

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
 Data File : PL062415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 20:52
 Operator : DD\AJ
 Sample : L4432-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:27:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	34717798	53617403	19.946	19.024
28)	SA Decachlor...	8.123	8.992	28270099	39943715	15.454	14.553
Target Compounds							
2)	A alpha-BHC	0.000	4.309f	0	5776776	N.D.	1.378 #
6)	B beta-BHC	4.375	0.000	531709	0	0.553	N.D. #
7)	B delta-BHC	0.000	4.984f	0	6613957	N.D.	1.907 #
8)	B Heptachlo...	5.112	5.802	6786447	3546020	3.714	1.091 #
10)	B gamma-Chl...	0.000	6.080f	0	800827	N.D.	0.244 #
11)	B alpha-Chl...	0.000	6.096f	0	158839	N.D.	0.049 #
15)	B Endosulfa...	0.000	6.870	0	4926223	N.D.	1.815 #
25)	Chlordane-3	0.000	6.080f	0	800827	N.D.	1.956 #
26)	Chlordane-4	0.000	6.096f	0	158839	N.D.	0.321 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
Data File : PL062415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 20:52
Operator : DD\AJ
Sample : L4432-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:27:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

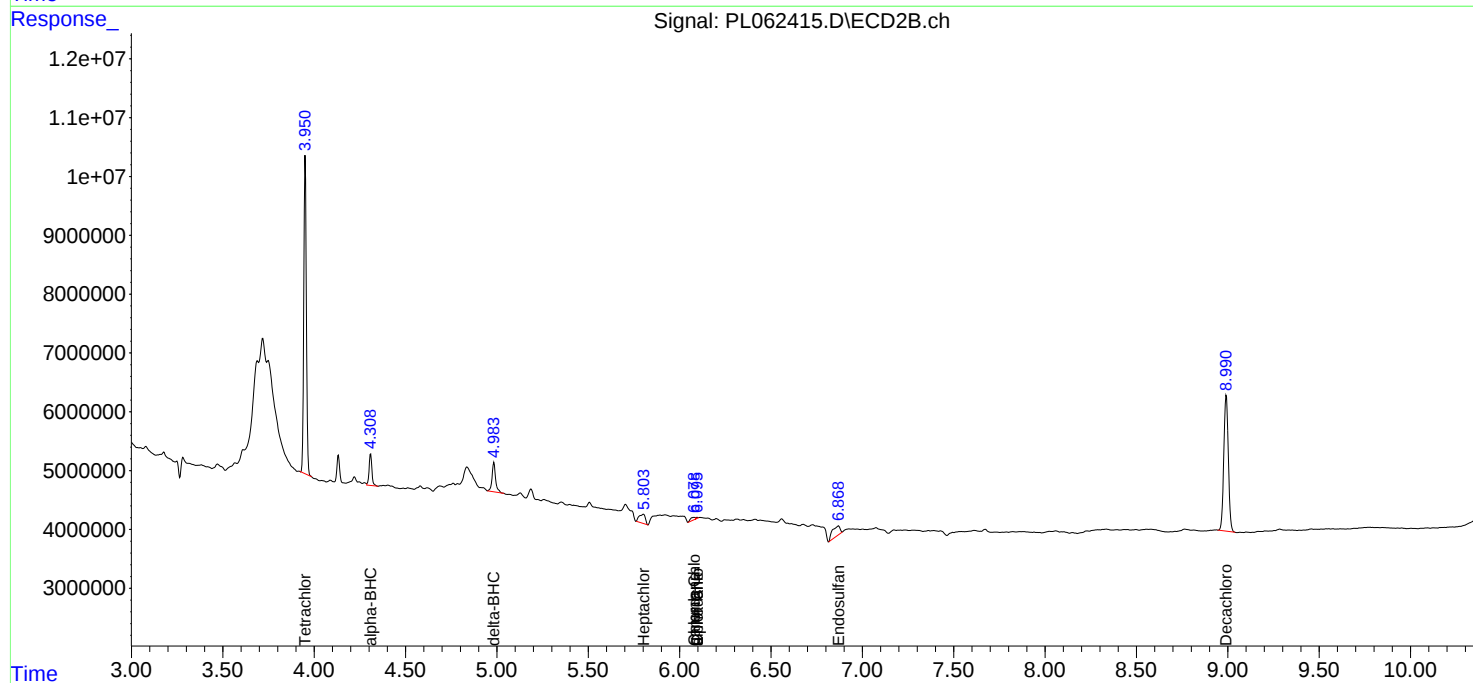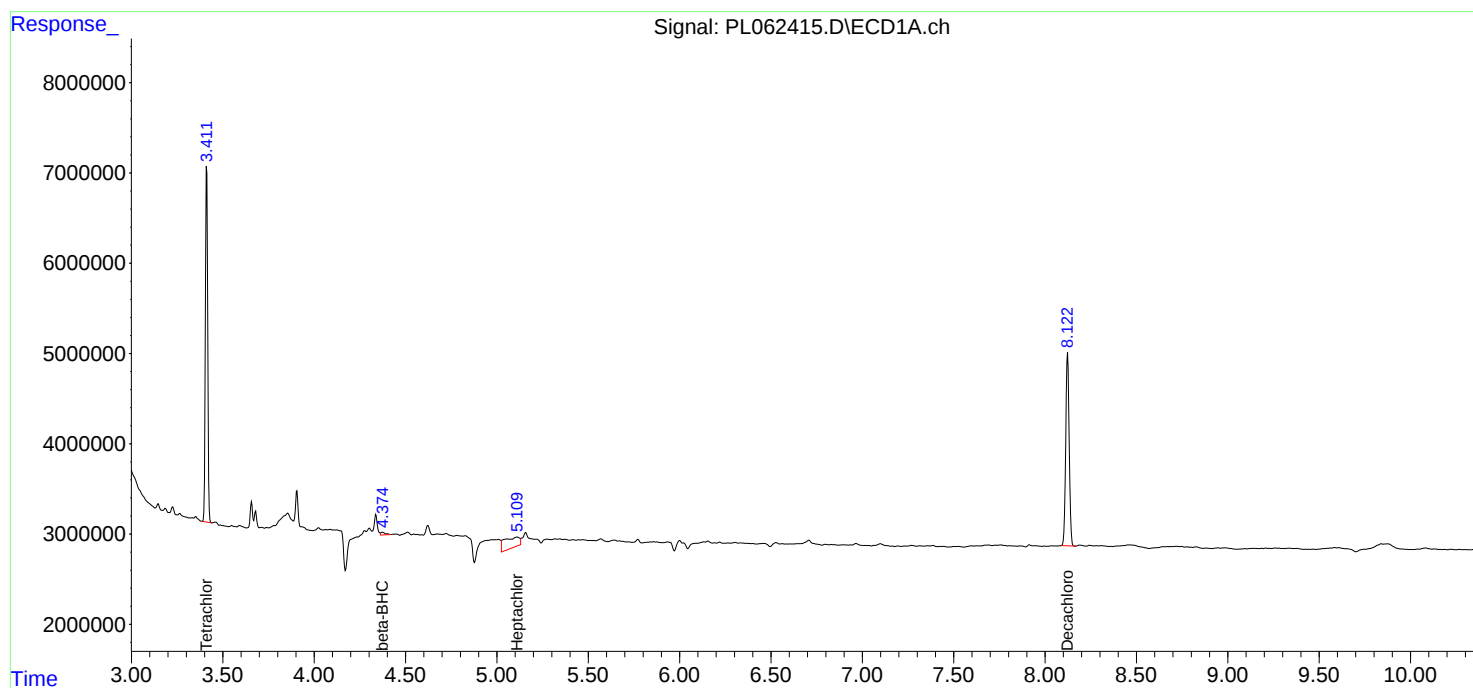


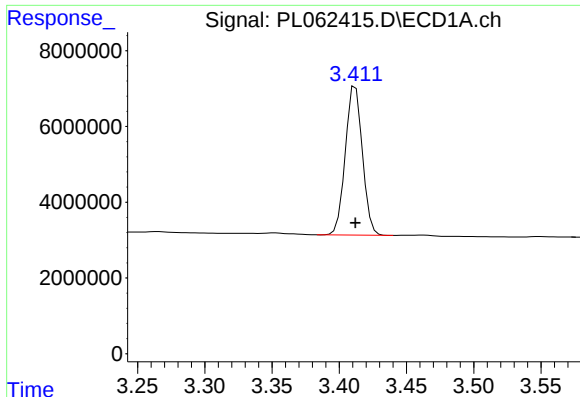

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 34717798
Conc: 19.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

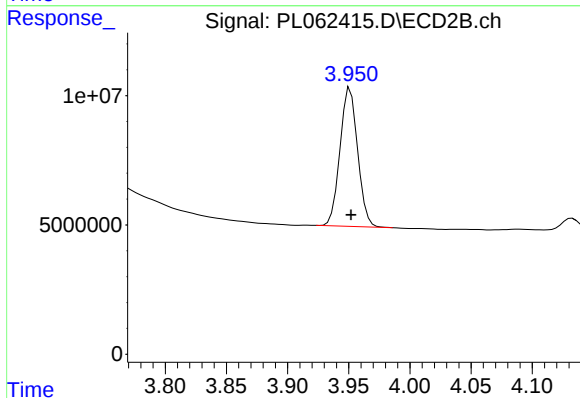


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 53617403
Conc: 19.02 ng/ml

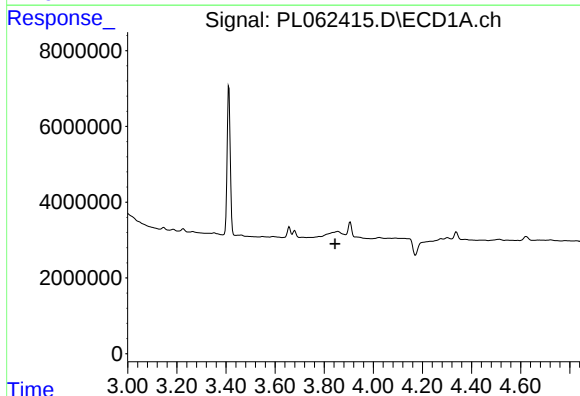


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.845 min
Response: 0
Conc: N.D.

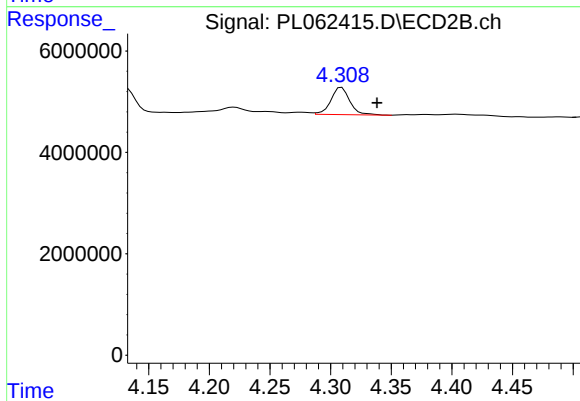

#2 alpha-BHC


R.T.: 4.309 min
Delta R.T.: -0.029 min
Response: 5776776
Conc: 1.38 ng/ml

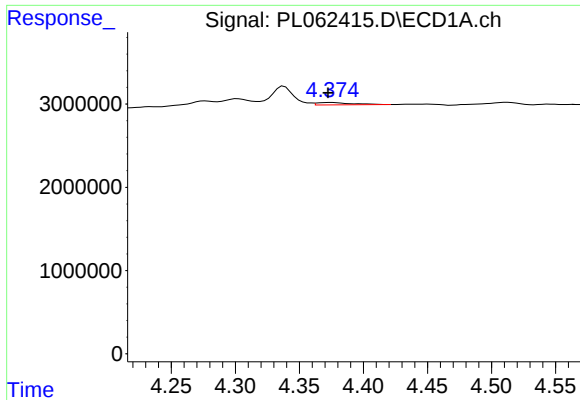

#6 beta-BHC


R.T.: 4.375 min
Delta R.T.: 0.003 min
Response: 531709
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

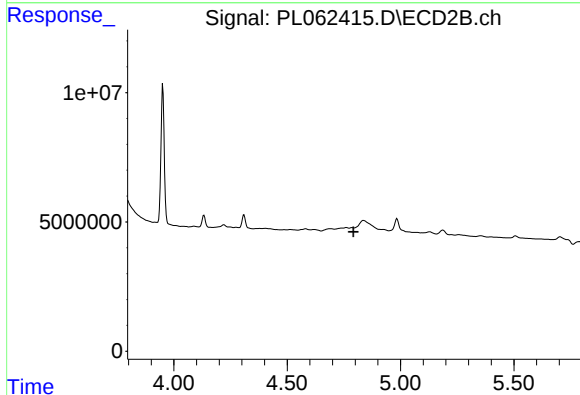


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

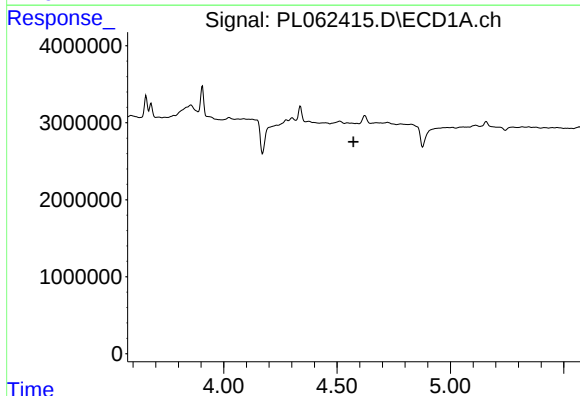


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

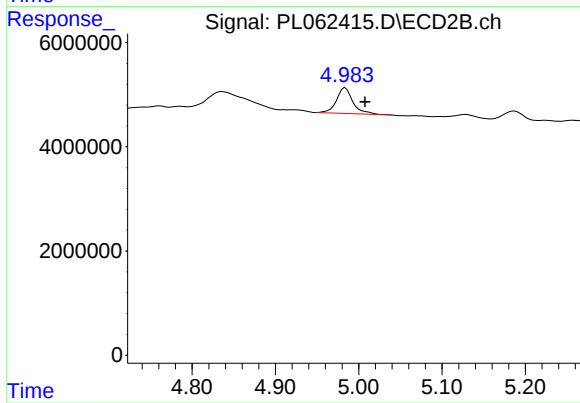

#7 delta-BHC


R.T.: 4.984 min
Delta R.T.: -0.024 min
Response: 6613957
Conc: 1.91 ng/ml

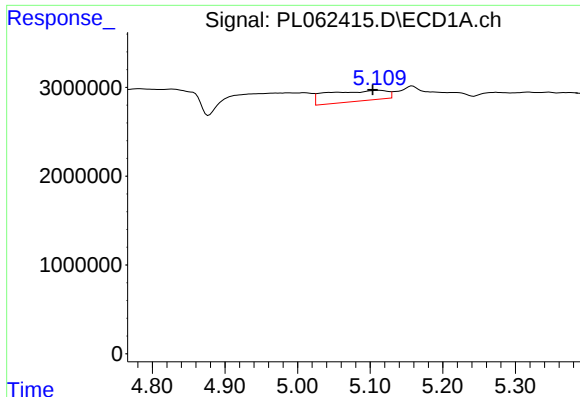

#8 Heptachlor epoxide


R.T.: 5.112 min
Delta R.T.: 0.009 min
Response: 6786447
Conc: 3.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

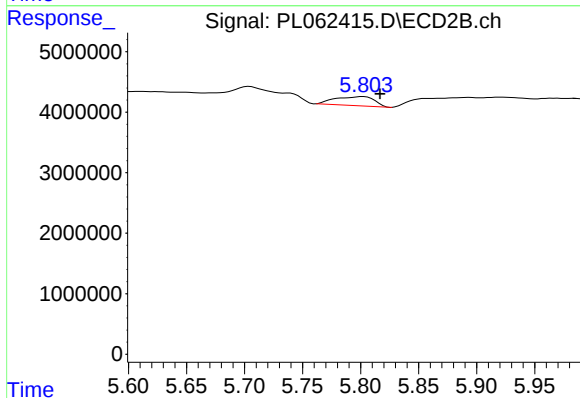


#8 Heptachlor epoxide

R.T.: 5.802 min
Delta R.T.: -0.014 min
Response: 3546020
Conc: 1.09 ng/ml

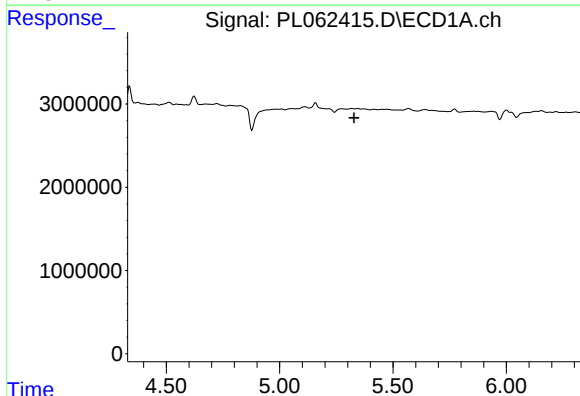


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

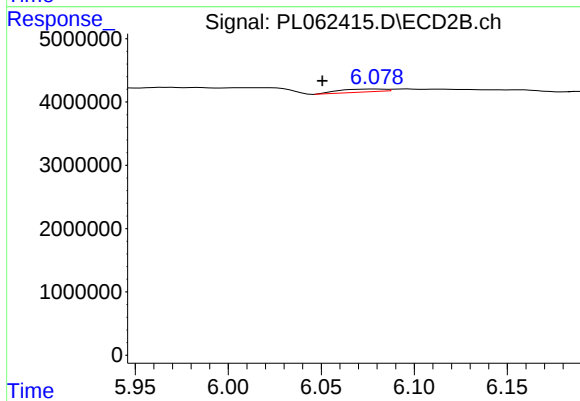

#10 gamma-Chlordane


R.T.: 6.080 min
Delta R.T.: 0.029 min
Response: 800827
Conc: 0.24 ng/ml

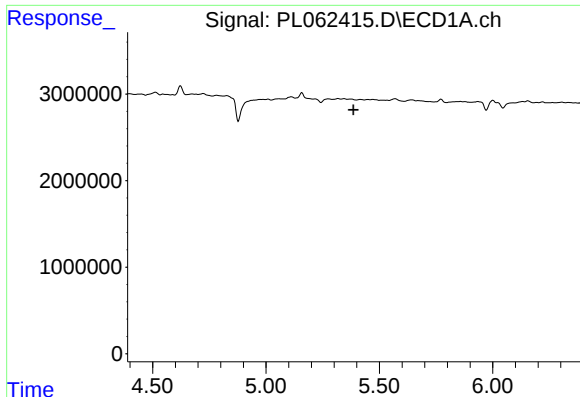

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

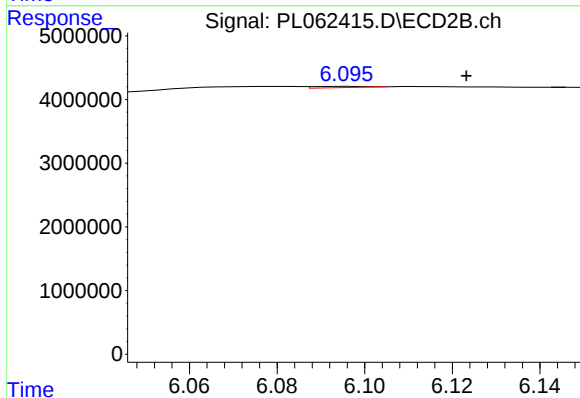


#11 alpha-Chlordane

R.T.: 6.096 min
Delta R.T.: -0.027 min
Response: 158839
Conc: 0.05 ng/ml

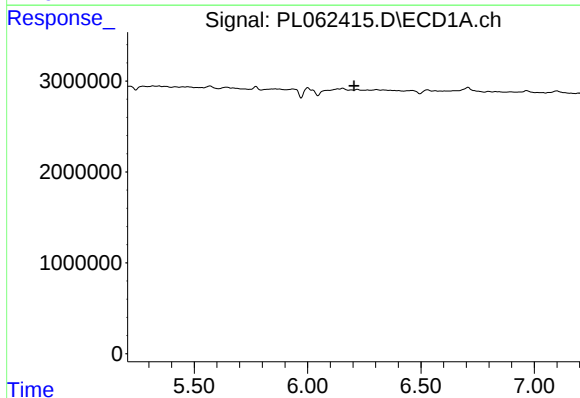


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

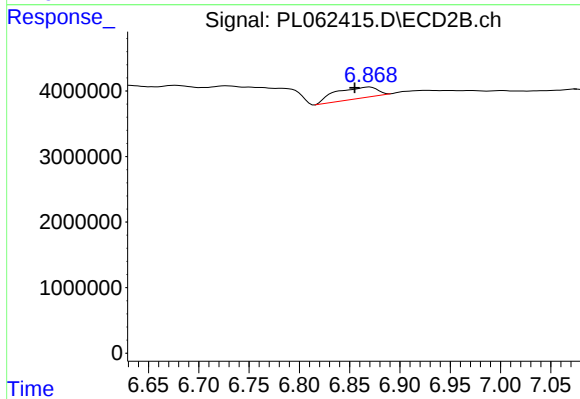

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 4926223
Conc: 1.82 ng/ml

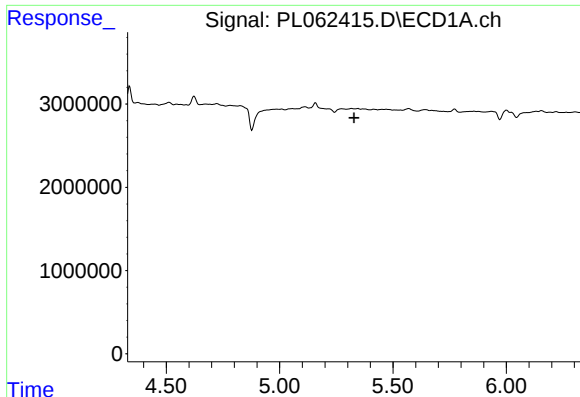

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

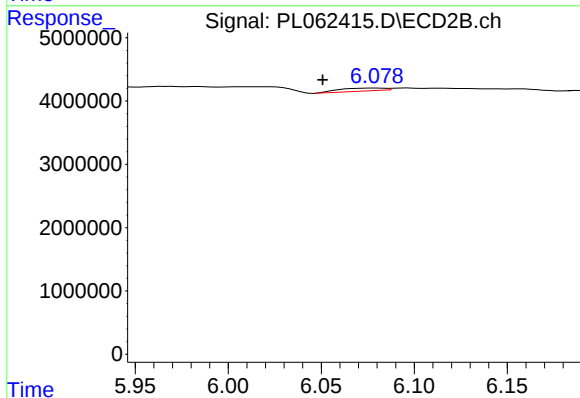


#25 Chlordane-3

R.T.: 6.080 min
Delta R.T.: 0.029 min
Response: 800827
Conc: 1.96 ng/ml

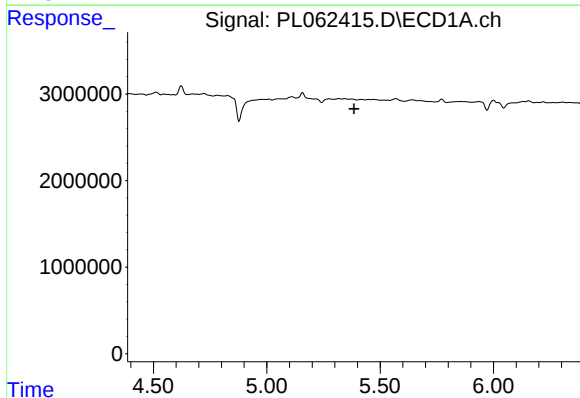


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

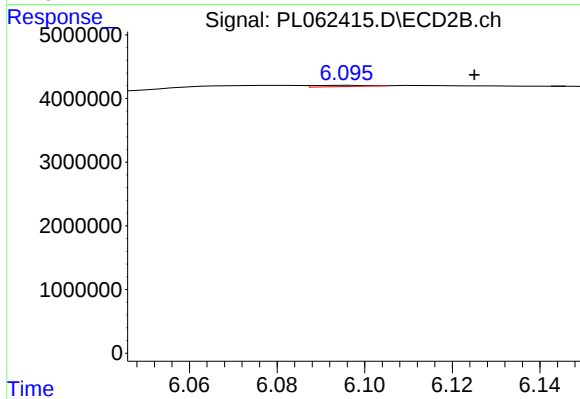

#26 Chlordane-4


R.T.: 6.096 min
Delta R.T.: -0.029 min
Response: 158839
Conc: 0.32 ng/ml

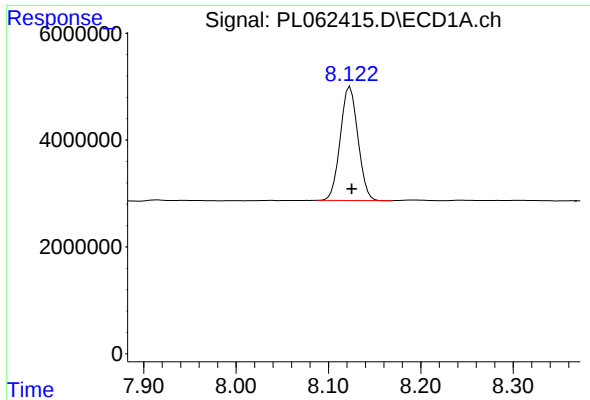

#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: -0.002 min
Response: 28270099
Conc: 15.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

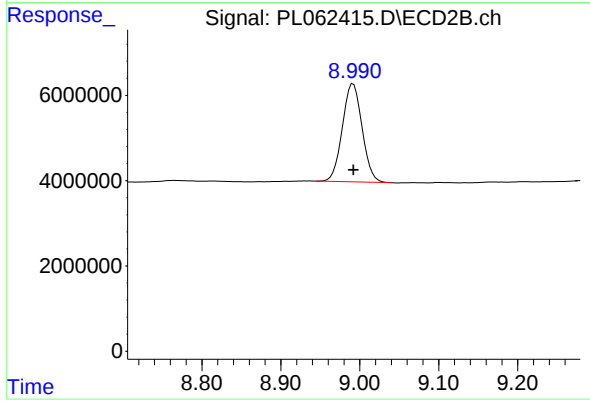

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 39943715
Conc: 14.55 ng/ml