

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
 Data File : PL062378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 10:09
 Operator : DD\AJ
 Sample : L4392-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 10/19/2020 3:05:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 02:20:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 13 05:04:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.949	21086332	28939395	12.114	10.268m
28)	SA Decachlor...	8.125	8.991	27755160	37972077	15.173	13.834
Target Compounds							
14)	MA Endrin	5.933	6.640	1433963	2398448	0.933m	0.964

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101720\
Data File : PL062378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 10:09
Operator : DD\AJ
Sample : L4392-06
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
10/19/2020 3:05:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 02:20:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101320.M
Quant Title : GC Extractables
QLast Update : Tue Oct 13 05:04:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

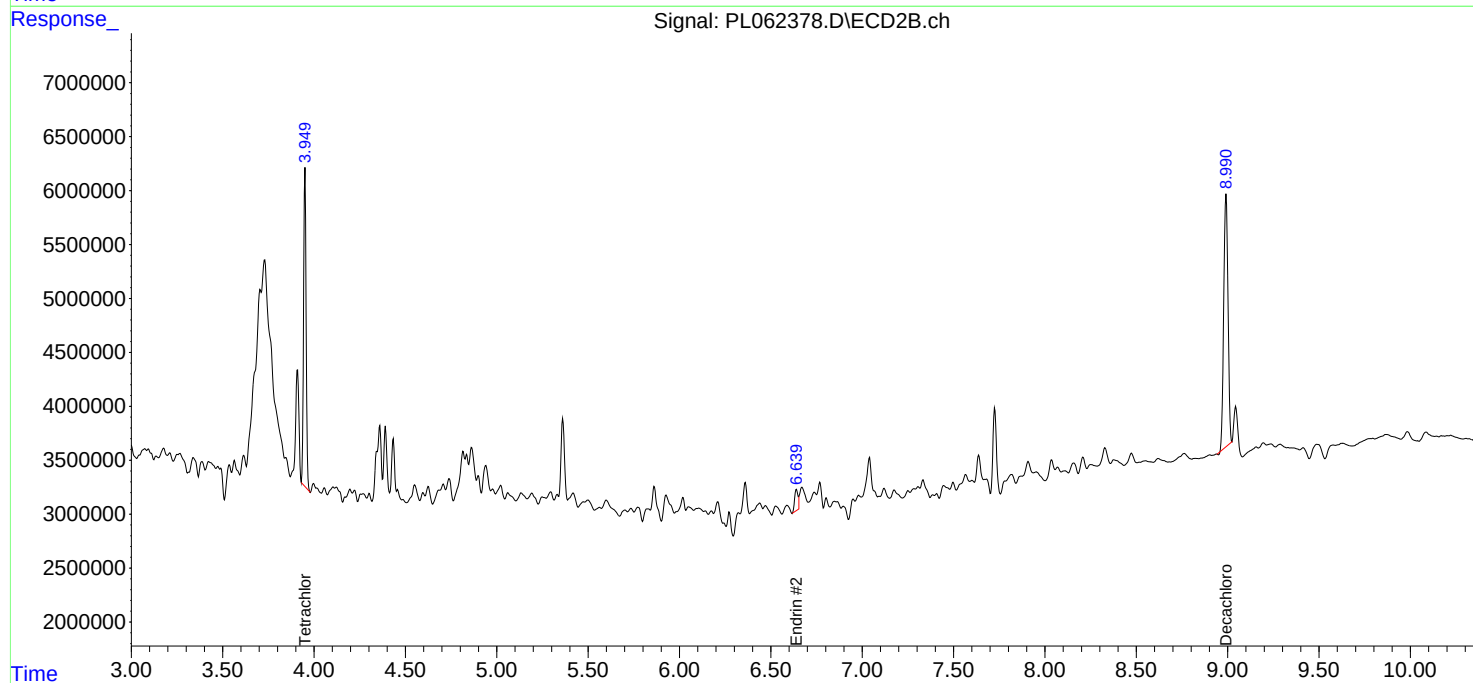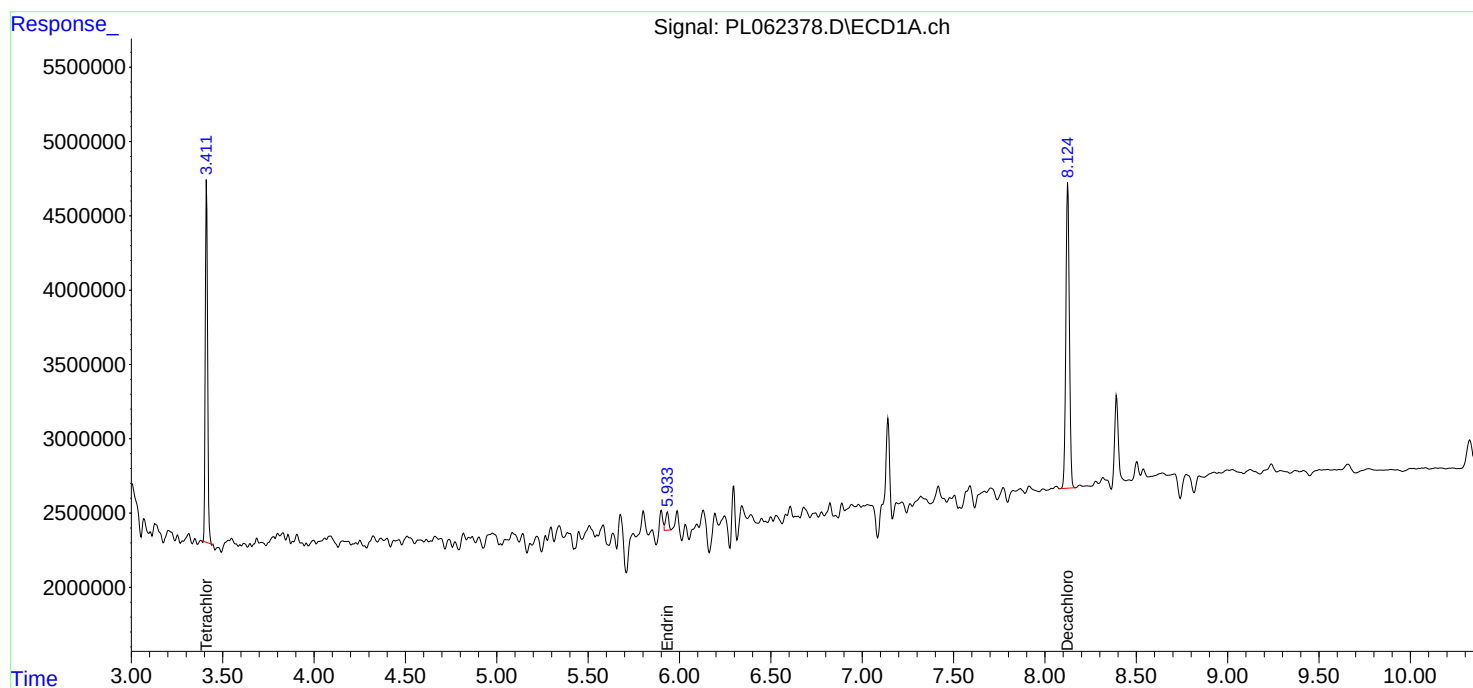

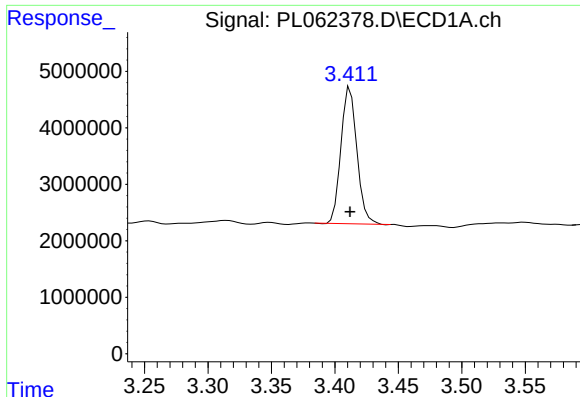


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 21086332
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
10/19/2020 3:05:49 PM

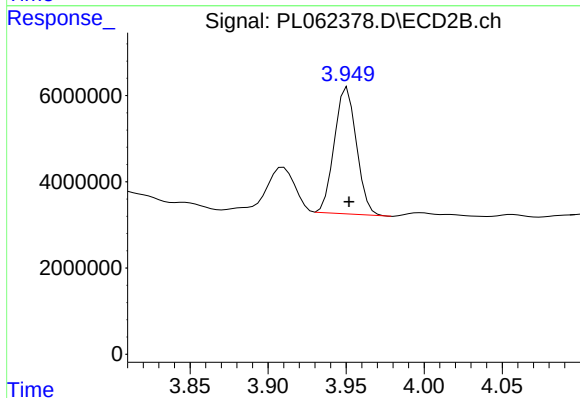


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.003 min
Response: 28939395
Conc: 10.27 ng/ml m

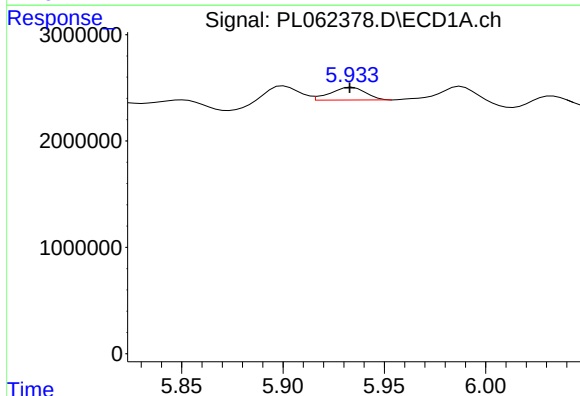


#14 Endrin

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 1433963
Conc: 0.93 ng/ml m

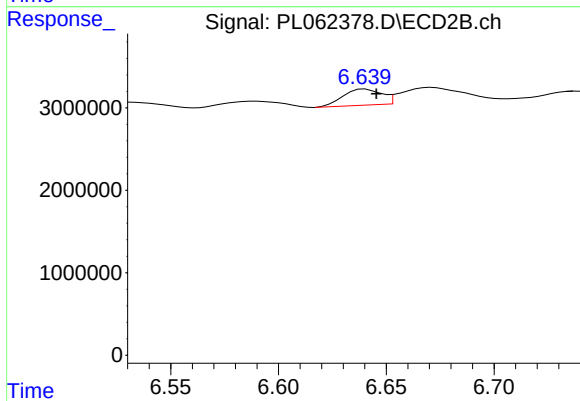

#14 Endrin

R.T.: 6.640 min
Delta R.T.: -0.005 min
Response: 2398448
Conc: 0.96 ng/ml

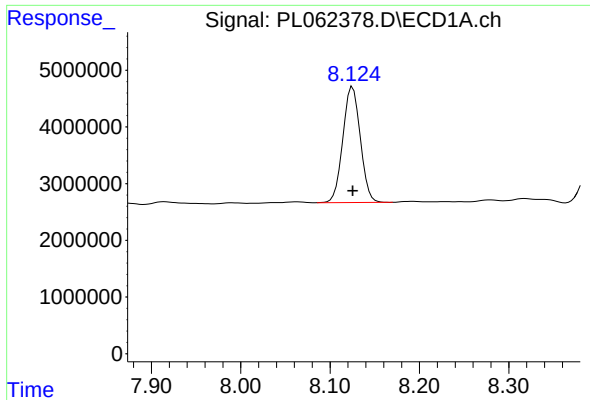


#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 27755160
Conc: 15.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
10/19/2020 3:05:49 PM

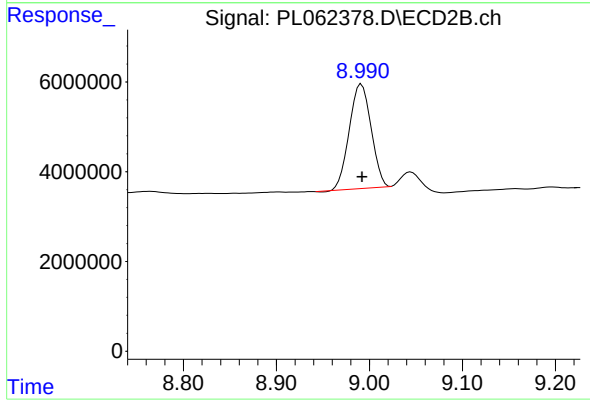

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.000 min
Response: 37972077
Conc: 13.83 ng/ml