

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101722\
 Data File : PL078395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2022 13:29
 Operator : AR\AJ
 Sample : N5122-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 QUARTERLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/18/2022
 Supervised By :Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 23:53:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.413	2.619	29125908	32907891	17.624m	12.450 #
28) SA Decachlor...	8.908	7.716	20462910	37362342	13.255	17.187 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101722\
Data File : PL078395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2022 13:29
Operator : AR\AJ
Sample : N5122-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/18/2022
Supervised By : Ankita Jodhani 10/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 23:53:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

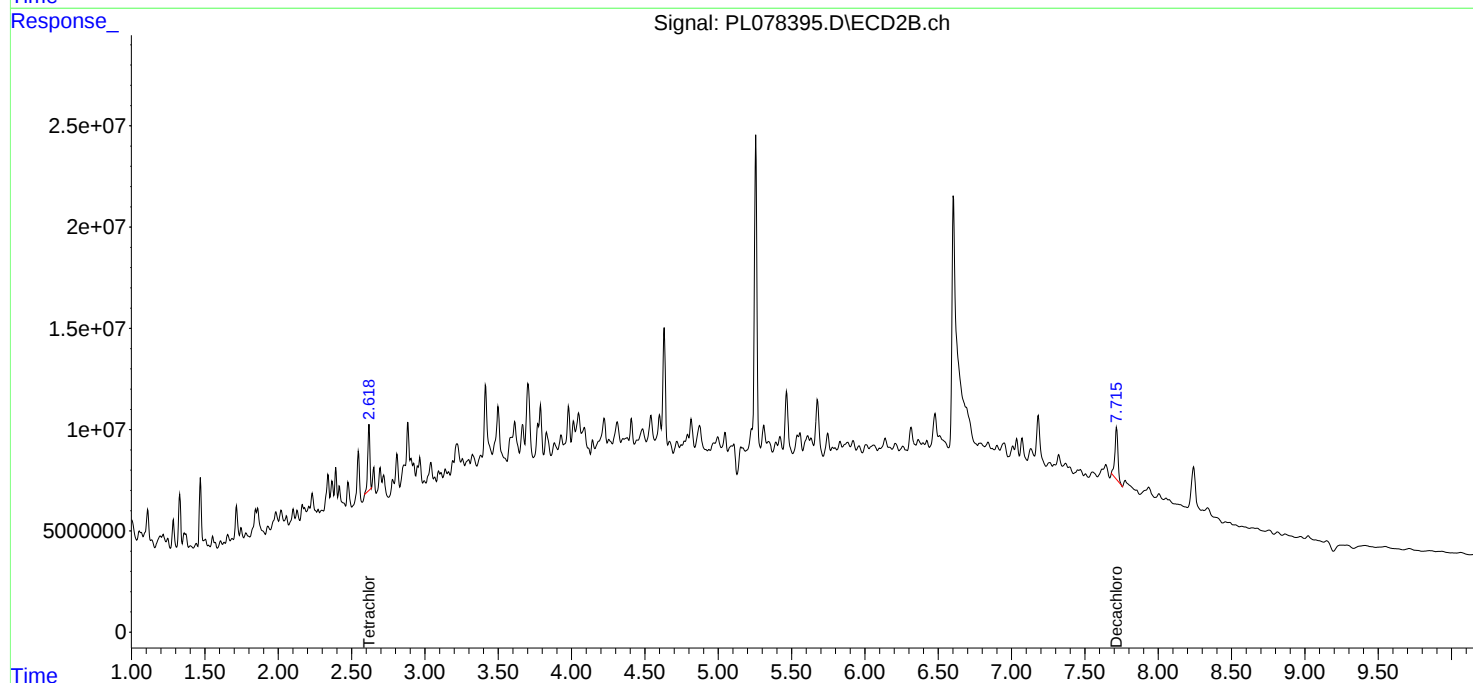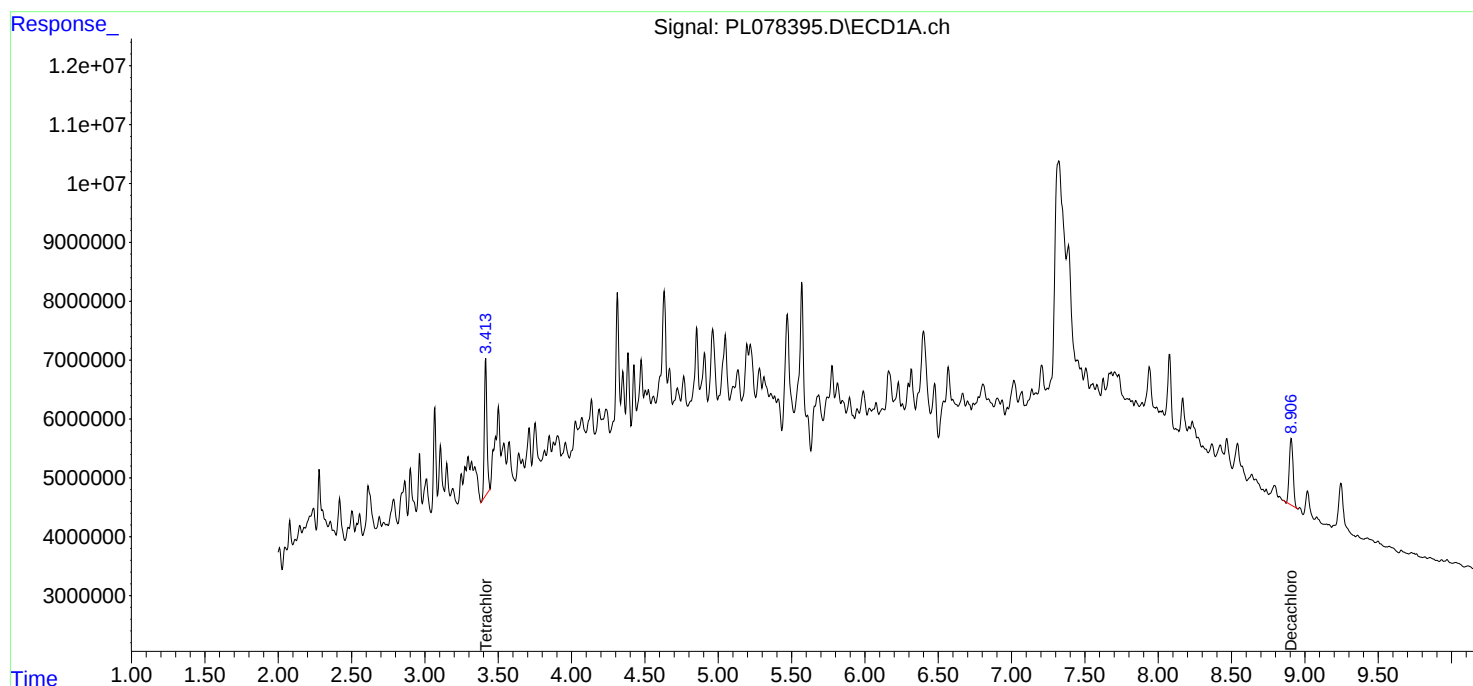

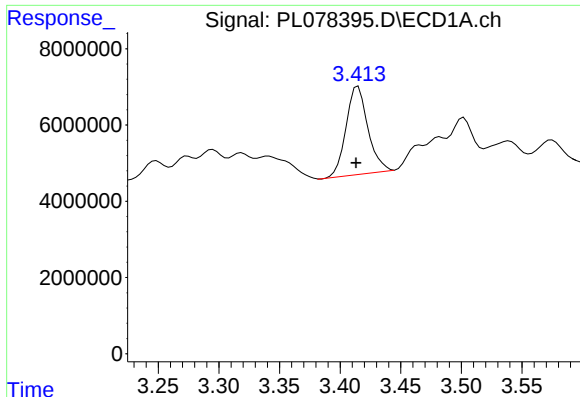


#1 Tetrachloro-m-xylene

R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 29125908
Conc: 17.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/18/2022
Supervised By :Ankita Jodhani 10/19/2022

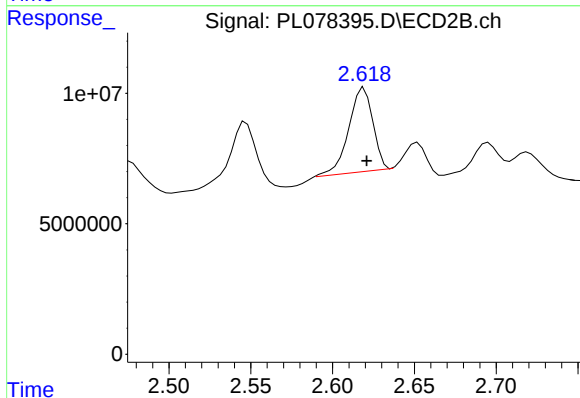


#1 Tetrachloro-m-xylene

R.T.: 2.619 min
Delta R.T.: -0.002 min
Response: 32907891
Conc: 12.45 ng/ml

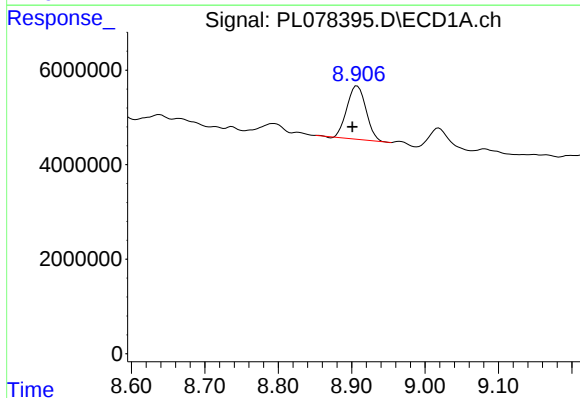

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.006 min
Response: 20462910
Conc: 13.25 ng/ml

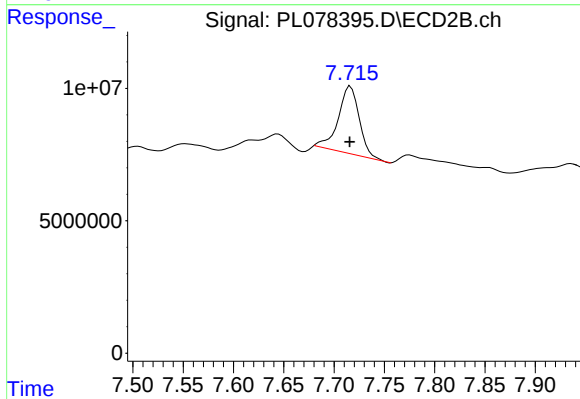

#28 Decachlorobiphenyl

R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 37362342
Conc: 17.19 ng/ml