

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101724\
 Data File : PL092443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 16:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 03:44:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.781	48636883	54567169	21.863	21.757
28)	SA Decachlor...	9.057	7.919	35705494	46682875	21.795	18.659
Target Compounds							
2)	A alpha-BHC	0.000	3.270f	0	152831	N.D.	0.042 #
4)	MA Heptachlor	0.000	3.950	0	188726	N.D.	0.055 #
5)	MB Aldrin	0.000	4.239	0	2335450	N.D.	0.687 #
6)	B beta-BHC	0.000	3.918	0	629831	N.D.	0.419 #
7)	B delta-BHC	4.765	4.143	5873092	497553	2.036	0.143 #
8)	B Heptachlo...	0.000	4.757f	0	1003167	N.D.	0.332 #
14)	MA Endrin	0.000	5.643	0	418007	N.D.	0.159 #
17)	MA 4,4'-DDT	0.000	6.040	0	4014932	N.D.	1.736 #
22)	Mirex	0.000	7.055f	0	417278	N.D.	0.172 #
23)	Chlordane-1	0.000	3.771	0	428420	N.D.	4.285 #
24)	Chlordane-2	0.000	4.359	0	53950	N.D.	0.481 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101724\
Data File : PL092443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 16:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 03:44:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

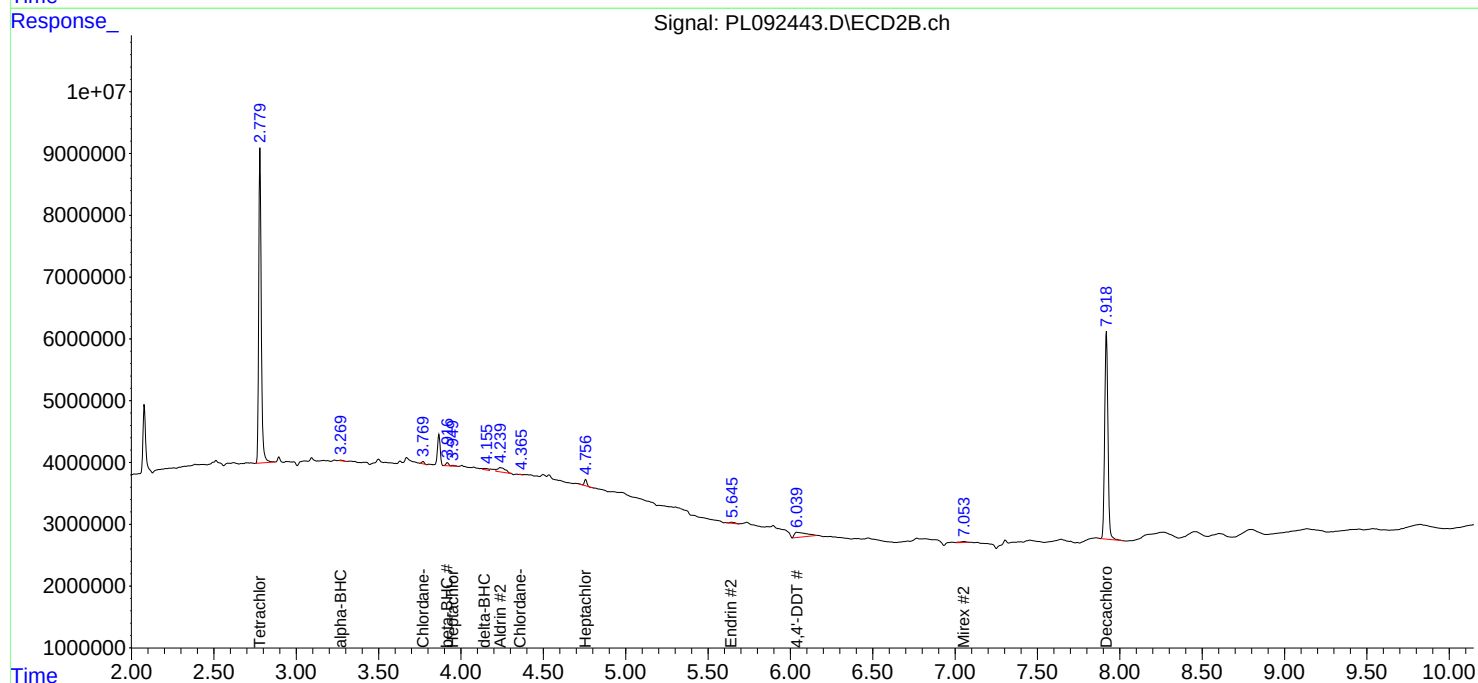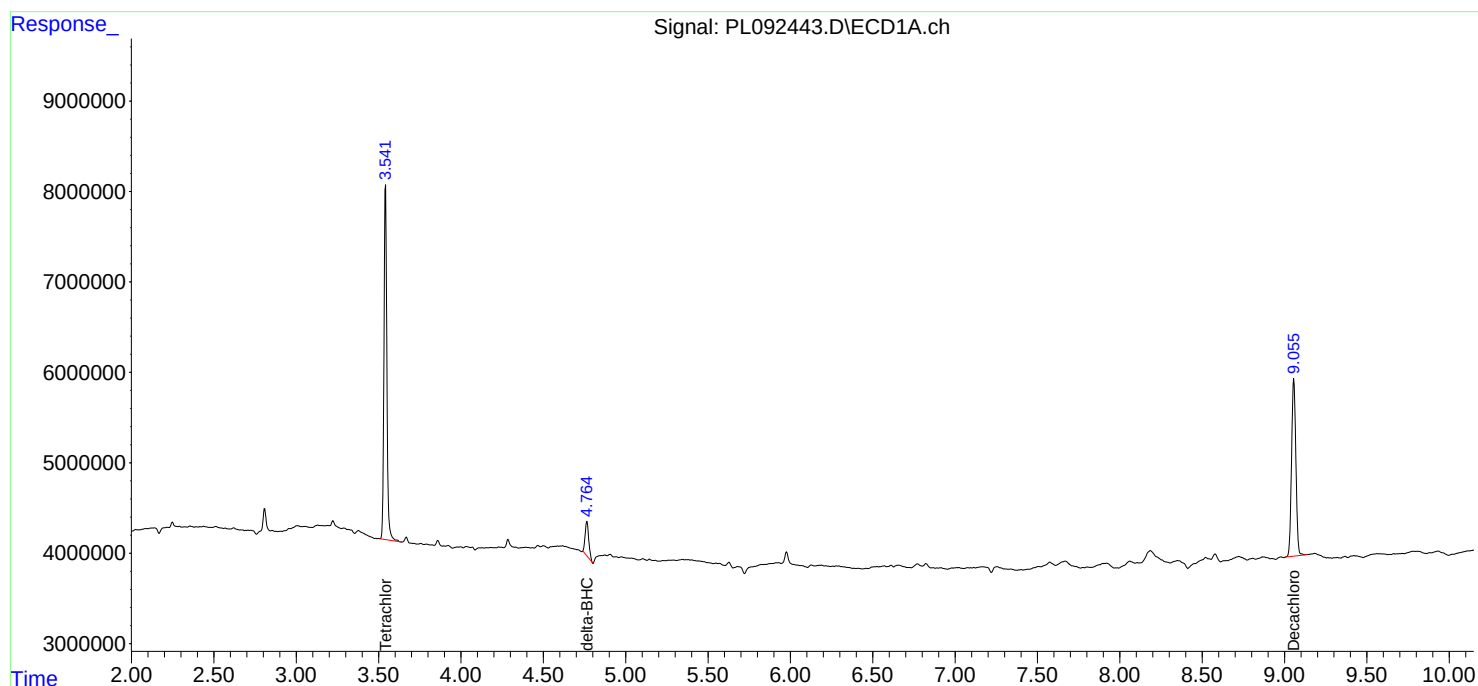


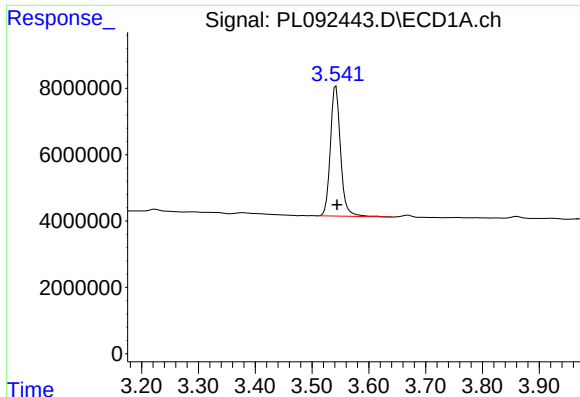

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 48636883
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

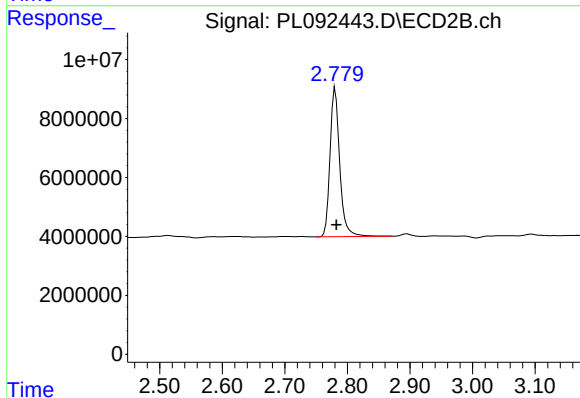


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.002 min
Response: 54567169
Conc: 21.76 ng/ml

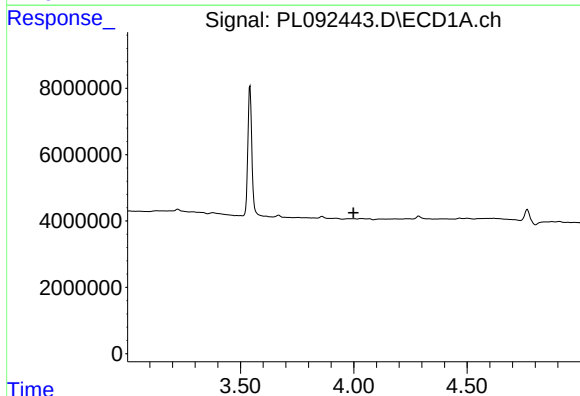


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.999 min
Response: 0
Conc: N.D.

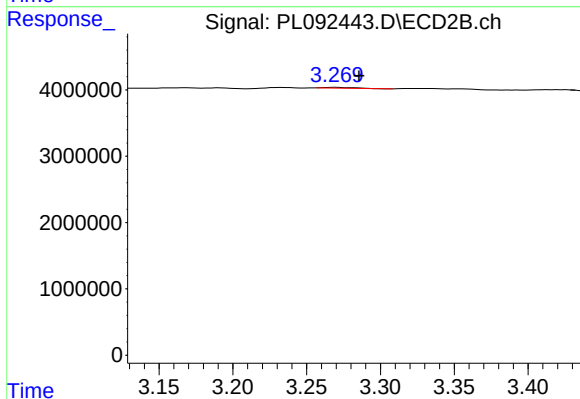

#2 alpha-BHC


R.T.: 3.270 min
Delta R.T.: -0.015 min
Response: 152831
Conc: 0.04 ng/ml

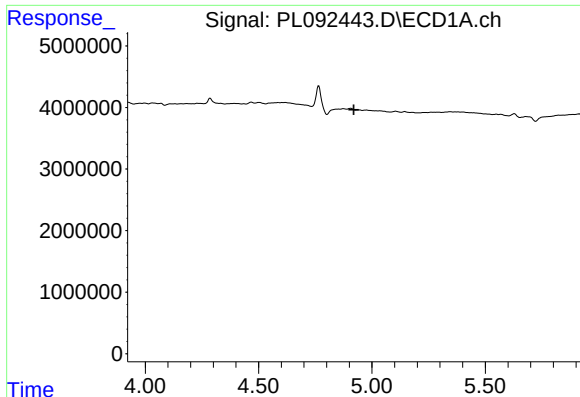

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

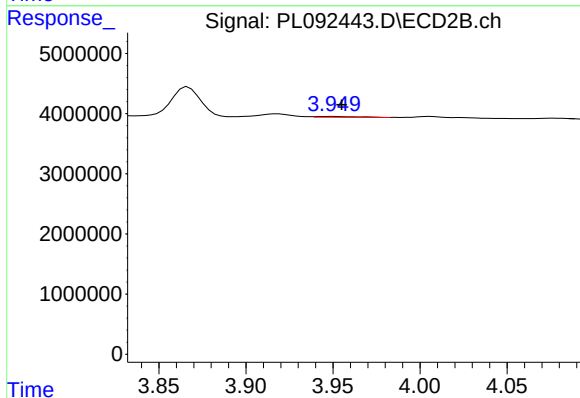


#4 Heptachlor

R.T.: 3.950 min
Delta R.T.: -0.005 min
Response: 188726
Conc: 0.05 ng/ml

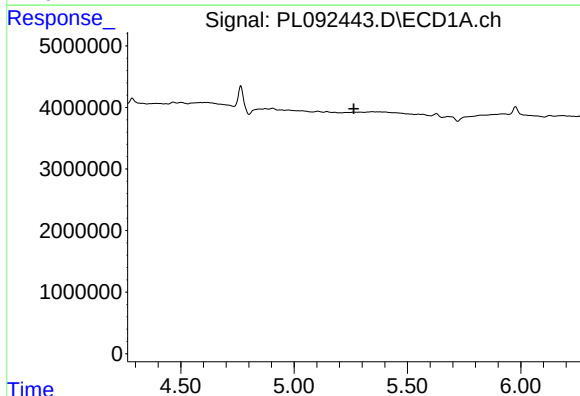


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.263 min
Response: 0
Conc: N.D.

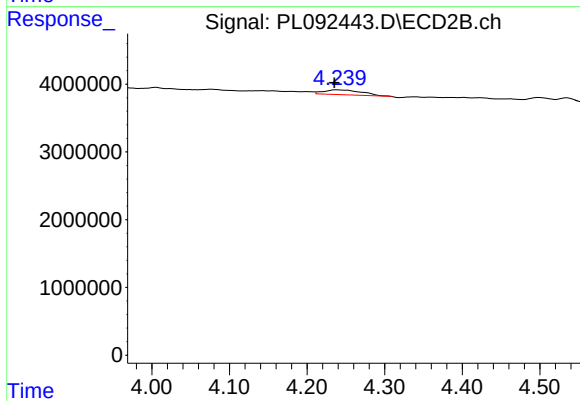

#5 Aldrin


R.T.: 4.239 min
Delta R.T.: 0.003 min
Response: 2335450
Conc: 0.69 ng/ml

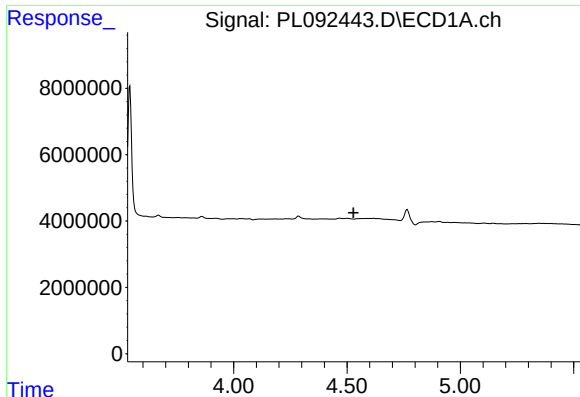

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

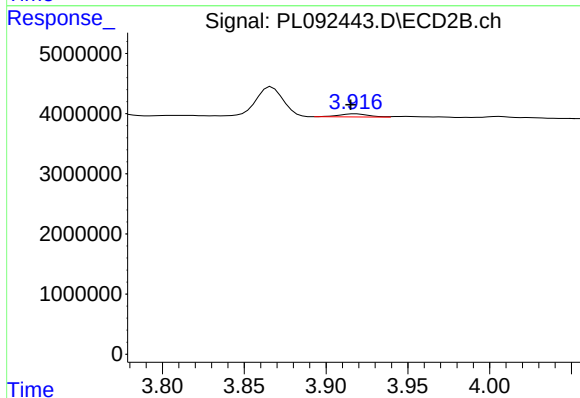


#6 beta-BHC

R.T.: 3.918 min
Delta R.T.: 0.003 min
Response: 629831
Conc: 0.42 ng/ml

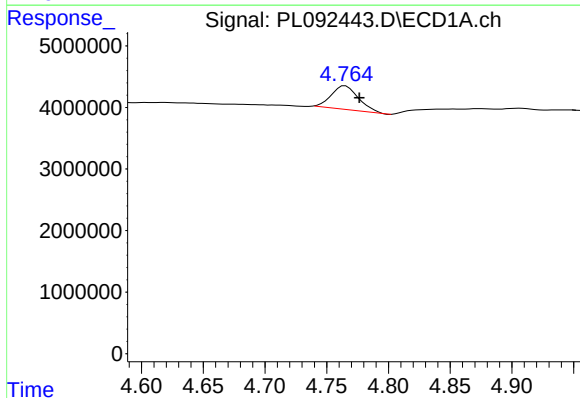


#7 delta-BHC

R.T.: 4.765 min
Delta R.T.: -0.011 min
Response: 5873092
Conc: 2.04 ng/ml

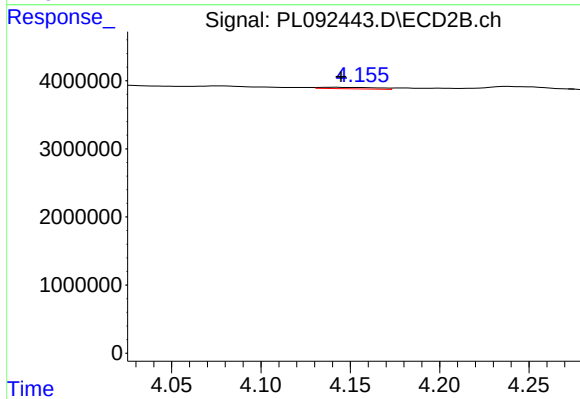

#7 delta-BHC


R.T.: 4.143 min
Delta R.T.: -0.002 min
Response: 497553
Conc: 0.14 ng/ml

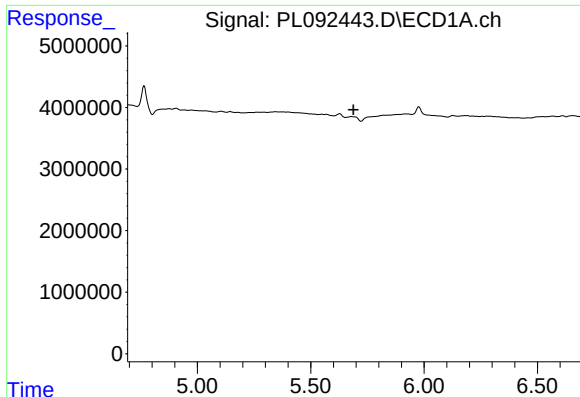

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

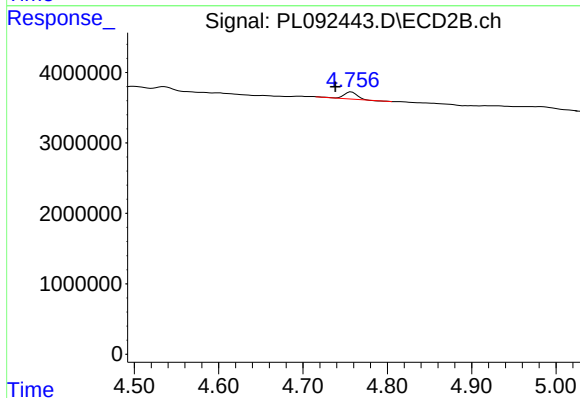


#8 Heptachlor epoxide

R.T.: 4.757 min
Delta R.T.: 0.019 min
Response: 1003167
Conc: 0.33 ng/ml

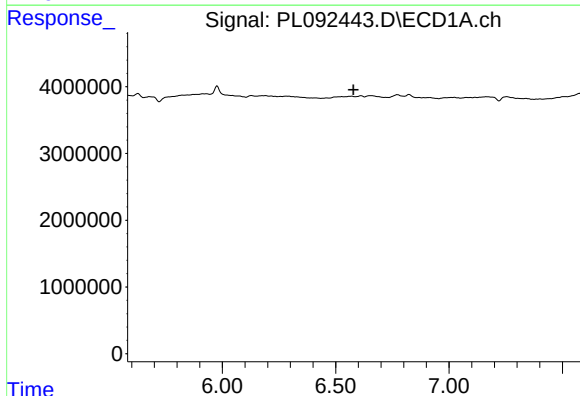


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.579 min
Response: 0
Conc: N.D.

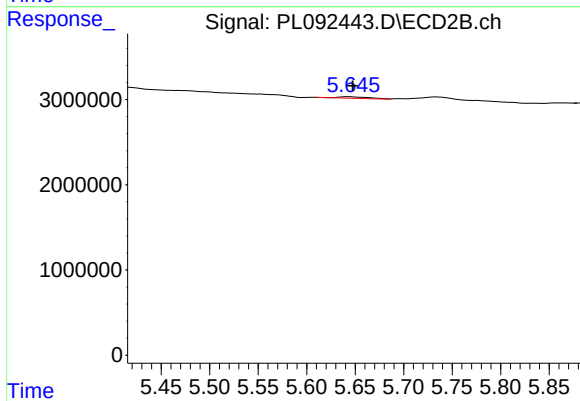

#14 Endrin


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 418007
Conc: 0.16 ng/ml

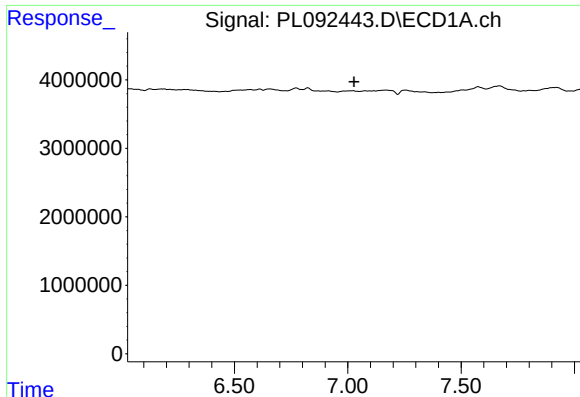

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

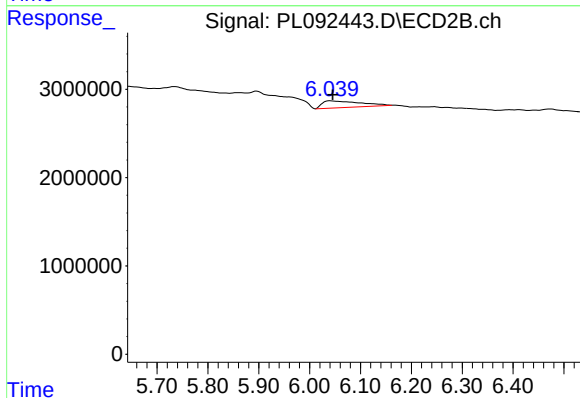


#17 4,4'-DDT

R.T.: 6.040 min
Delta R.T.: -0.006 min
Response: 4014932
Conc: 1.74 ng/ml

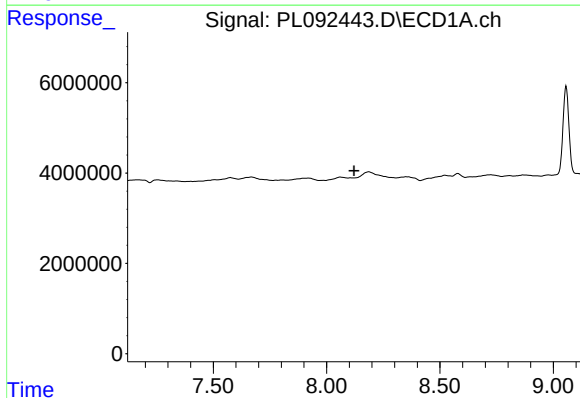


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

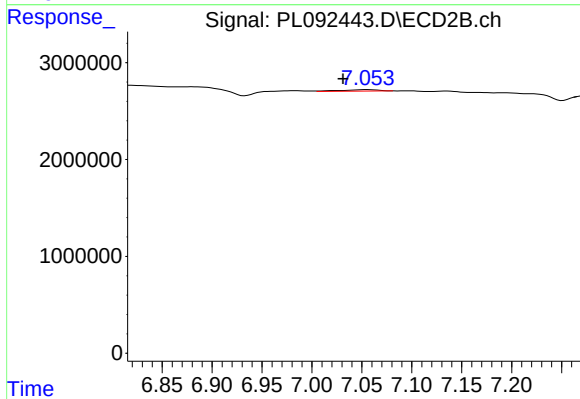

#22 Mirex


R.T.: 7.055 min
Delta R.T.: 0.024 min
Response: 417278
Conc: 0.17 ng/ml

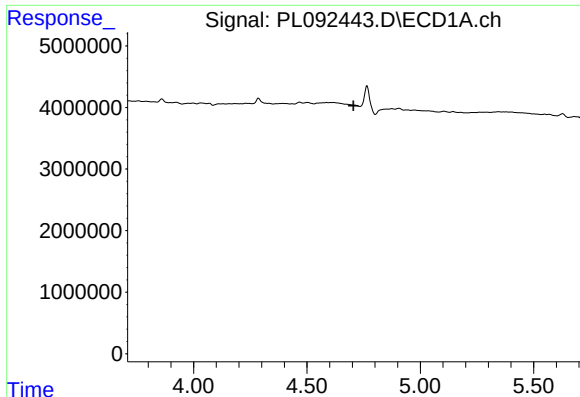

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

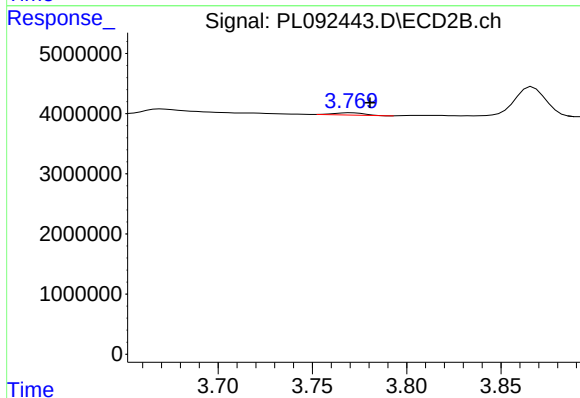


#23 Chlordane-1

R.T.: 3.771 min
Delta R.T.: -0.010 min
Response: 428420
Conc: 4.29 ng/ml

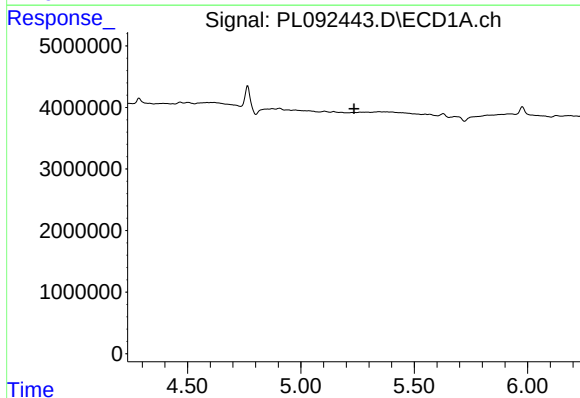


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.235 min
Response: 0
Conc: N.D.

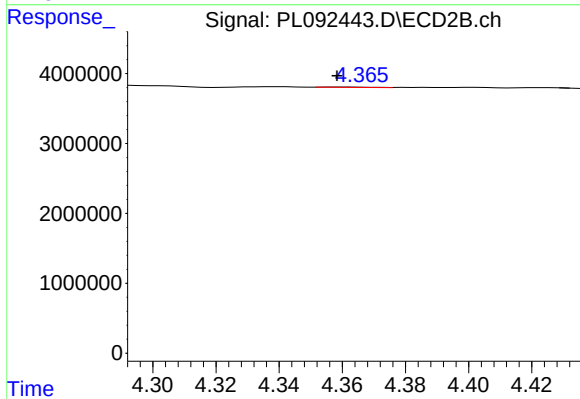

#24 Chlordane-2


R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 53950
Conc: 0.48 ng/ml

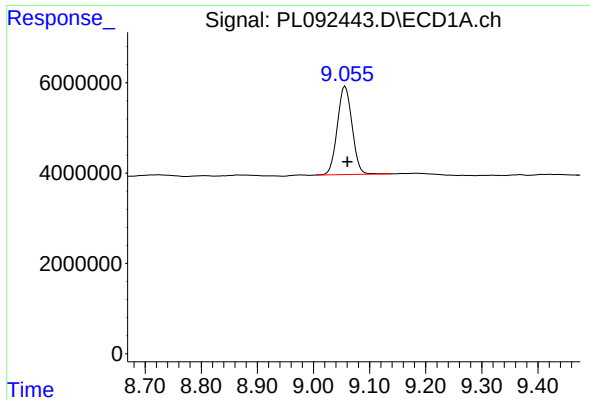

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.004 min
Response: 35705494
Conc: 21.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

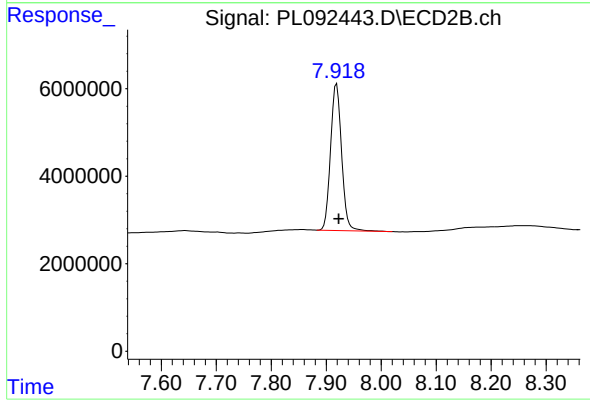

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.004 min
Response: 46682875
Conc: 18.66 ng/ml