

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101724\
 Data File : PL092445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 16:30
 Operator : AR\AJ
 Sample : PB164207BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164207BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 03:45:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.780	43742425	49348437	19.663	19.676
28)	SA Decachlor...	9.057	7.919	32581404	43192769	19.888	17.264
Target Compounds							
2)	A alpha-BHC	0.000	3.285	0	175888	N.D.	0.048 #
5)	MB Aldrin	0.000	4.236	0	2593410	N.D.	0.763 #
6)	B beta-BHC	0.000	3.915	0	283106	N.D.	0.188 #
7)	B delta-BHC	0.000	4.145	0	977302	N.D.	0.282 #
8)	B Heptachlo...	0.000	4.758f	0	69228	N.D.	0.023 #
9)	A Endosulfan I	0.000	5.135f	0	1414041	N.D.	0.515 #
14)	MA Endrin	0.000	5.663f	0	1309905	N.D.	0.500 #
19)	B Endosulfa...	0.000	6.342	0	100105	N.D.	0.041 #
22)	Mirex	0.000	7.061f	0	8344	N.D.	0.003 #
24)	Chlordane-2	0.000	4.365	0	2352678	N.D.	20.964 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101724\
Data File : PL092445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 16:30
Operator : AR\AJ
Sample : PB164207BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164207BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 03:45:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

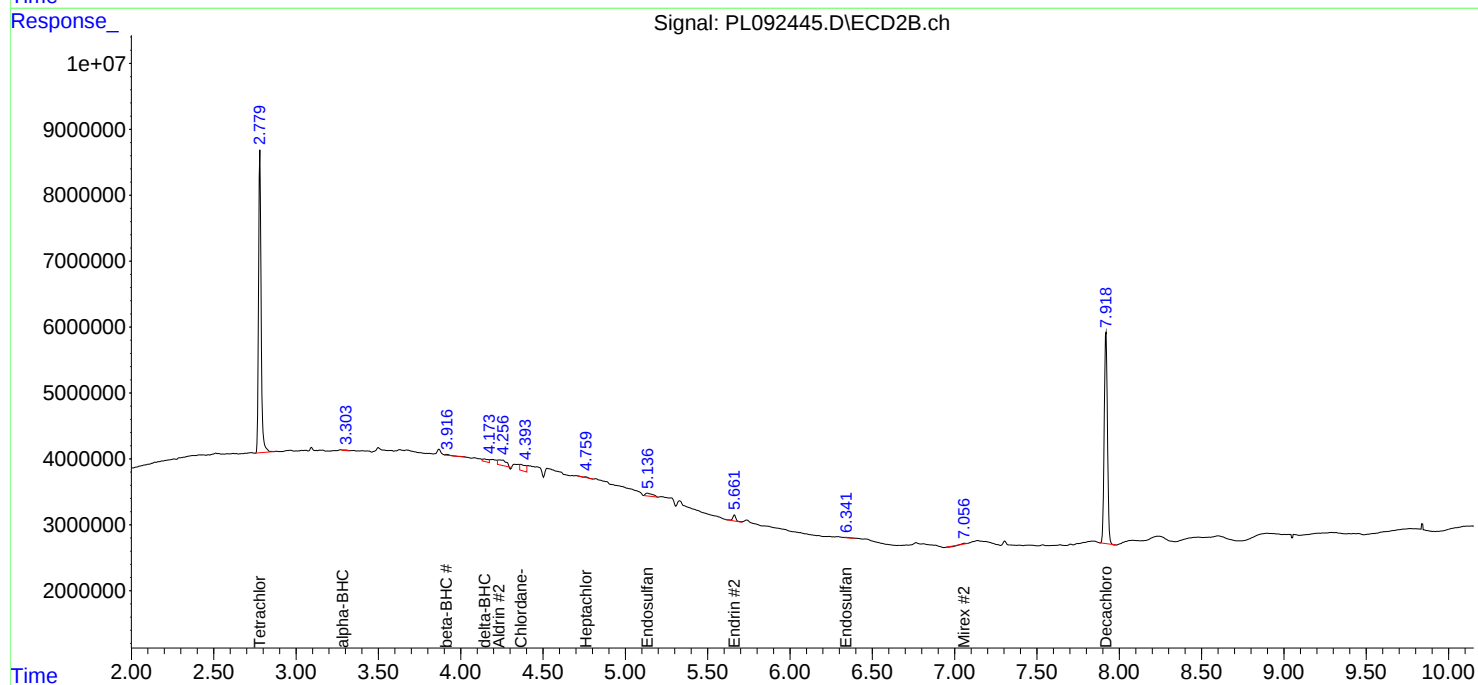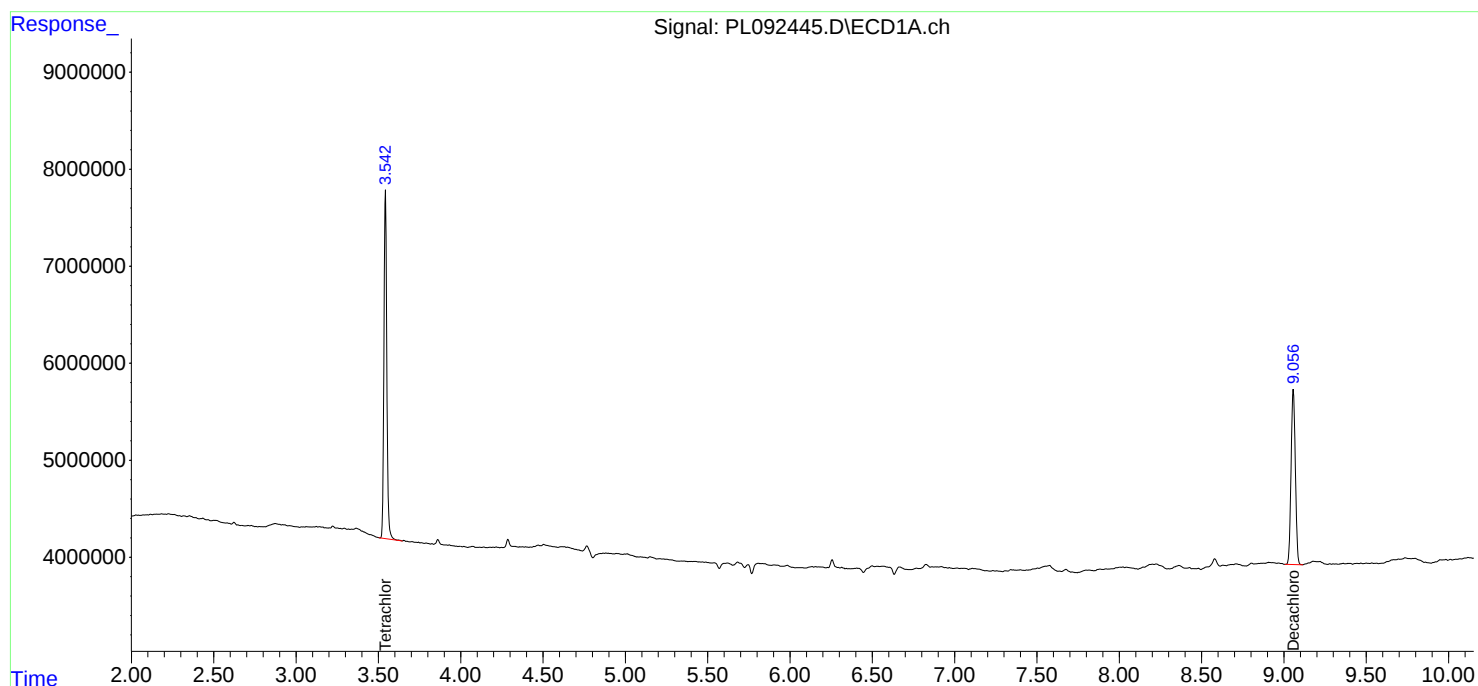


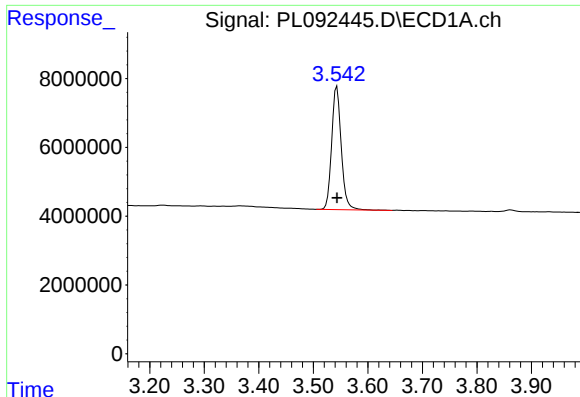

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 43742425
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164207BL

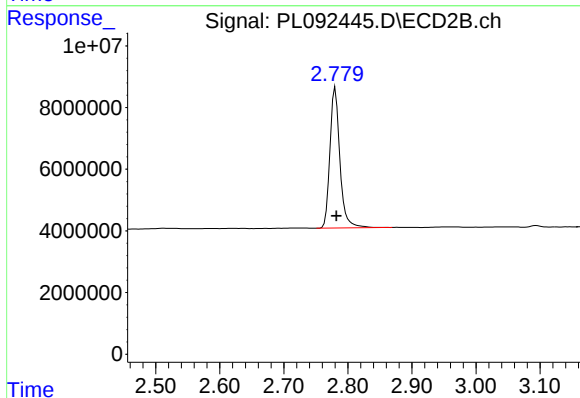


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.002 min
Response: 49348437
Conc: 19.68 ng/ml

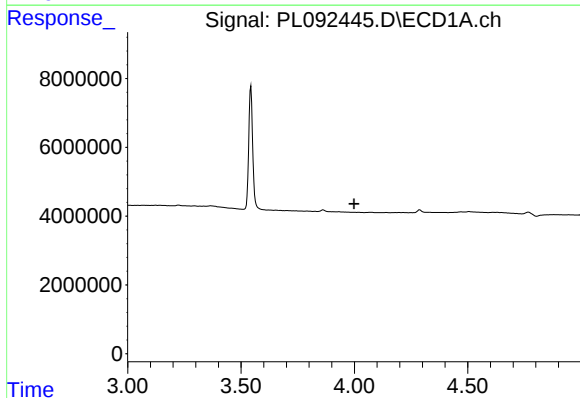


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.999 min
Response: 0
Conc: N.D.

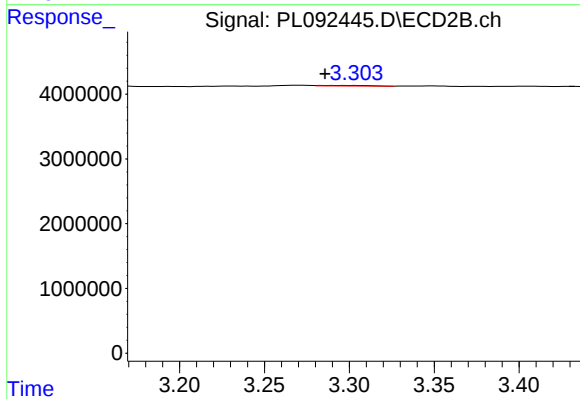

#2 alpha-BHC


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 175888
Conc: 0.05 ng/ml

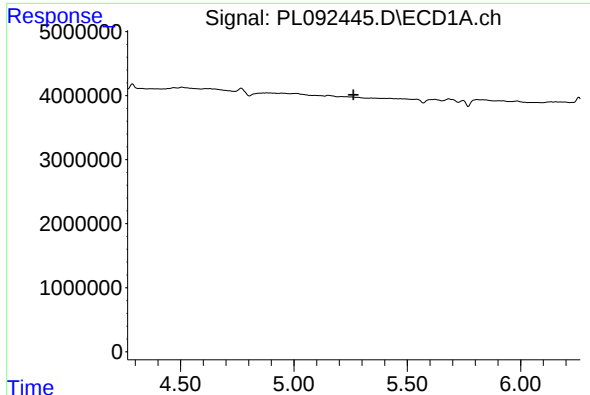

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164207BL

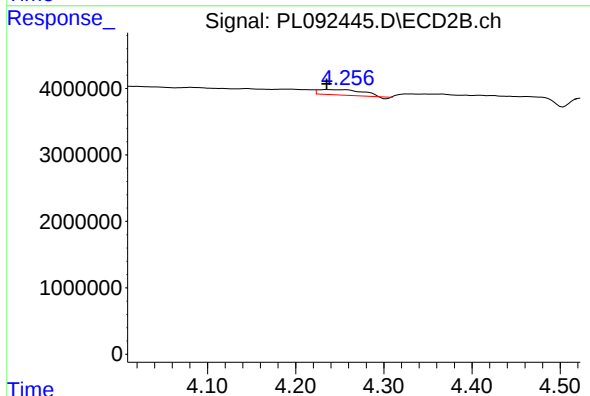


#5 Aldrin

R.T.: 4.236 min
Delta R.T.: 0.000 min
Response: 2593410
Conc: 0.76 ng/ml

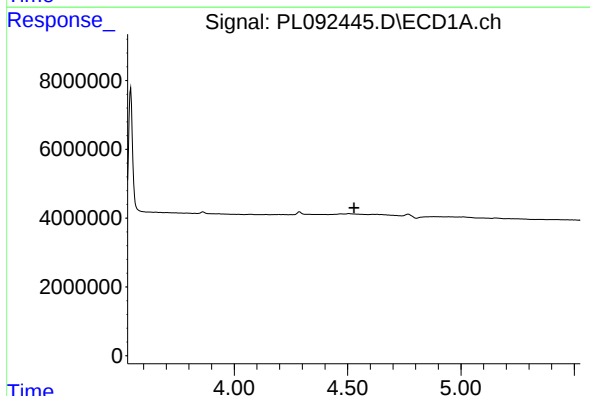


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.529 min
Response: 0
Conc: N.D.

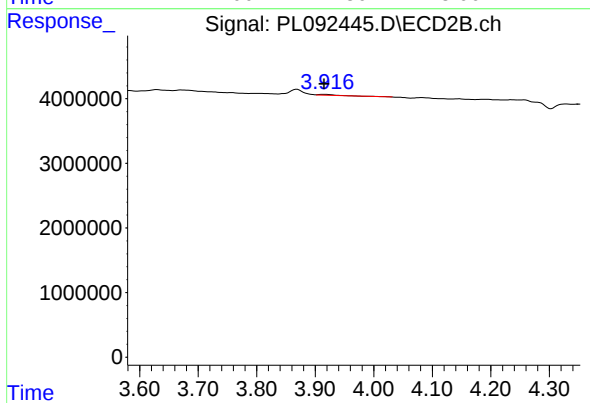

#6 beta-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 283106
Conc: 0.19 ng/ml

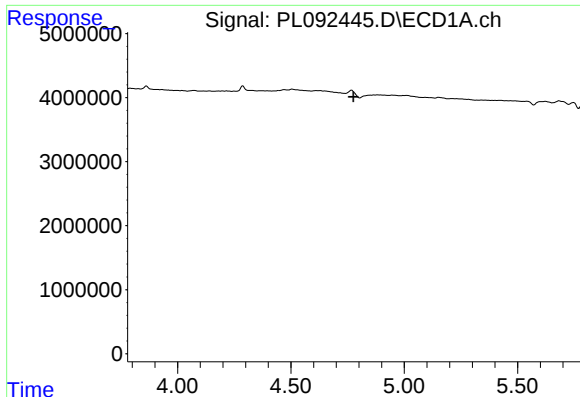

#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164207BL

#7 delta-BHC


R.T.: 4.145 min
Delta R.T.: 0.000 min
Response: 977302
Conc: 0.28 ng/ml

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.689 min
Response: 0
Conc: N.D.

#8 Heptachlor epoxide


R.T.: 4.758 min
Delta R.T.: 0.019 min
Response: 69228
Conc: 0.02 ng/ml

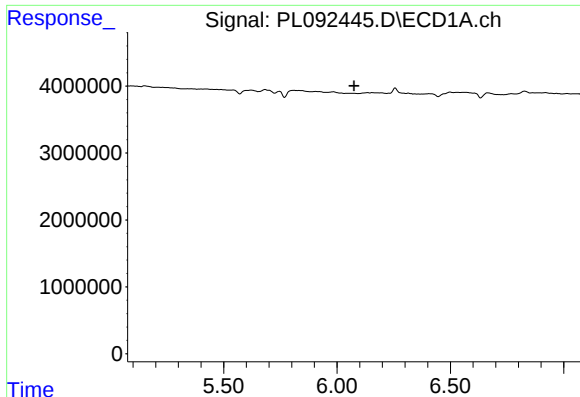

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164207BL

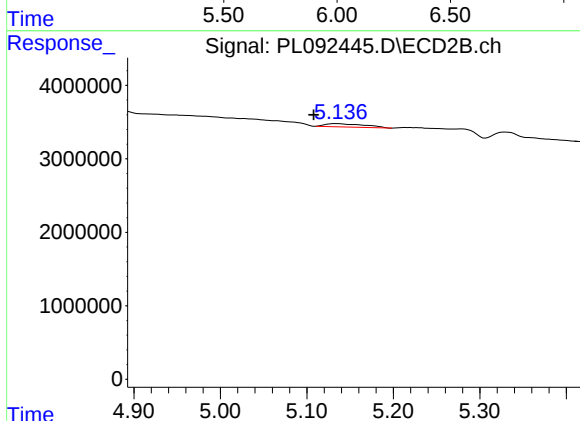


#9 Endosulfan I

R.T.: 5.135 min
Delta R.T.: 0.026 min
Response: 1414041
Conc: 0.52 ng/ml

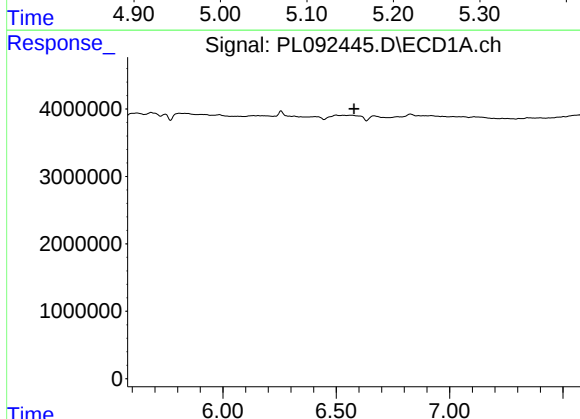


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.579 min
Response: 0
Conc: N.D.

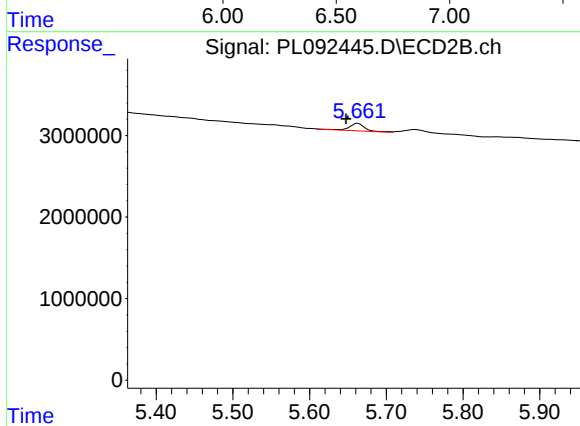

#14 Endrin


R.T.: 5.663 min
Delta R.T.: 0.015 min
Response: 1309905
Conc: 0.50 ng/ml

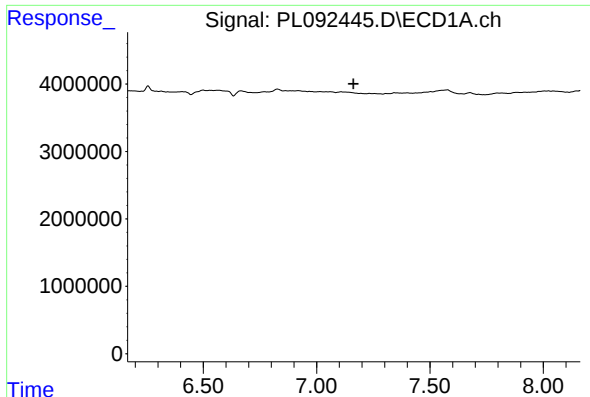

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164207BL

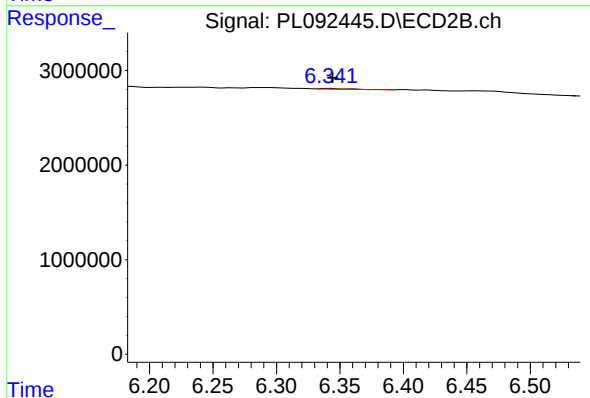


#19 Endosulfan Sulfate

R.T.: 6.342 min
Delta R.T.: -0.002 min
Response: 100105
Conc: 0.04 ng/ml

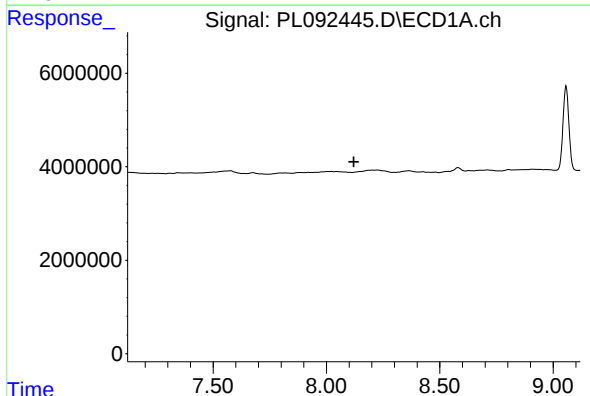


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

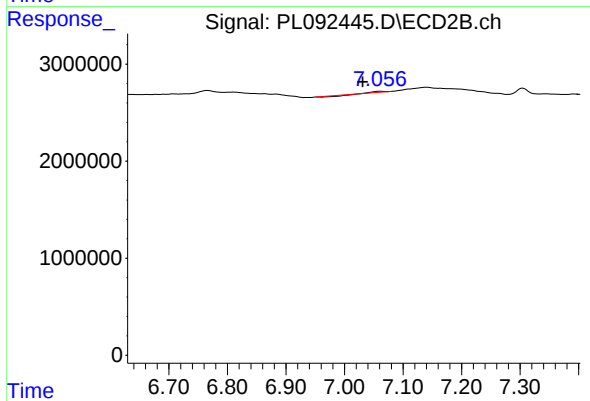

#22 Mirex


R.T.: 7.061 min
Delta R.T.: 0.029 min
Response: 8344
Conc: 0.00 ng/ml

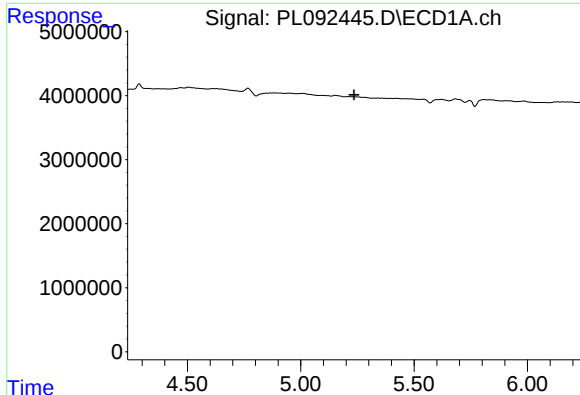

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164207BL

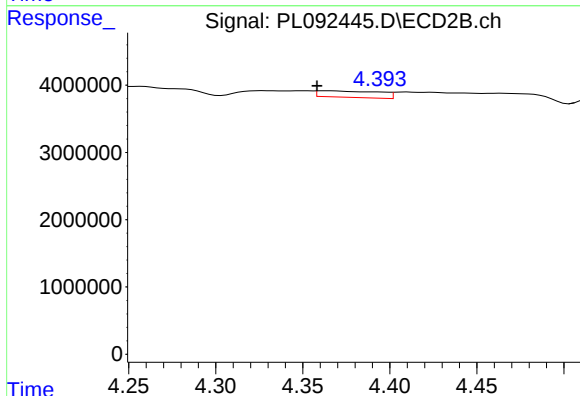


#24 Chlordane-2

R.T.: 4.365 min
Delta R.T.: 0.006 min
Response: 2352678
Conc: 20.96 ng/ml

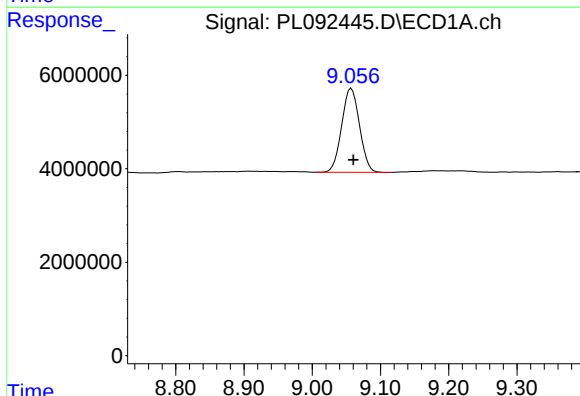

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.003 min
Response: 32581404
Conc: 19.89 ng/ml

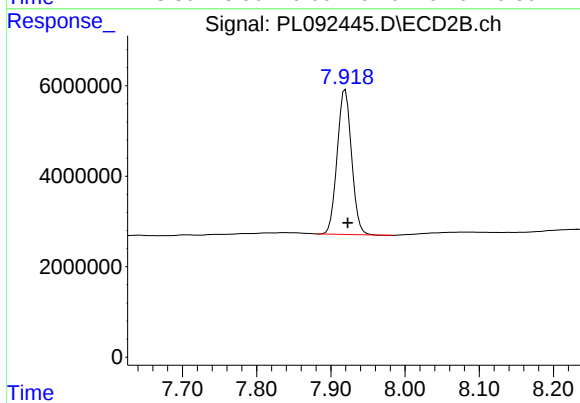

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: -0.003 min
Response: 43192769
Conc: 17.26 ng/ml