

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101818\
 Data File : PL041120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2018 18:08
 Operator : AJ\SJ
 Sample : J5570-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:53:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	49795181	25336338	9.085	9.087
28)	SA Decachlor...	8.222	9.232	48635926	20620131	9.354	7.974
Target Compounds							
6)	B beta-BHC	0.000	4.998f	0	7477830	N.D.	4.666 #
9)	A Endosulfan I	5.472f	6.309f	2000518	1674620	0.334	0.654 #
10)	B gamma-Chl...	5.435	0.000	2534206	0	0.385	N.D. #
11)	B alpha-Chl...	5.472	6.309	2000518	1674620	0.307	0.603 #
12)	B 4,4'-DDE	5.639	6.462	116.0E6	54174537	20.407	20.479
13)	MA Dieldrin	5.763	0.000	864985	0	0.137	N.D. #
14)	MA Endrin	6.027	6.860	5797070	1495870	1.009	0.670 #
16)	A 4,4'-DDD	6.154	6.958	1877554	3068733	0.416	1.465 #
17)	MA 4,4'-DDT	6.392	7.254	20575432	9157107	4.517	4.402
24)	Chlordane-2	4.851	0.000	3510887	0	13.008	N.D. #
25)	Chlordane-3	5.435	0.000	2534206	0	3.311	N.D. #
26)	Chlordane-4	5.472	6.309	2000518	1674620	2.984	3.528



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101818\
Data File : PL041120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2018 18:08
Operator : AJ\SJ
Sample : J5570-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:53:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

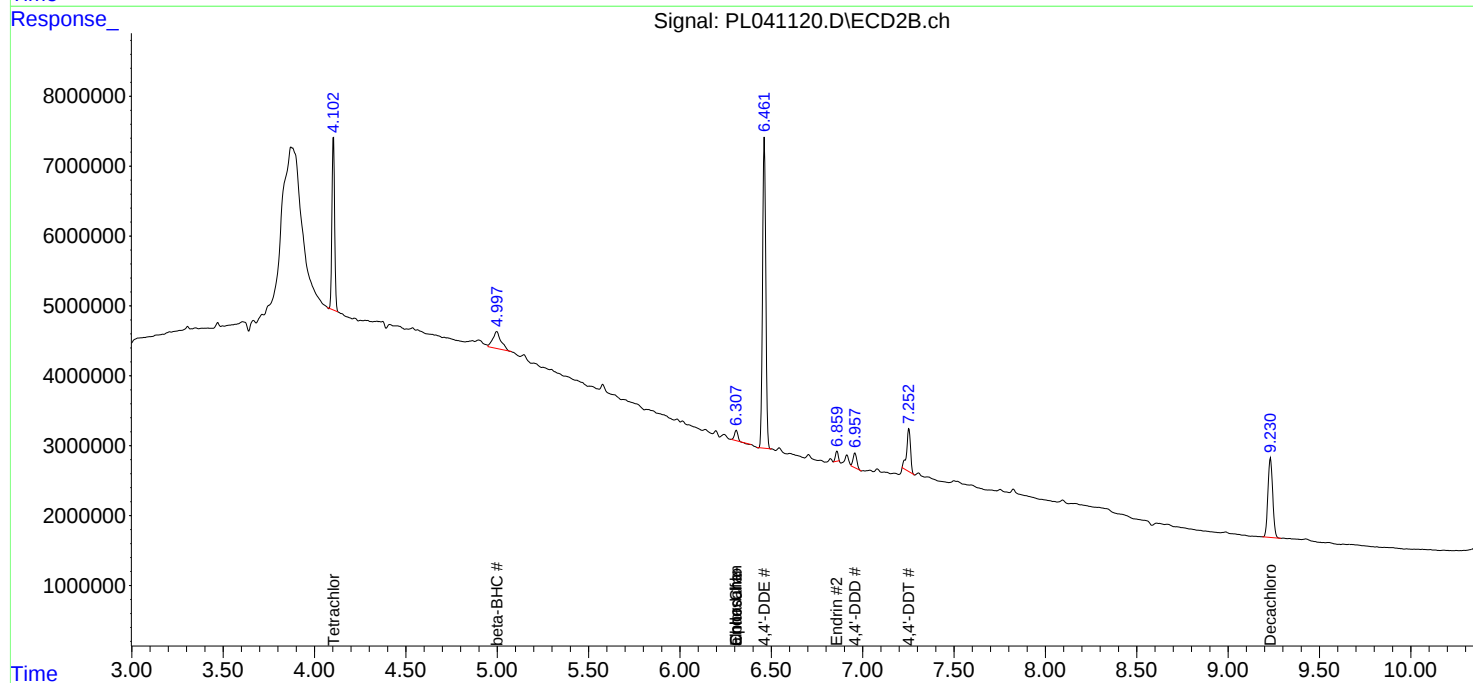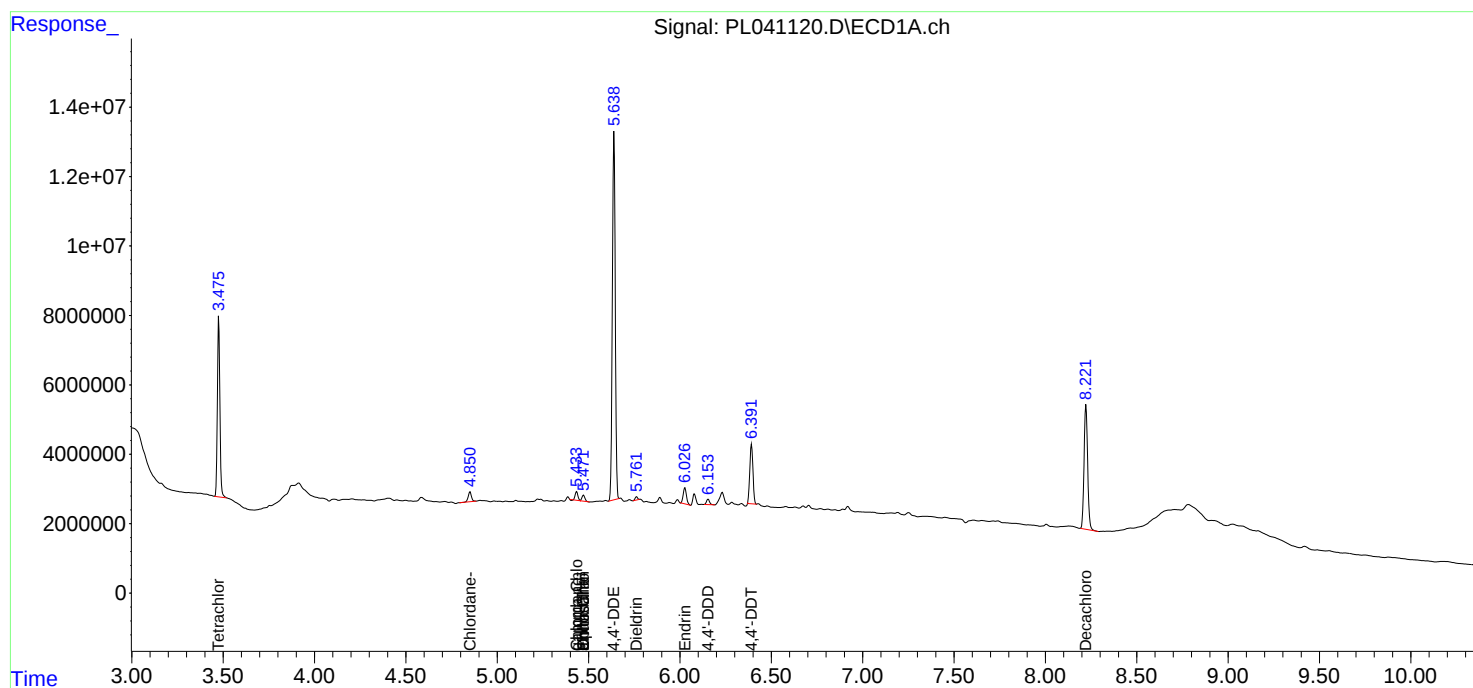


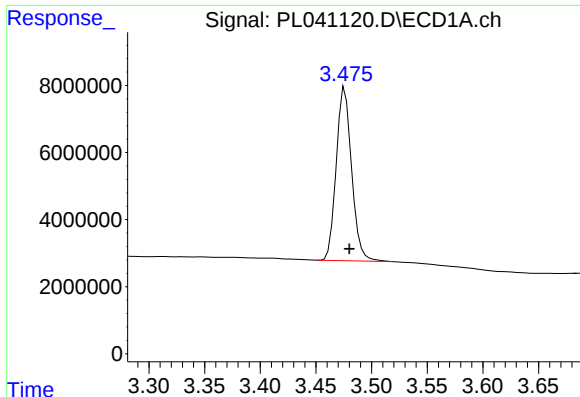

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 49795181
Conc: 9.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

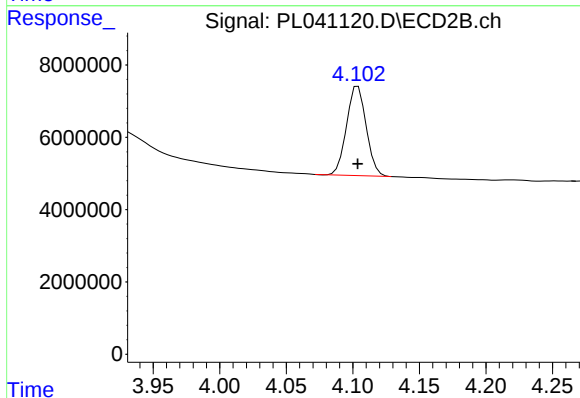


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 25336338
Conc: 9.09 ng/ml

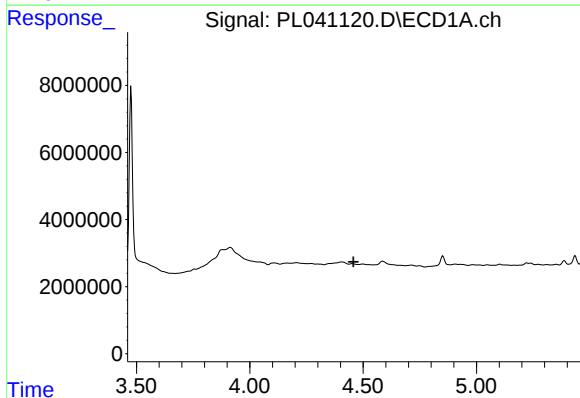


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.458 min
Response: 0
Conc: N.D.

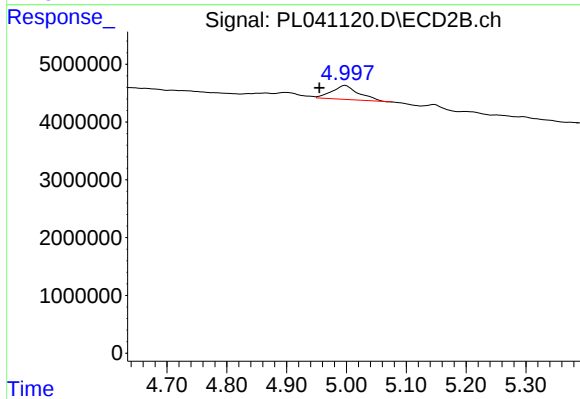

#6 beta-BHC


R.T.: 4.998 min
Delta R.T.: 0.043 min
Response: 7477830
Conc: 4.67 ng/ml

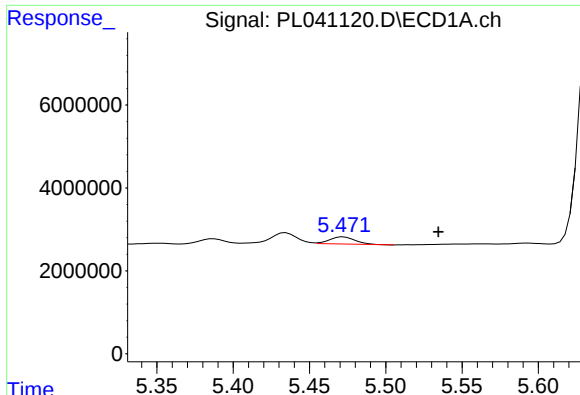

#9 Endosulfan I


R.T.: 5.472 min
Delta R.T.: -0.062 min
Response: 2000518
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

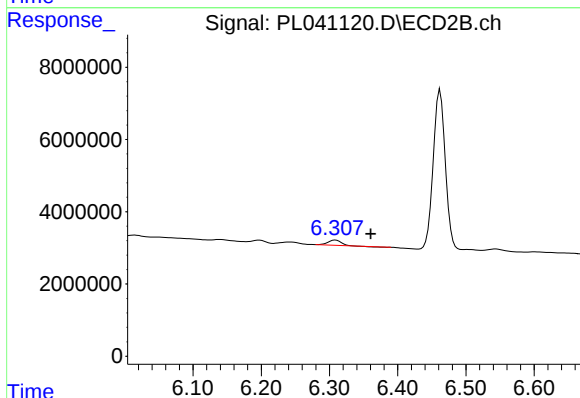


#9 Endosulfan I

R.T.: 6.309 min
Delta R.T.: -0.052 min
Response: 1674620
Conc: 0.65 ng/ml

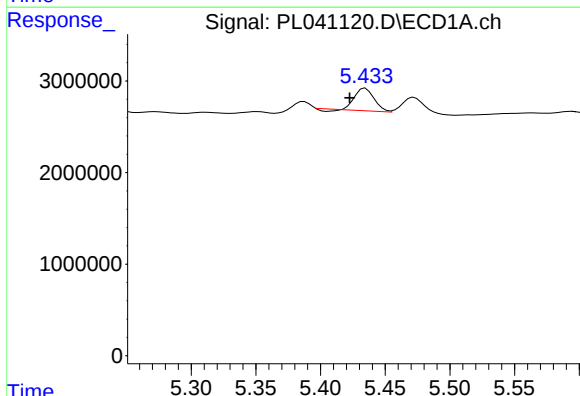


#10 gamma-Chlordane

R.T.: 5.435 min
Delta R.T.: 0.012 min
Response: 2534206
Conc: 0.39 ng/ml

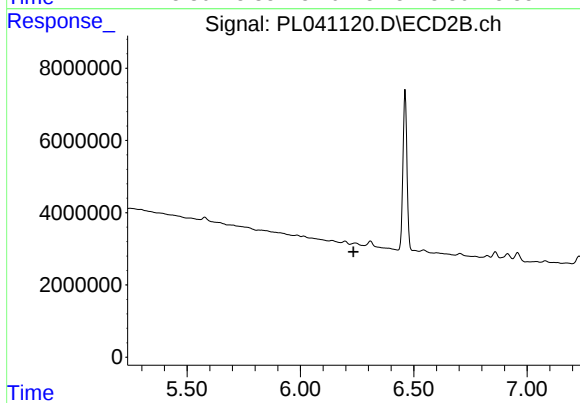

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.235 min
Response: 0
Conc: N.D.

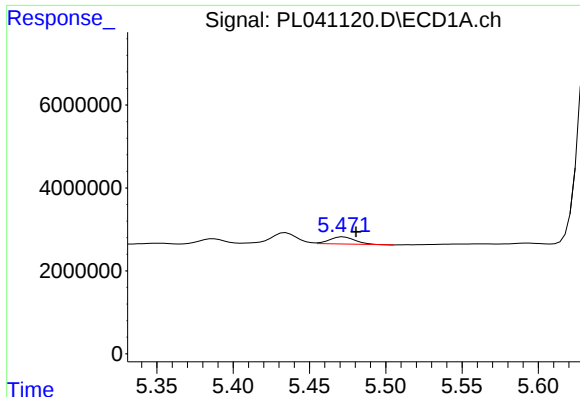

#11 alpha-Chlordane


R.T.: 5.472 min
Delta R.T.: -0.008 min
Response: 2000518
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

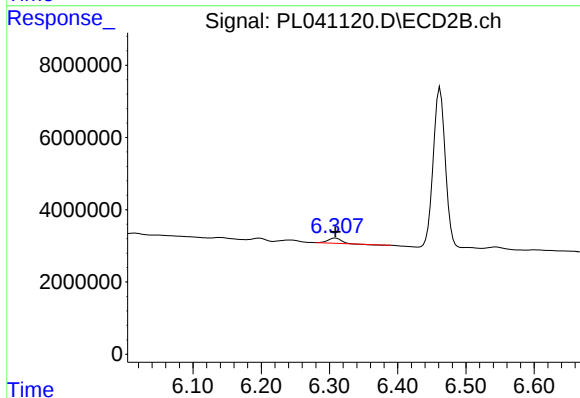


#11 alpha-Chlordane

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 1674620
Conc: 0.60 ng/ml

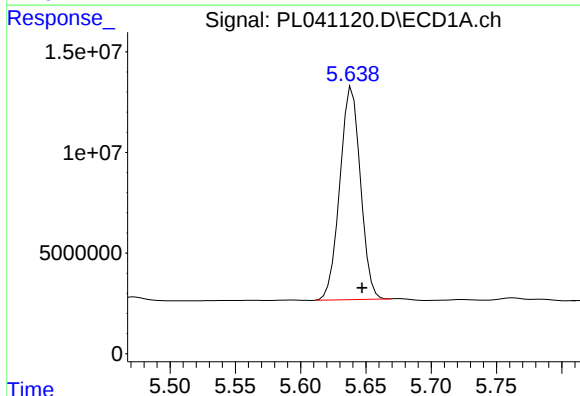


#12 4,4'-DDE

R.T.: 5.639 min
Delta R.T.: -0.008 min
Response: 115988469
Conc: 20.41 ng/ml

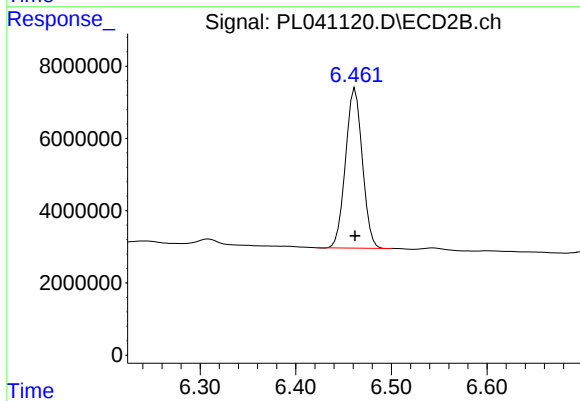

#12 4,4'-DDE


R.T.: 6.462 min
Delta R.T.: 0.000 min
Response: 54174537
Conc: 20.48 ng/ml

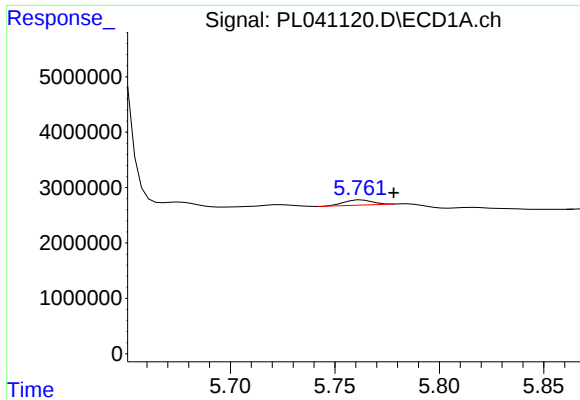

#13 Dieldrin


R.T.: 5.763 min
Delta R.T.: -0.016 min
Response: 864985
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

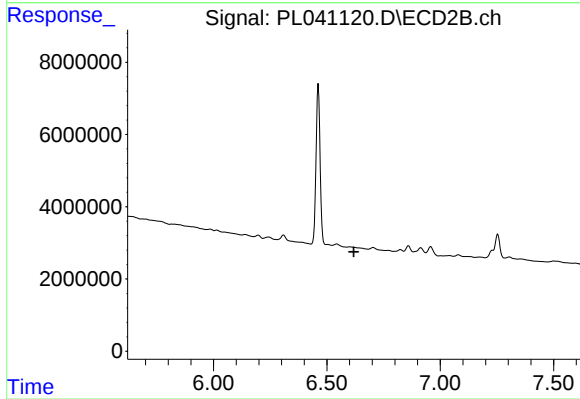


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.618 min
Response: 0
Conc: N.D.

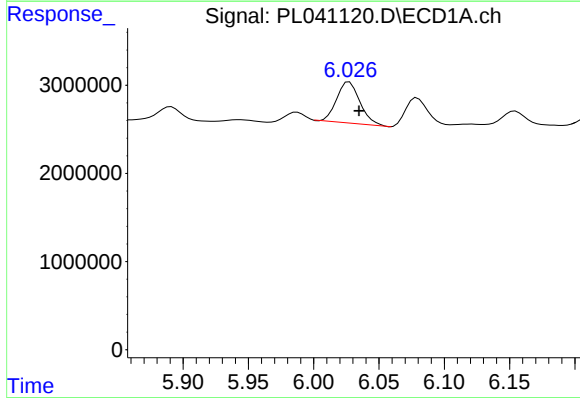


#14 Endrin

R.T.: 6.027 min
Delta R.T.: -0.007 min
Response: 5797070
Conc: 1.01 ng/ml

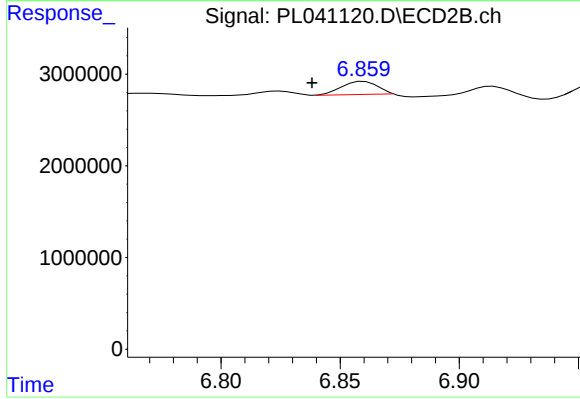

#14 Endrin


R.T.: 6.860 min
Delta R.T.: 0.022 min
Response: 1495870
Conc: 0.67 ng/ml

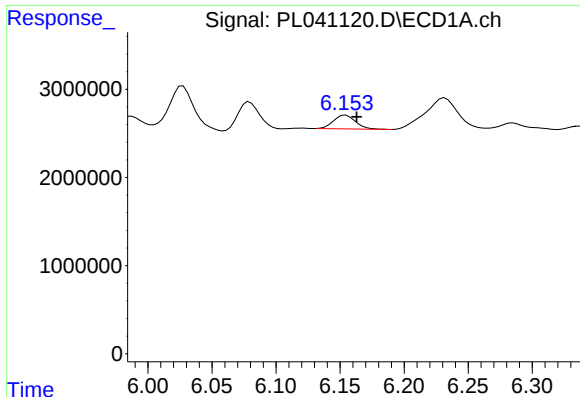

#16 4,4'-DDD


R.T.: 6.154 min
Delta R.T.: -0.009 min
Response: 1877554
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

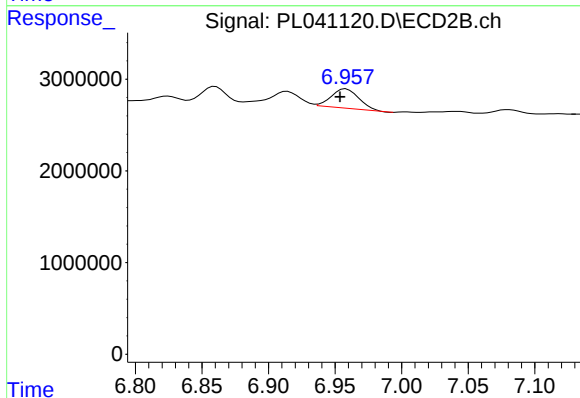


#16 4,4'-DDD

R.T.: 6.958 min
Delta R.T.: 0.004 min
Response: 3068733
Conc: 1.46 ng/ml

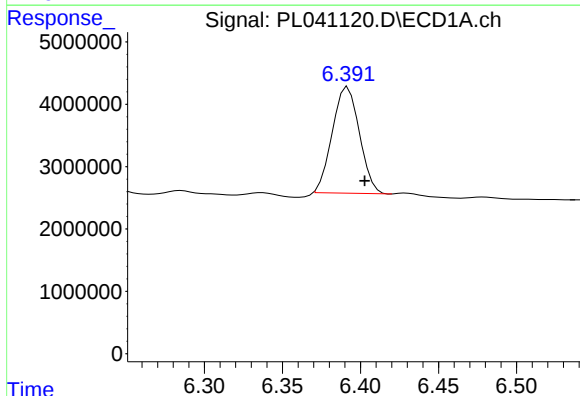


#17 4,4'-DDT

R.T.: 6.392 min
Delta R.T.: -0.011 min
Response: 20575432
Conc: 4.52 ng/ml

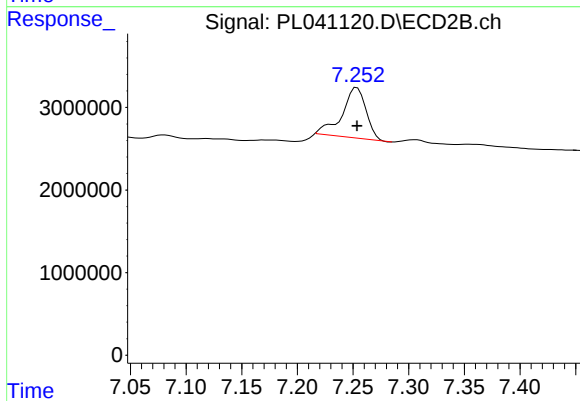

#17 4,4'-DDT


R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 9157107
Conc: 4.40 ng/ml

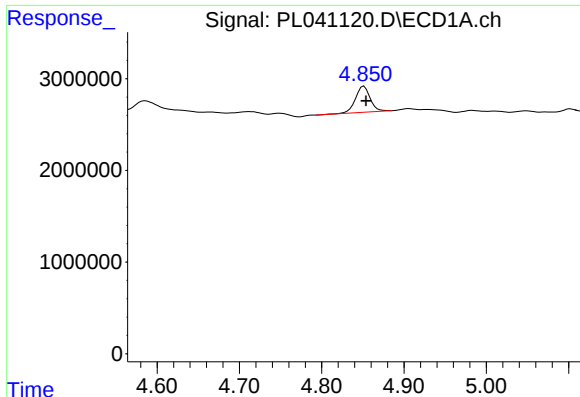

#24 Chlordane-2


R.T.: 4.851 min
Delta R.T.: -0.003 min
Response: 3510887
Conc: 13.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

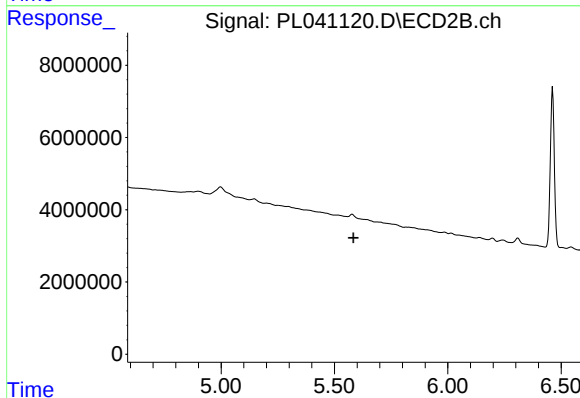


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

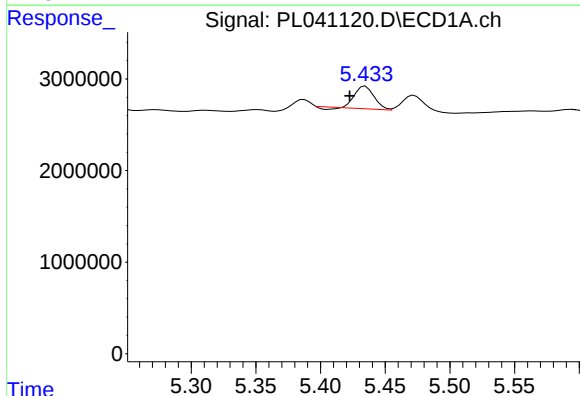


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.012 min
Response: 2534206
Conc: 3.31 ng/ml

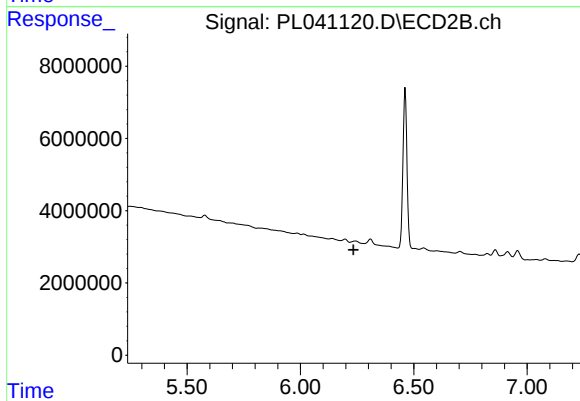

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

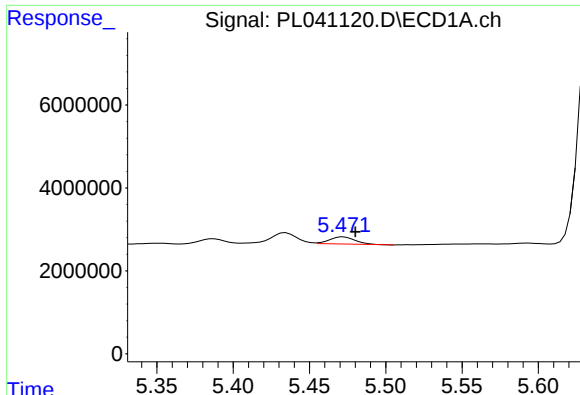

#26 Chlordane-4


R.T.: 5.472 min
Delta R.T.: -0.008 min
Response: 2000518
Conc: 2.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

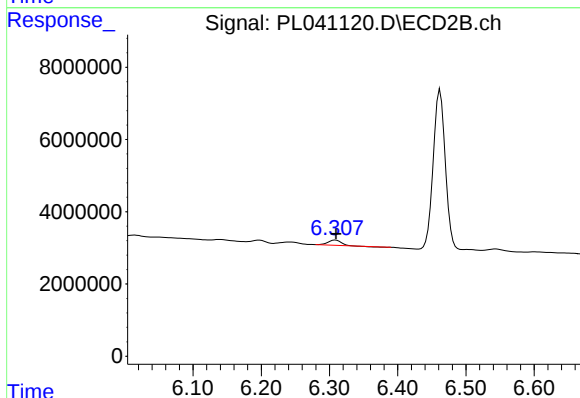


#26 Chlordane-4

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 1674620
Conc: 3.53 ng/ml

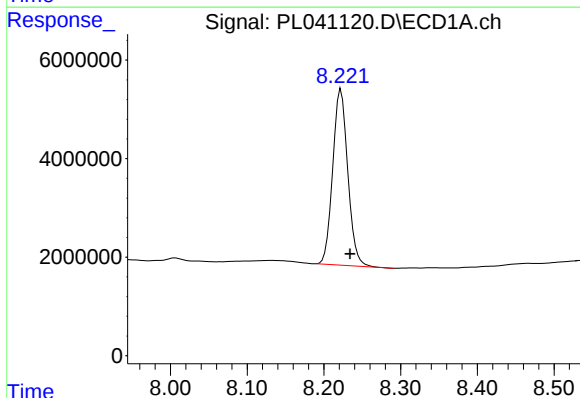

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.012 min
Response: 48635926
Conc: 9.35 ng/ml

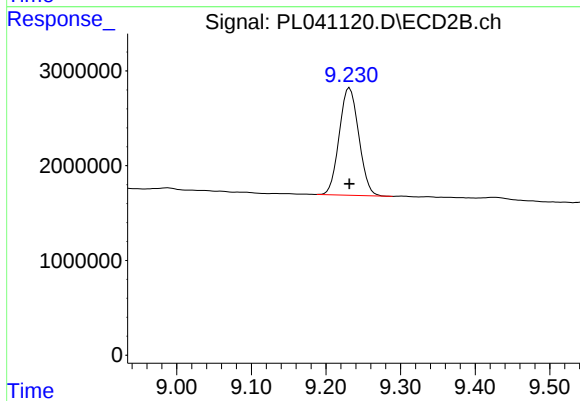

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 20620131
Conc: 7.97 ng/ml