

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101818\
 Data File : PL041116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2018 17:12
 Operator : AJ\SJ
 Sample : J5575-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1015-S-DH-25A-T

Manual Integrations
 APPROVED

Sohil
 10/19/2018 5:39:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:53:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.103	117.3E6	56057269	21.408	20.105
28)	SA Decachlor...	8.222	9.230	104.0E6	43985906	20.007	17.010m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101818\
Data File : PL041116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2018 17:12
Operator : AJ\SJ
Sample : J5575-08
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SSSI-1015-S-DH-25A-T


Manual Integrations
APPROVED

Sohil
10/19/2018 5:39:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:53:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

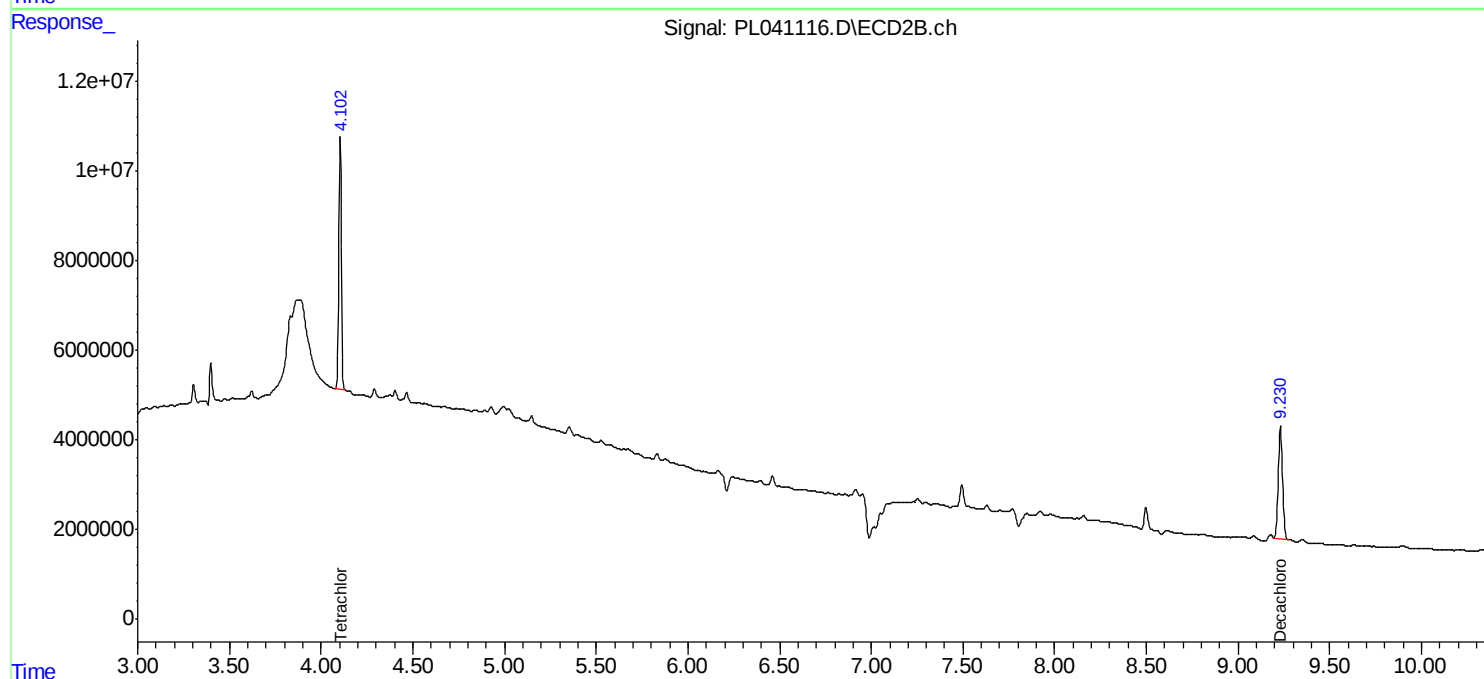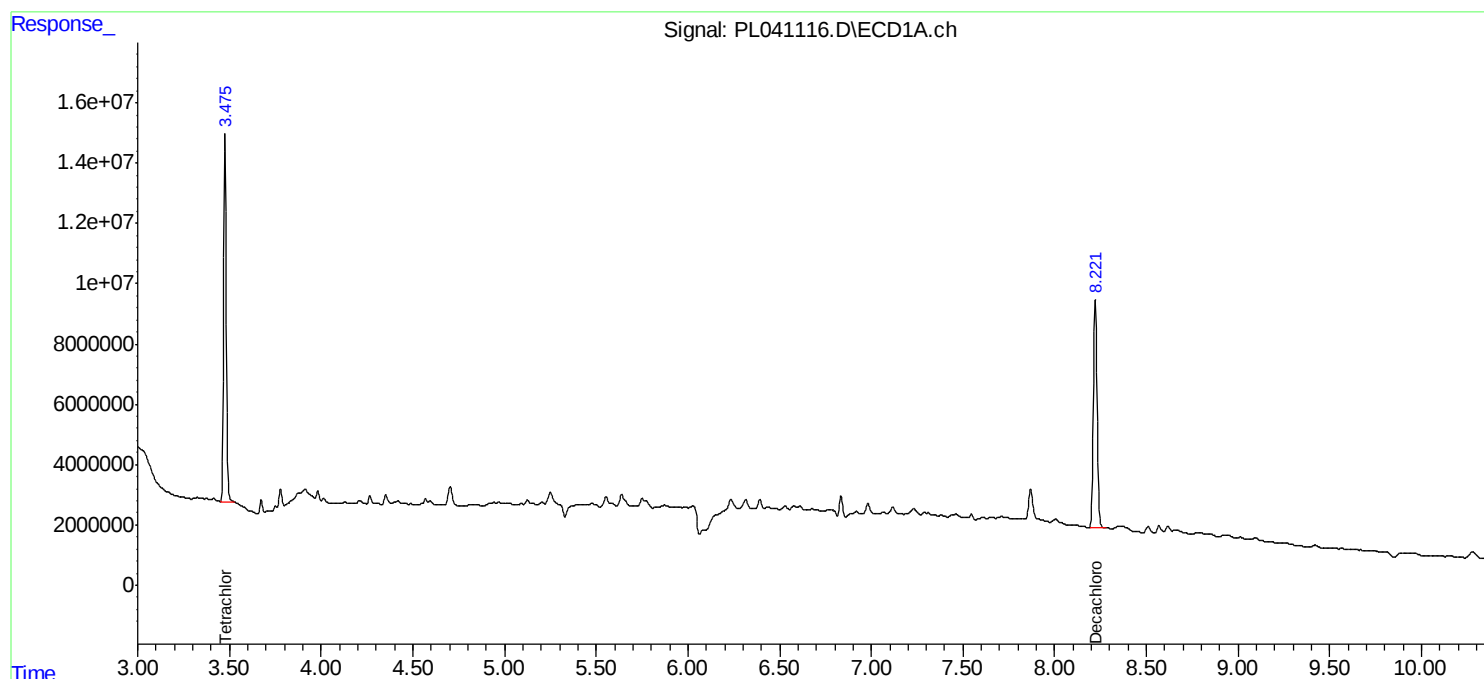

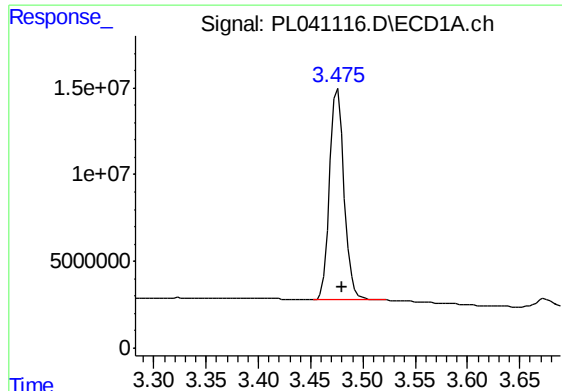


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 117333974
Conc: 21.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1015-S-DH-25A-T


Manual Integrations
APPROVED

Sohil
10/19/2018 5:39:13 PM

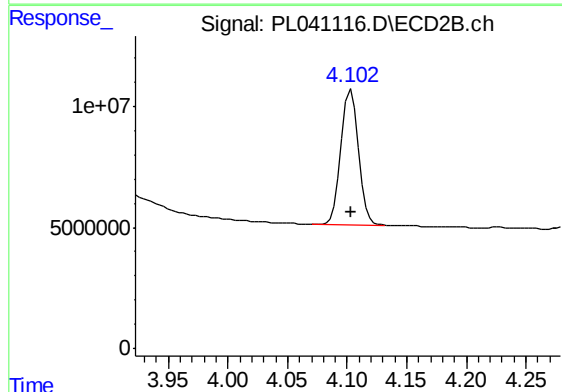


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 56057269
Conc: 20.10 ng/ml

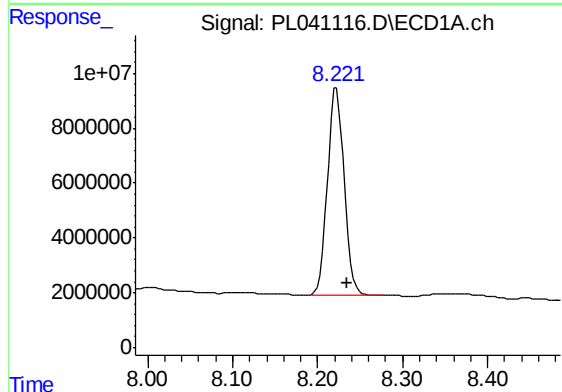

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: -0.012 min
Response: 104029110
Conc: 20.01 ng/ml

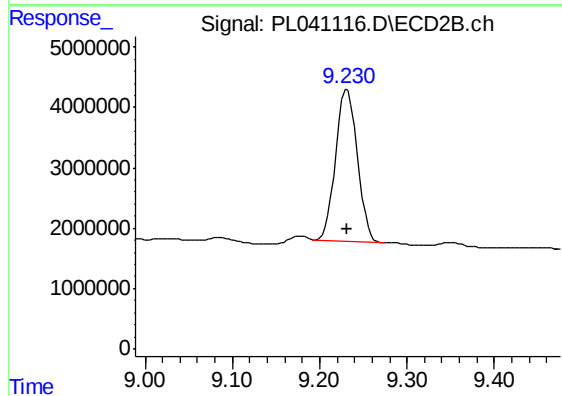

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.001 min
Response: 43985906
Conc: 17.01 ng/ml m