

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
 Data File : PL053410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 15:53
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 03:29:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 03:23:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.047	680.1E6	125.6E6	50.000	50.000
28)	SA Decachlor...	8.337	9.131	502.6E6	140.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.430	5.045	198.2E6	47230036	500.000	500.000
24)	Chlordane-2	4.936	5.513	219.7E6	52434425	500.000	500.000
25)	Chlordane-3	5.512	6.161	666.9E6	200.1E6	500.000	500.000
26)	Chlordane-4	5.570	6.235	550.1E6	243.3E6	500.000	500.000
27)	Chlordane-5	6.412	7.041	207.4E6	42151739	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
Data File : PL053410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 15:53
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 03:29:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 03:23:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

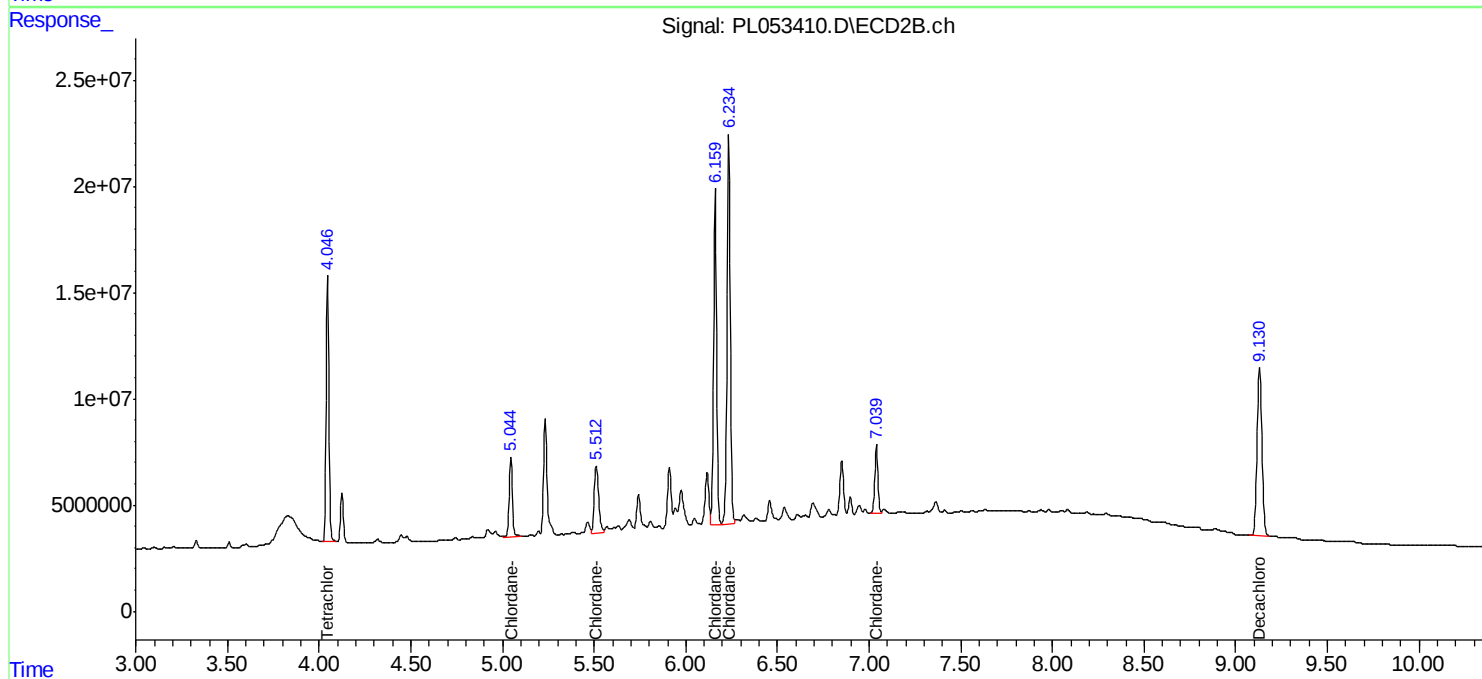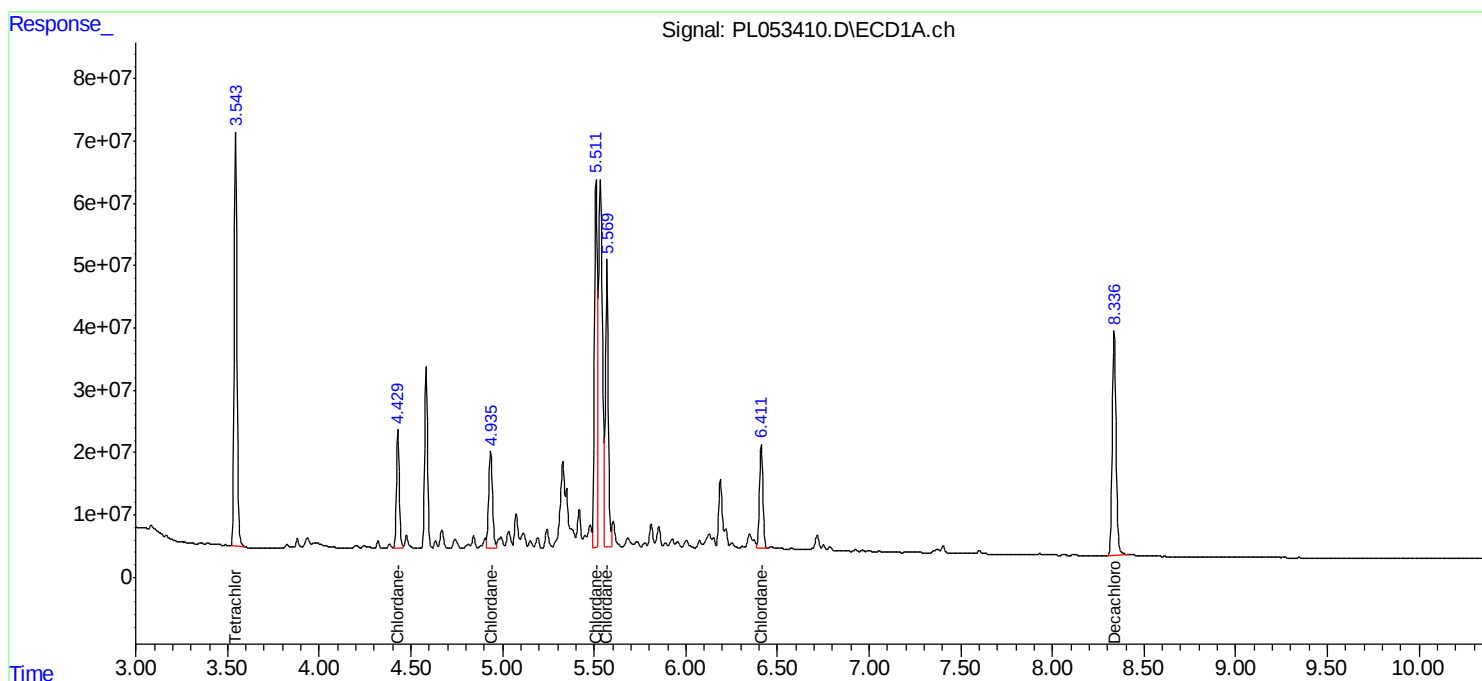


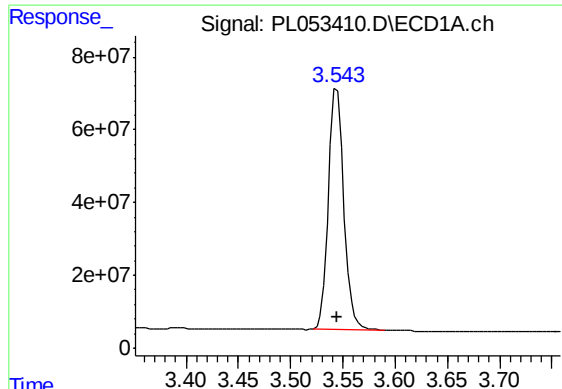

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 680126200
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

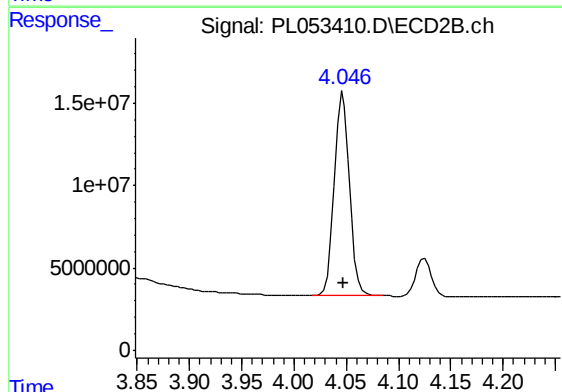


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 125646590
Conc: 50.00 ng/ml

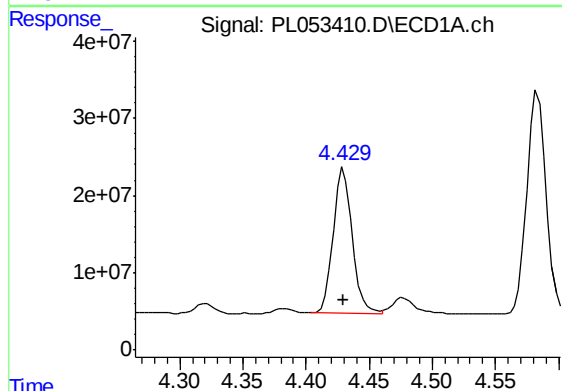


#23 Chlordane-1

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 198225083
Conc: 500.00 ng/ml

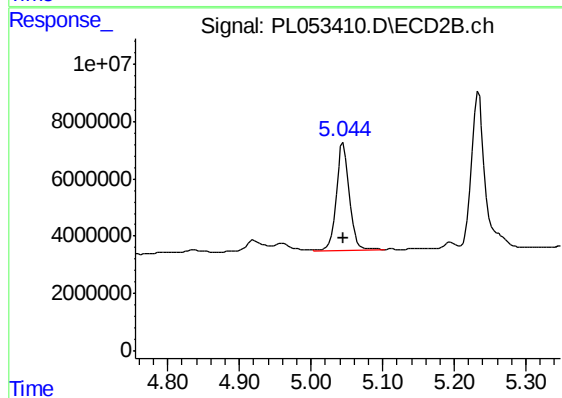

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 47230036
Conc: 500.00 ng/ml

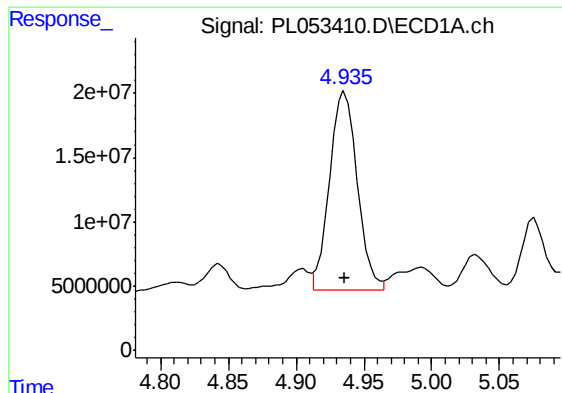

#24 Chlordane-2


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 219741956
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

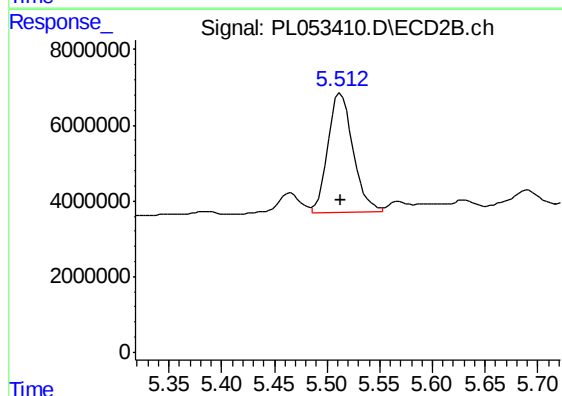


#24 Chlordane-2

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 52434425
Conc: 500.00 ng/ml

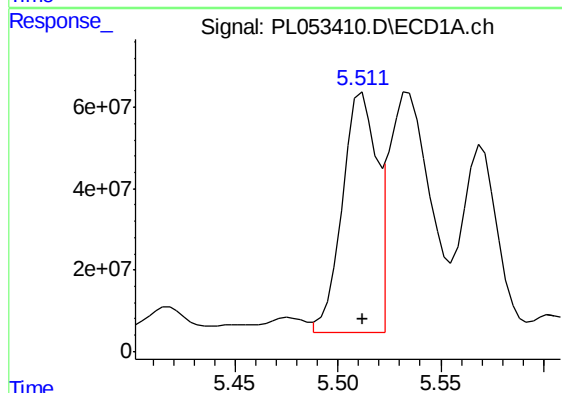


#25 Chlordane-3

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 666948263
Conc: 500.00 ng/ml

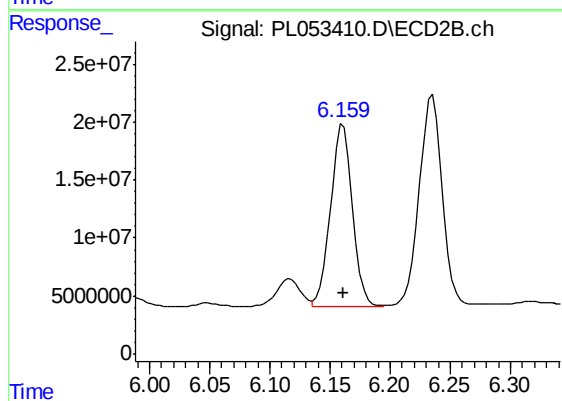

#25 Chlordane-3


R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 200106848
Conc: 500.00 ng/ml

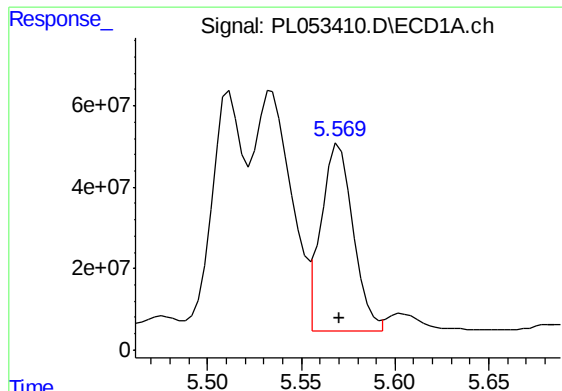

#26 Chlordane-4


R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 550106521
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

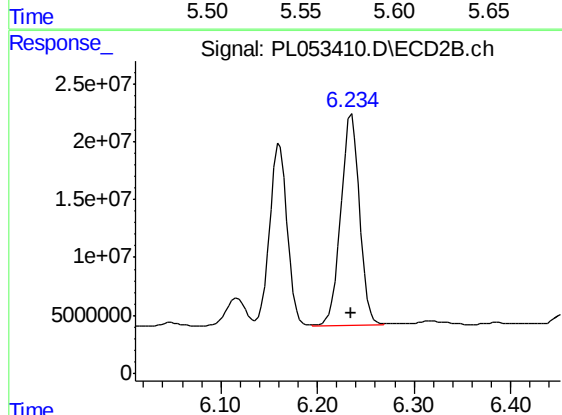


#26 Chlordane-4

R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 243289618
Conc: 500.00 ng/ml

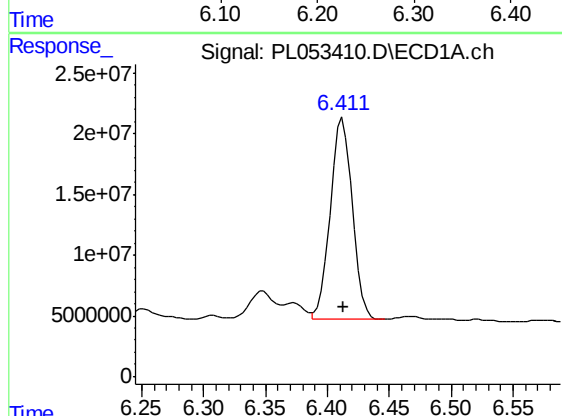


#27 Chlordane-5

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 207415567
Conc: 500.00 ng/ml

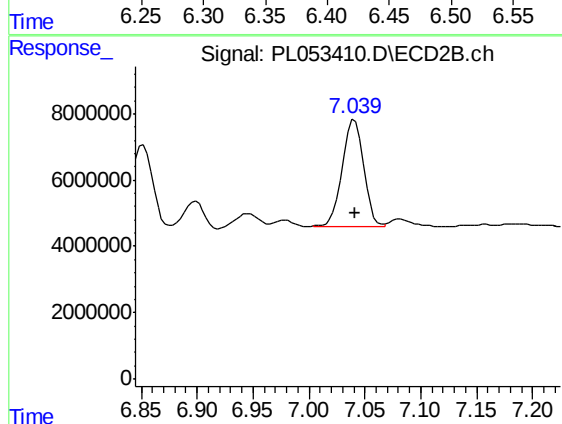

#27 Chlordane-5


R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 42151739
Conc: 500.00 ng/ml

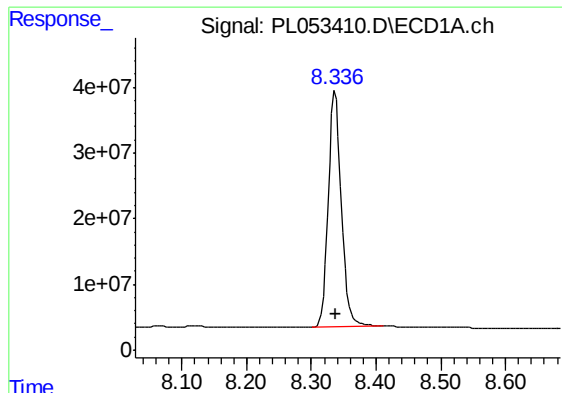

#28 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: 0.000 min
Response: 502640987
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

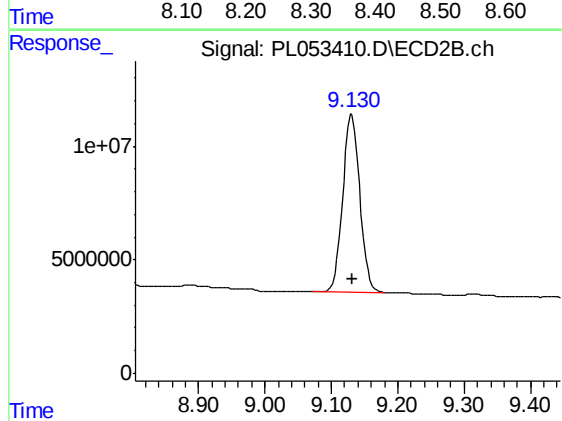

#28 Decachlorobiphenyl

R.T.: 9.131 min
Delta R.T.: 0.000 min
Response: 140166790
Conc: 50.00 ng/ml