

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
 Data File : PL053419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 19:08
 Operator : SG\AJ
 Sample : PB124066BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 08:24:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 04:15:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.047	211.8E6	48345259	18.689	18.632
28)	SA Decachlor...	8.336	9.130	196.4E6	55665604	18.638	19.094
Target Compounds							
10)	B gamma-Chl...	0.000	6.138f	0	1392288	N.D.	0.447 #
25)	Chlordane-3	0.000	6.138f	0	1392288	N.D.	3.549 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
Data File : PL053419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 19:08
Operator : SG\AJ
Sample : PB124066BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 08:24:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 04:15:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

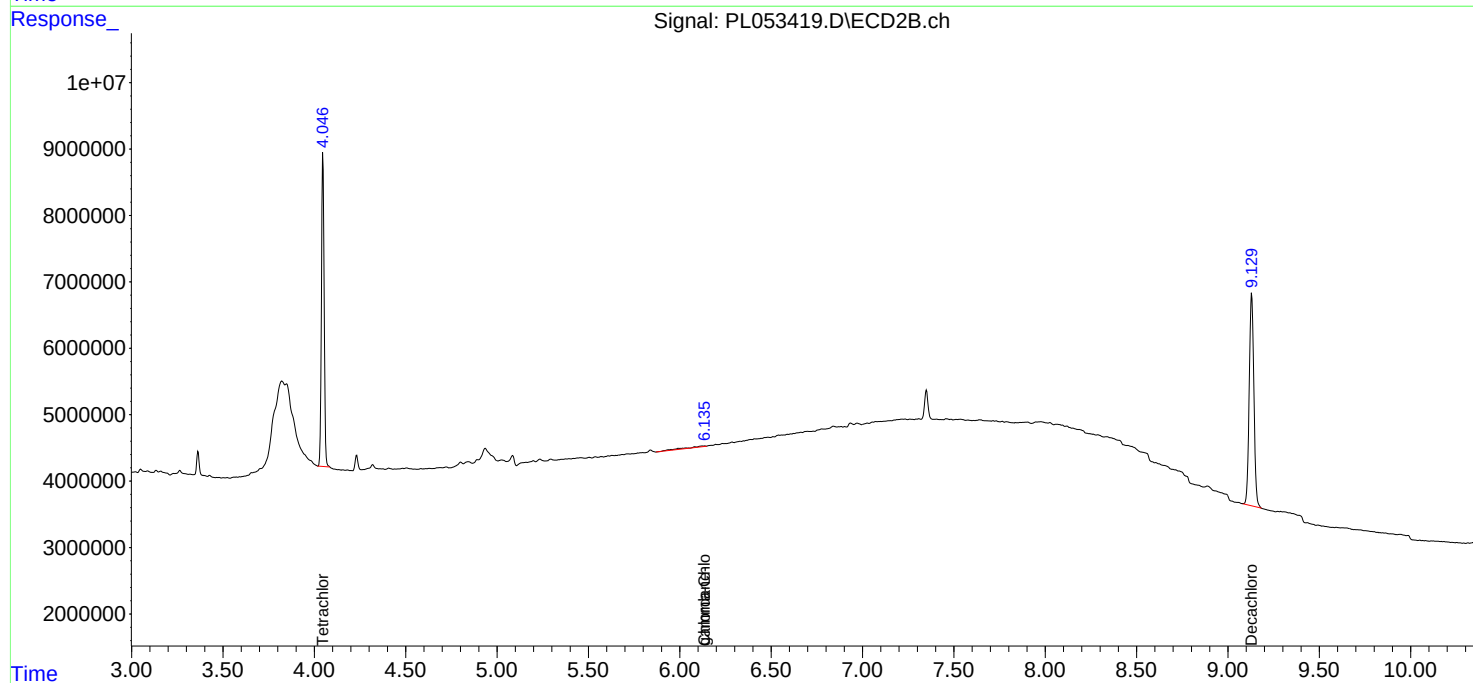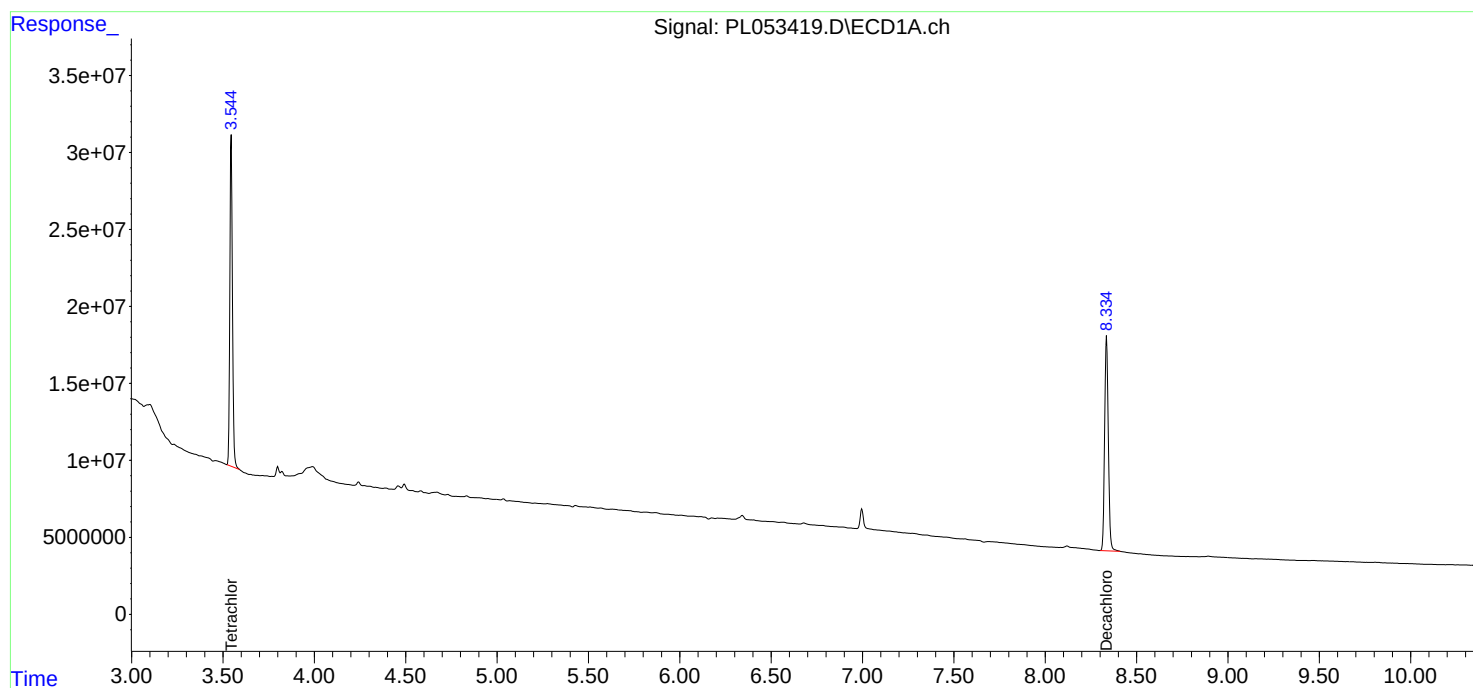


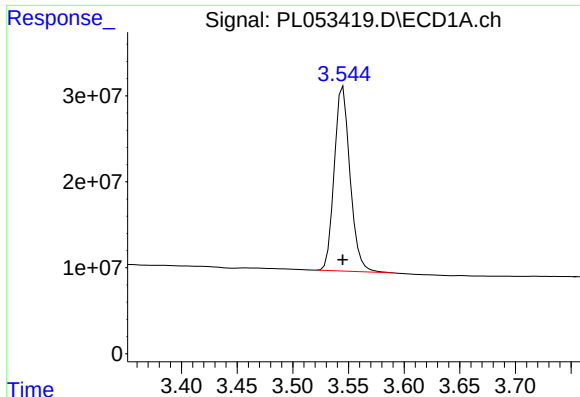

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 211808535
Conc: 18.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

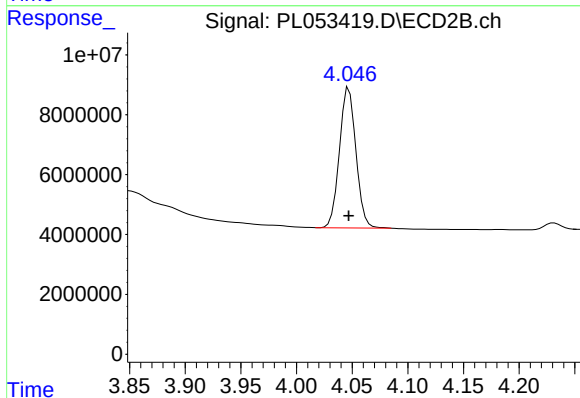


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 48345259
Conc: 18.63 ng/ml

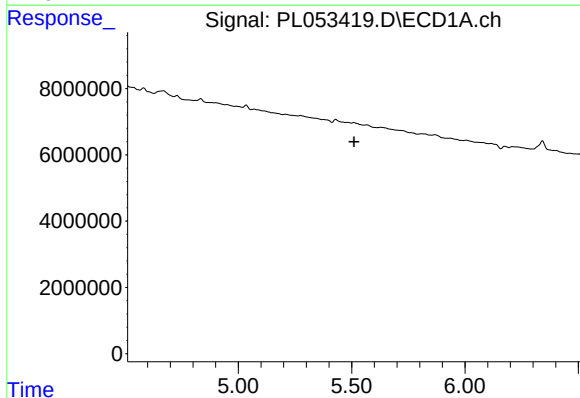


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

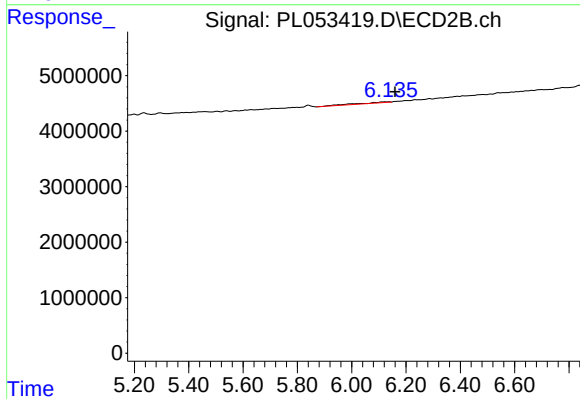

#10 gamma-Chlordane


R.T.: 6.138 min
Delta R.T.: -0.022 min
Response: 1392288
Conc: 0.45 ng/ml

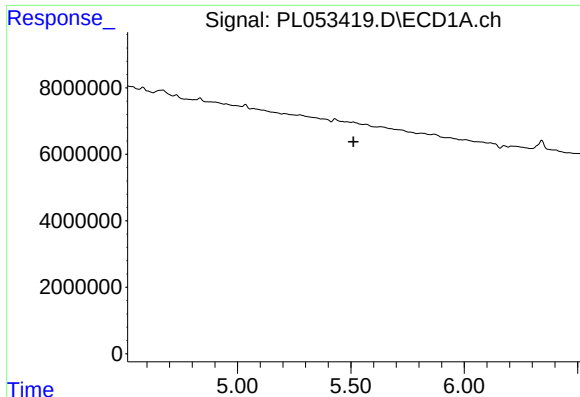

#25 Chlorodane-3


R.T.: 0.000 min
Exp R.T.: 5.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

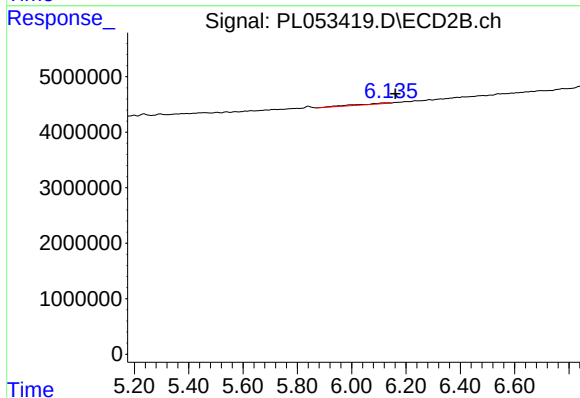


#25 Chlorodane-3

R.T.: 6.138 min
Delta R.T.: -0.023 min
Response: 1392288
Conc: 3.55 ng/ml

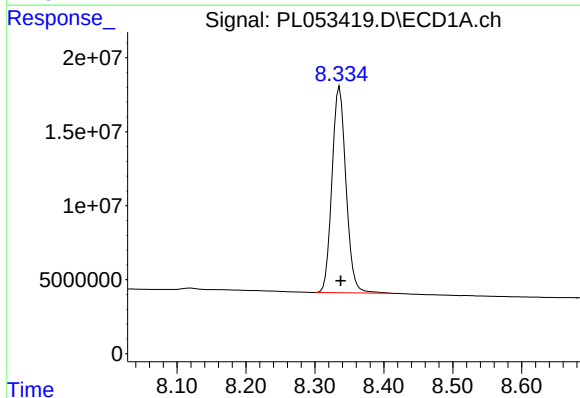

#28 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.001 min
Response: 196421157
Conc: 18.64 ng/ml

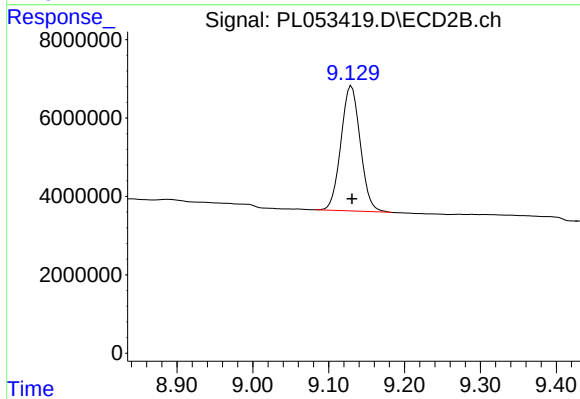

#28 Decachlorobiphenyl

R.T.: 9.130 min
Delta R.T.: 0.000 min
Response: 55665604
Conc: 19.09 ng/ml