

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
 Data File : PL053408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 15:25
 Operator : SG\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 03:28:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 03:23:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.047	1338.4E6	247.2E6	98.392	98.386
28)	SA Decachlor...	8.337	9.131	962.2E6	273.4E6	95.719	97.530
Target Compounds							
23)	Chlordane-1	4.430	5.045	405.7E6	93793545	1023.300	992.944
24)	Chlordane-2	4.936	5.514	429.0E6	102.4E6	976.078	976.379
25)	Chlordane-3	5.512	6.160	1344.1E6	413.0E6	1007.675	1031.864
26)	Chlordane-4	5.570	6.235	1108.1E6	494.3E6	1007.178	1015.880
27)	Chlordane-5	6.412	7.041	430.5E6	84486612	1037.862	1002.172



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
Data File : PL053408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 15:25
Operator : SG\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 03:28:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 03:23:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

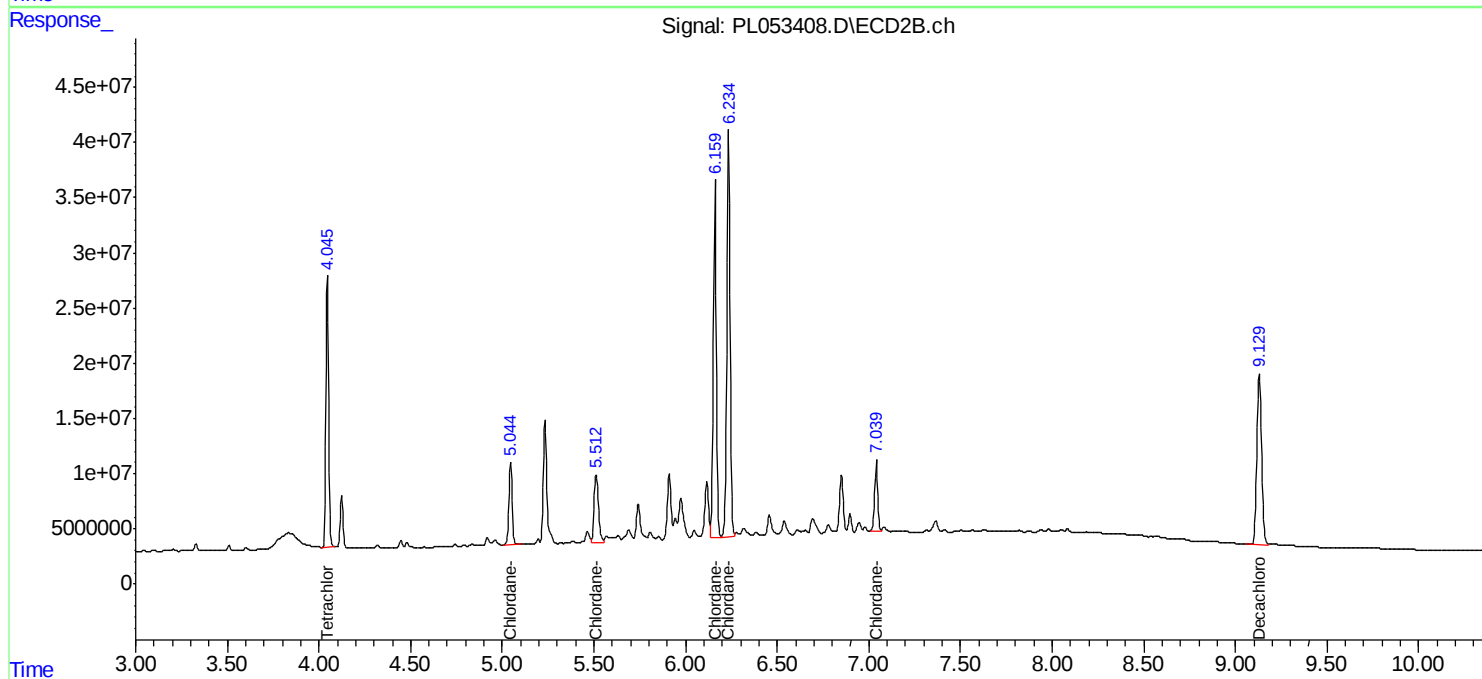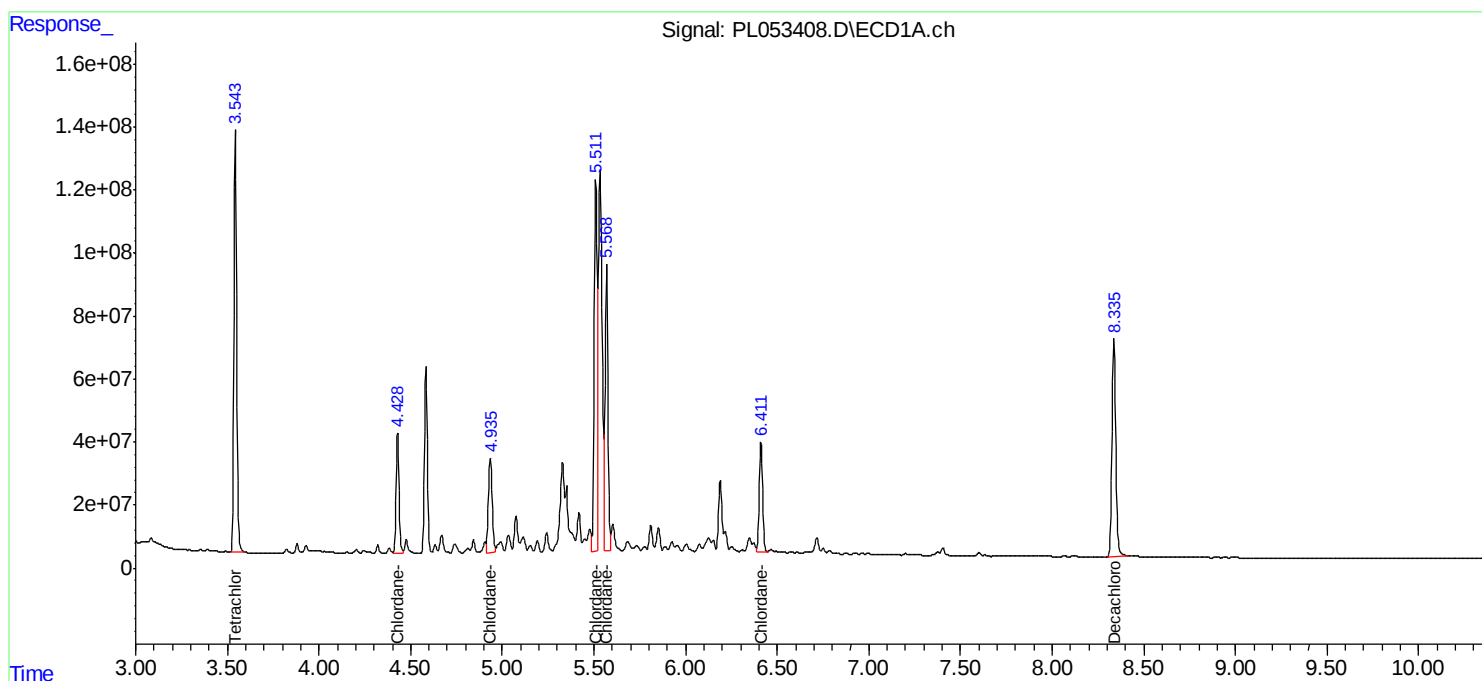


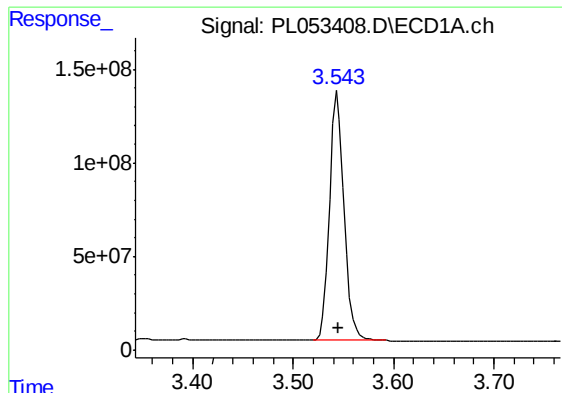

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 1338375862
Conc: 98.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

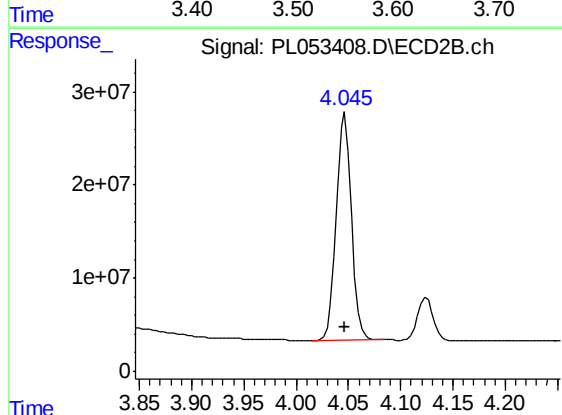


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 247237906
Conc: 98.39 ng/ml

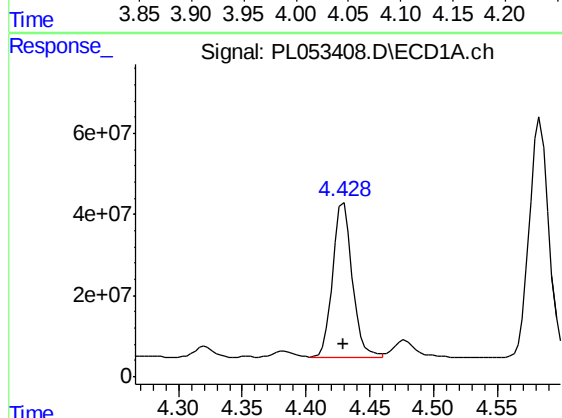


#23 Chlordane-1

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 405687409
Conc: 1023.30 ng/ml

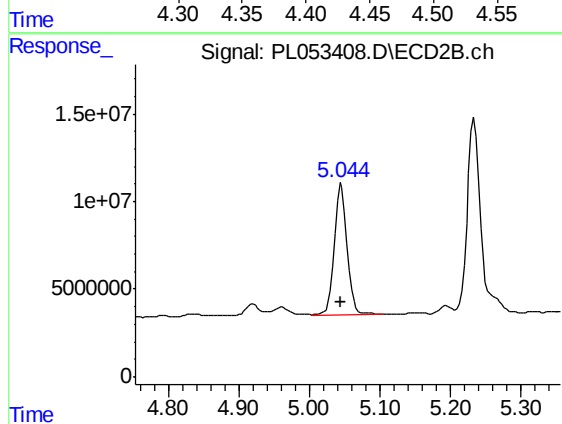

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 93793545
Conc: 992.94 ng/ml

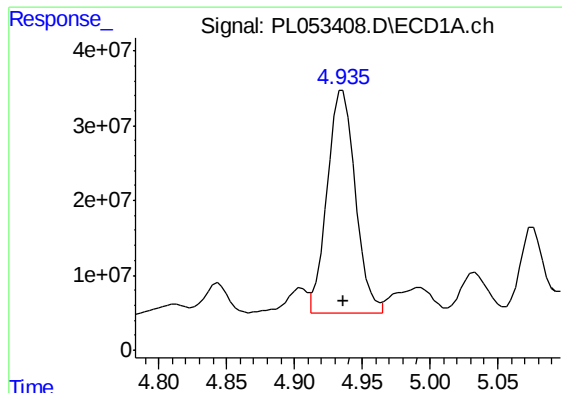

#24 Chlordane-2


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 428970778
Conc: 976.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

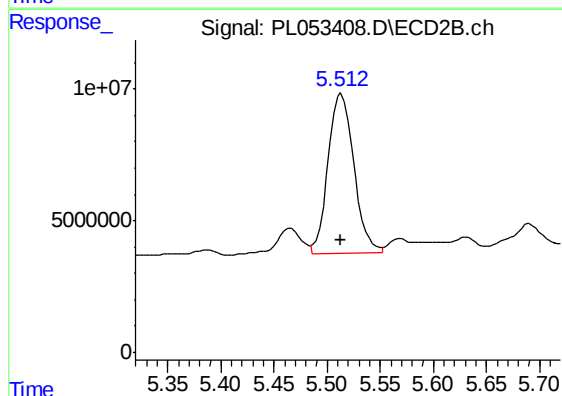


#24 Chlordane-2

R.T.: 5.514 min
Delta R.T.: 0.000 min
Response: 102391726
Conc: 976.38 ng/ml

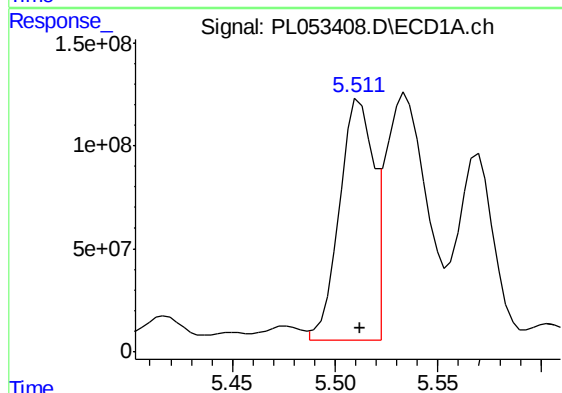


#25 Chlordane-3

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 1344133851
Conc: 1007.67 ng/ml

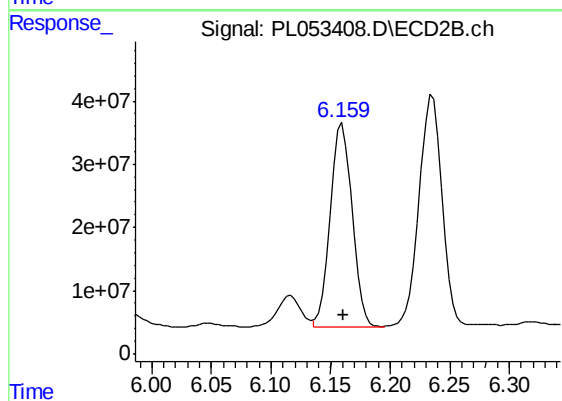

#25 Chlordane-3


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 412966227
Conc: 1031.86 ng/ml

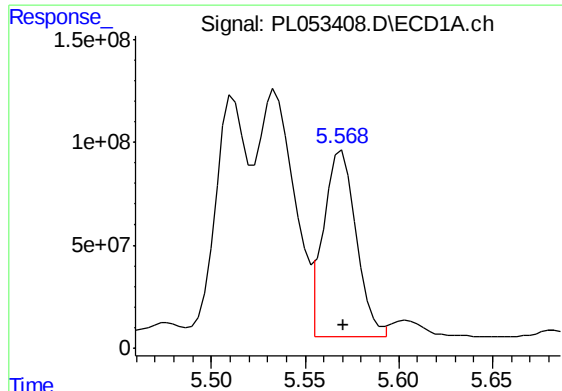

#26 Chlordane-4


R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 1108110299
Conc: 1007.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

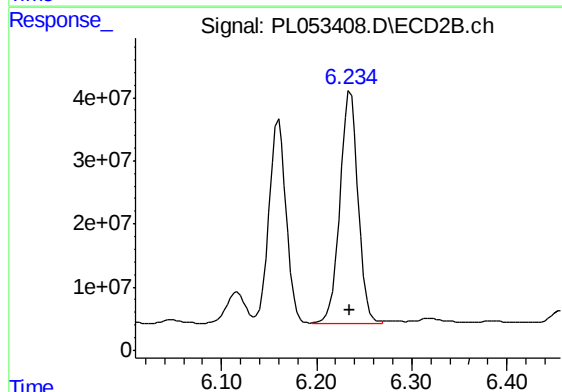


#26 Chlordane-4

R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 494306300
Conc: 1015.88 ng/ml

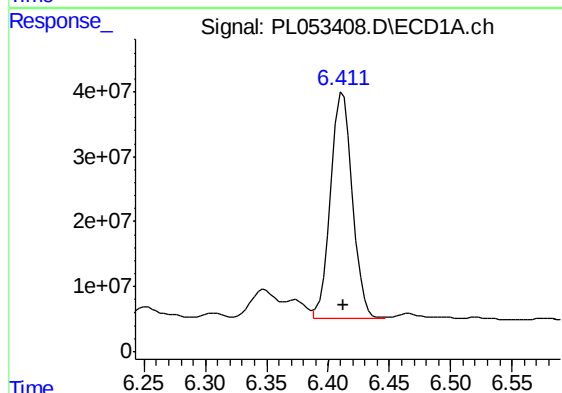


#27 Chlordane-5

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 430537414
Conc: 1037.86 ng/ml

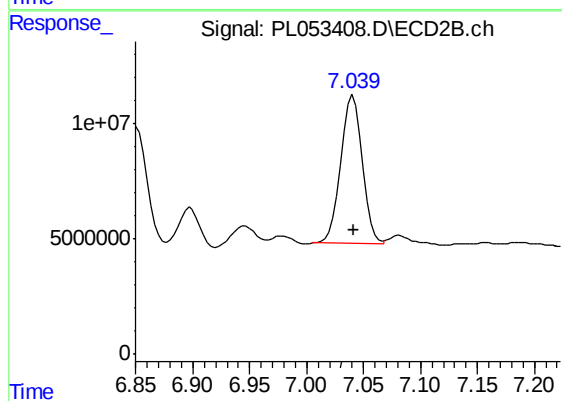

#27 Chlordane-5


R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 84486612
Conc: 1002.17 ng/ml

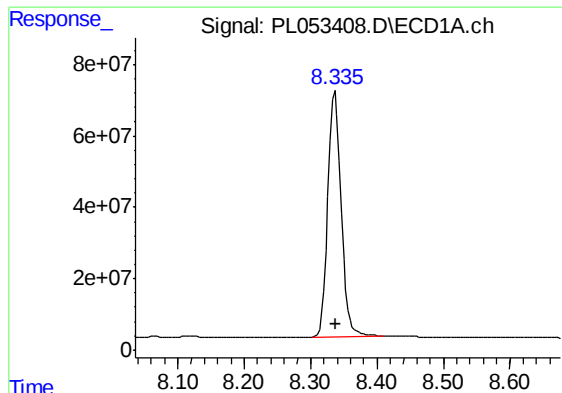

#28 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: 0.000 min
Response: 962246068
Conc: 95.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

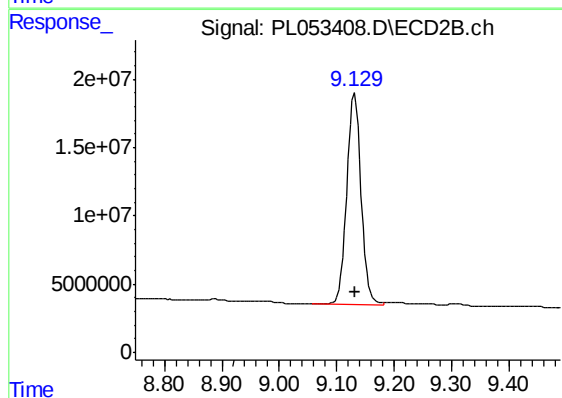

#28 Decachlorobiphenyl

R.T.: 9.131 min
Delta R.T.: 0.000 min
Response: 273409670
Conc: 97.53 ng/ml