

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
 Data File : PL053409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 15:39
 Operator : SG\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 03:29:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 03:23:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	4.047	971.2E6	180.1E6	71.402	71.667
28)	SA Decachlor...	8.338	9.131	712.6E6	198.1E6	70.887	70.679
Target Compounds							
23)	Chlordane-1	4.430	5.045	290.1E6	68018861	731.678	720.081
24)	Chlordane-2	4.936	5.513	313.0E6	74925018	712.245	714.464
25)	Chlordane-3	5.512	6.160	967.9E6	293.7E6	725.636	733.897
26)	Chlordane-4	5.570	6.235	800.4E6	354.9E6	727.494	729.451
27)	Chlordane-5	6.413	7.040	309.0E6	60677437	744.793	719.750


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
Data File : PL053409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 15:39
Operator : SG\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 03:29:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 03:23:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

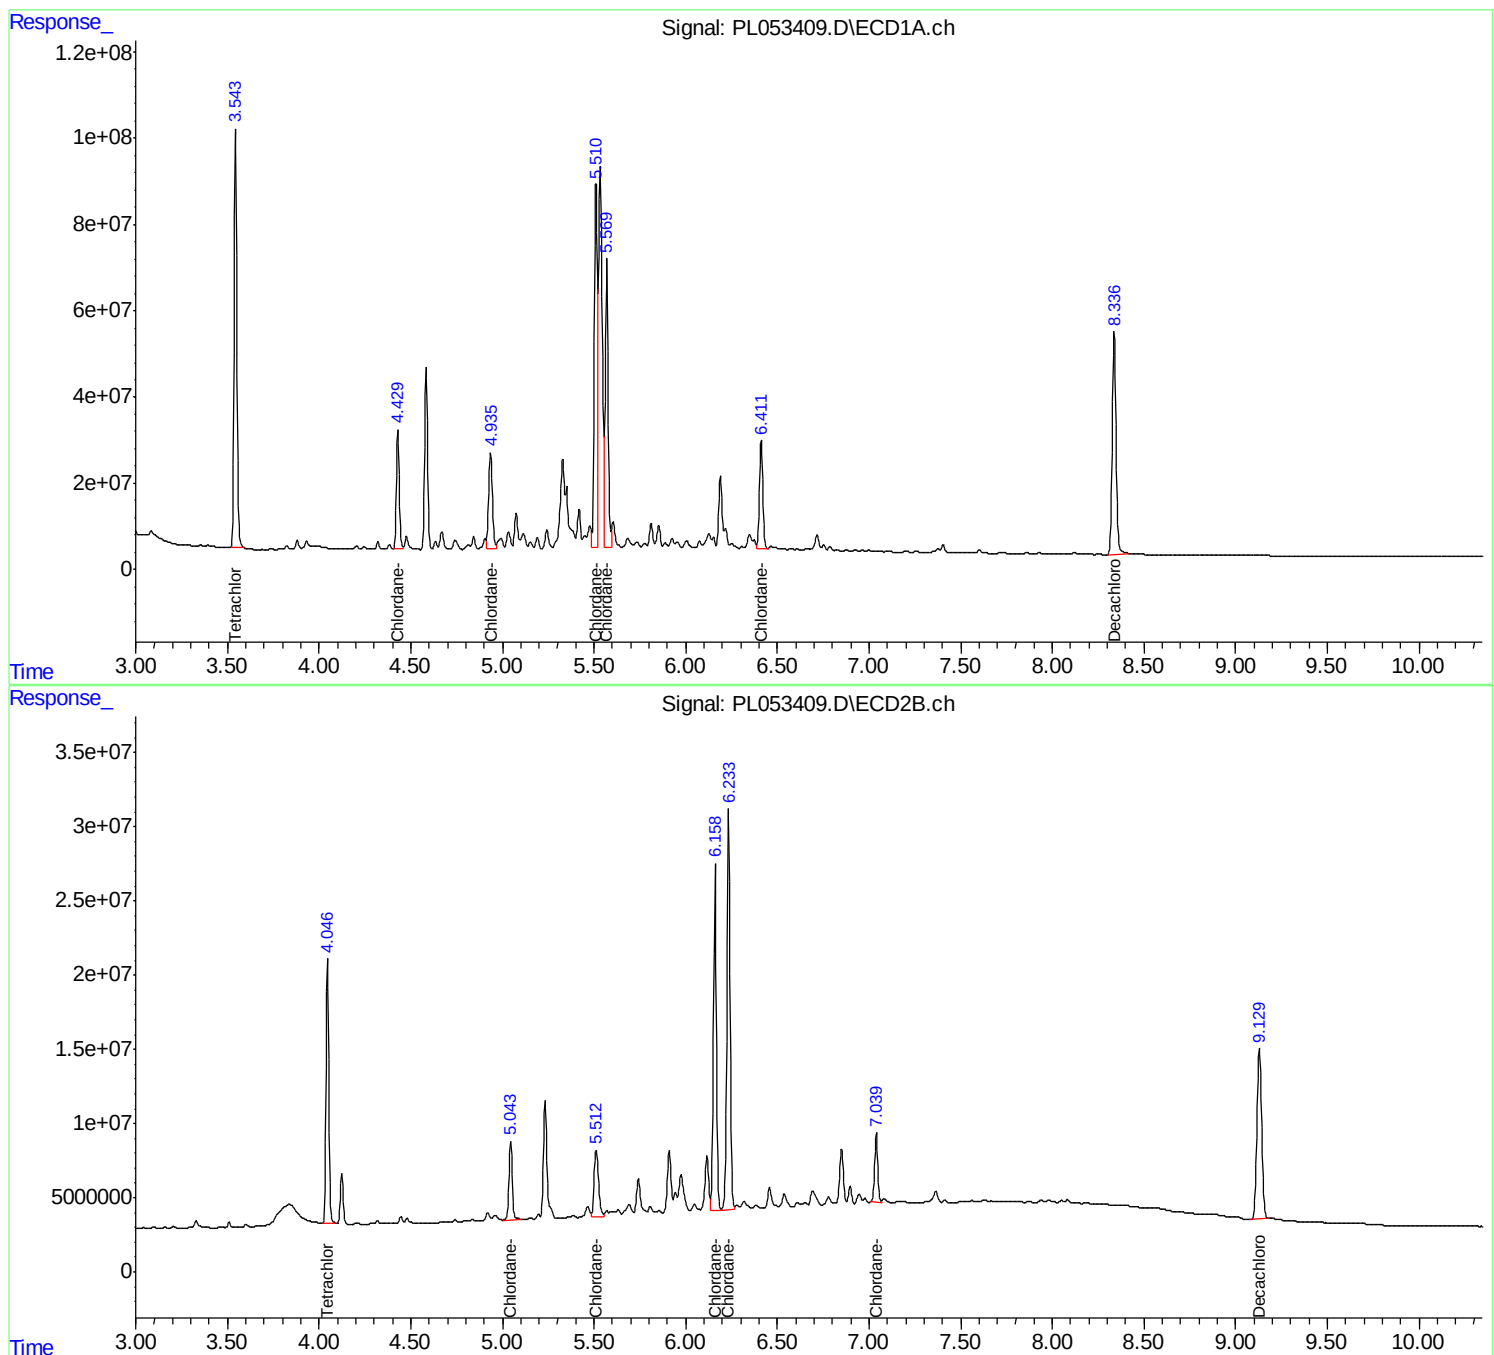


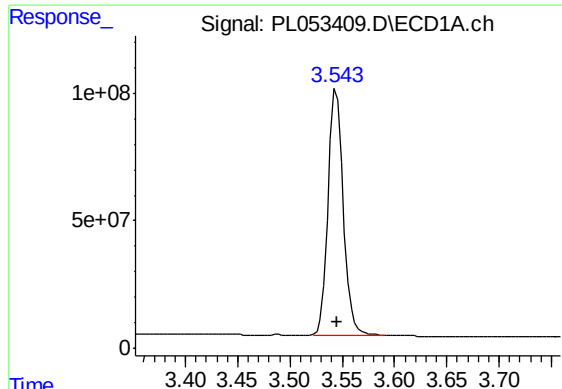

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 971242660
Conc: 71.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

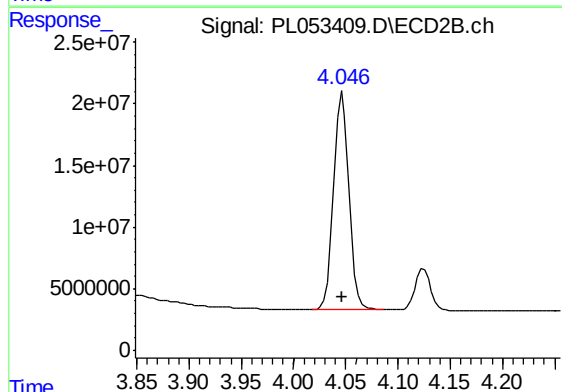


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 180093838
Conc: 71.67 ng/ml

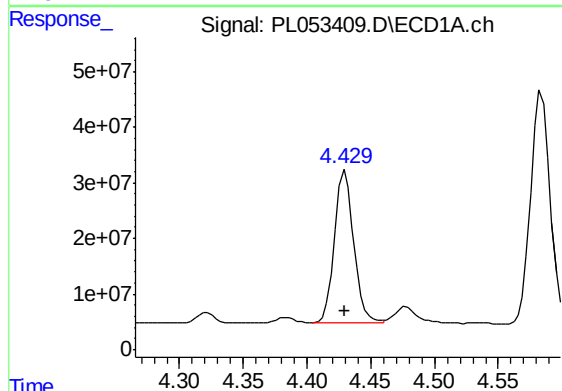


#23 Chlordane-1

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 290073841
Conc: 731.68 ng/ml

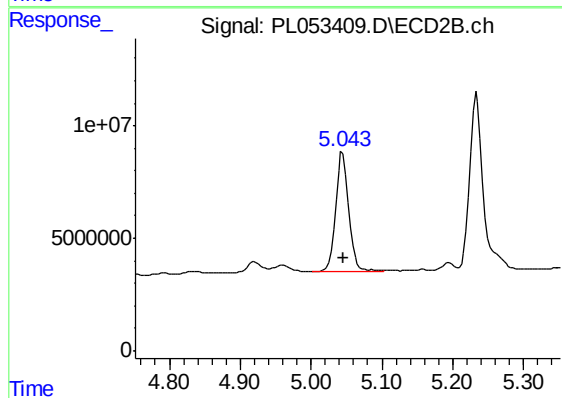

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 68018861
Conc: 720.08 ng/ml

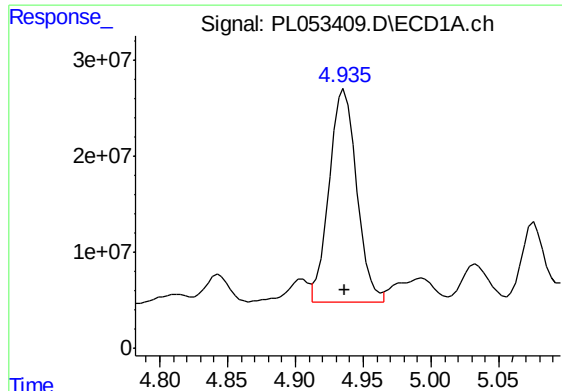

#24 Chlordane-2


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 313020036
Conc: 712.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

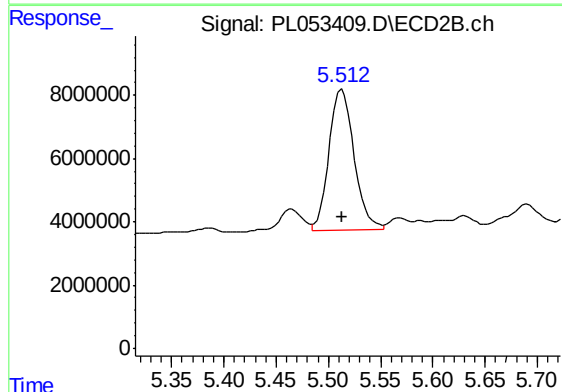


#24 Chlordane-2

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 74925018
Conc: 714.46 ng/ml

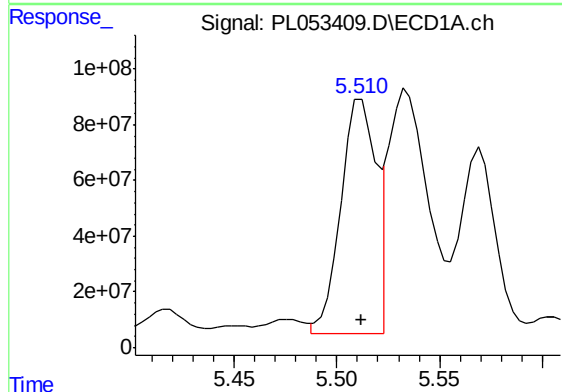


#25 Chlordane-3

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 967923924
Conc: 725.64 ng/ml

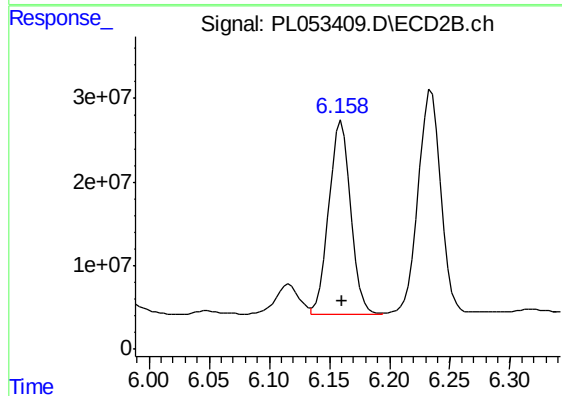

#25 Chlordane-3


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 293715758
Conc: 733.90 ng/ml

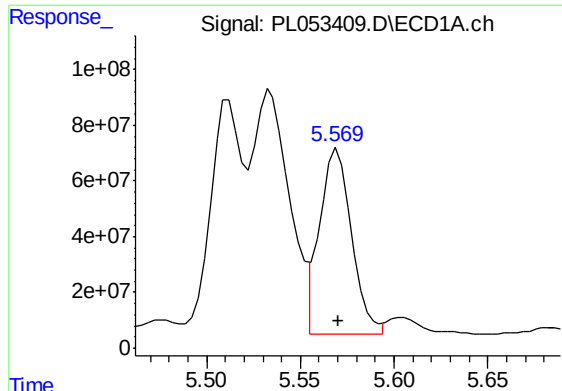

#26 Chlordane-4


R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 800398028
Conc: 727.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

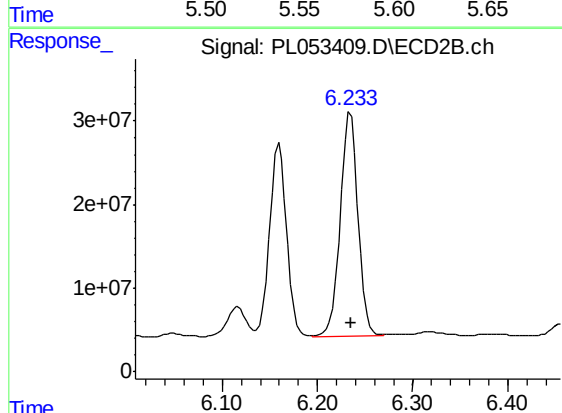


#26 Chlordane-4

R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 354935522
Conc: 729.45 ng/ml

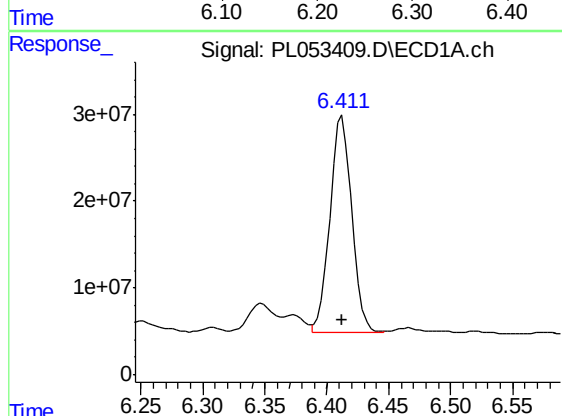


#27 Chlordane-5

R.T.: 6.413 min
Delta R.T.: 0.000 min
Response: 308963336
Conc: 744.79 ng/ml

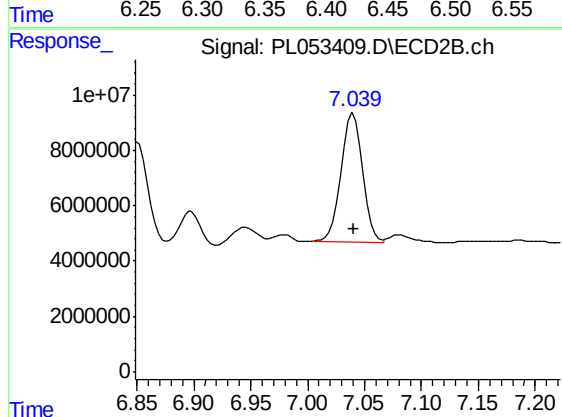

#27 Chlordane-5


R.T.: 7.040 min
Delta R.T.: 0.000 min
Response: 60677437
Conc: 719.75 ng/ml

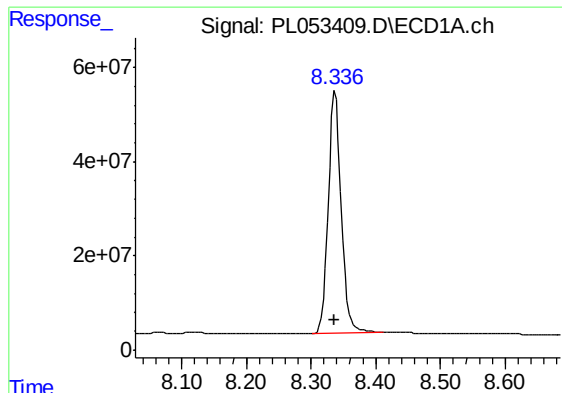

#28 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: 0.000 min
Response: 712609925
Conc: 70.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

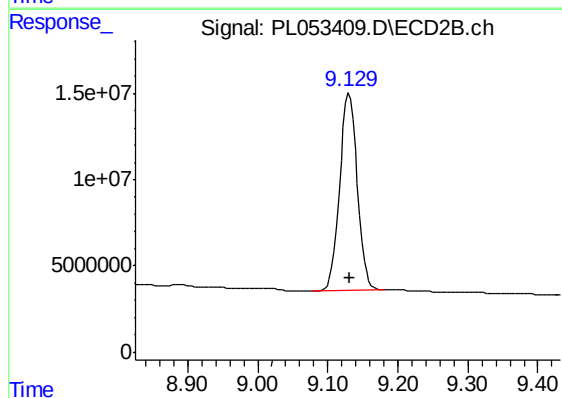

#28 Decachlorobiphenyl

R.T.: 9.131 min
Delta R.T.: 0.000 min
Response: 198135944
Conc: 70.68 ng/ml