

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
 Data File : PL053415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 17:58
 Operator : SG\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL101819CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 04:44:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 04:15:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.047	663.3E6	121.8E6	58.524	46.924
28)	SA Decachlor...	8.336	9.130	495.5E6	135.6E6	47.015	46.512
Target Compounds							
23)	Chlordane-1	4.429	5.045	196.7E6	47074599	511.568	500.509
24)	Chlordane-2	4.936	5.513	217.6E6	51737342	506.574	501.315
25)	Chlordane-3	5.512	6.160	661.2E6	197.9E6	529.779	504.595
26)	Chlordane-4	5.570	6.234	545.3E6	240.3E6	532.236	501.982
27)	Chlordane-5	6.412	7.040	203.8E6	41927398	500.280	507.627



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101819\
Data File : PL053415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 17:58
Operator : SG\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL101819CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 04:44:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101819.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 04:15:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

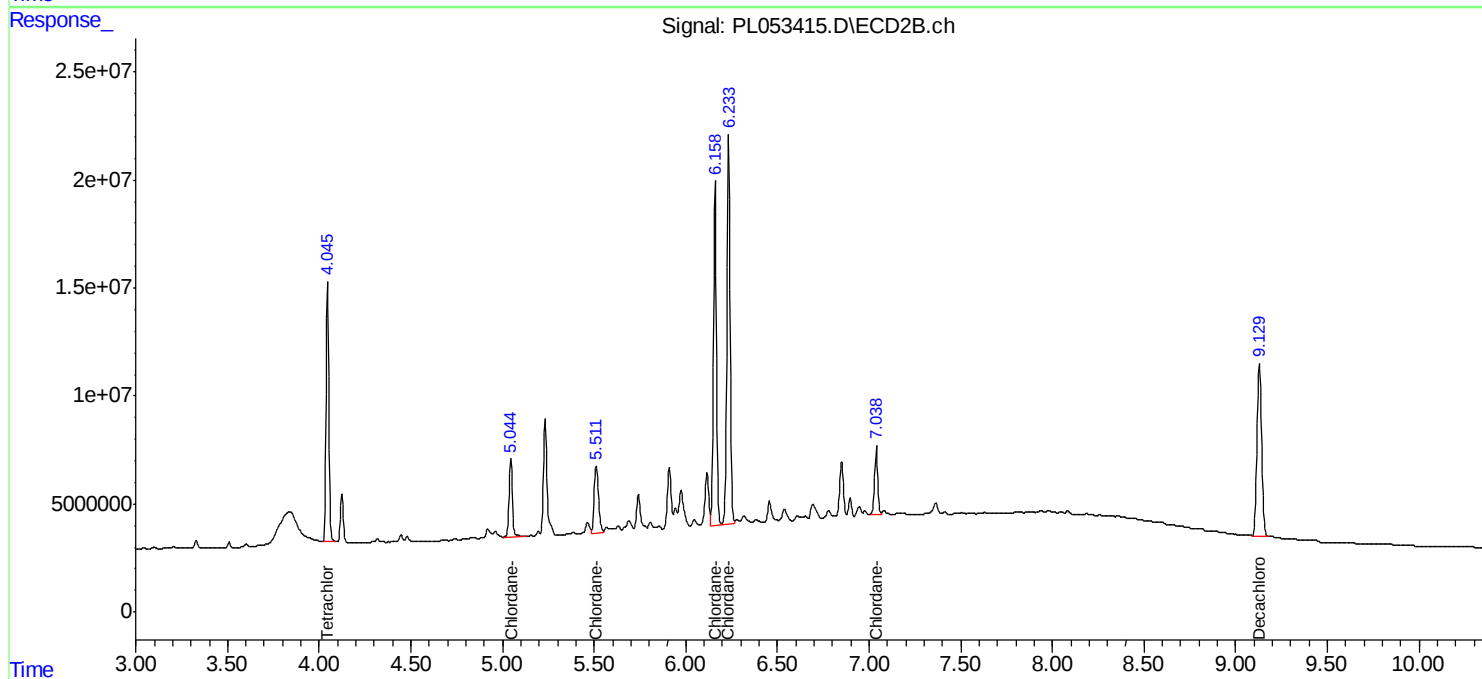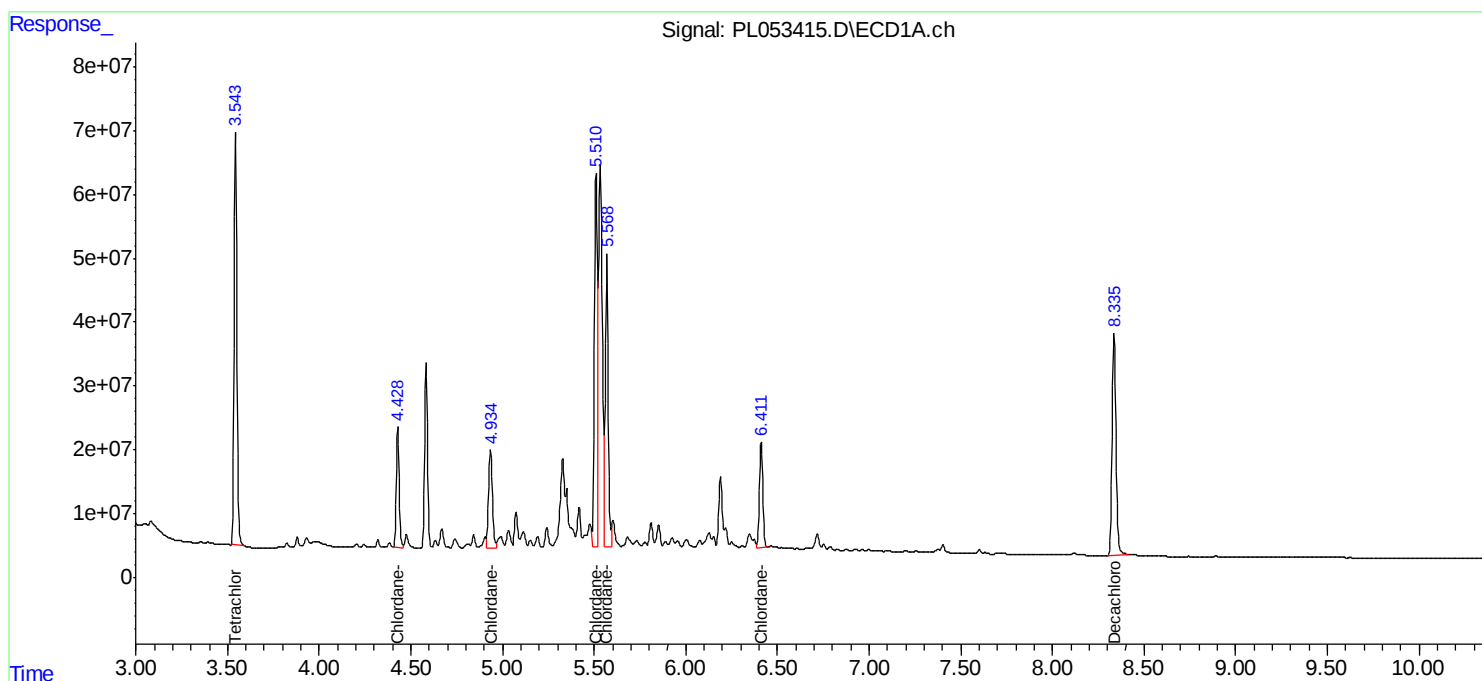


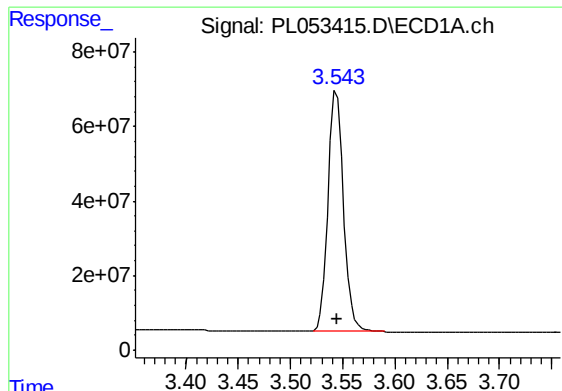

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 663262199
Conc: 58.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101819CHLOR

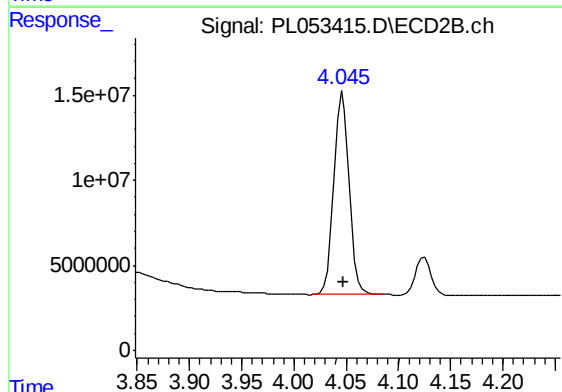


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 121755755
Conc: 46.92 ng/ml

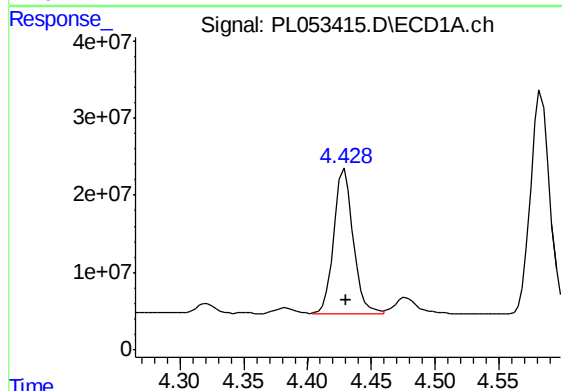


#23 Chlordane-1

R.T.: 4.429 min
Delta R.T.: 0.000 min
Response: 196712133
Conc: 511.57 ng/ml

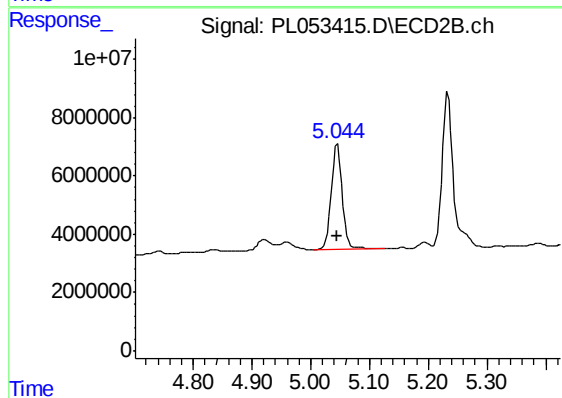

#23 Chlordane-1


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 47074599
Conc: 500.51 ng/ml

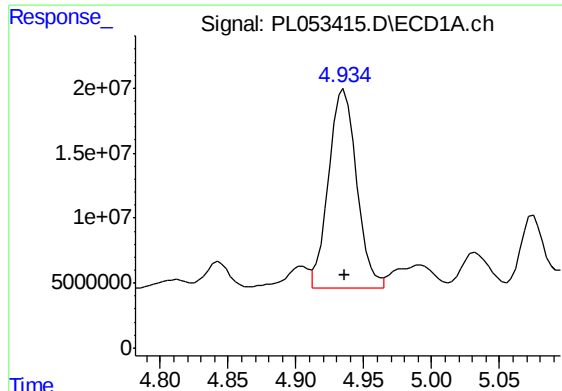

#24 Chlordane-2


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 217614035
Conc: 506.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101819CHLOR

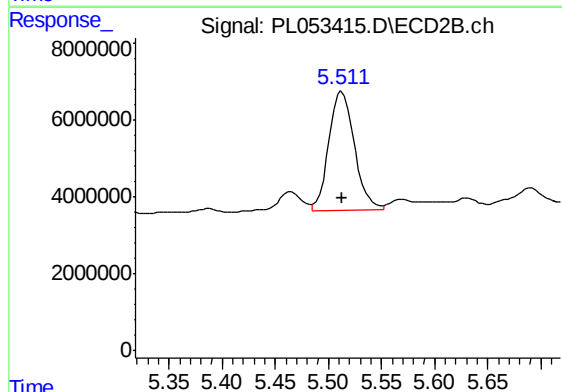


#24 Chlordane-2

R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 51737342
Conc: 501.32 ng/ml

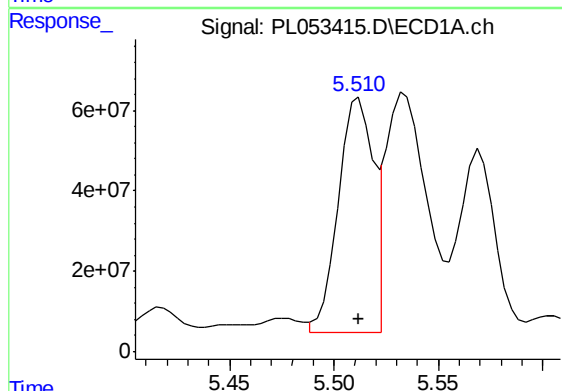


#25 Chlordane-3

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 661173104
Conc: 529.78 ng/ml

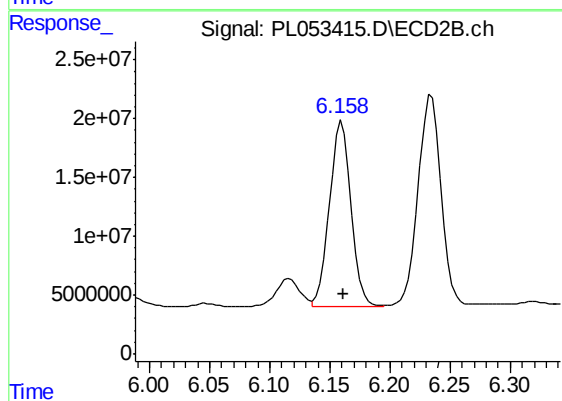

#25 Chlordane-3


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 197936759
Conc: 504.60 ng/ml

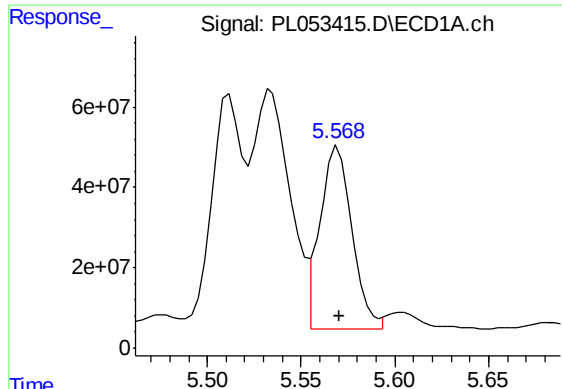

#26 Chlordane-4


R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 545268549
Conc: 532.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101819CHLOR

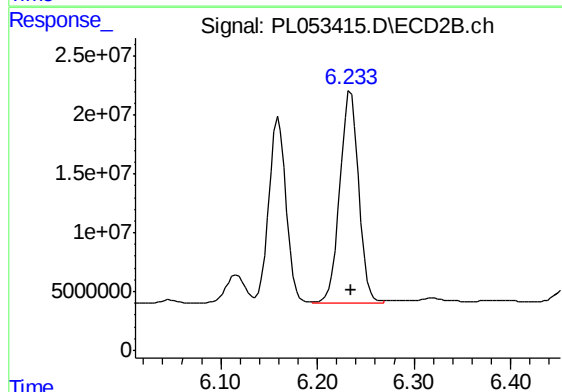


#26 Chlordane-4

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 240265161
Conc: 501.98 ng/ml

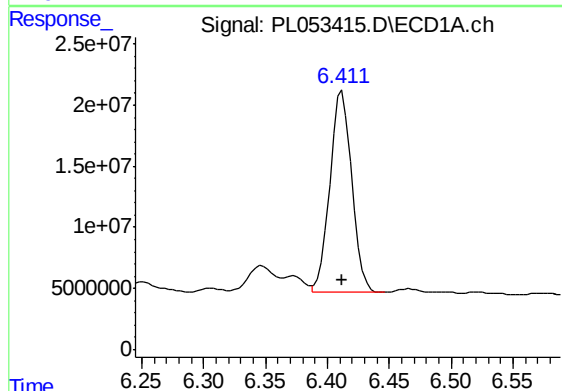


#27 Chlordane-5

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 203813444
Conc: 500.28 ng/ml

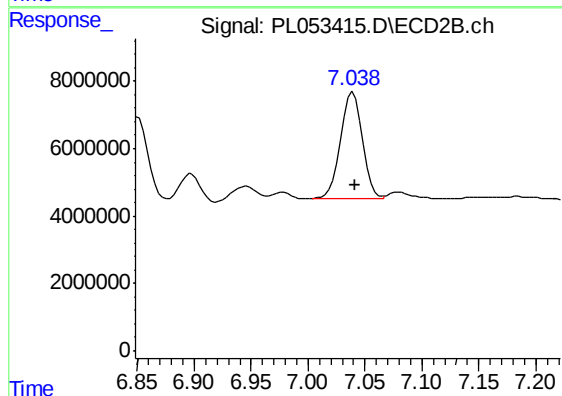

#27 Chlordane-5


R.T.: 7.040 min
Delta R.T.: -0.001 min
Response: 41927398
Conc: 507.63 ng/ml

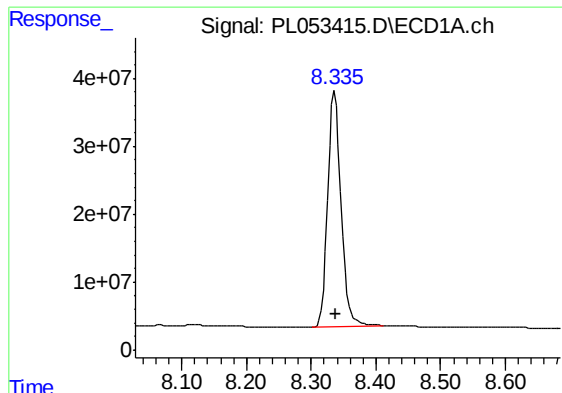

#28 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: 0.000 min
Response: 495481806
Conc: 47.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101819CHLOR

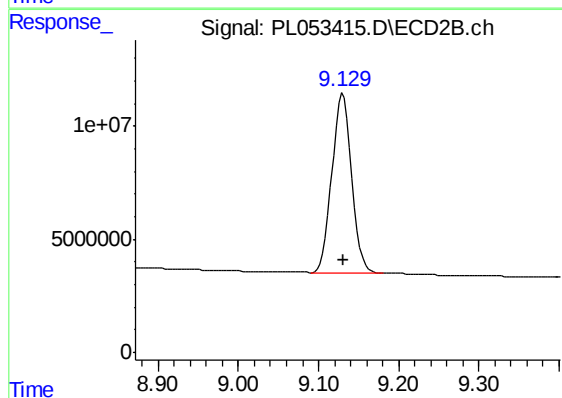

#28 Decachlorobiphenyl

R.T.: 9.130 min
Delta R.T.: 0.000 min
Response: 135601212
Conc: 46.51 ng/ml