

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101821\
 Data File : PL070390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2021 22:06
 Operator : AR\AJ
 Sample : M4252-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-BA-(1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 05:40:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.624	5.562	6961321	17916237	13.912	13.546
28)	SA Decachlor...	10.390	11.484	9930418	15646506	14.351	12.929
Target Compounds							
17)	MA 4,4'-DDT	8.468	9.423	729529	1166658	1.193	0.893 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101821\
Data File : PL070390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2021 22:06
Operator : AR\AJ
Sample : M4252-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-BA-(1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 05:40:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

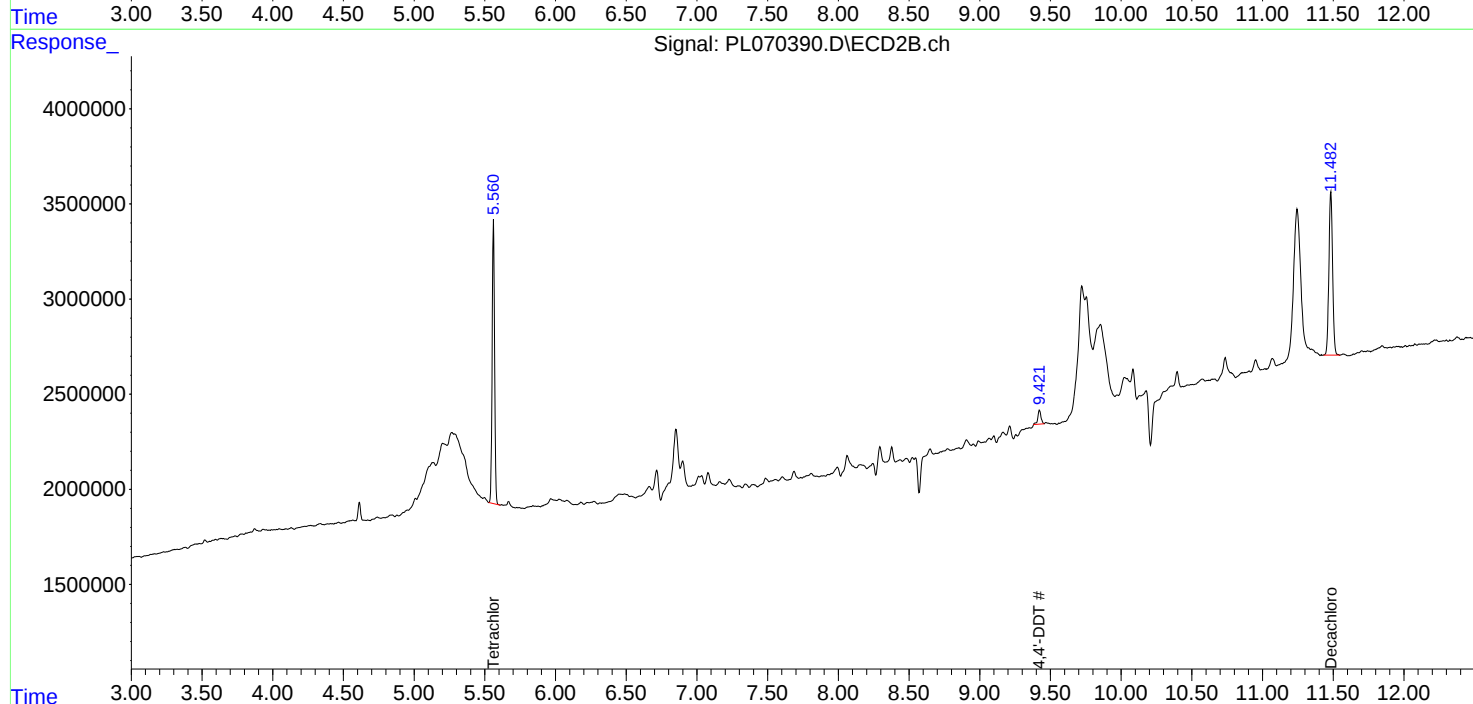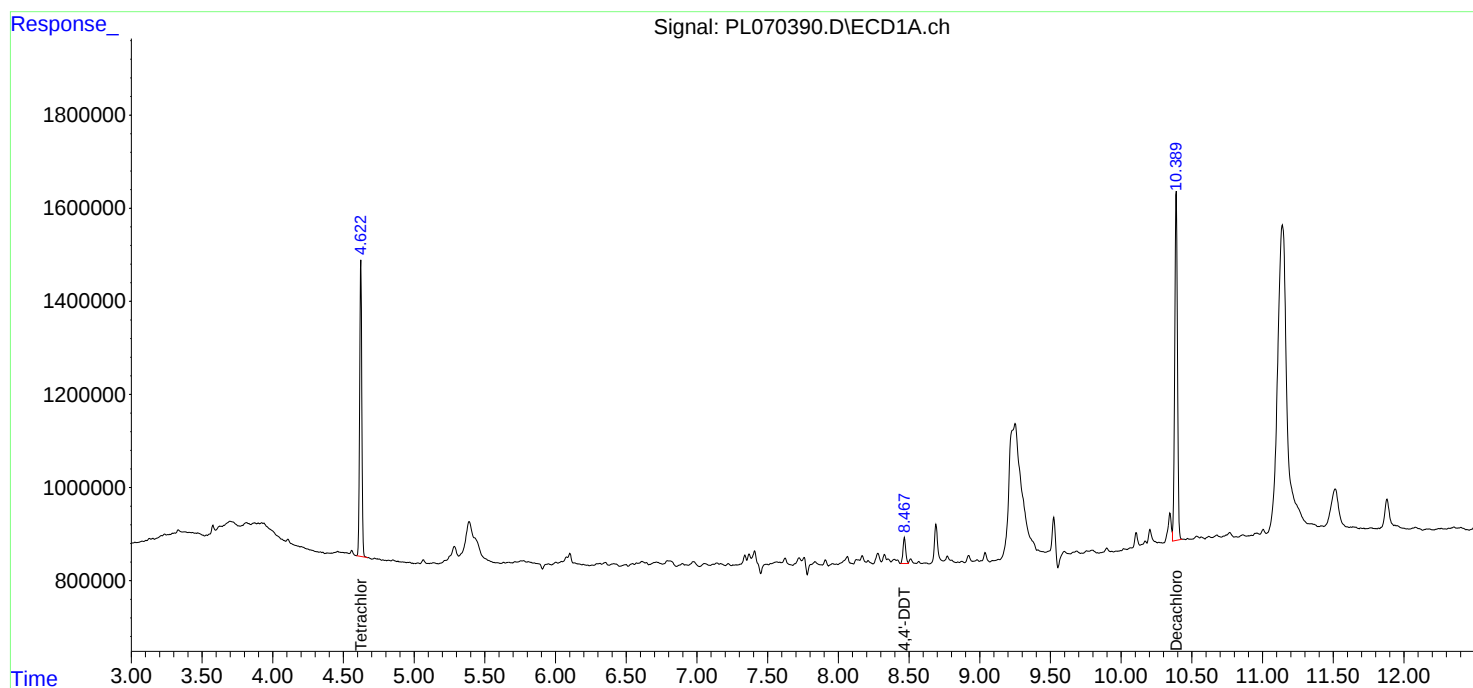


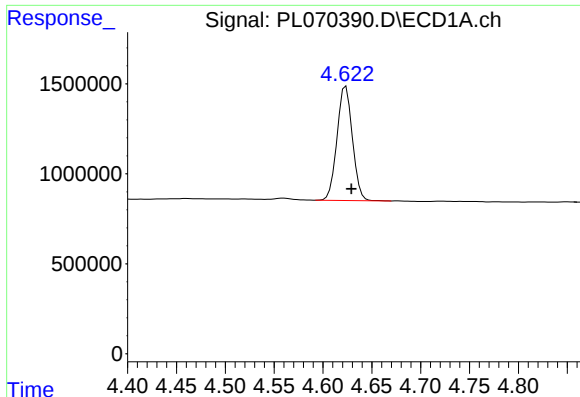

#1 Tetrachloro-m-xylene


R.T.: 4.624 min
Delta R.T.: -0.005 min
Response: 6961321
Conc: 13.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-BA-(1)

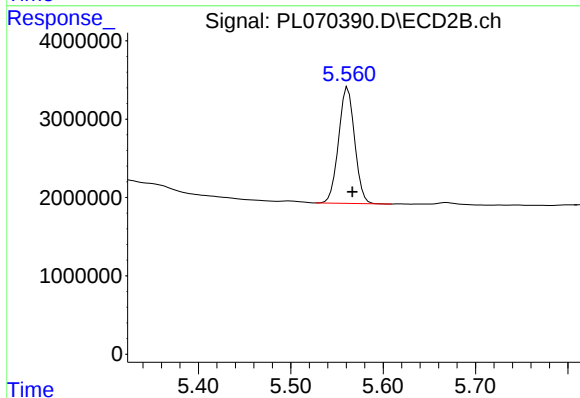


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 17916237
Conc: 13.55 ng/ml

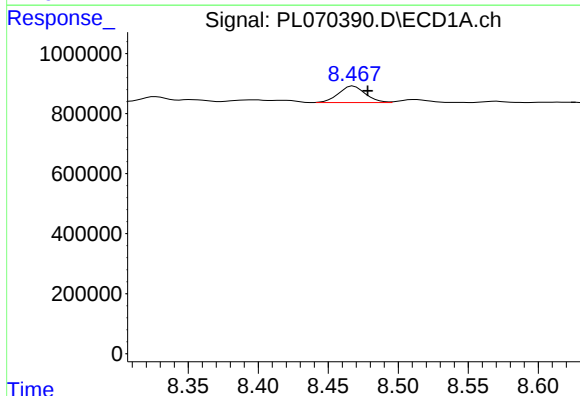


#17 4,4'-DDT

R.T.: 8.468 min
Delta R.T.: -0.010 min
Response: 729529
Conc: 1.19 ng/ml

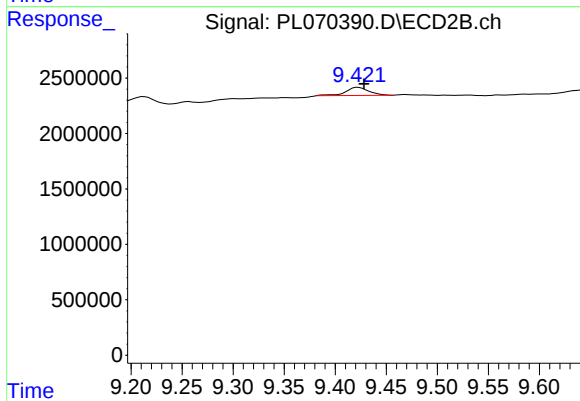

#17 4,4'-DDT


R.T.: 9.423 min
Delta R.T.: -0.006 min
Response: 1166658
Conc: 0.89 ng/ml

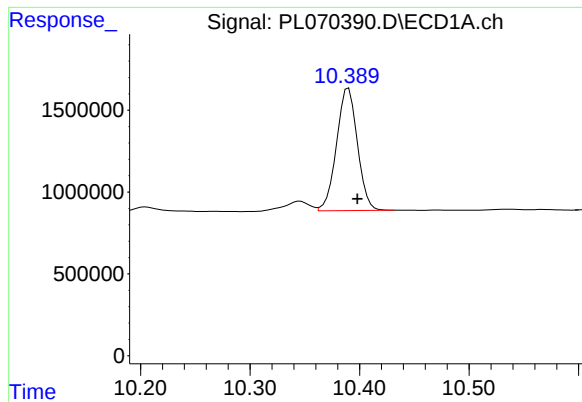

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.008 min
Response: 9930418
Conc: 14.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-BA-(1)

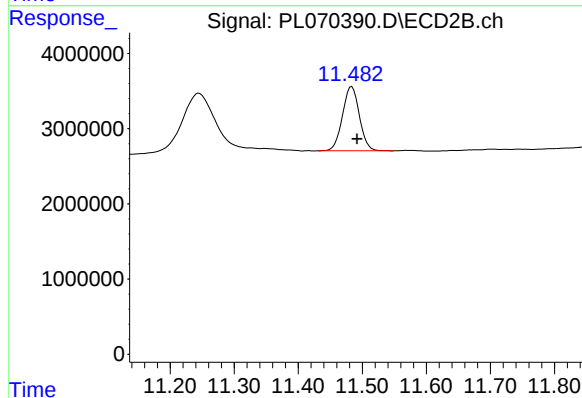

#28 Decachlorobiphenyl

R.T.: 11.484 min
Delta R.T.: -0.008 min
Response: 15646506
Conc: 12.93 ng/ml