

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101823\
 Data File : PL085998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2023 15:04
 Operator : AR\AJ
 Sample : 04872-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 QUARTERLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/19/2023
 Supervised By :Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 16:52:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	2.622	51225270	20786395	17.223m	22.253 #
2)	SA Decachlor...	8.862	7.775	50527309	20241886	23.198	21.931

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101823\
Data File : PL085998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2023 15:04
Operator : AR\AJ
Sample : 04872-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/19/2023
Supervised By : Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 16:52:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

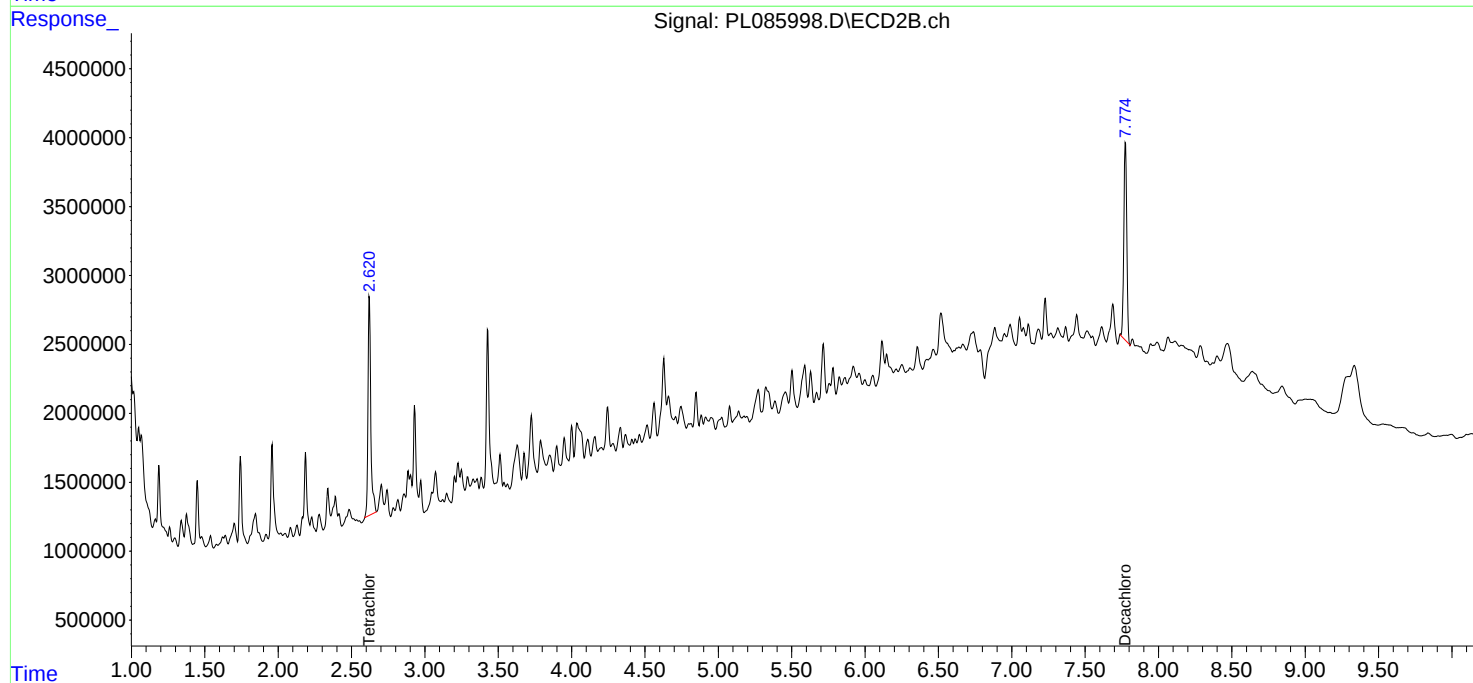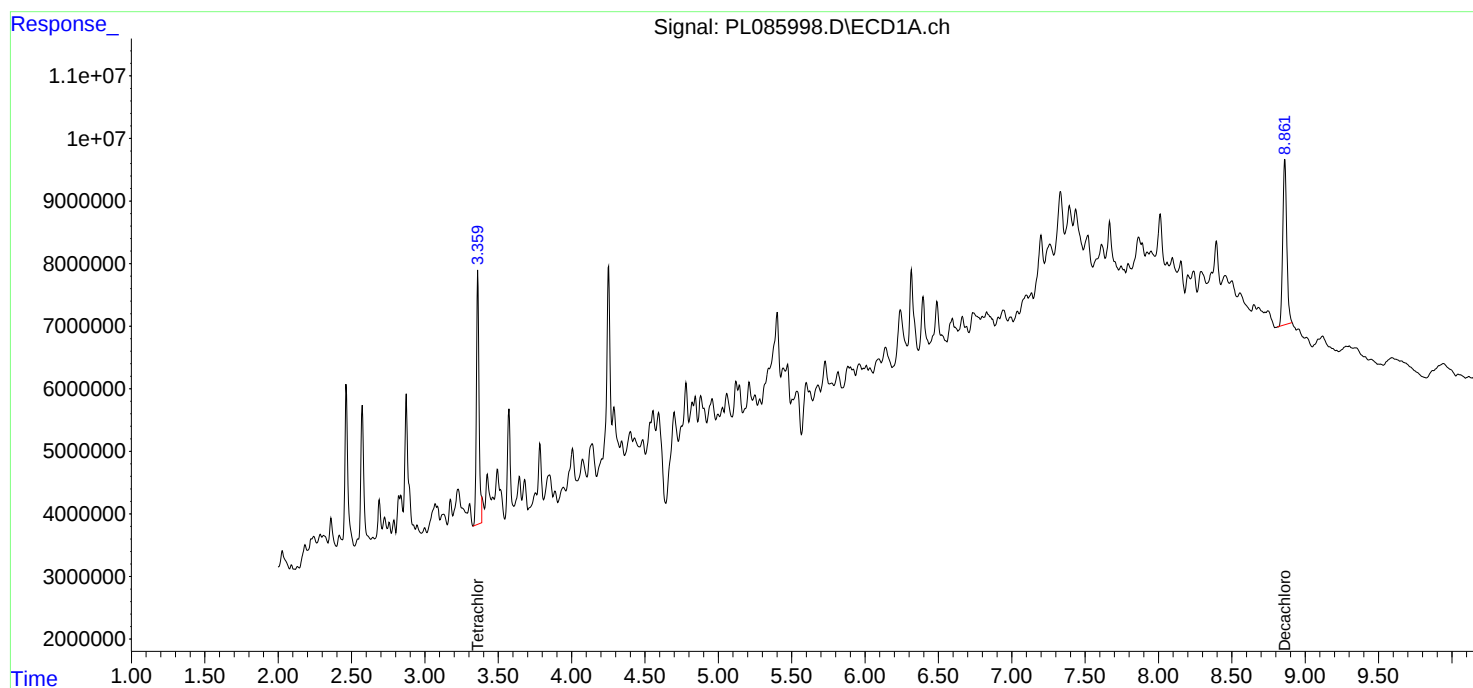

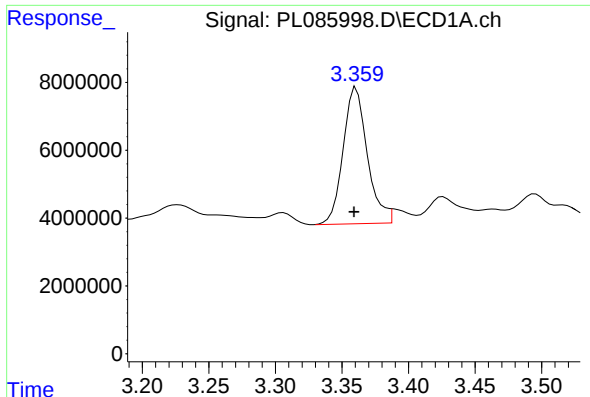


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 51225270
Conc: 17.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/19/2023
Supervised By :Ankita Jodhani 10/19/2023

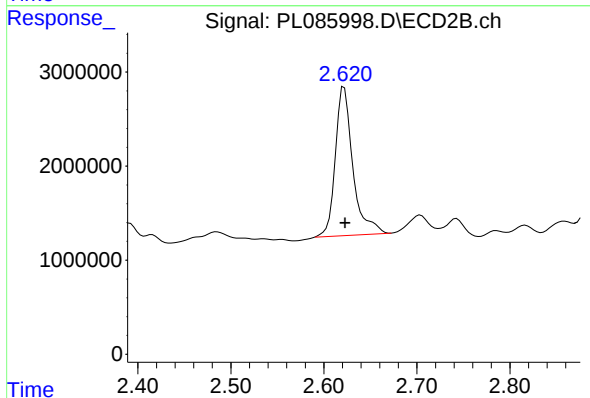


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 20786395
Conc: 22.25 ng/ml

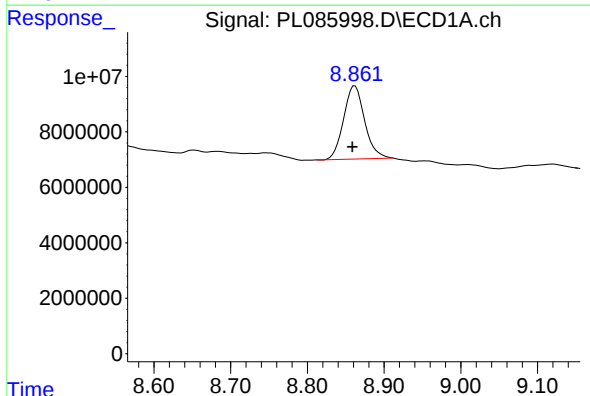

#28 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.003 min
Response: 50527309
Conc: 23.20 ng/ml

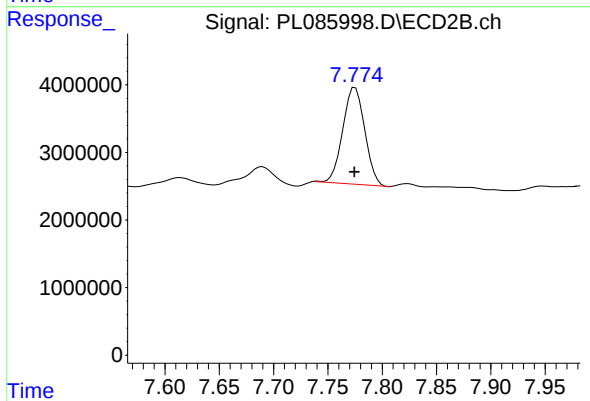

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 20241886
Conc: 21.93 ng/ml