

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101823\
 Data File : PL086009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2023 18:28
 Operator : AR\AJ
 Sample : 04938-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A-2(0-2)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/19/2023
 Supervised By : Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 22:22:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.354	2.621	23214569	6966320	7.805	7.458
2) SA Decachlor...	8.856	7.772	8856521	5409936	4.066m	5.861 #
Target Compounds						
13) MA Dieldrin	6.166	5.208	9320841	2756652	2.837	2.841

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101823\
Data File : PL086009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2023 18:28
Operator : AR\AJ
Sample : 04938-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
A-2(0-2)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/19/2023
Supervised By : Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 22:22:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

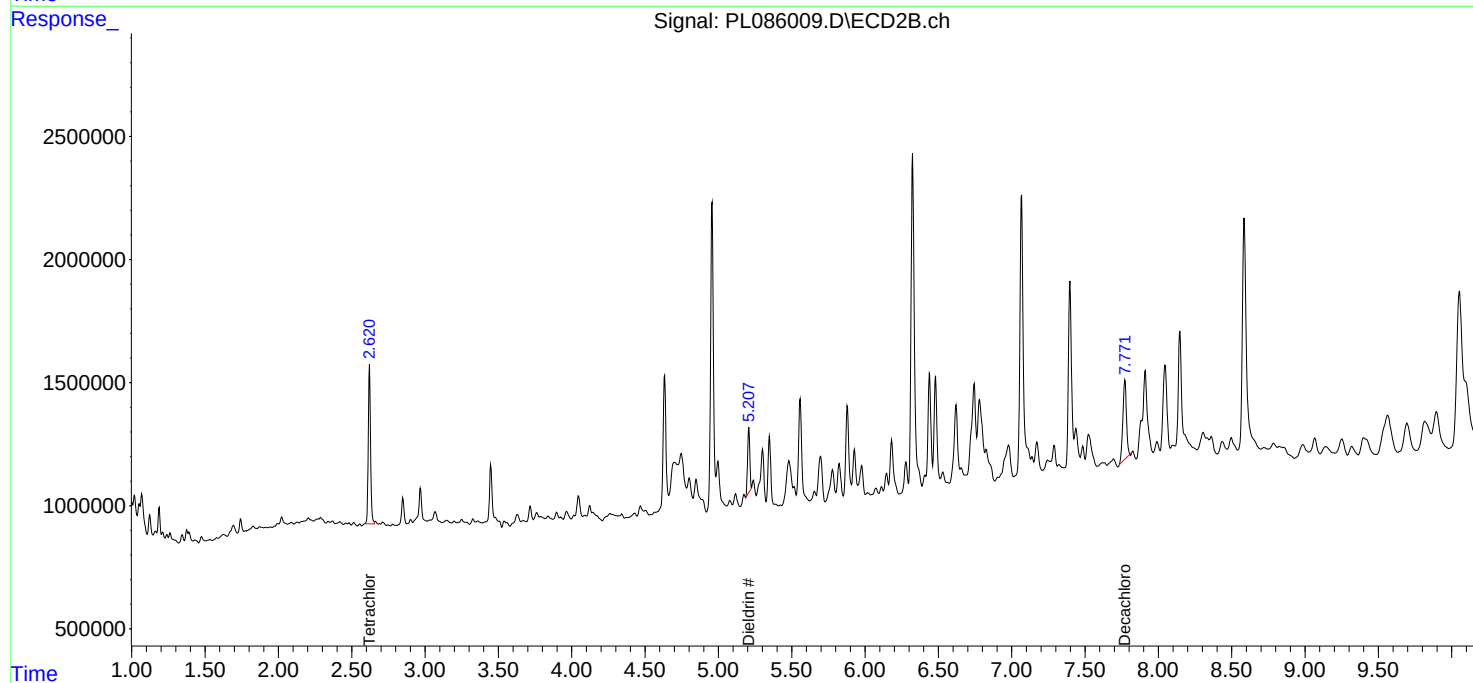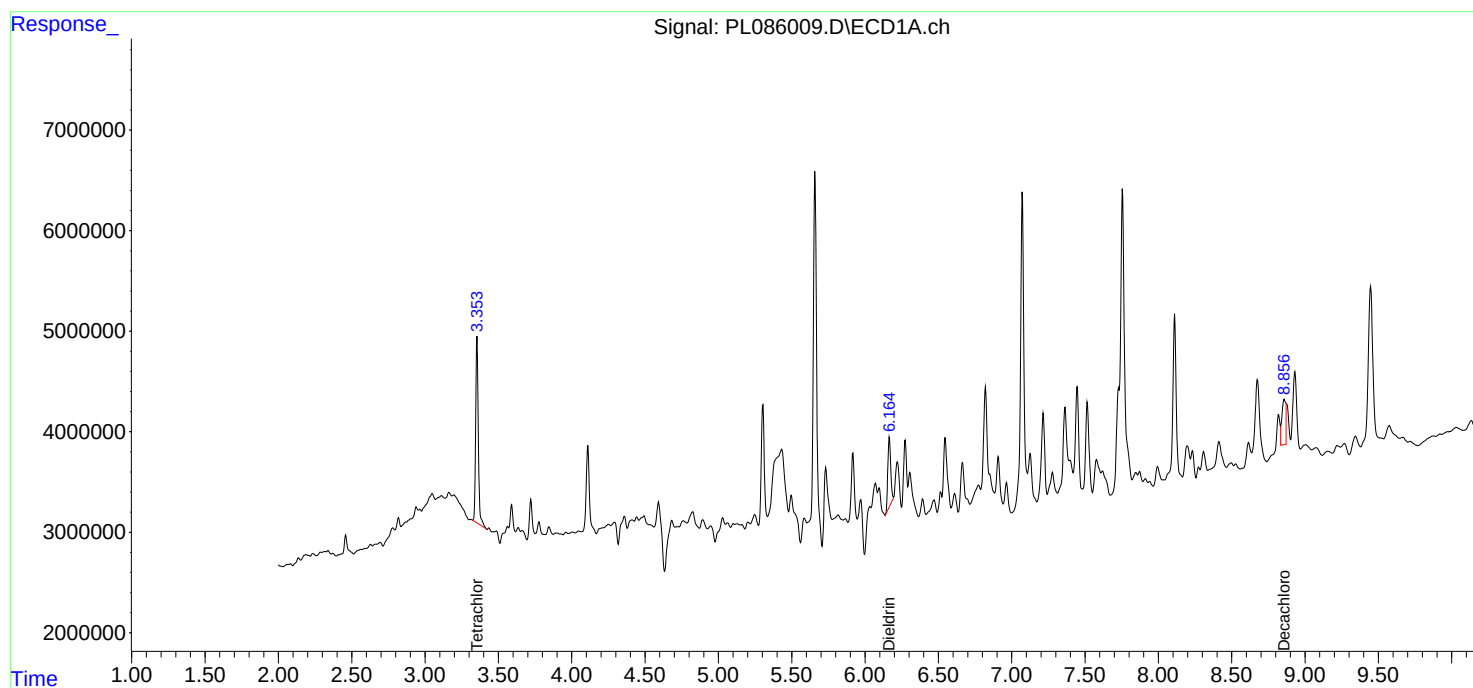

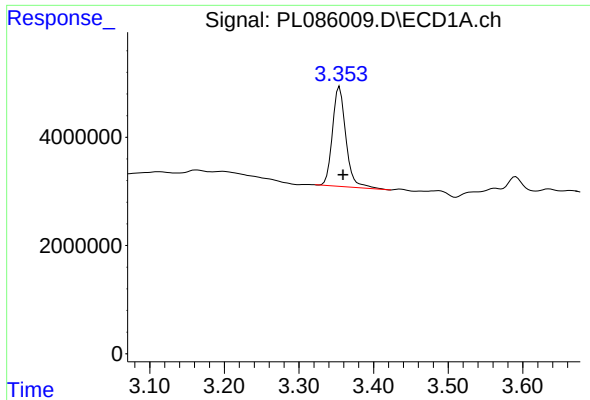


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: -0.005 min
Response: 23214569
Conc: 7.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
A-2(0-2)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/19/2023
Supervised By :Ankita Jodhani 10/19/2023

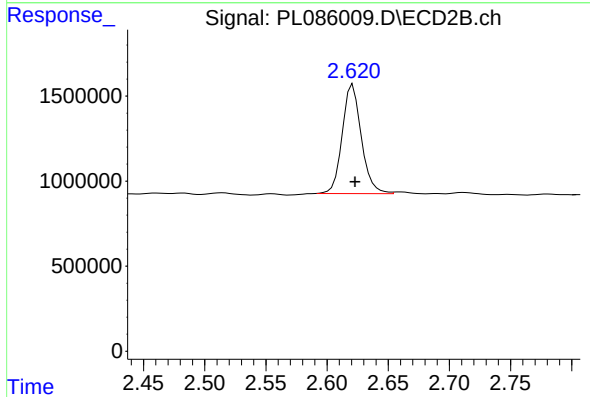


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 6966320
Conc: 7.46 ng/ml

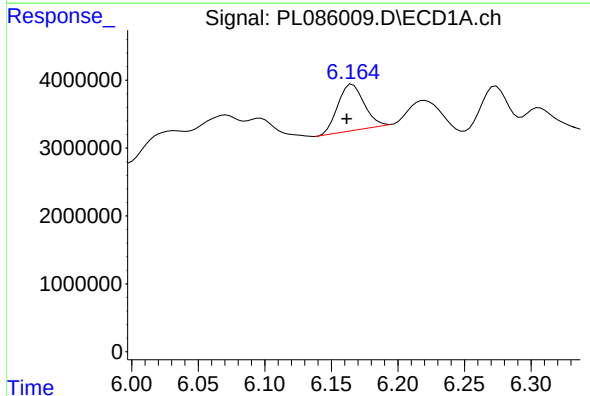


#13 Dieldrin

R.T.: 6.166 min
Delta R.T.: 0.004 min
Response: 9320841
Conc: 2.84 ng/ml

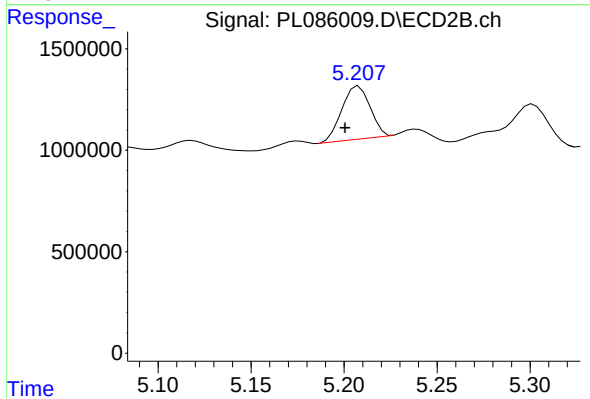

#13 Dieldrin

R.T.: 5.208 min
Delta R.T.: 0.007 min
Response: 2756652
Conc: 2.84 ng/ml

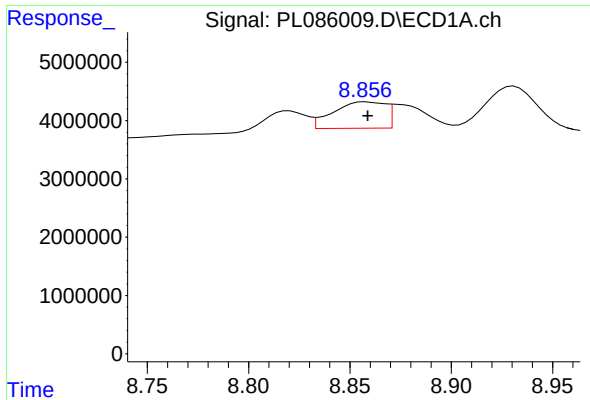


#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: -0.003 min
Response: 8856521
Conc: 4.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
A-2(0-2)

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/19/2023
Supervised By :Ankita Jodhani 10/19/2023

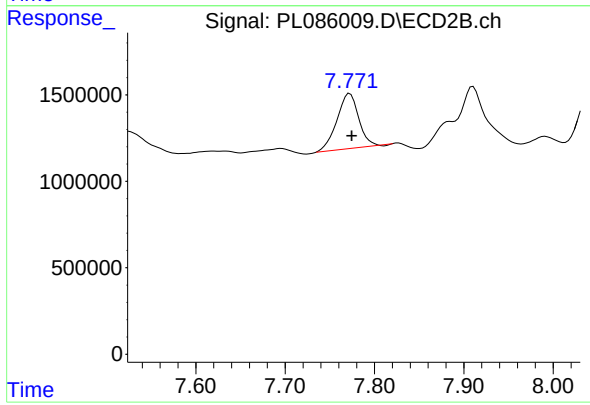

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: -0.002 min
Response: 5409936
Conc: 5.86 ng/ml