

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101823\
 Data File : PL086015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2023 20:19
 Operator : AR\AJ
 Sample : 04938-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A-5(0-2)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/19/2023
 Supervised By : Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 22:24:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.621	10024461	5574452	3.371m	5.968 #
28)	SA Decachlor...	8.880	7.759	471.5E6	28608770	216.469m	30.996m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101823\
Data File : PL086015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2023 20:19
Operator : AR\AJ
Sample : 04938-09
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
A-5(0-2)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/19/2023
Supervised By : Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 22:24:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

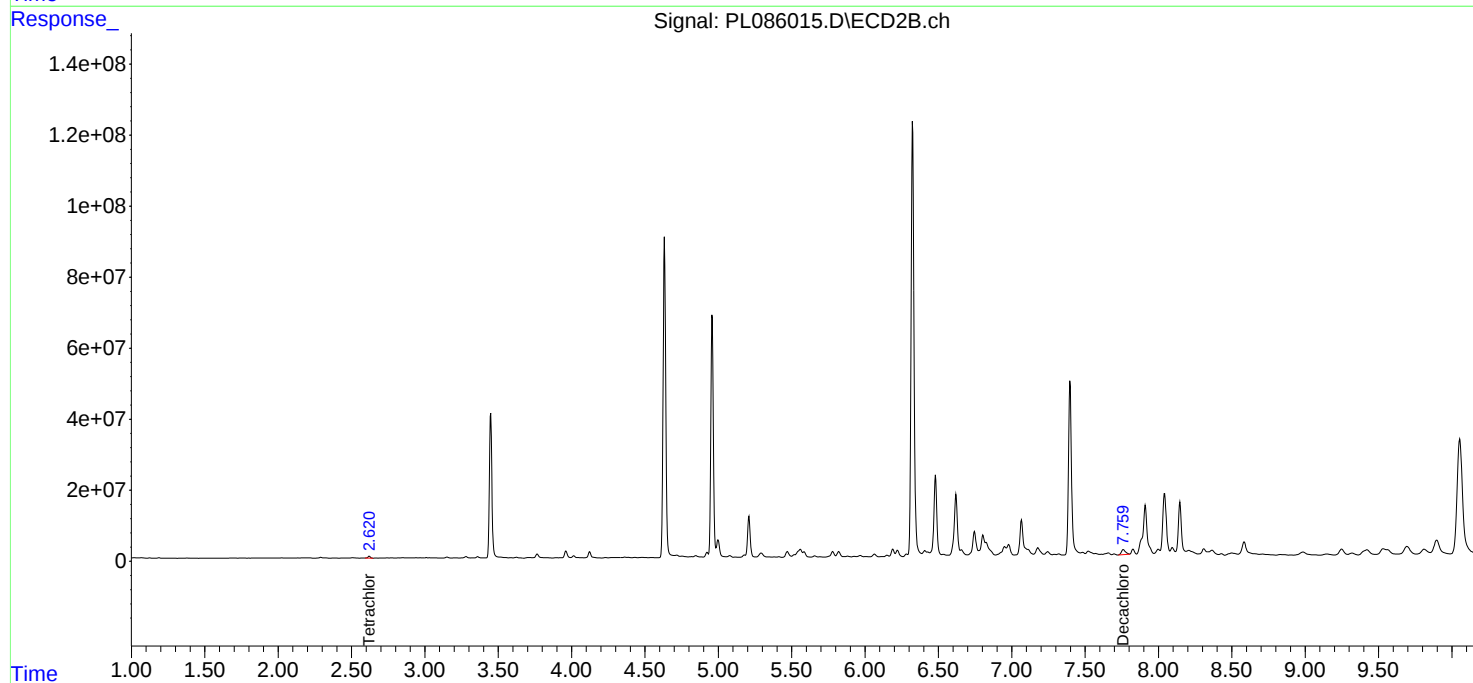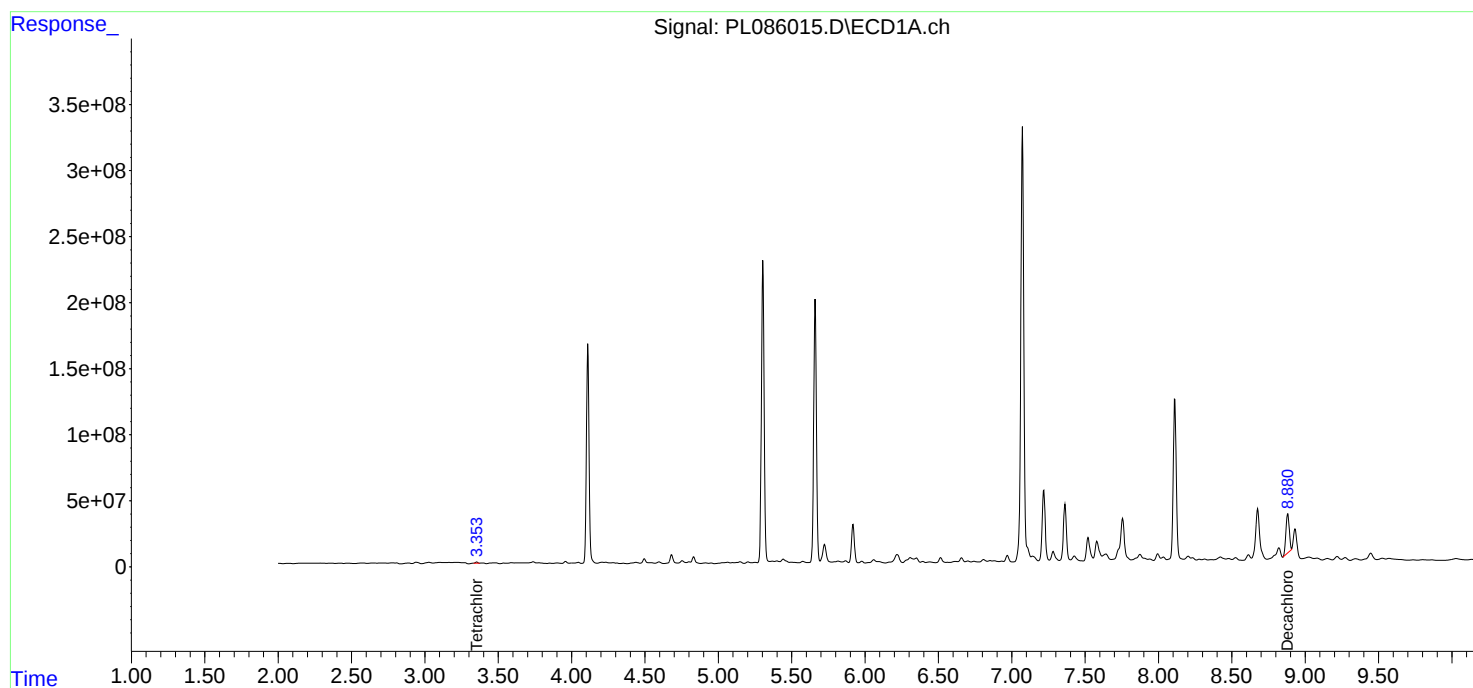

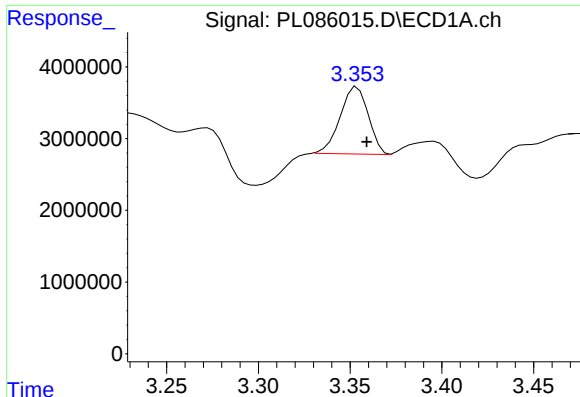


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: -0.006 min
Response: 10024461
Conc: 3.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
A-5(0-2)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/19/2023
Supervised By :Ankita Jodhani 10/19/2023

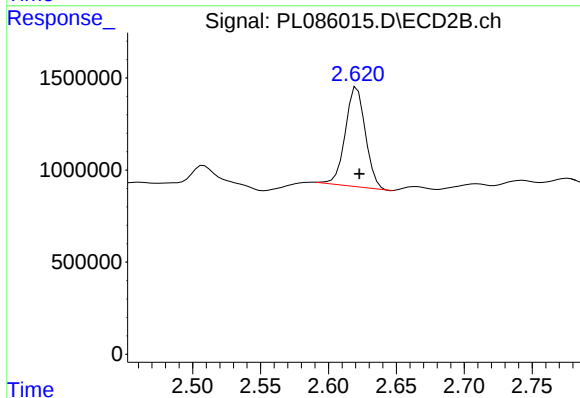


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 5574452
Conc: 5.97 ng/ml

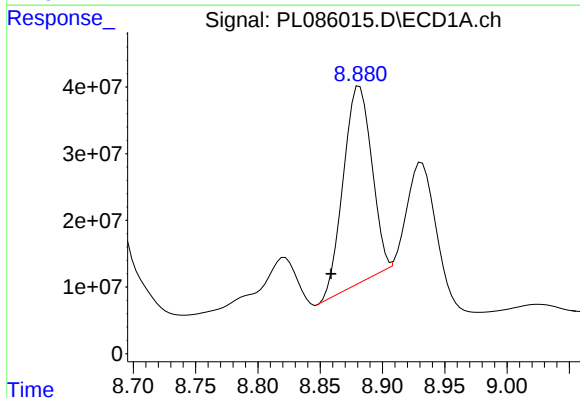

#28 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: 0.022 min
Response: 471480741
Conc: 216.47 ng/ml m

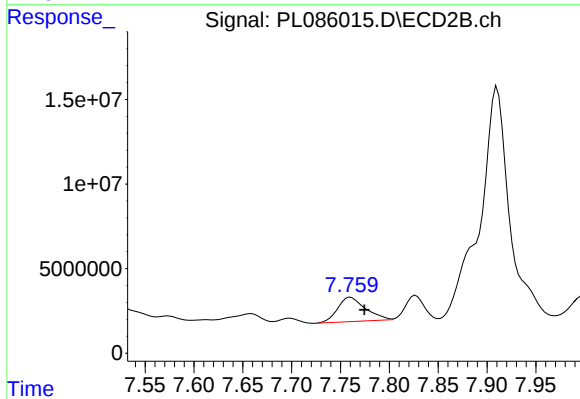

#28 Decachlorobiphenyl

R.T.: 7.759 min
Delta R.T.: -0.016 min
Response: 28608770
Conc: 31.00 ng/ml m