

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
 Data File : PL041157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 12:04
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 23:57:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.261f	5.990	63227118	51009155	9.640	17.785 #
9) A	Endosulfan I	5.554	0.000	8186040	0	1.366	N.D. #
14) MA	Endrin	6.033	0.000	16153602	0	2.812	N.D. #
15) B	Endosulfa...	0.000	6.999f	0	4952144	N.D.	2.085 #
16) A	4,4'-DDD	6.231f	6.913f	9858842	6778902	2.183	3.236 #
20) A	Methoxychlor	0.000	7.643f	0	47186259	N.D.	40.085 #
21) B	Endrin ke...	7.131f	0.000	86882981	0	16.597	N.D. #
23) A	Chlordane-1	4.402	0.000	3673932	0	14.395	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
Data File : PL041157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 12:04
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 23:57:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

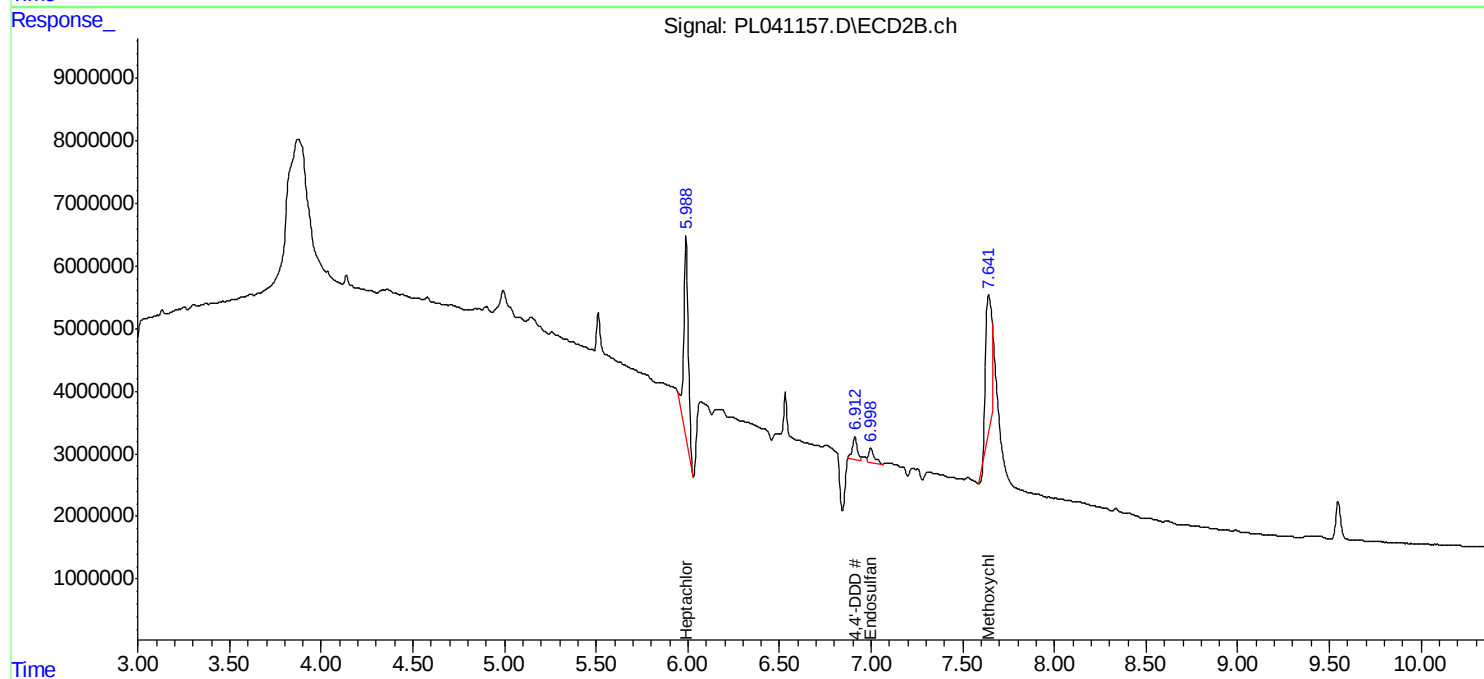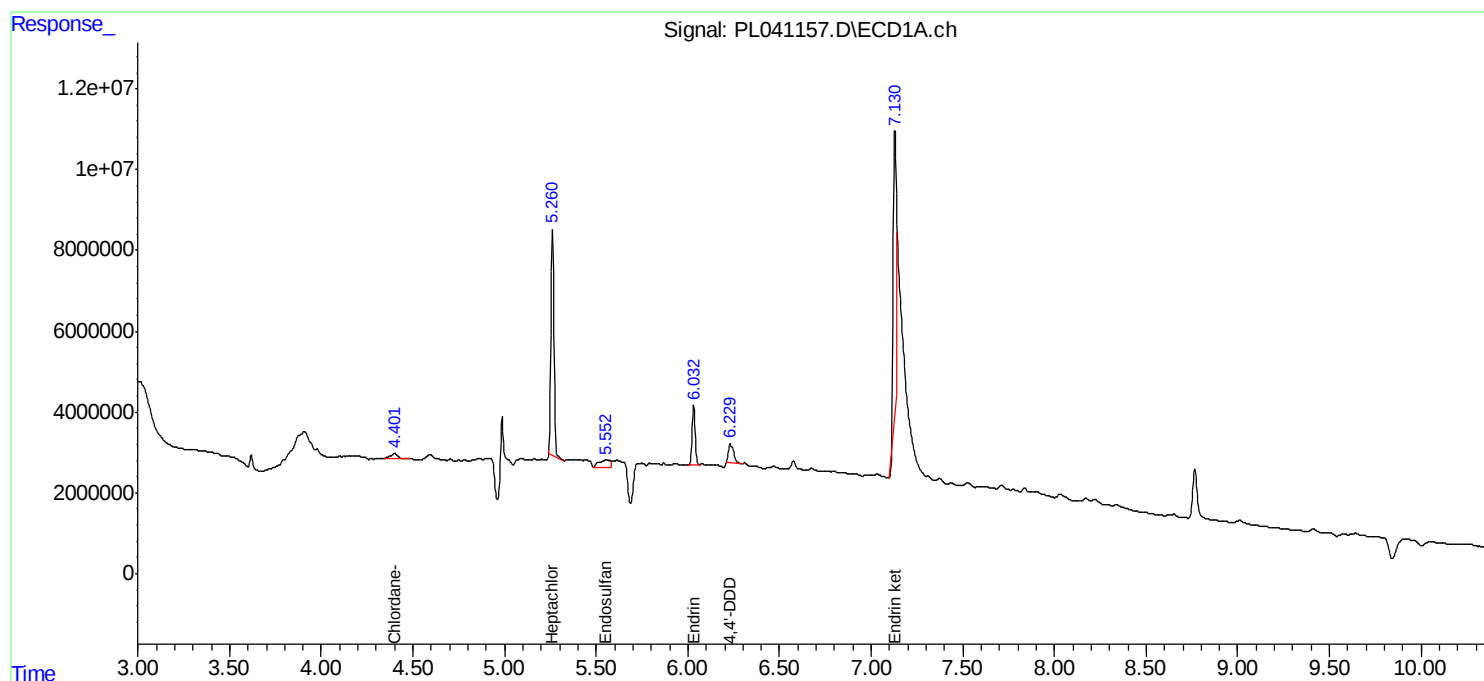


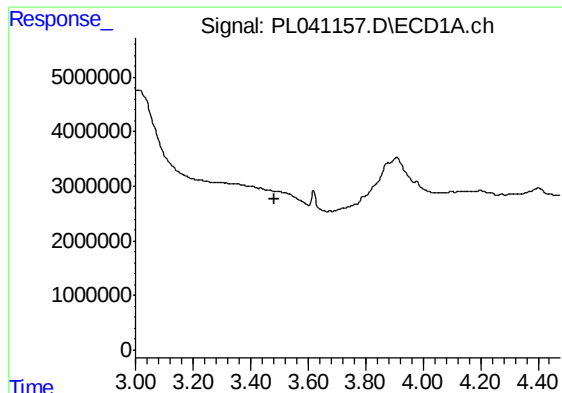

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

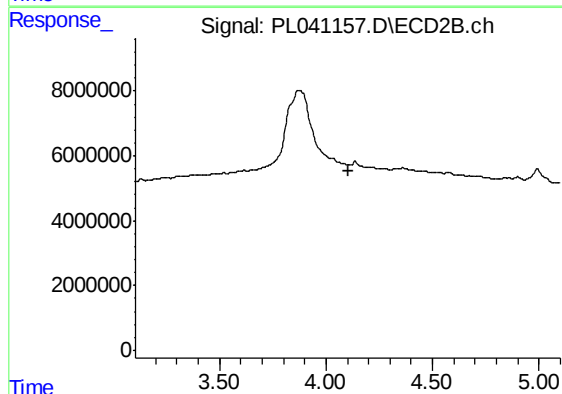


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.104 min
Response: 0
Conc: N.D.

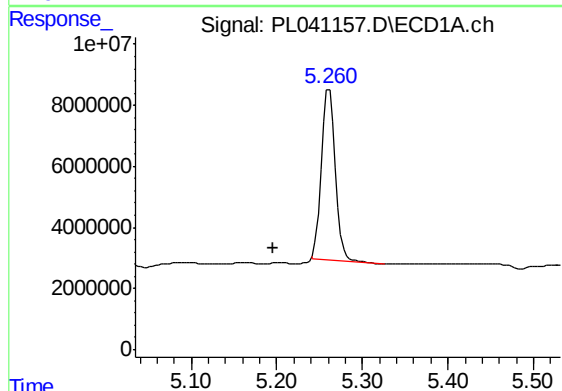


#8 Heptachlor epoxide

R.T.: 5.261 min
Delta R.T.: 0.065 min
Response: 63227118
Conc: 9.64 ng/ml

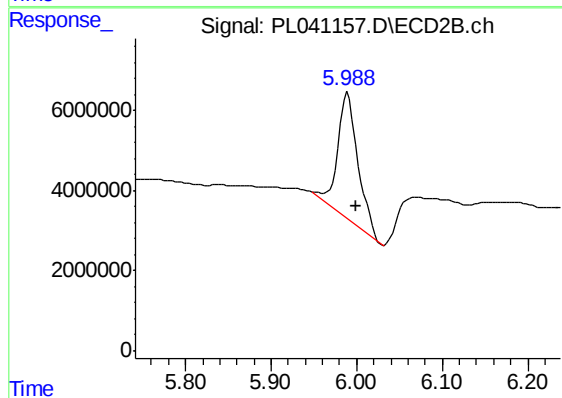

#8 Heptachlor epoxide


R.T.: 5.990 min
Delta R.T.: -0.010 min
Response: 51009155
Conc: 17.78 ng/ml

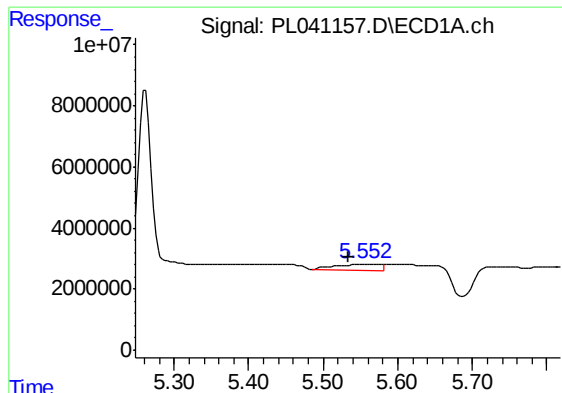

#9 Endosulfan I


R.T.: 5.554 min
Delta R.T.: 0.019 min
Response: 8186040
Conc: 1.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

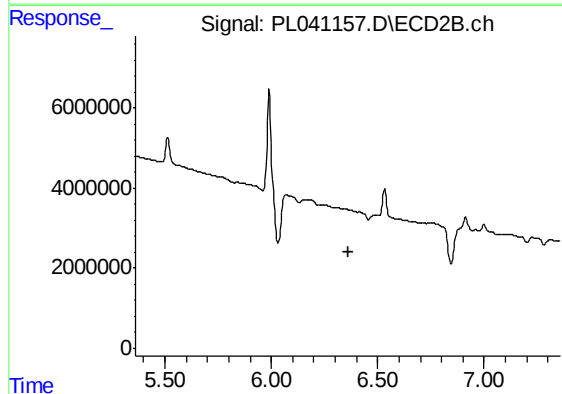


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.360 min
Response: 0
Conc: N.D.

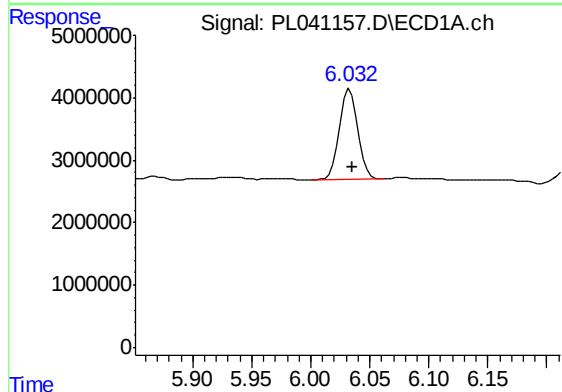


#14 Endrin

R.T.: 6.033 min
Delta R.T.: -0.002 min
Response: 16153602
Conc: 2.81 ng/ml

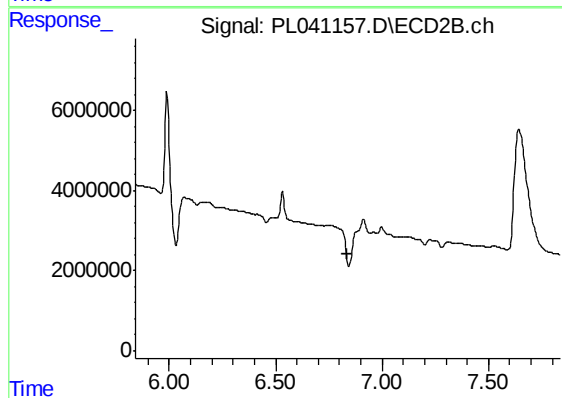

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

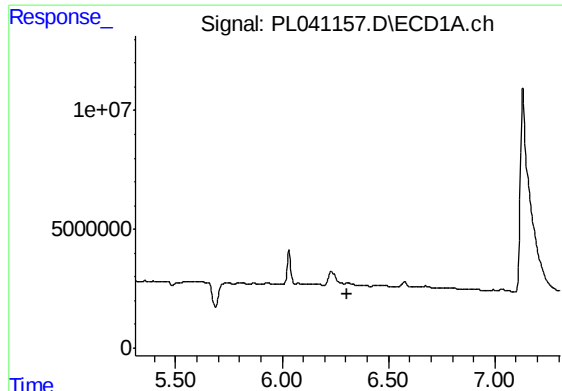

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.309 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

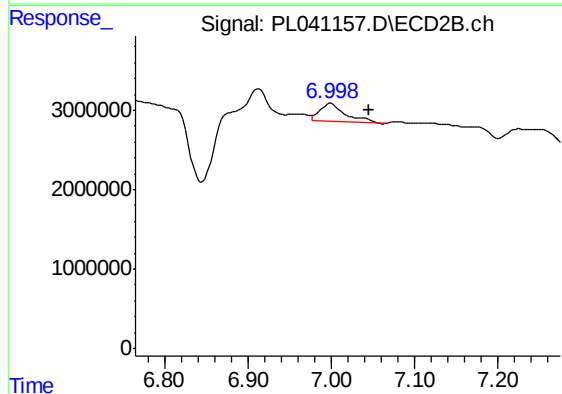


#15 Endosulfan II

R.T.: 6.999 min
Delta R.T.: -0.046 min
Response: 4952144
Conc: 2.09 ng/ml

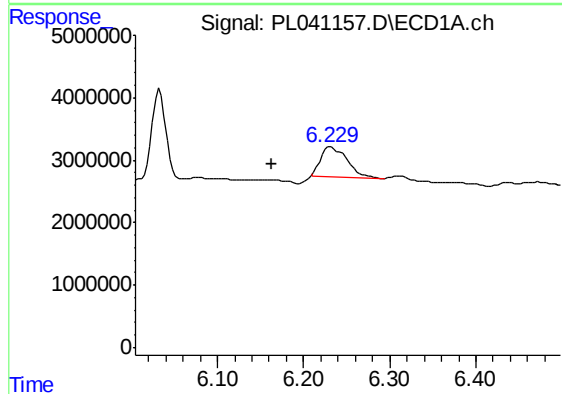


#16 4,4'-DDD

R.T.: 6.231 min
Delta R.T.: 0.068 min
Response: 9858842
Conc: 2.18 ng/ml

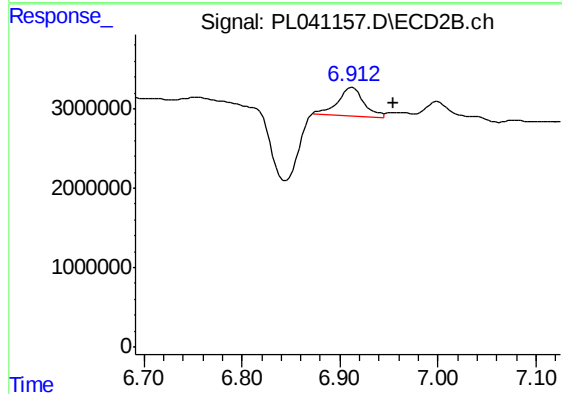

#16 4,4'-DDD


R.T.: 6.913 min
Delta R.T.: -0.041 min
Response: 6778902
Conc: 3.24 ng/ml

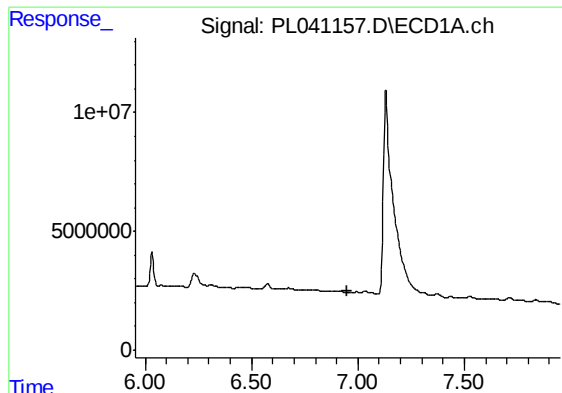

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.952 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

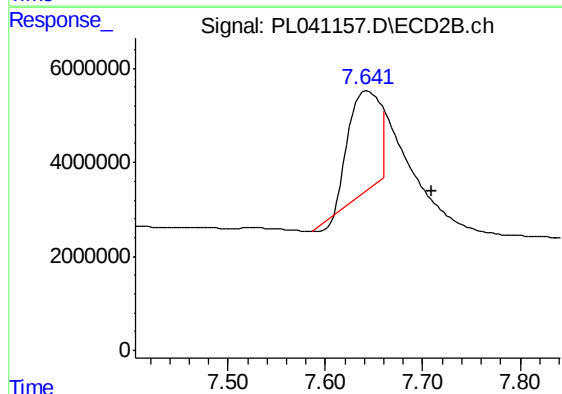


#20 Methoxychlor

R.T.: 7.643 min
Delta R.T.: -0.066 min
Response: 47186259
Conc: 40.09 ng/ml

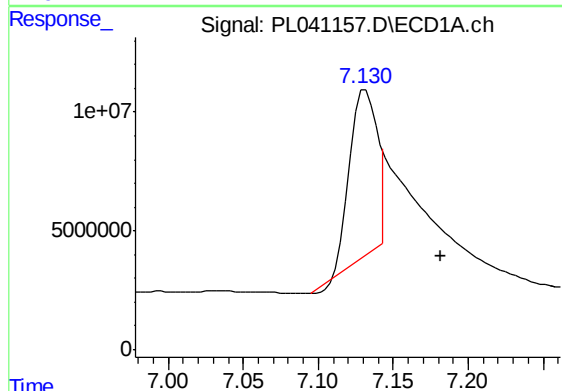


#21 Endrin ketone

R.T.: 7.131 min
Delta R.T.: -0.050 min
Response: 86882981
Conc: 16.60 ng/ml

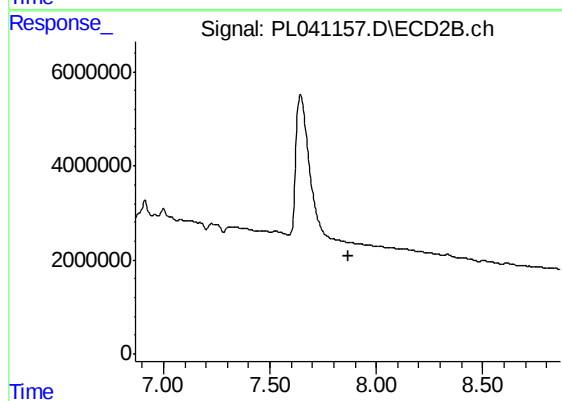

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.867 min
Response: 0
Conc: N.D.

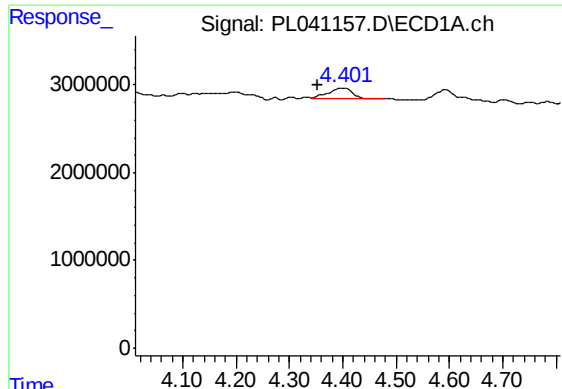

#23 Chlordane-1


R.T.: 4.402 min
Delta R.T.: 0.049 min
Response: 3673932
Conc: 14.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

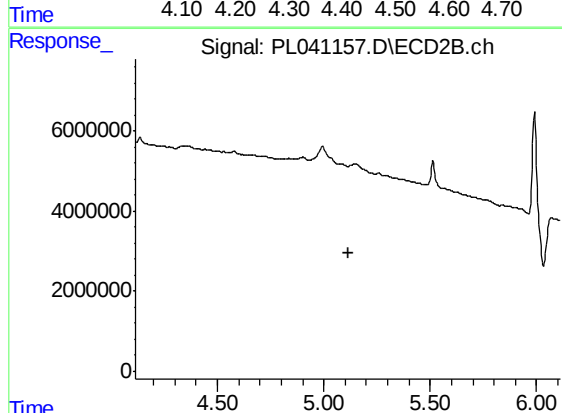


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

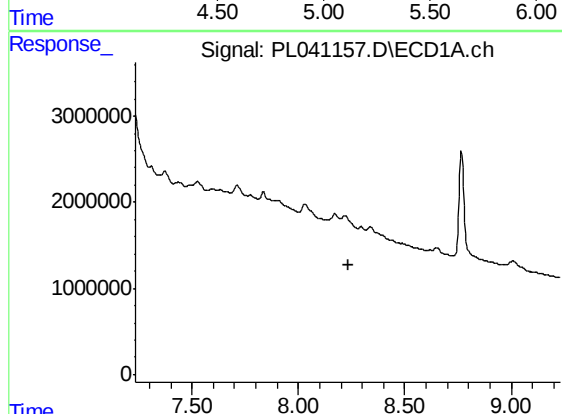

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.234 min
Response: 0
Conc: N.D.

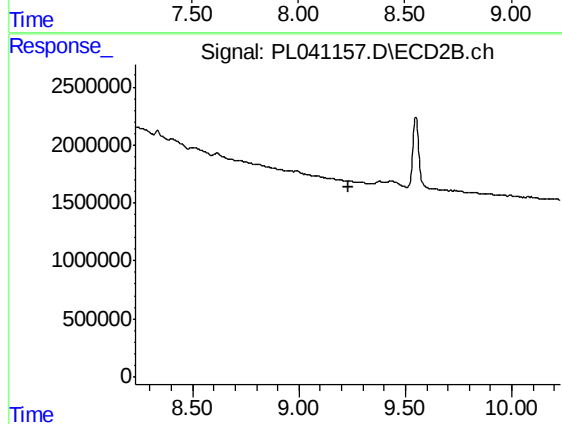

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.