

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
 Data File : PL041191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 21:28
 Operator : AJ\SJ
 Sample : J5577-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1016-S-DH-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:59:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	78946426	40105610	14.404	14.384
28)	SA Decachlor...	8.224	9.236	74186230	33429933	14.268	12.928
Target Compounds							
3)	MA gamma-BHC...	4.167f	0.000	2229271	0	0.305	N.D. #
9)	A Endosulfan I	0.000	6.413f	0	949052	N.D.	0.371 #
12)	B 4,4'-DDE	5.644	6.413f	3578418	949052	0.630	0.359 #
15)	B Endosulfa...	0.000	7.044	0	3545144	N.D.	1.493 #
16)	A 4,4'-DDD	0.000	6.915f	0	9113307	N.D.	4.351 #
23)	Chlordane-1	4.389	0.000	678302	0	2.658	N.D. #
24)	Chlordane-2	4.910	0.000	3315458	0	12.284	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
Data File : PL041191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 21:28
Operator : AJ\SJ
Sample : J5577-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:59:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

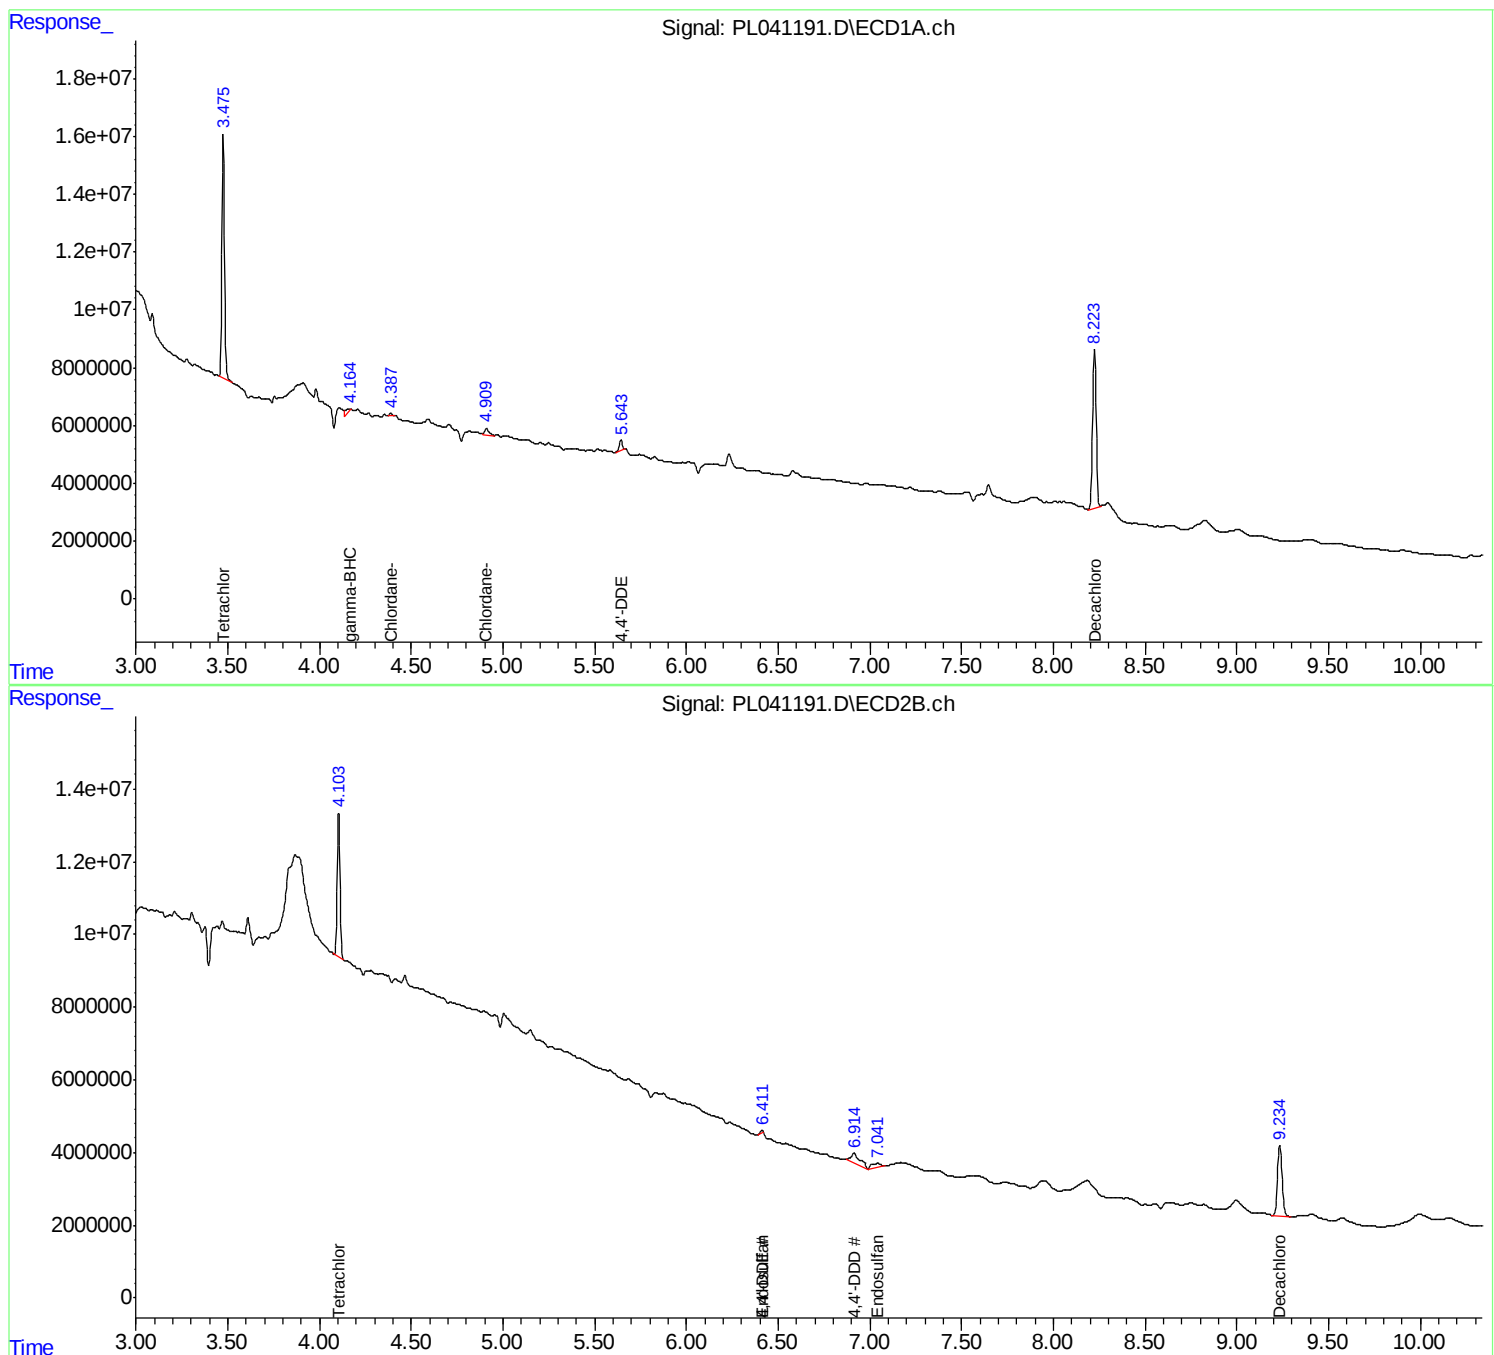


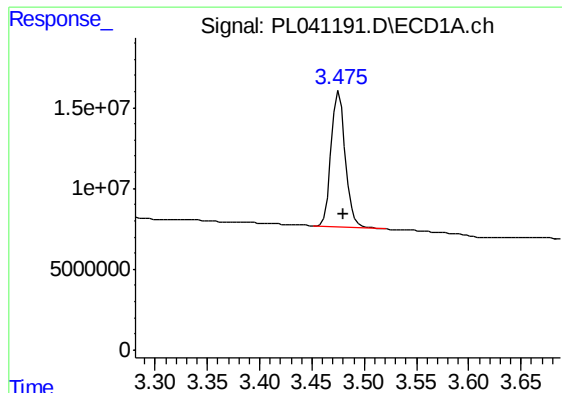

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 78946426
Conc: 14.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-21

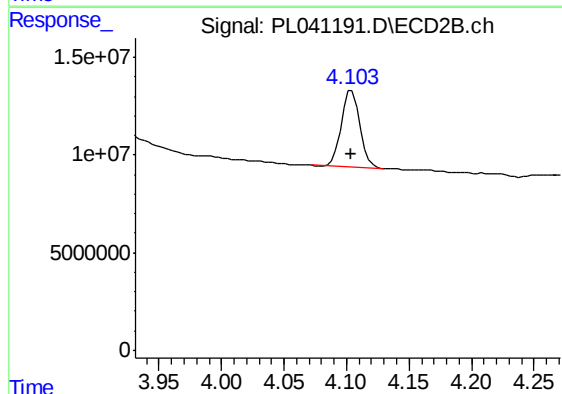


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 40105610
Conc: 14.38 ng/ml

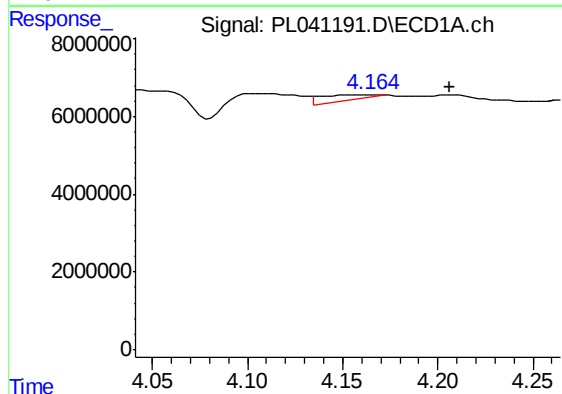


#3 gamma-BHC (Lindane)

R.T.: 4.167 min
Delta R.T.: -0.039 min
Response: 2229271
Conc: 0.31 ng/ml

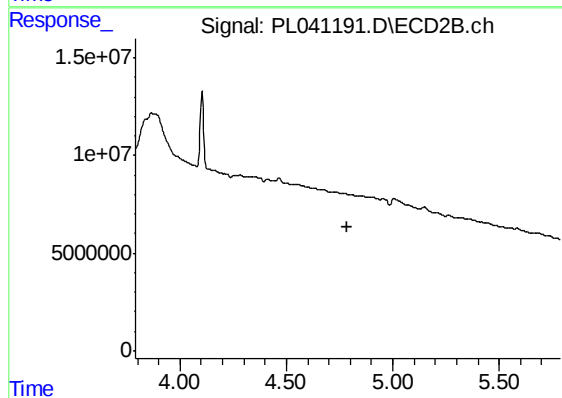

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

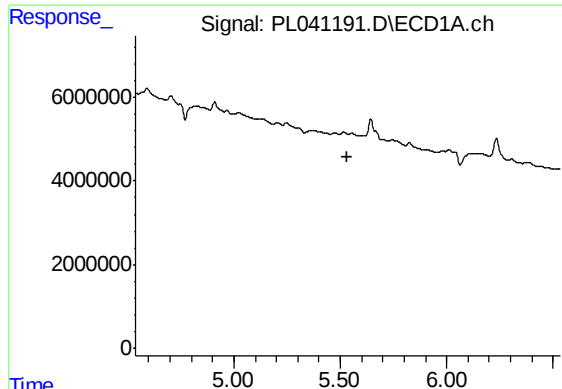

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.534 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-21

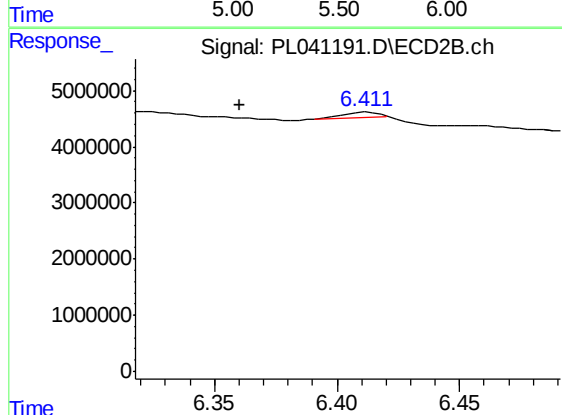


#9 Endosulfan I

R.T.: 6.413 min
Delta R.T.: 0.052 min
Response: 949052
Conc: 0.37 ng/ml

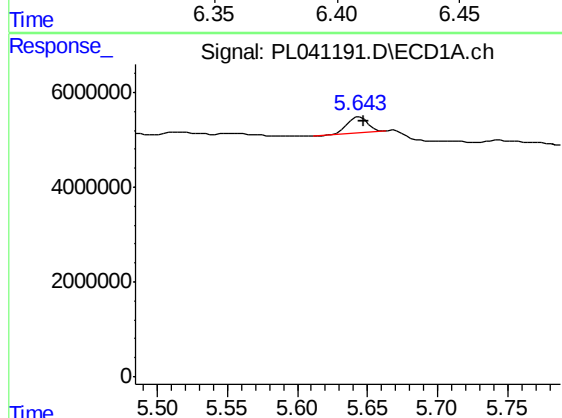


#12 4,4'-DDE

R.T.: 5.644 min
Delta R.T.: -0.003 min
Response: 3578418
Conc: 0.63 ng/ml

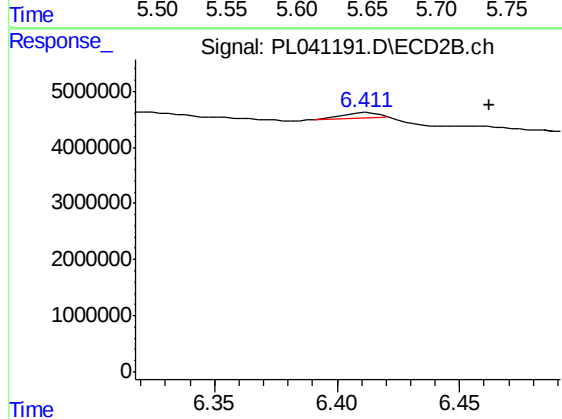

#12 4,4'-DDE


R.T.: 6.413 min
Delta R.T.: -0.049 min
Response: 949052
Conc: 0.36 ng/ml

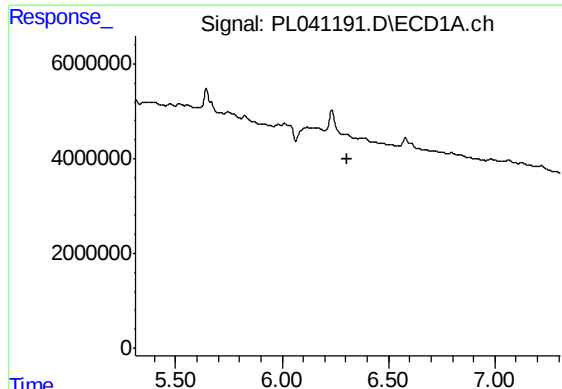

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.309 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-21

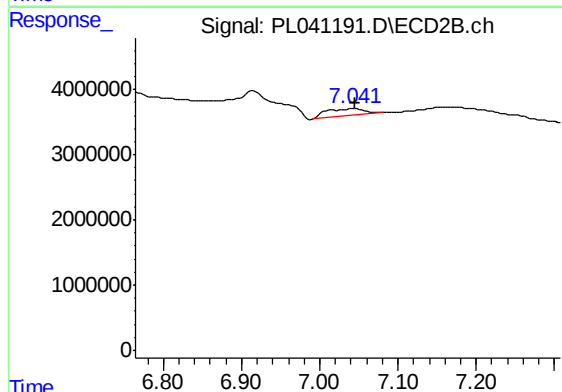


#15 Endosulfan II

R.T.: 7.044 min
Delta R.T.: -0.002 min
Response: 3545144
Conc: 1.49 ng/ml

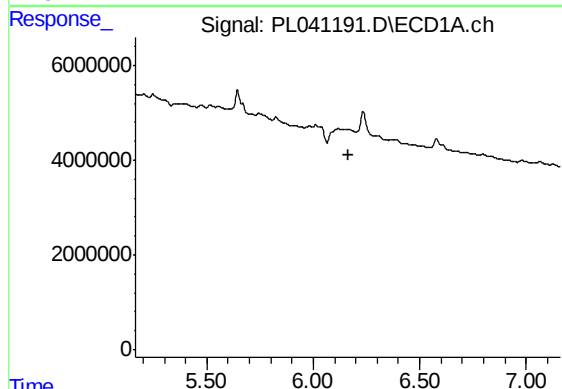


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.163 min
Response: 0
Conc: N.D.

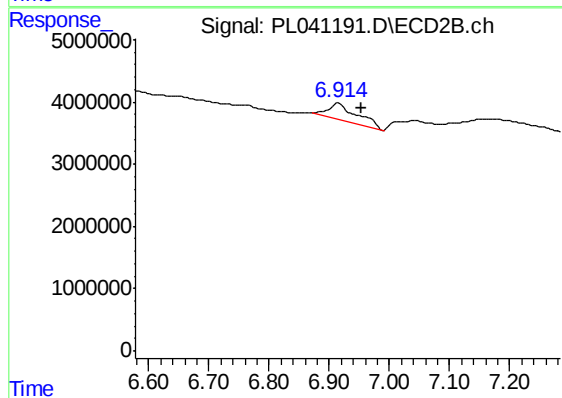

#16 4,4'-DDD


R.T.: 6.915 min
Delta R.T.: -0.039 min
Response: 9113307
Conc: 4.35 ng/ml

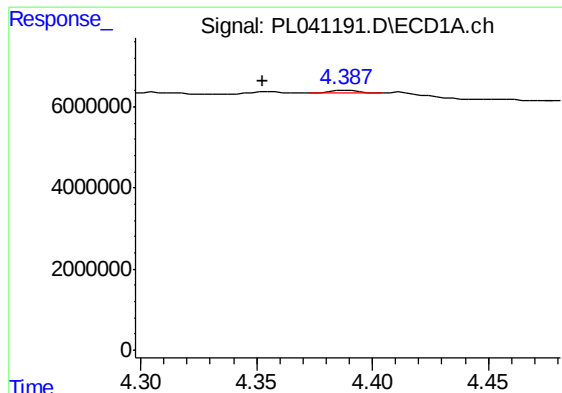

#23 Chlordane-1


R.T.: 4.389 min
Delta R.T.: 0.036 min
Response: 678302
Conc: 2.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-21

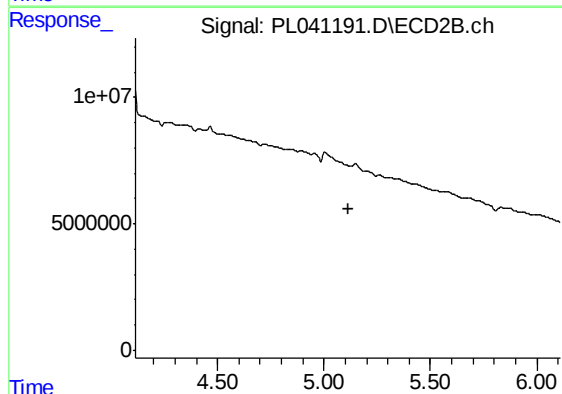


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

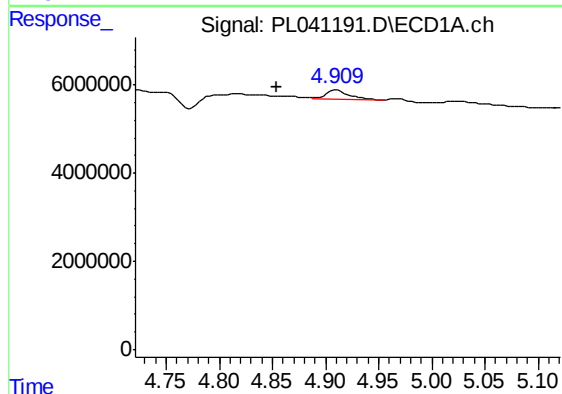


#24 Chlordane-2

R.T.: 4.910 min
Delta R.T.: 0.056 min
Response: 3315458
Conc: 12.28 ng/ml

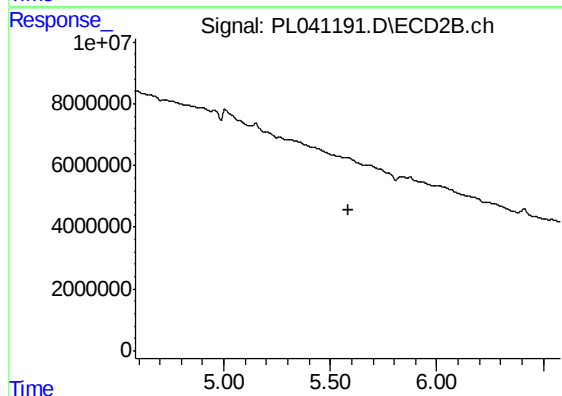

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

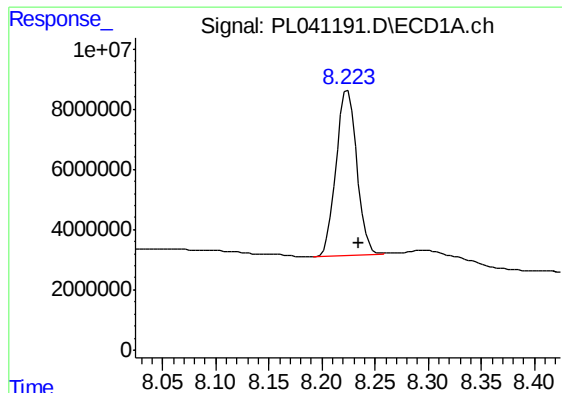

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.010 min
Response: 74186230
Conc: 14.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-21

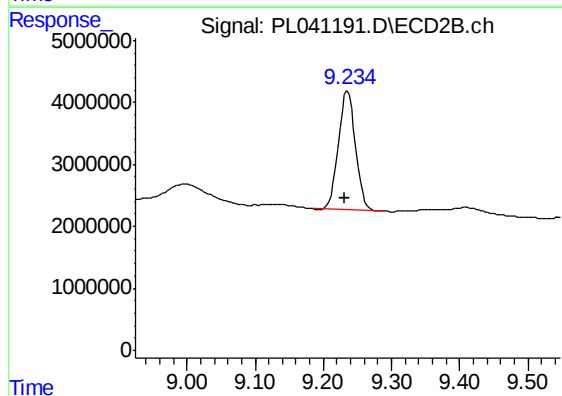

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.004 min
Response: 33429933
Conc: 12.93 ng/ml