

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
 Data File : PL041192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 21:42
 Operator : AJ\SJ
 Sample : J5579-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 7-1-ROLLOFFS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:59:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	64748109	31934218	11.814	11.453
28)	SA Decachlor...	8.223	9.234	71151588	30104966	13.684	11.642
Target Compounds							
4)	MA Heptachlor	4.508	0.000	3021548	0	0.410	N.D. #
6)	B beta-BHC	4.410f	0.000	5959137	0	1.878	N.D. #
10)	B gamma-Chl...	5.435	0.000	1179437	0	0.179	N.D. #
11)	B alpha-Chl...	5.435f	0.000	1179437	0	0.181	N.D. #
12)	B 4,4'-DDE	5.638	6.463	2862016	2457740	0.504	0.929 #
13)	MA Dieldrin	5.763	0.000	2855259	0	0.452	N.D. #
16)	A 4,4'-DDD	6.233f	6.915f	5103402	2512301	1.130	1.199
17)	MA 4,4'-DDT	6.388	0.000	2358026	0	0.518	N.D. #
19)	B Endosulfa...	6.676	0.000	2915772	0	0.573	N.D. #
23)	Chlordane-1	4.348	0.000	3091400	0	12.113	N.D. #
24)	Chlordane-2	4.827	5.553	5304728	2794682	19.655	22.598
25)	Chlordane-3	5.435	0.000	1179437	0	1.541	N.D. #
26)	Chlordane-4	5.435	0.000	1179437	0	1.759	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
Data File : PL041192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 21:42
Operator : AJ\SJ
Sample : J5579-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:59:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

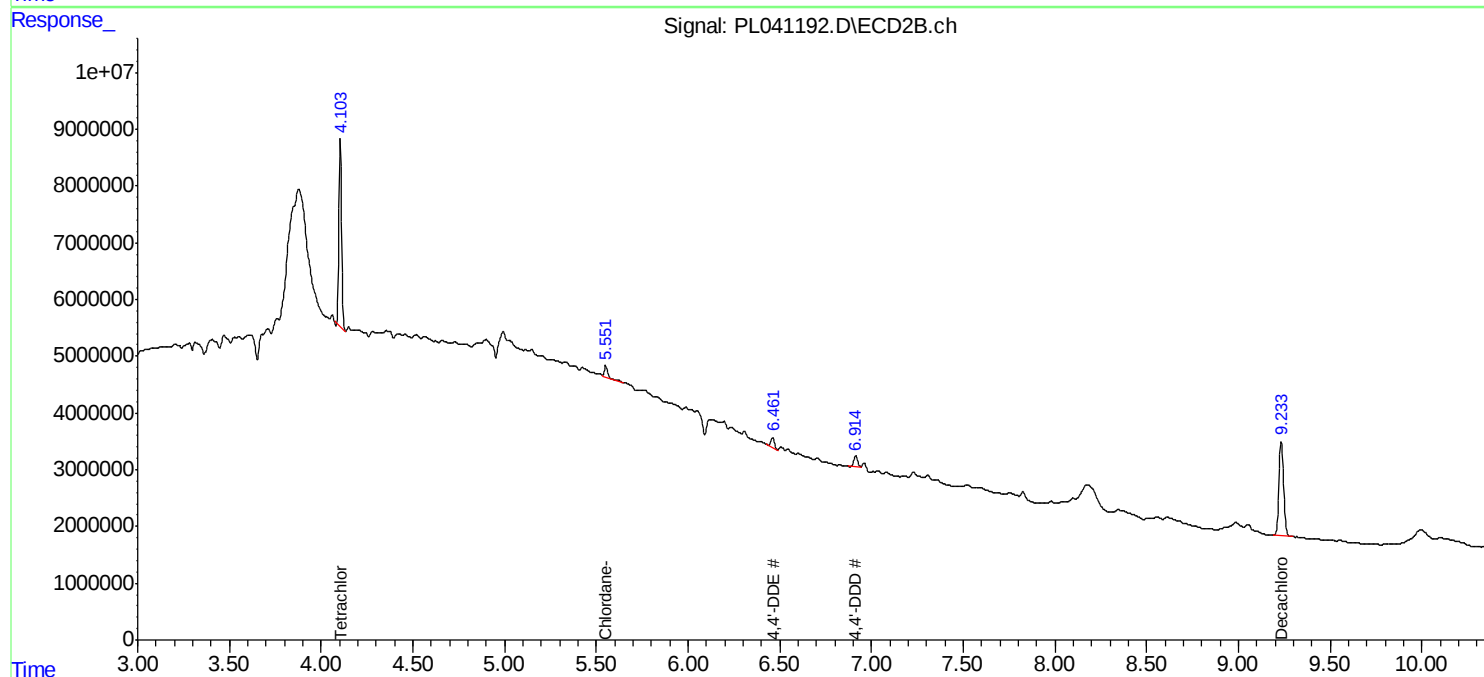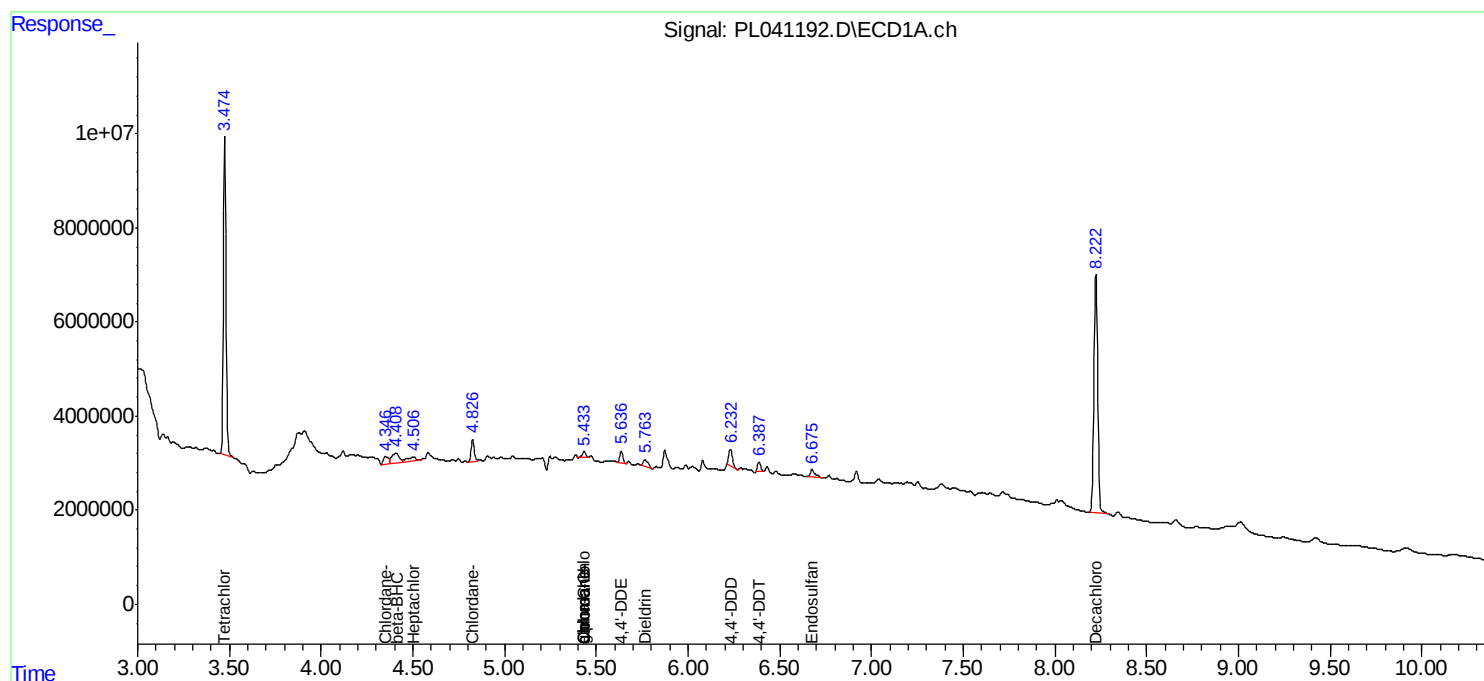


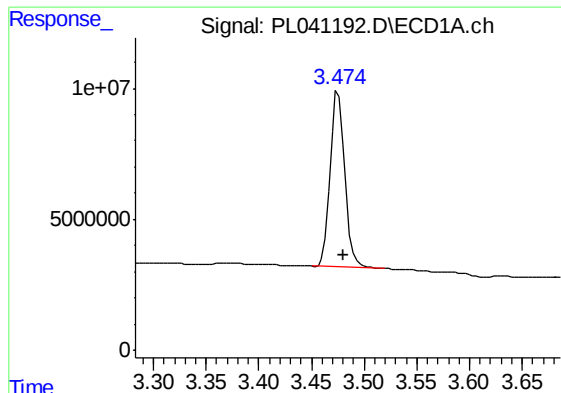

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 64748109
Conc: 11.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

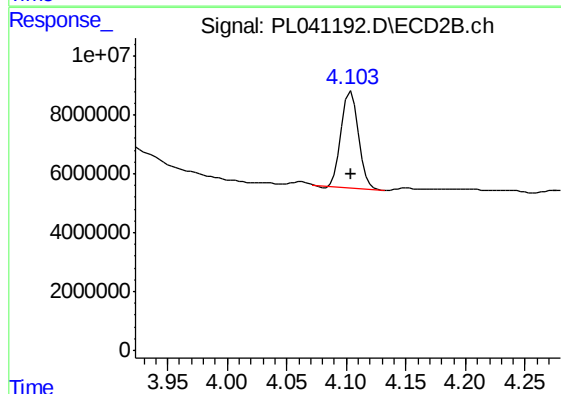


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 31934218
Conc: 11.45 ng/ml

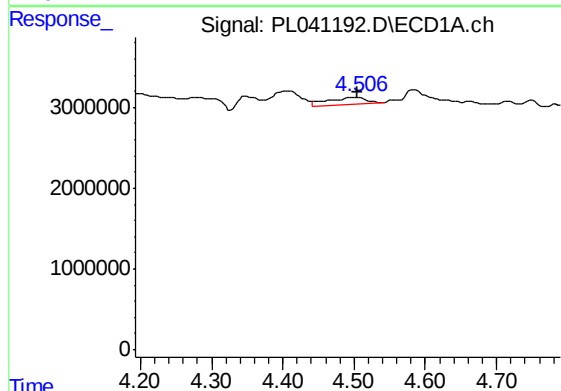


#4 Heptachlor

R.T.: 4.508 min
Delta R.T.: 0.003 min
Response: 3021548
Conc: 0.41 ng/ml

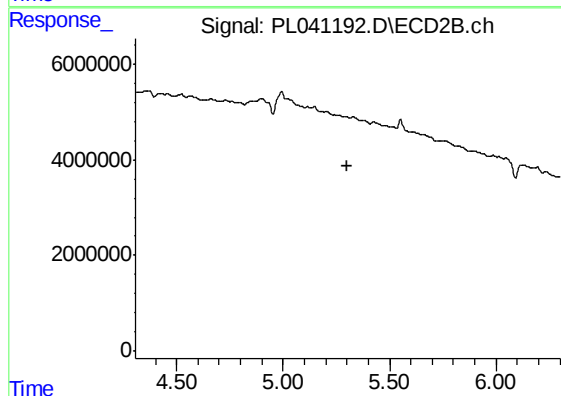

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.304 min
Response: 0
Conc: N.D.

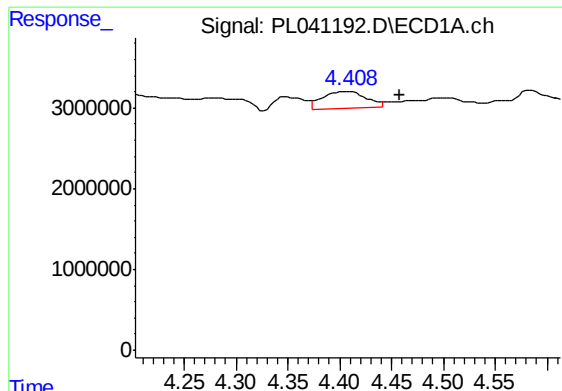

#6 beta-BHC


R.T.: 4.410 min
Delta R.T.: -0.048 min
Response: 5959137
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

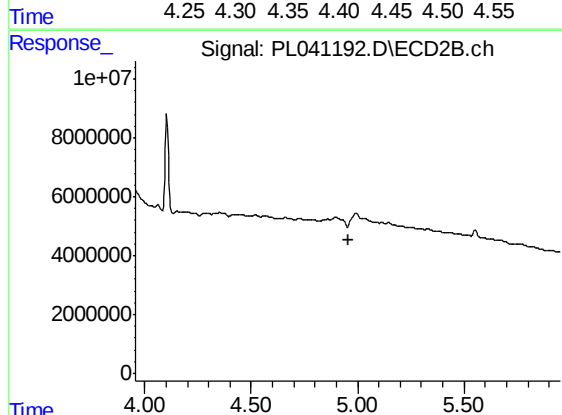


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.955 min
Response: 0
Conc: N.D.

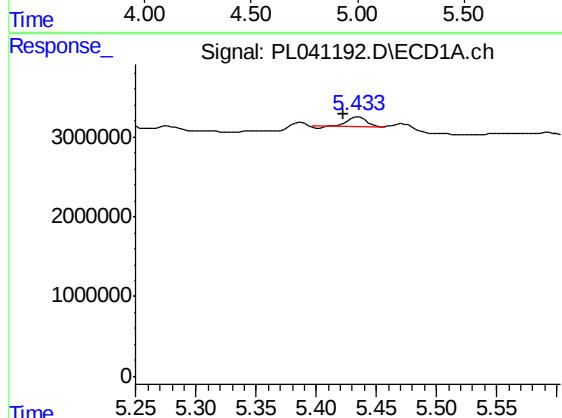


#10 gamma-Chlordane

R.T.: 5.435 min
Delta R.T.: 0.012 min
Response: 1179437
Conc: 0.18 ng/ml

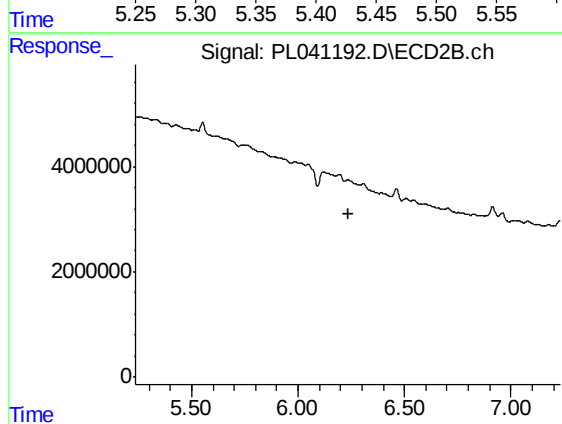

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

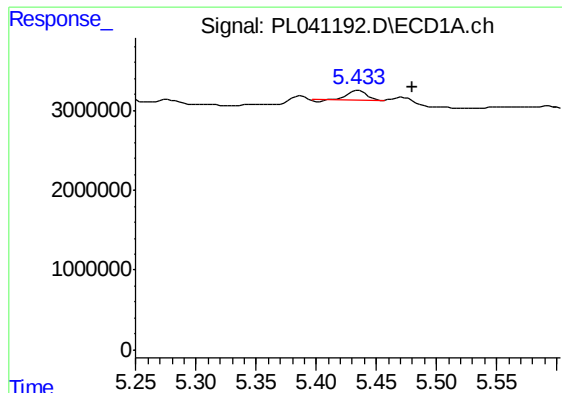

#11 alpha-Chlordane


R.T.: 5.435 min
Delta R.T.: -0.046 min
Response: 1179437
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

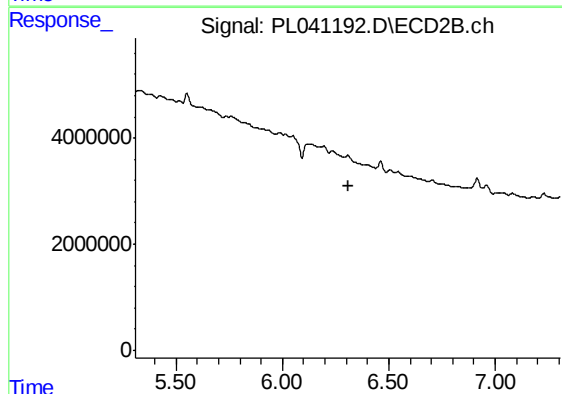


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

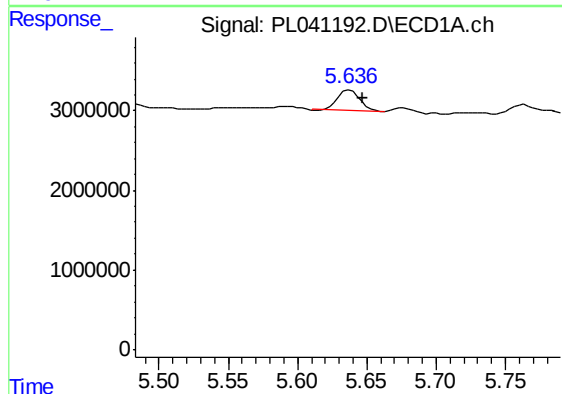


#12 4,4'-DDE

R.T.: 5.638 min
Delta R.T.: -0.009 min
Response: 2862016
Conc: 0.50 ng/ml

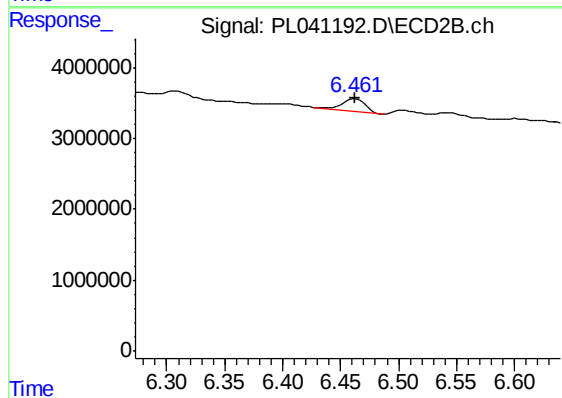

#12 4,4'-DDE


R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 2457740
Conc: 0.93 ng/ml

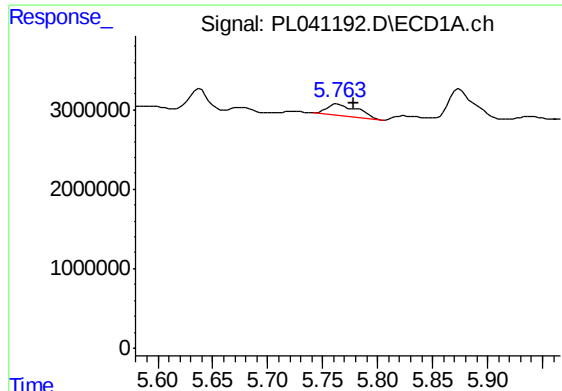

#13 Dieldrin


R.T.: 5.763 min
Delta R.T.: -0.015 min
Response: 2855259
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

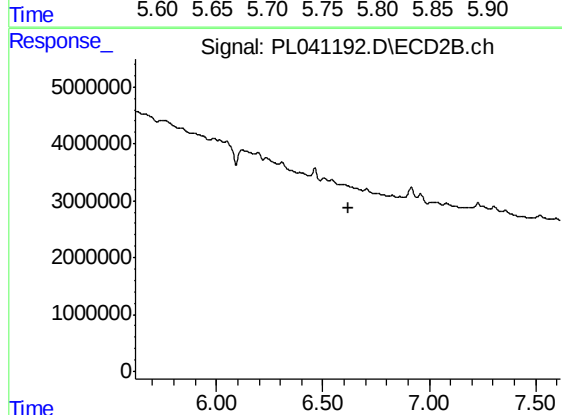


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.618 min
Response: 0
Conc: N.D.

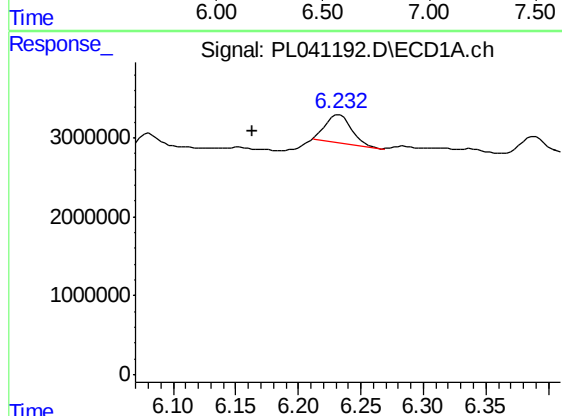


#16 4,4'-DDD

R.T.: 6.233 min
Delta R.T.: 0.070 min
Response: 5103402
Conc: 1.13 ng/ml

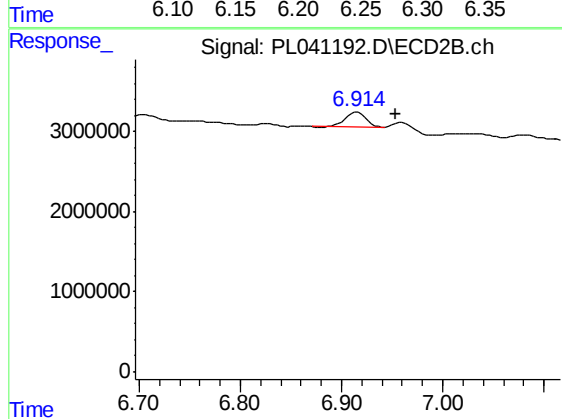

#16 4,4'-DDD


R.T.: 6.915 min
Delta R.T.: -0.038 min
Response: 2512301
Conc: 1.20 ng/ml

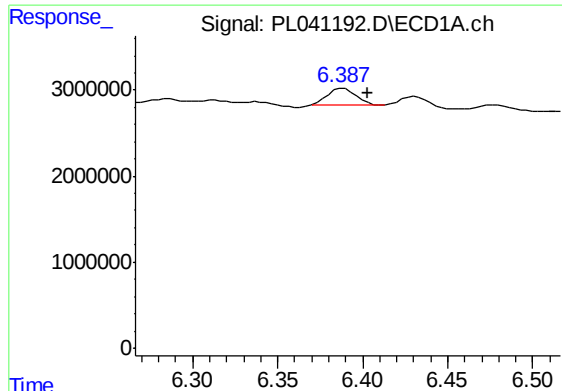

#17 4,4'-DDT


R.T.: 6.388 min
Delta R.T.: -0.014 min
Response: 2358026
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

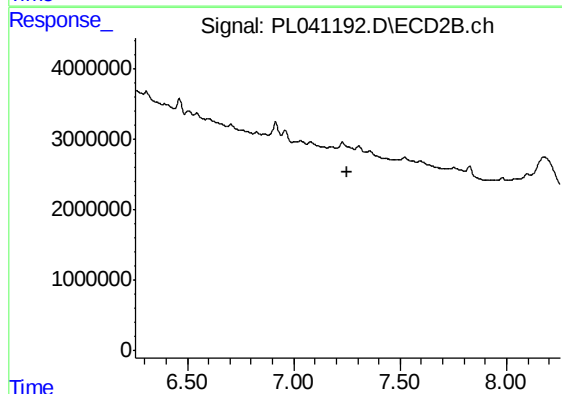


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

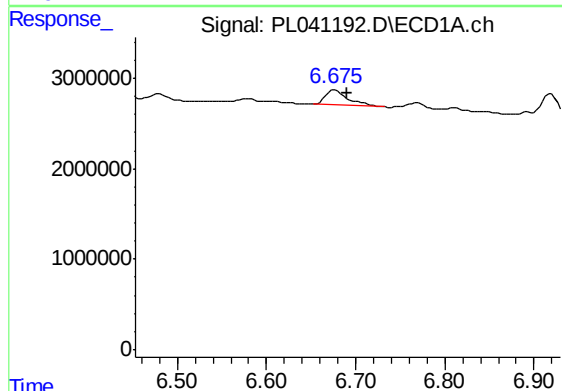


#19 Endosulfan Sulfate

R.T.: 6.676 min
Delta R.T.: -0.014 min
Response: 2915772
Conc: 0.57 ng/ml

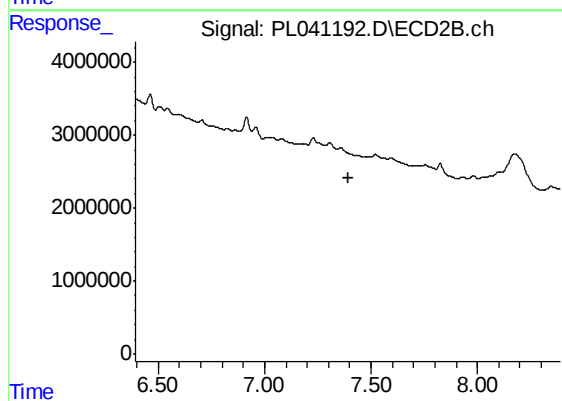

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

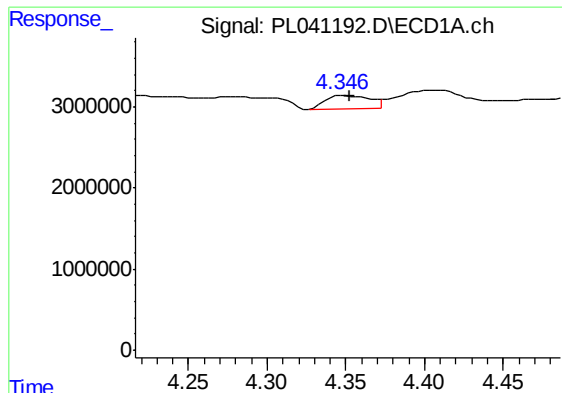

#23 Chlordane-1


R.T.: 4.348 min
Delta R.T.: -0.005 min
Response: 3091400
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

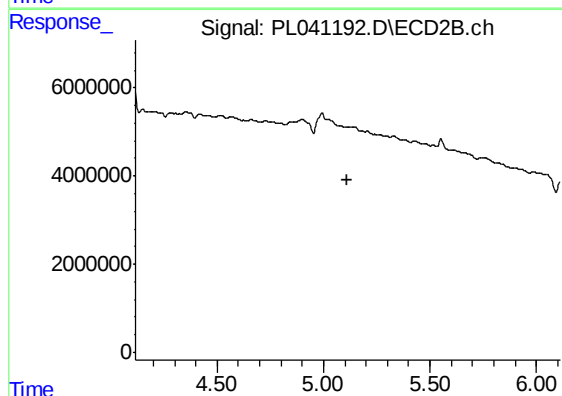


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

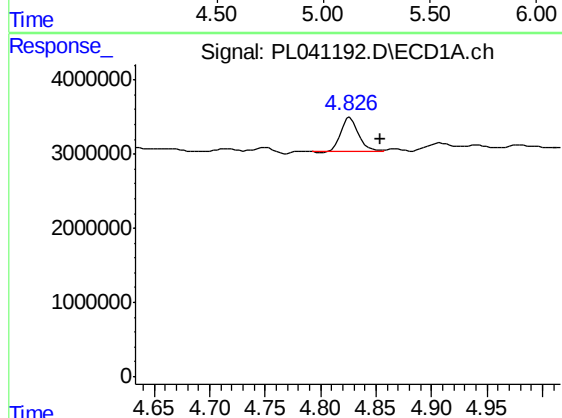


#24 Chlordane-2

R.T.: 4.827 min
Delta R.T.: -0.027 min
Response: 5304728
Conc: 19.65 ng/ml

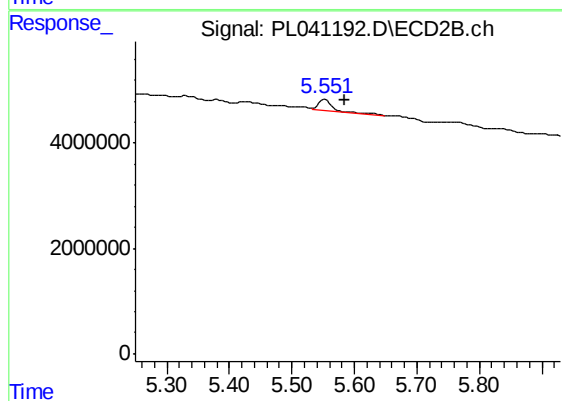

#24 Chlordane-2


R.T.: 5.553 min
Delta R.T.: -0.032 min
Response: 2794682
Conc: 22.60 ng/ml

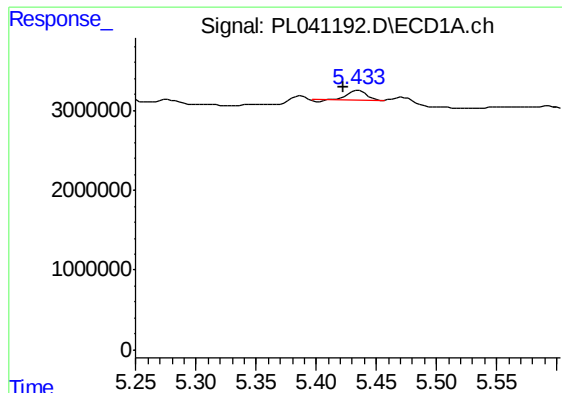

#25 Chlordane-3


R.T.: 5.435 min
Delta R.T.: 0.012 min
Response: 1179437
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

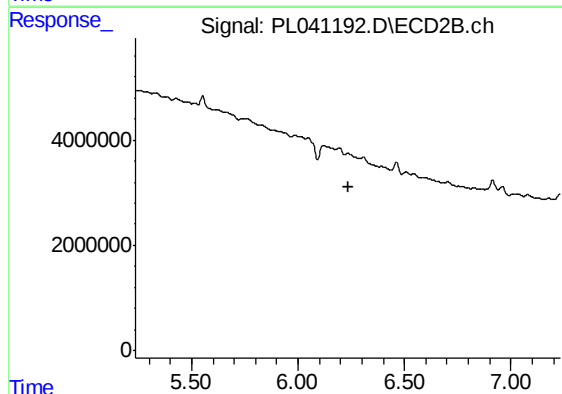


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.235 min
Response: 0
Conc: N.D.

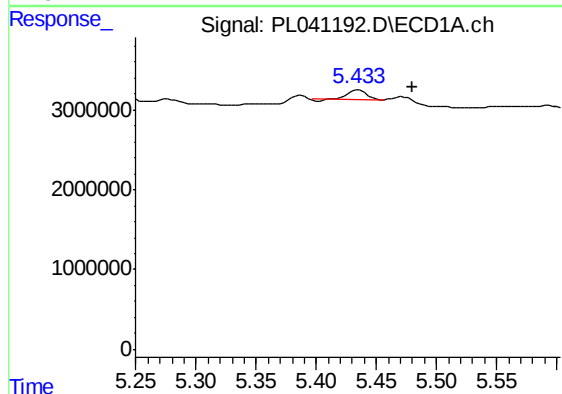


#26 Chlordane-4

R.T.: 5.435 min
Delta R.T.: -0.045 min
Response: 1179437
Conc: 1.76 ng/ml

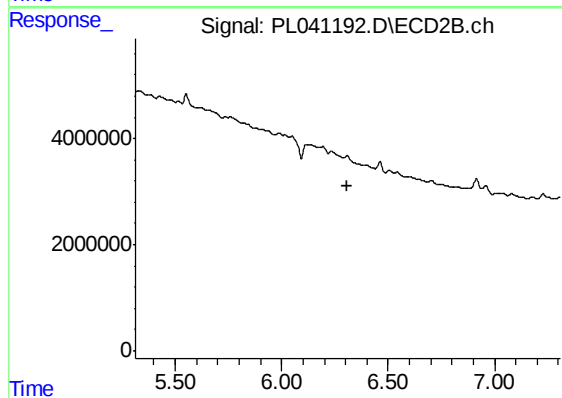

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.310 min
Response: 0
Conc: N.D.

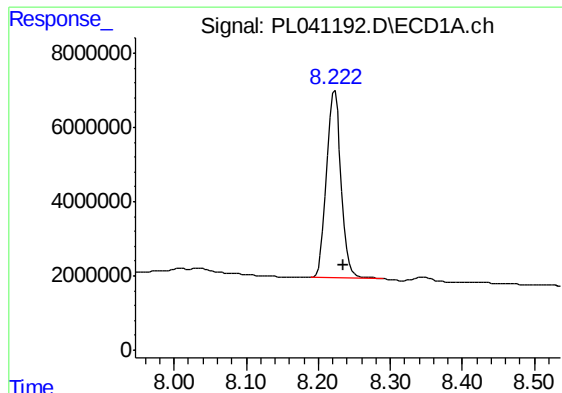

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: -0.011 min
Response: 71151588
Conc: 13.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
7-1-ROLLOFFS

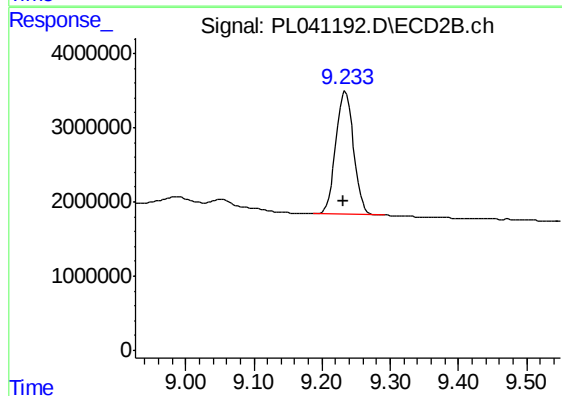

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.003 min
Response: 30104966
Conc: 11.64 ng/ml