

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
 Data File : PL041190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 21:14
 Operator : AJ\SJ
 Sample : J5577-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1016-S-DH-22

Manual Integrations
 APPROVED

sohil
 10/22/2018 3:49:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:58:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	53752151	28175980	9.807	10.105
28)	SA Decachlor...	8.224	9.235	70713350	33462778	13.600	12.941
Target Compounds							
12)	B 4,4'-DDE	5.637	6.461	5781666	3323720	1.017m	1.256m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101918\
Data File : PL041190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 21:14
Operator : AJ\SJ
Sample : J5577-02
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-22


Manual Integrations
APPROVED

sohil
10/22/2018 3:49:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:58:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

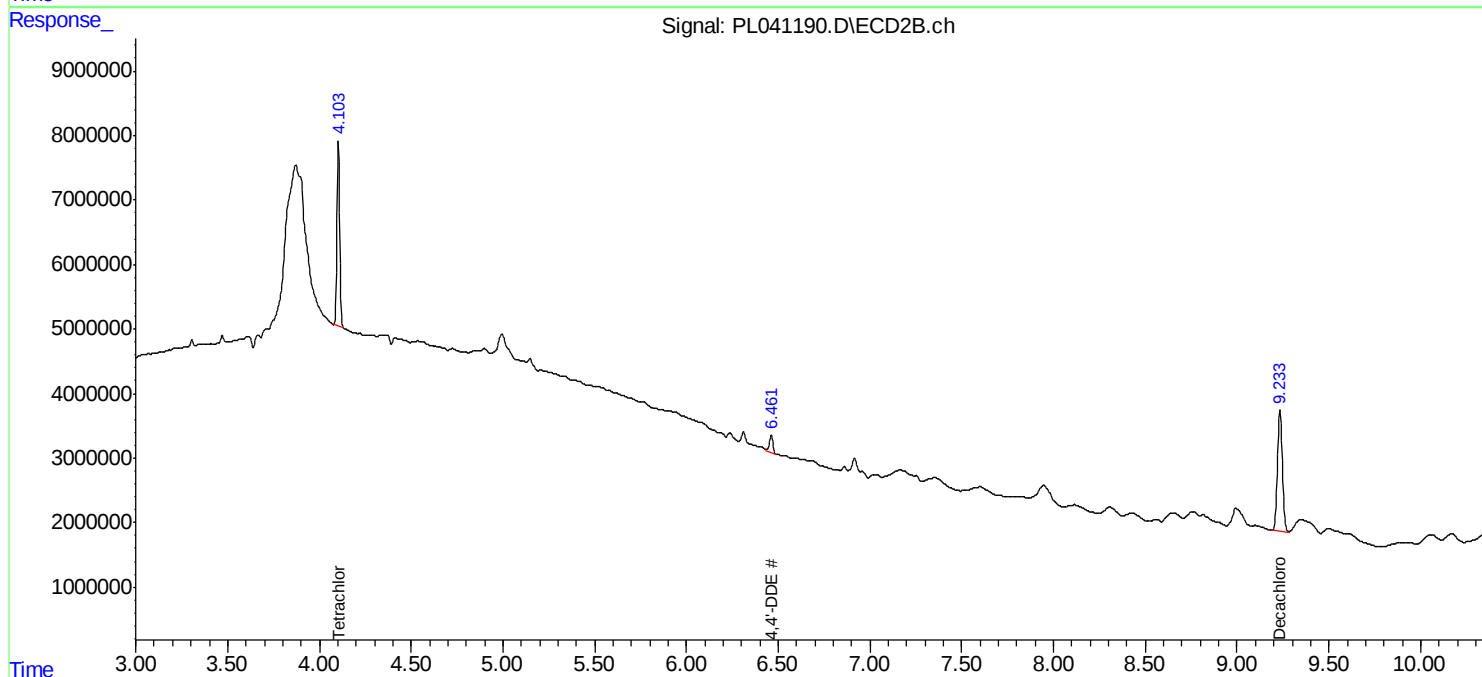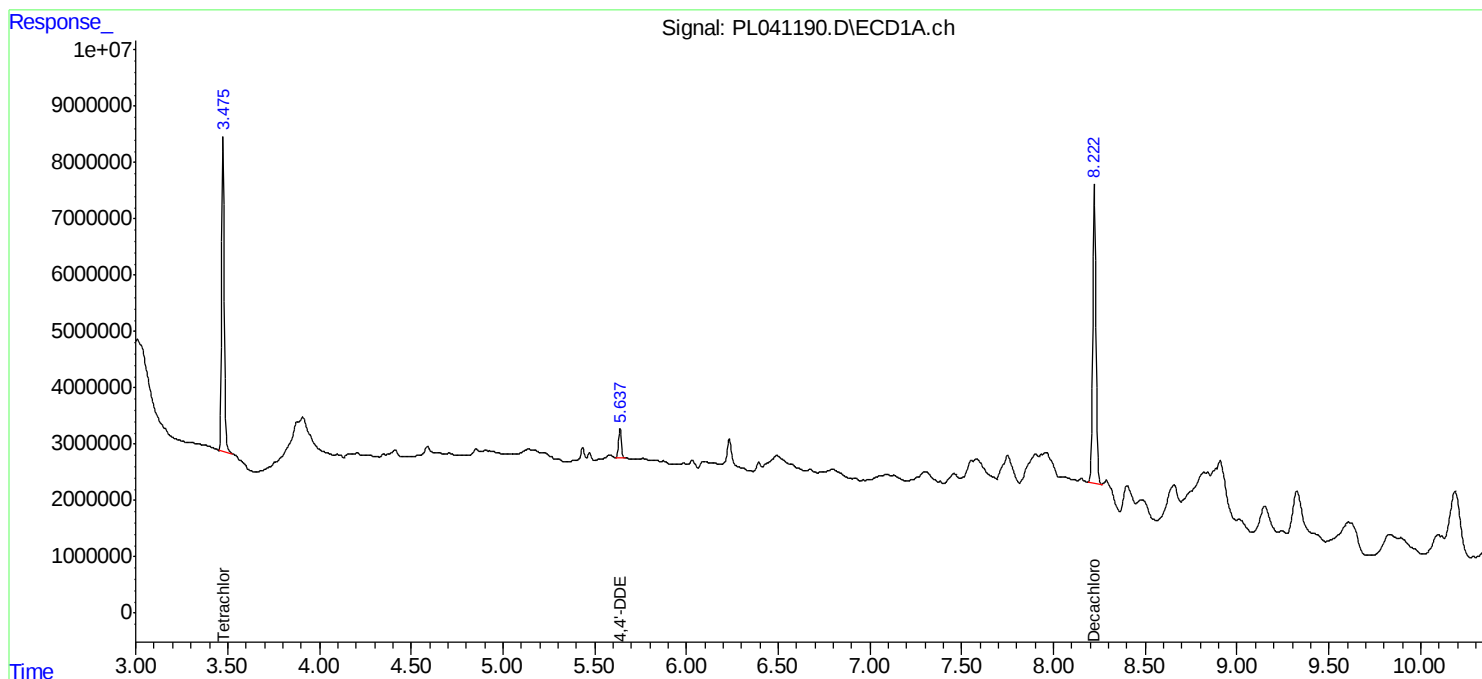

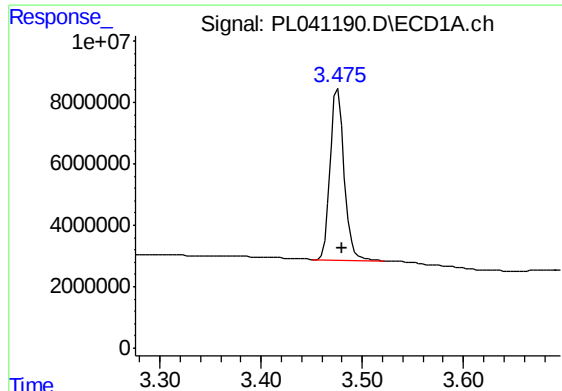


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 53752151
Conc: 9.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-22


Manual Integrations
APPROVED

sohil
10/22/2018 3:49:59 PM

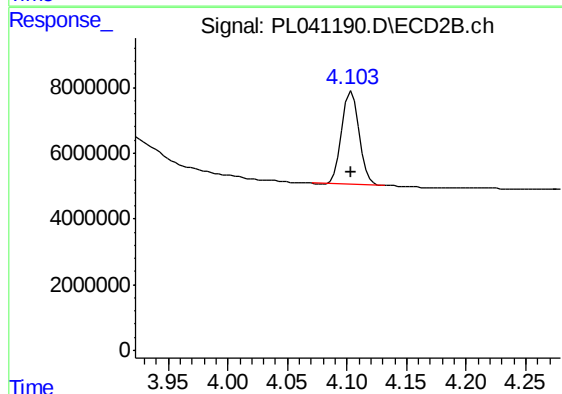


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 28175980
Conc: 10.11 ng/ml

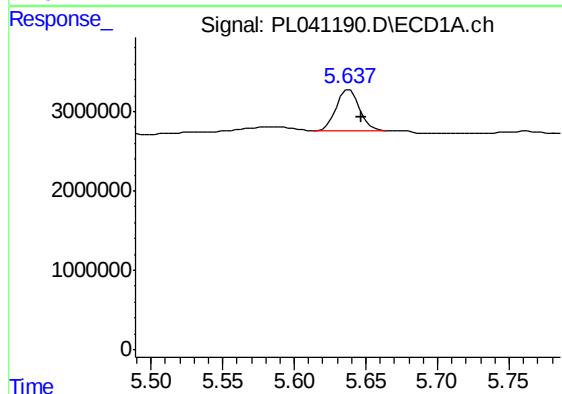


#12 4,4'-DDE

R.T.: 5.637 min
Delta R.T.: -0.010 min
Response: 5781666
Conc: 1.02 ng/ml m

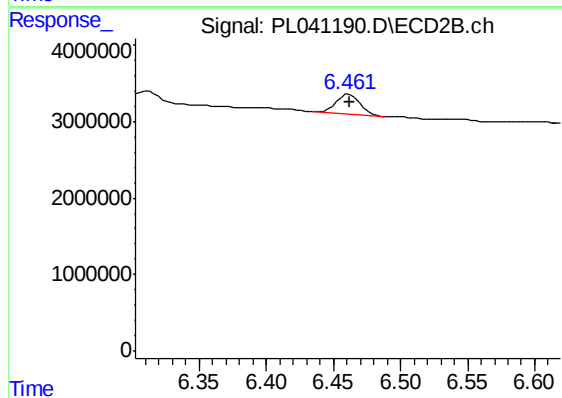

#12 4,4'-DDE

R.T.: 6.461 min
Delta R.T.: -0.001 min
Response: 3323720
Conc: 1.26 ng/ml m

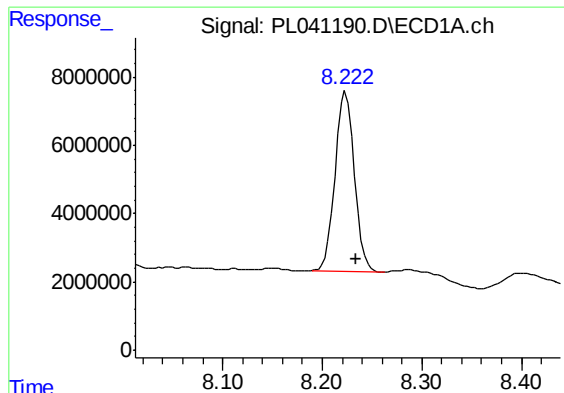


#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.011 min
Response: 70713350
Conc: 13.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1016-S-DH-22

Manual Integrations
APPROVED

sohil
10/22/2018 3:49:59 PM

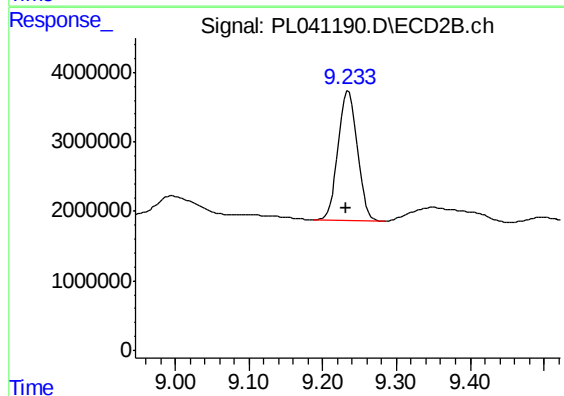

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.004 min
Response: 33462778
Conc: 12.94 ng/ml