

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 13:18
 Operator : SG\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 13:30:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	62652434	12935900	5.147	5.626
28)	SA Decachlor...	8.333	9.127	54858243	16807602	6.078	6.455
Target Compounds							
23)	Chlordane-1	4.428	5.043	17105149	4498760	47.805	54.637
24)	Chlordane-2	4.934	5.511	22298230	5352320	58.997	55.744
25)	Chlordane-3	5.509	6.158	53116996	18734244	45.195	51.628
26)	Chlordane-4	5.567	6.233	43540775	23736689	45.635	53.644
27)	Chlordane-5	6.409	7.038	18799412	3870755	51.799	50.793


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 13:18
Operator : SG\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 13:30:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

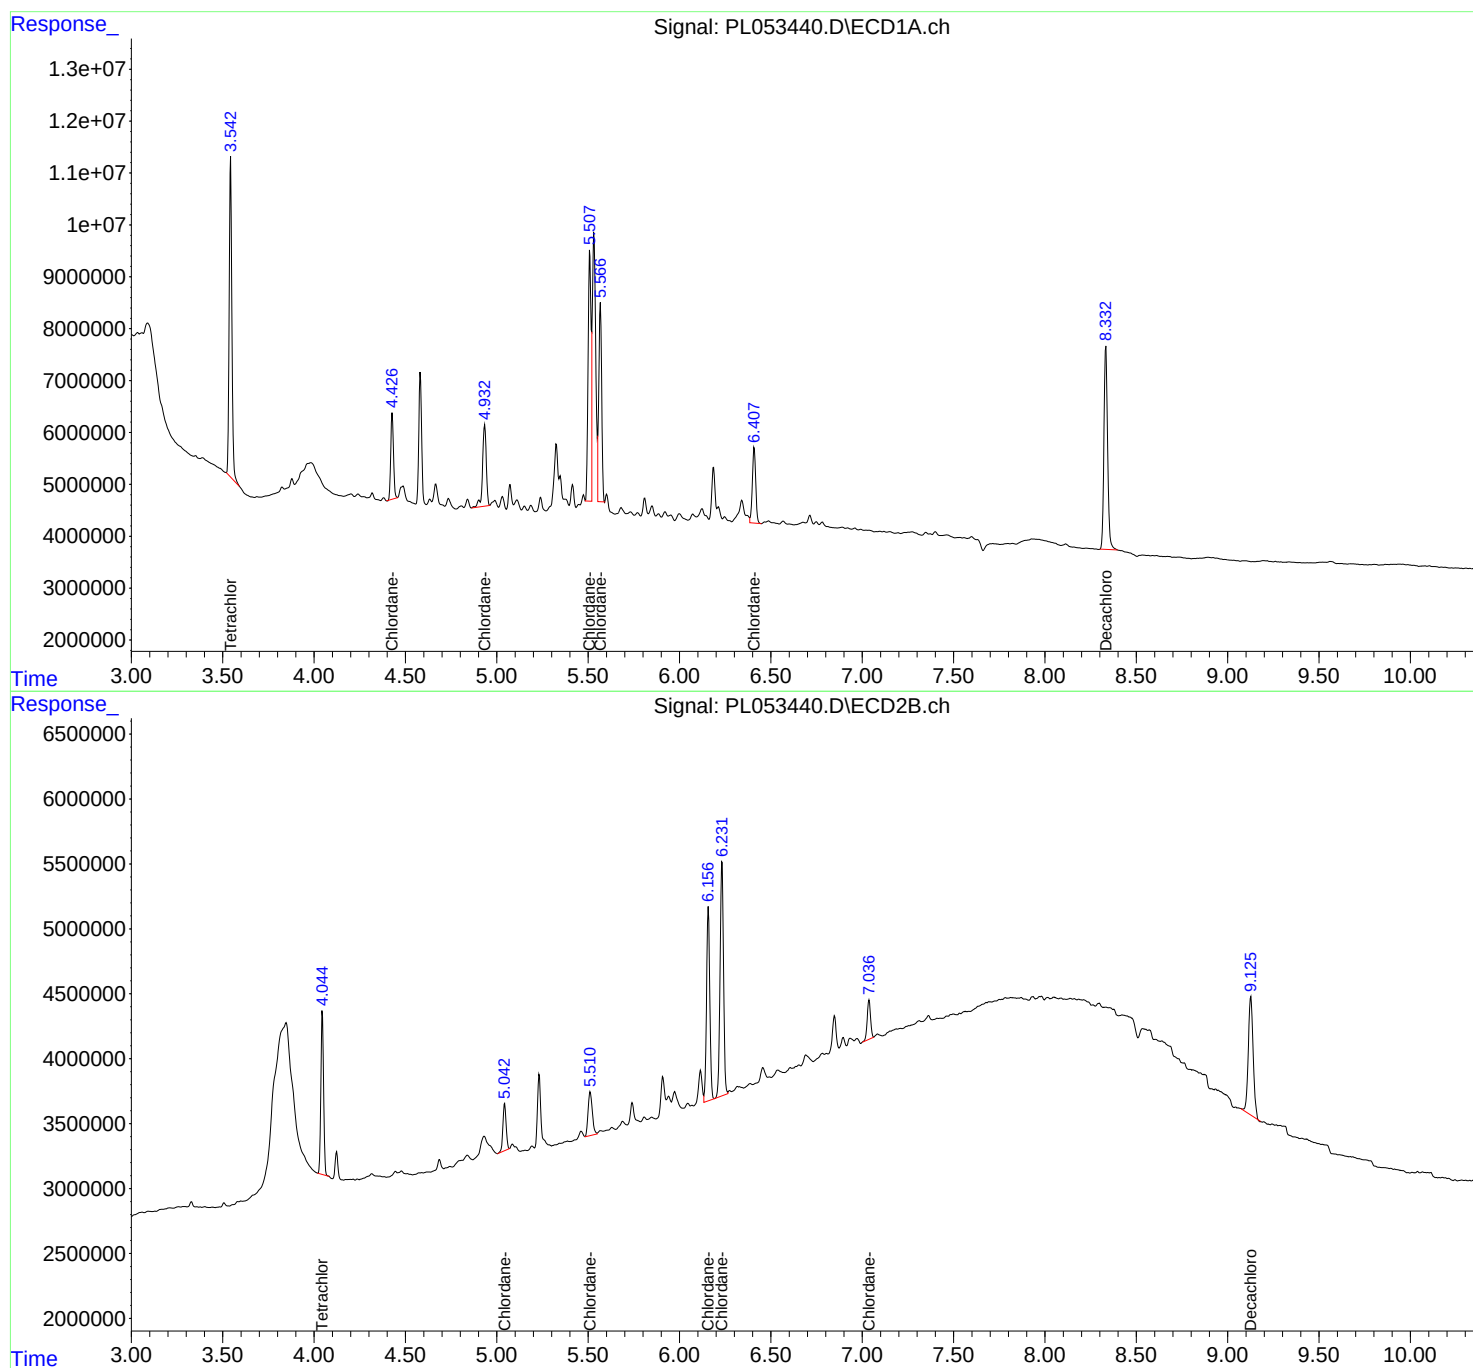


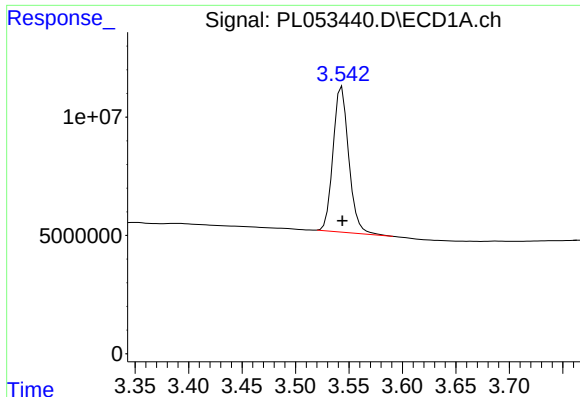

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 62652434
Conc: 5.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

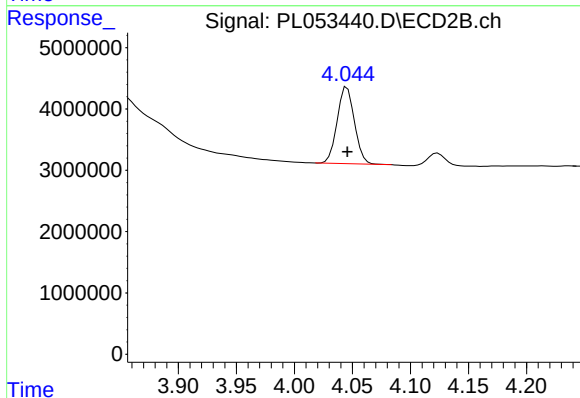


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 12935900
Conc: 5.63 ng/ml

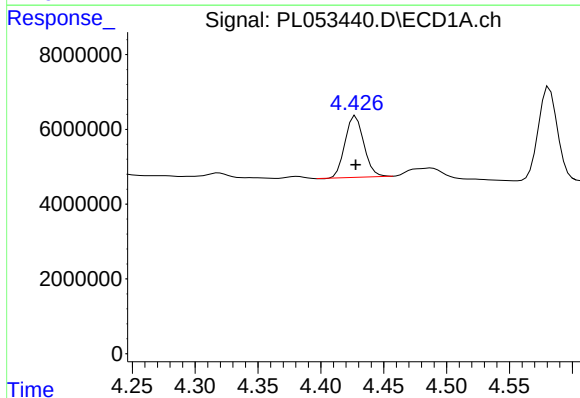


#23 Chlordane-1

R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 17105149
Conc: 47.80 ng/ml

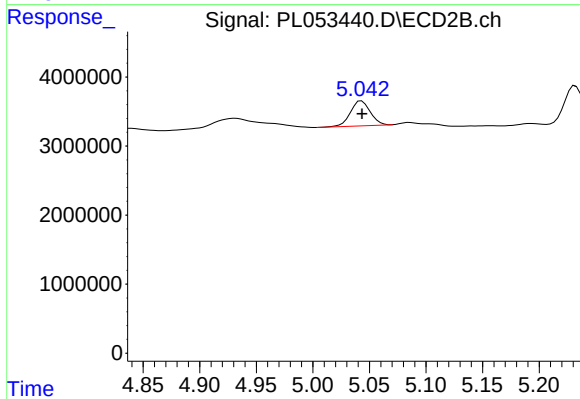

#23 Chlordane-1


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 4498760
Conc: 54.64 ng/ml

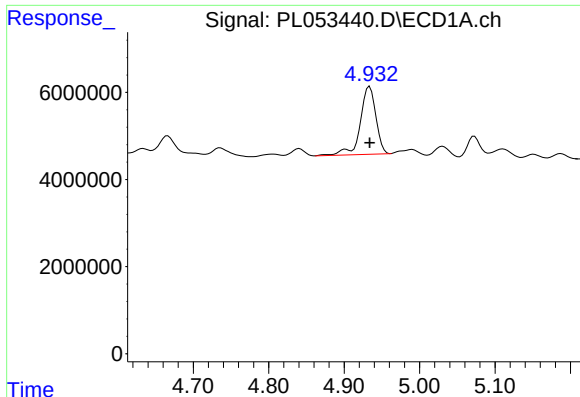

#24 Chlordane-2


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 22298230
Conc: 59.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

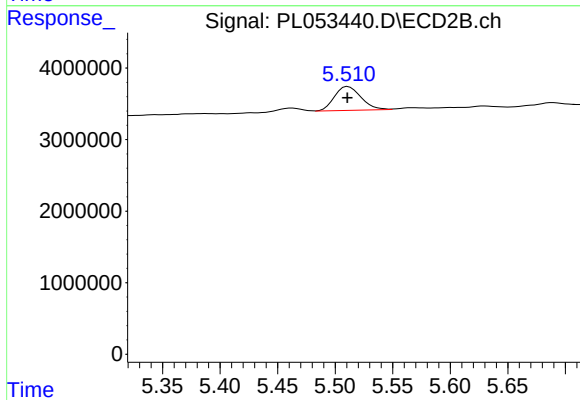


#24 Chlordane-2

R.T.: 5.511 min
Delta R.T.: 0.000 min
Response: 5352320
Conc: 55.74 ng/ml

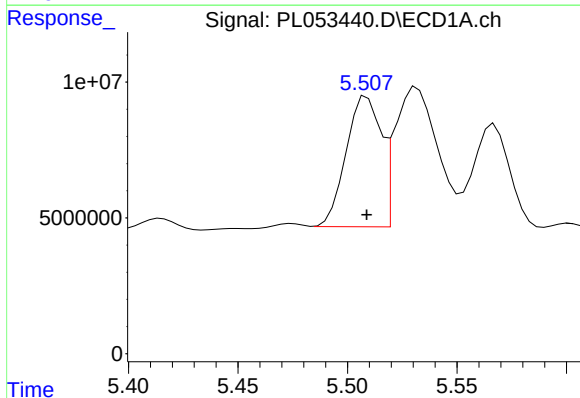


#25 Chlordane-3

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 53116996
Conc: 45.20 ng/ml

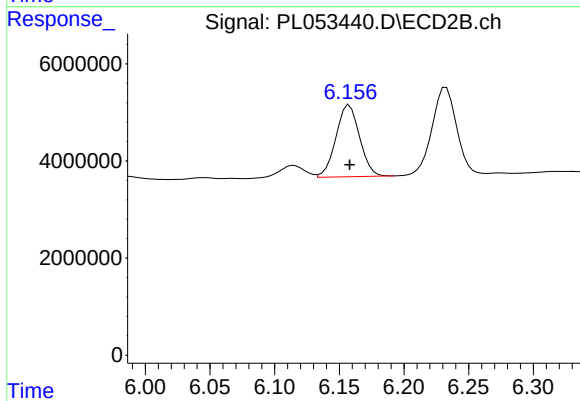

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 18734244
Conc: 51.63 ng/ml

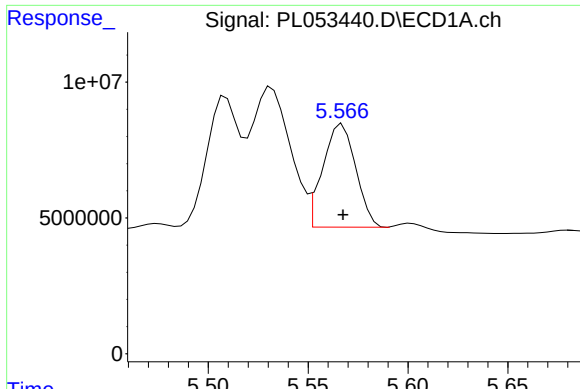

#26 Chlordane-4


R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 43540775
Conc: 45.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

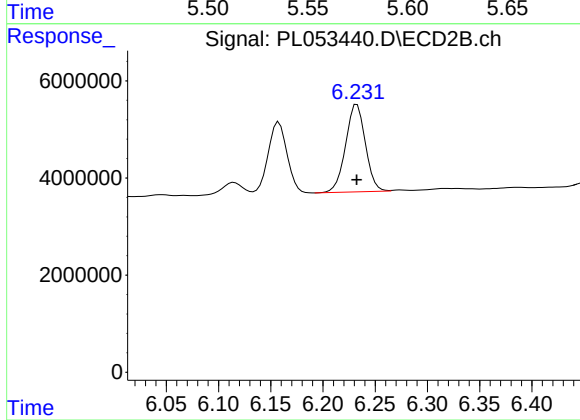


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 23736689
Conc: 53.64 ng/ml

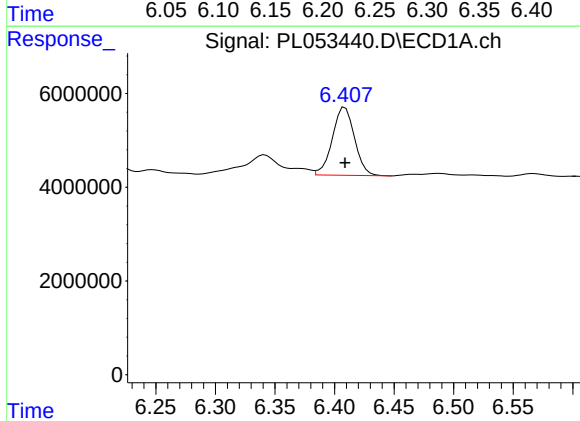


#27 Chlordane-5

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 18799412
Conc: 51.80 ng/ml

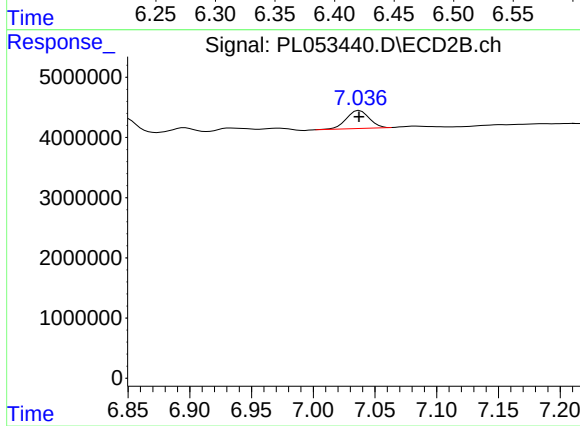

#27 Chlordane-5


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 3870755
Conc: 50.79 ng/ml

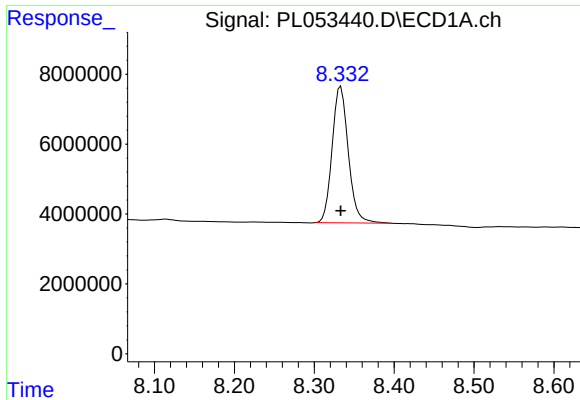

#28 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: 0.000 min
Response: 54858243
Conc: 6.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

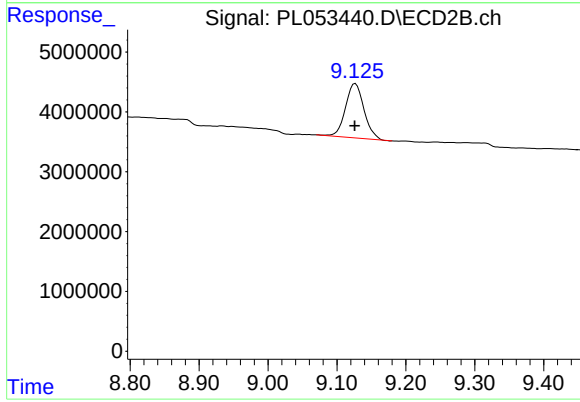

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.001 min
Response: 16807602
Conc: 6.45 ng/ml