

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 17:59
 Operator : SG\AJ
 Sample : K5152-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:01:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.046	171.9E6	40659439	15.859	16.248
28)	SA Decachlor...	8.332	9.125	149.2E6	41971631	15.207	14.905
Target Compounds							
5)	MB Aldrin	0.000	5.544	0	2425308	N.D.	0.813 #
7)	B delta-BHC	0.000	5.083f	0	1961667	N.D.	0.649 #
9)	A Endosulfan I	0.000	6.281	0	1742462	N.D.	0.643 #
10)	B gamma-Chl...	0.000	6.175f	0	434213	N.D.	0.149 #
12)	B 4,4'-DDE	0.000	6.391	0	399514	N.D.	0.142 #
15)	B Endosulfa...	0.000	6.971	0	7101041	N.D.	2.780 #
25)	Chlordane-3	0.000	6.175f	0	434213	N.D.	1.189 #
27)	Chlordane-5	0.000	7.023	0	3677791	N.D.	48.108 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 17:59
Operator : SG\AJ
Sample : K5152-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:01:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

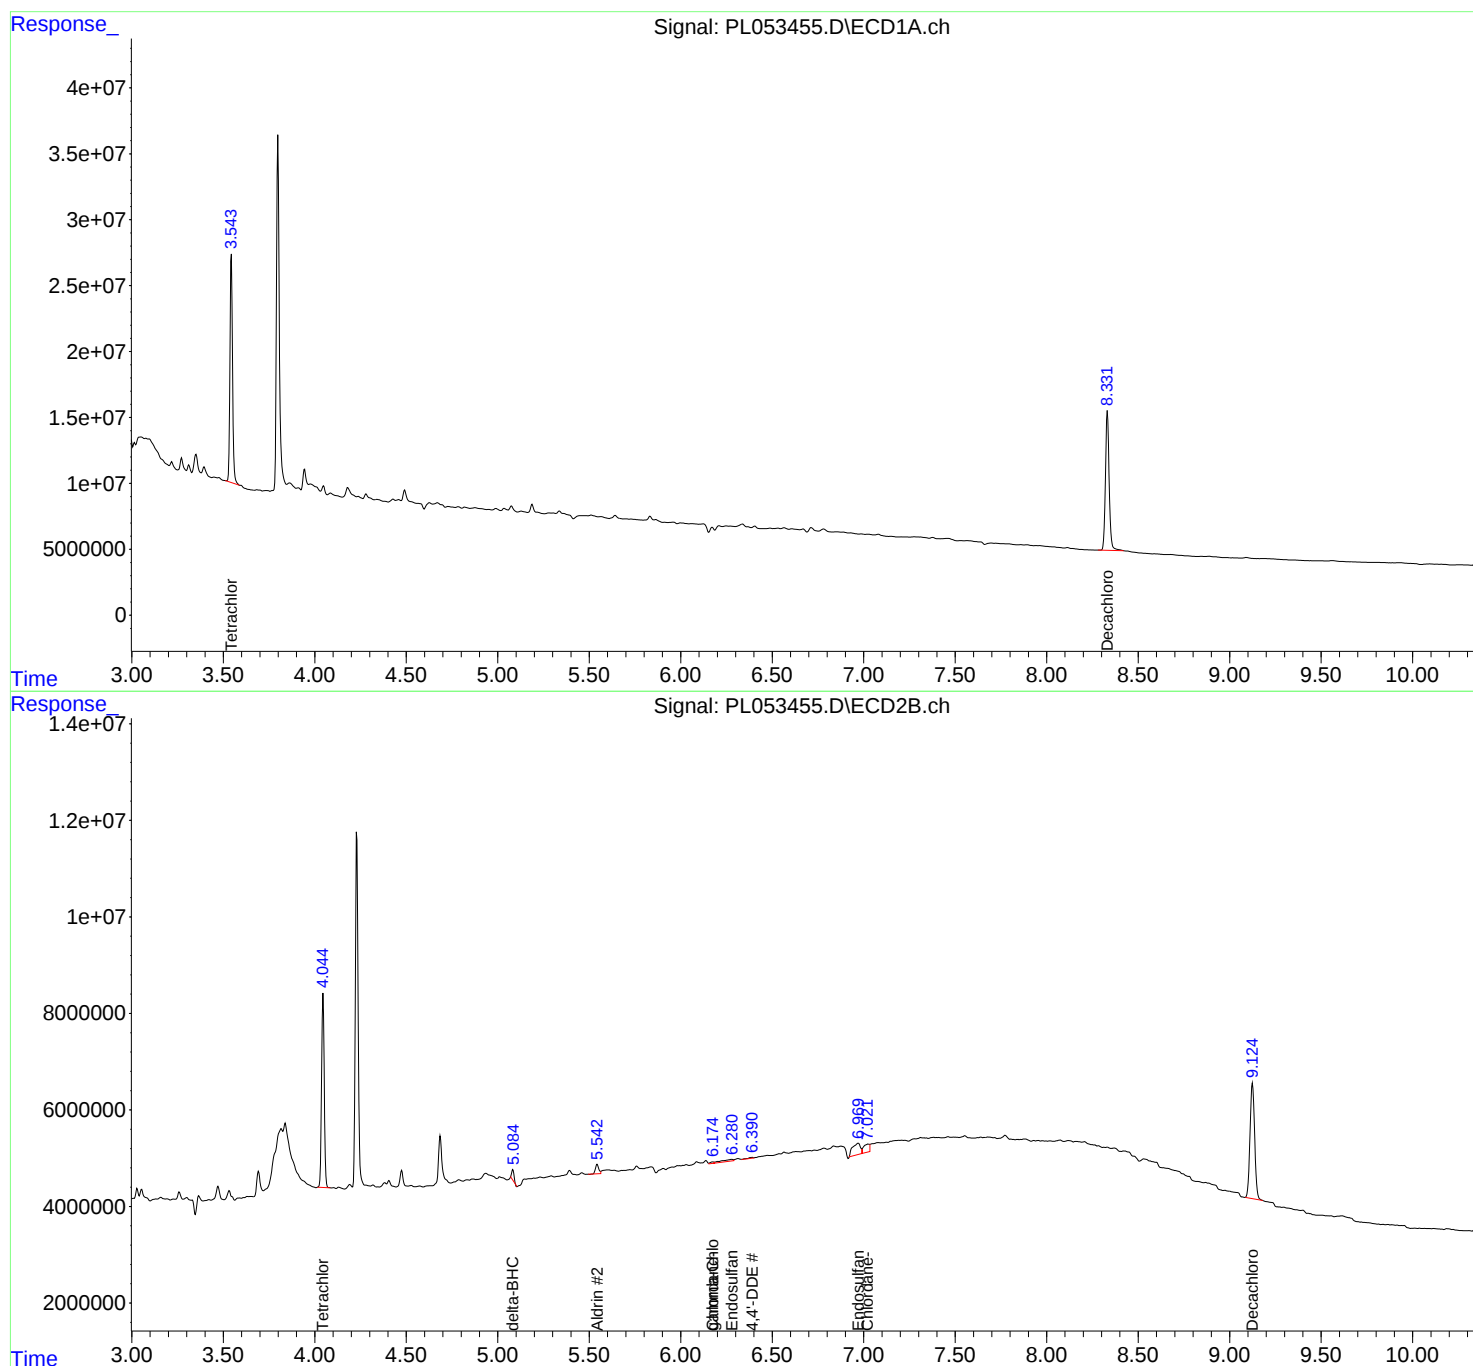


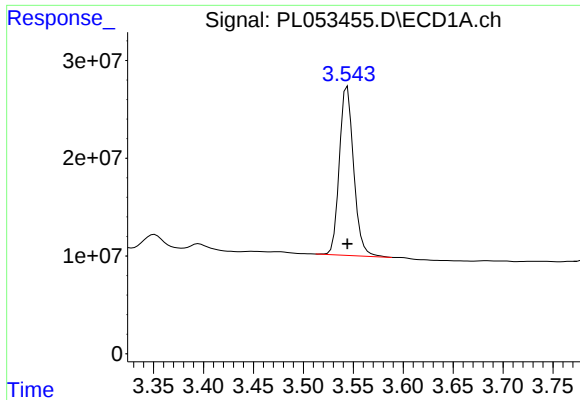

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 171899485
Conc: 15.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

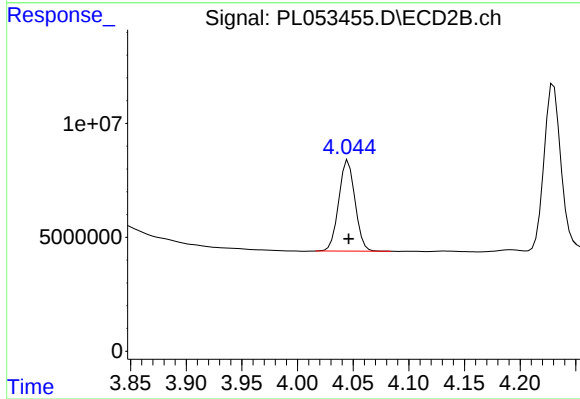


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 40659439
Conc: 16.25 ng/ml

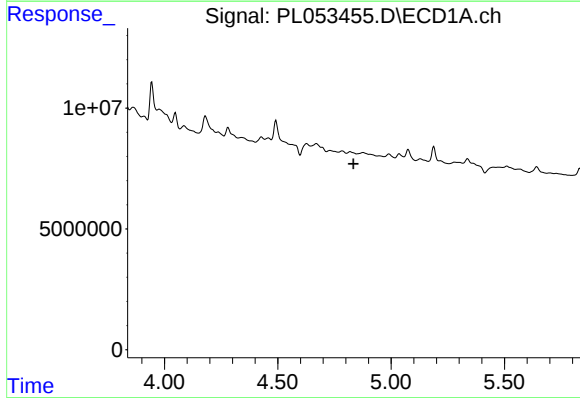


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.834 min
Response: 0
Conc: N.D.

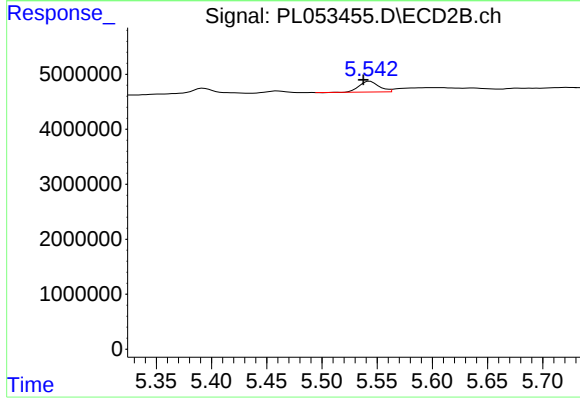

#5 Aldrin


R.T.: 5.544 min
Delta R.T.: 0.006 min
Response: 2425308
Conc: 0.81 ng/ml

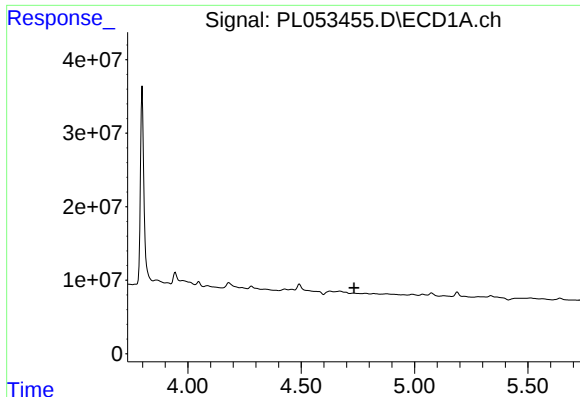

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

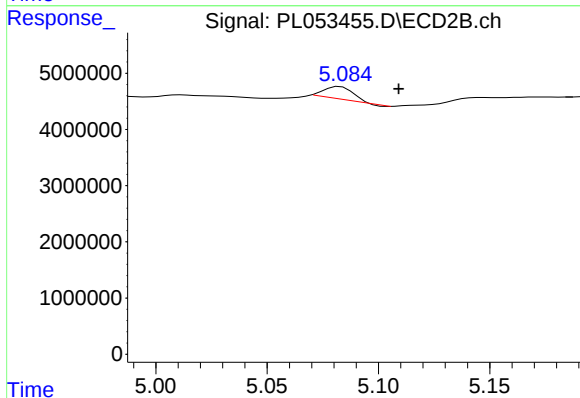


#7 delta-BHC

R.T.: 5.083 min
Delta R.T.: -0.026 min
Response: 1961667
Conc: 0.65 ng/ml

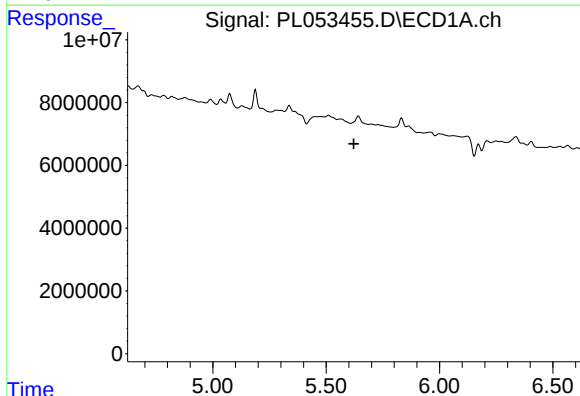


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.623 min
Response: 0
Conc: N.D.

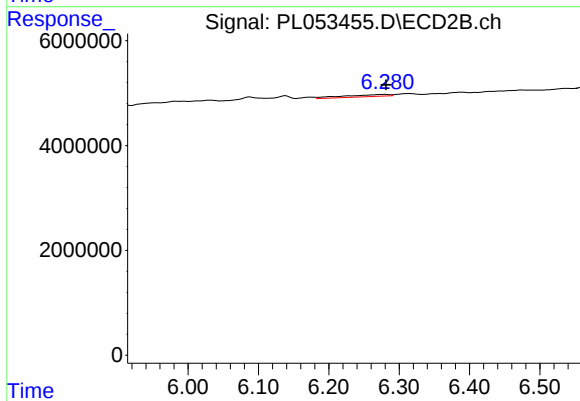

#9 Endosulfan I


R.T.: 6.281 min
Delta R.T.: 0.000 min
Response: 1742462
Conc: 0.64 ng/ml

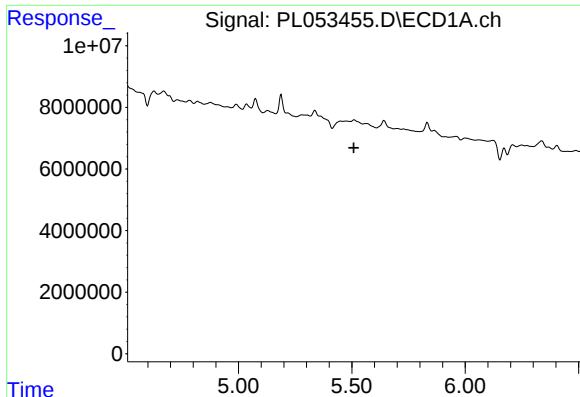

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

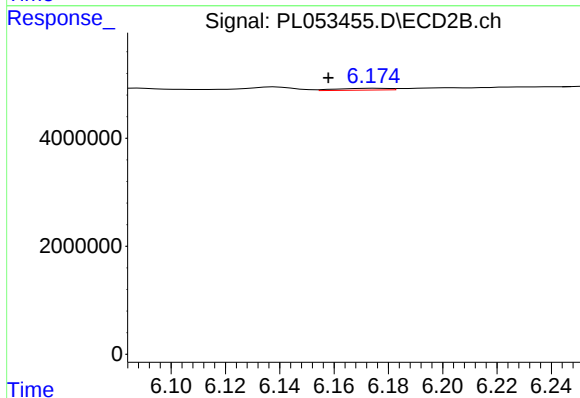


#10 gamma-Chlordane

R.T.: 6.175 min
Delta R.T.: 0.017 min
Response: 434213
Conc: 0.15 ng/ml

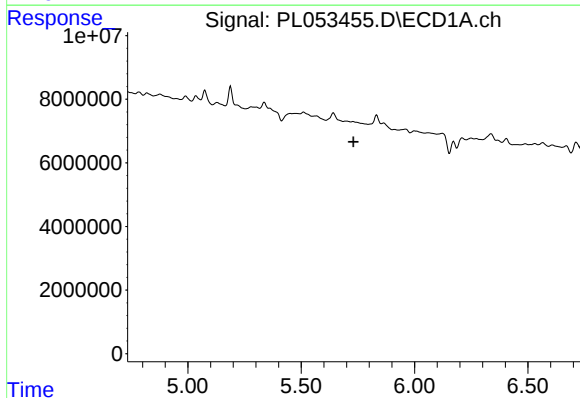


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

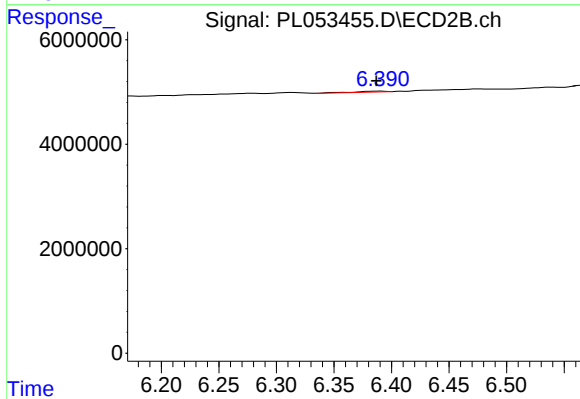

#12 4,4'-DDE


R.T.: 6.391 min
Delta R.T.: 0.004 min
Response: 399514
Conc: 0.14 ng/ml

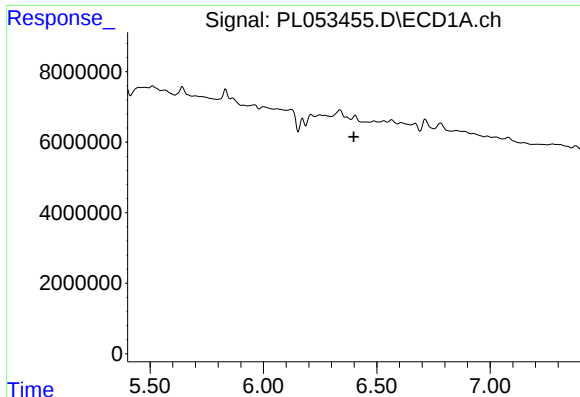

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

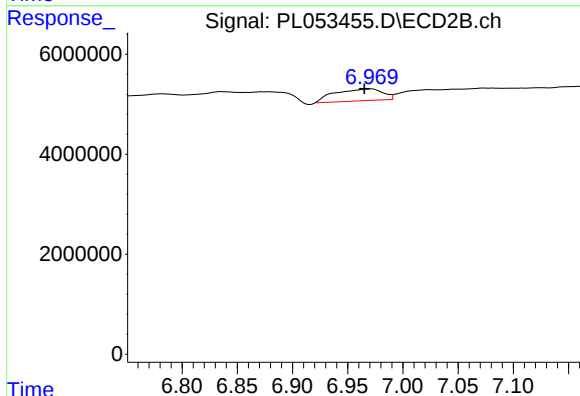


#15 Endosulfan II

R.T.: 6.971 min
Delta R.T.: 0.006 min
Response: 7101041
Conc: 2.78 ng/ml

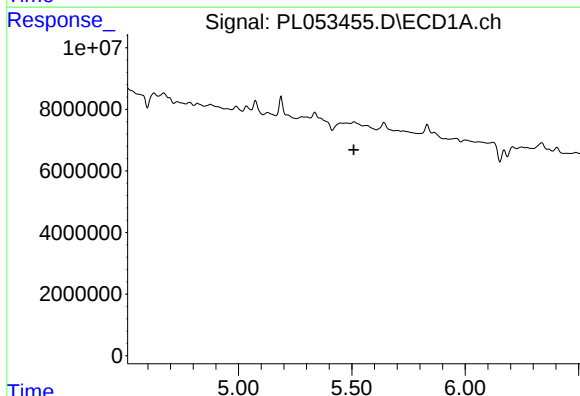


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

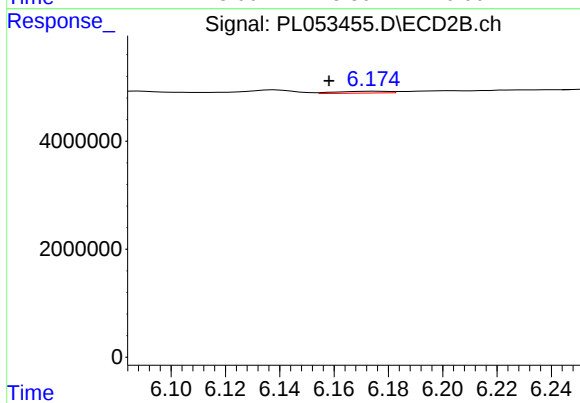

#25 Chlordane-3


R.T.: 6.175 min
Delta R.T.: 0.017 min
Response: 434213
Conc: 1.19 ng/ml

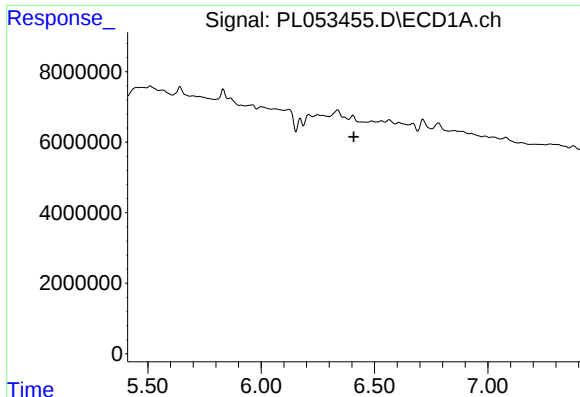

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

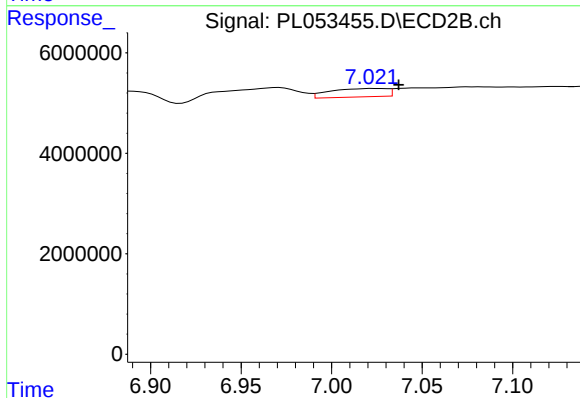


#27 Chlordane-5

R.T.: 7.023 min
Delta R.T.: -0.014 min
Response: 3677791
Conc: 48.11 ng/ml

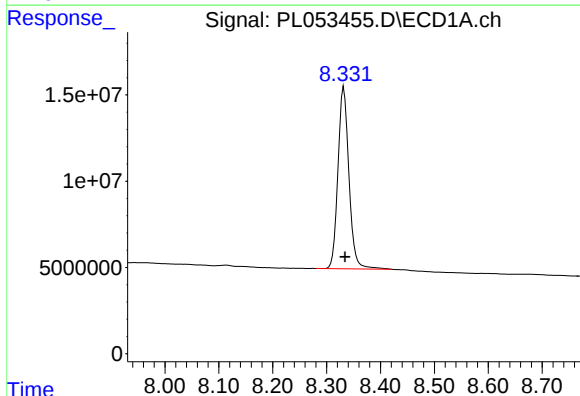

#28 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.002 min
Response: 149206061
Conc: 15.21 ng/ml

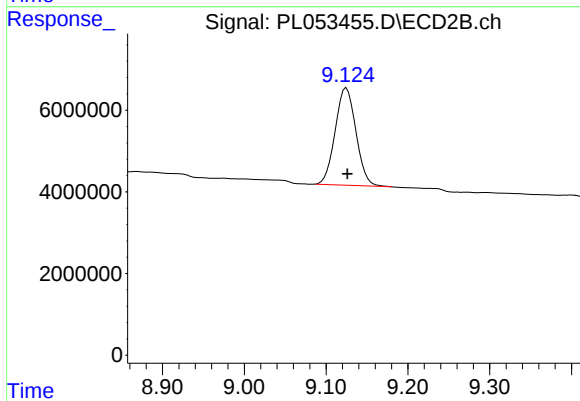

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.001 min
Response: 41971631
Conc: 14.90 ng/ml