

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 19:37
 Operator : SG\AJ
 Sample : K5393-26
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:03:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.045	185.7E6	44888134	17.134	17.938
28)	SA Decachlor...	8.333	9.125	189.4E6	52387623	19.300	18.603
Target Compounds							
2)	A alpha-BHC	3.985	0.000	22345490	0	1.282	N.D. #
7)	B delta-BHC	0.000	5.084f	0	4409717	N.D.	1.460 #
8)	B Heptachlo...	0.000	5.933	0	7248260	N.D.	2.485 #
9)	A Endosulfan I	0.000	6.310f	0	2746701	N.D.	1.013 #
11)	B alpha-Chl...	0.000	6.232	0	3889170	N.D.	1.332 #
12)	B 4,4'-DDE	0.000	6.386	0	324907	N.D.	0.115 #
15)	B Endosulfa...	0.000	6.968	0	6786708	N.D.	2.657 #
26)	Chlordane-4	0.000	6.232	0	3889170	N.D.	8.663 #
27)	Chlordane-5	0.000	7.045	0	6550092	N.D.	85.680 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 19:37
Operator : SG\AJ
Sample : K5393-26
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:03:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

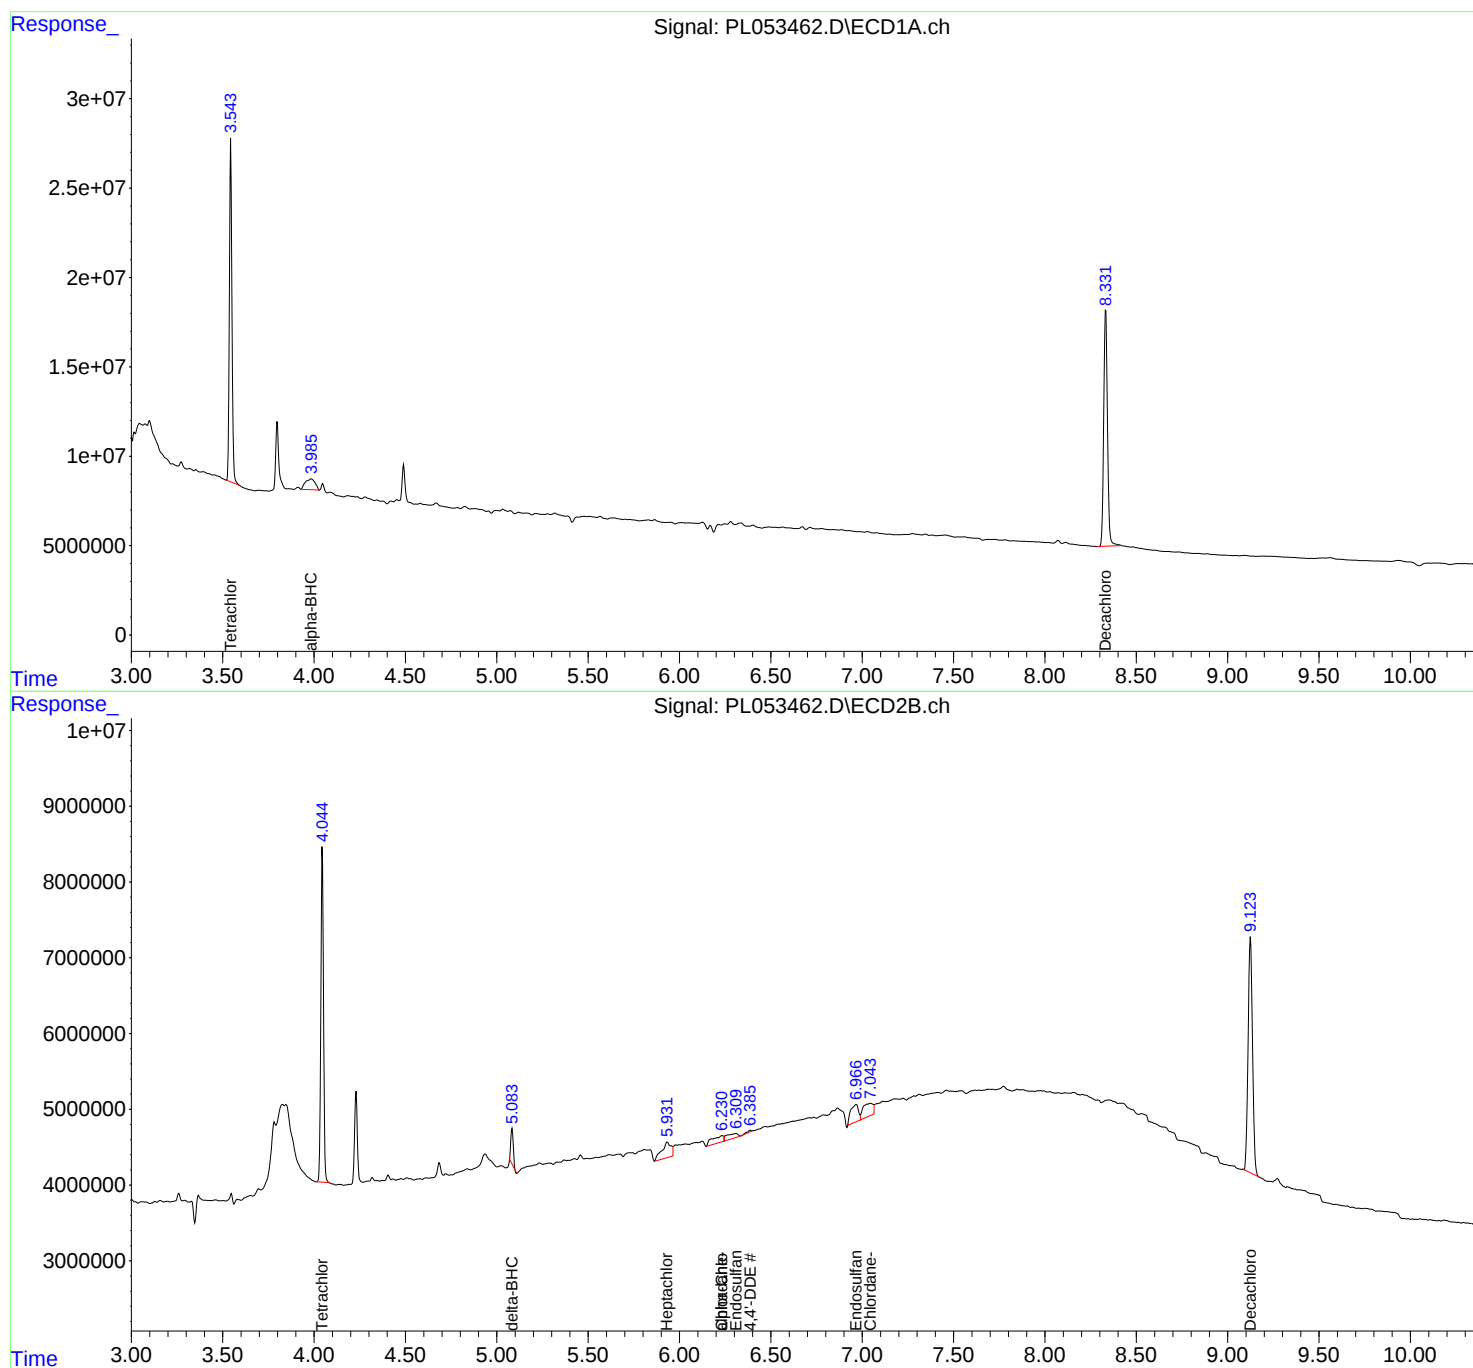


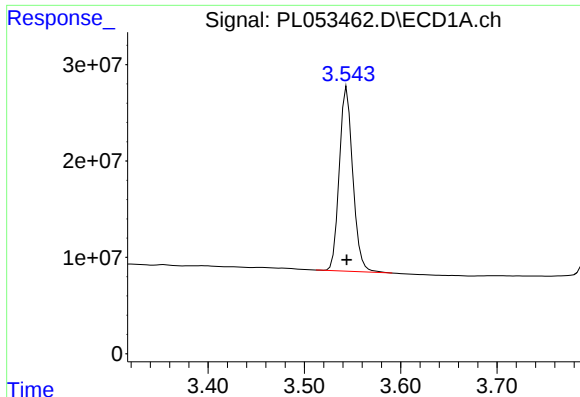

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 185721319
Conc: 17.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

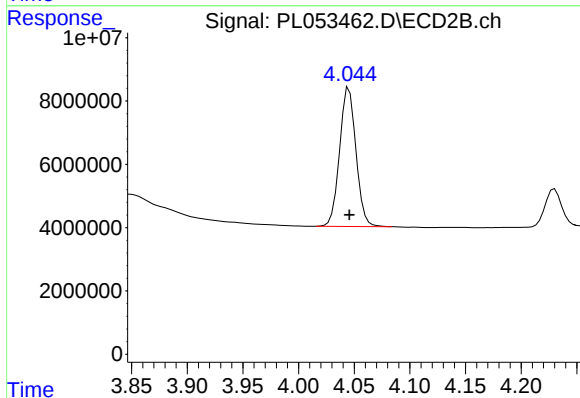


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 44888134
Conc: 17.94 ng/ml

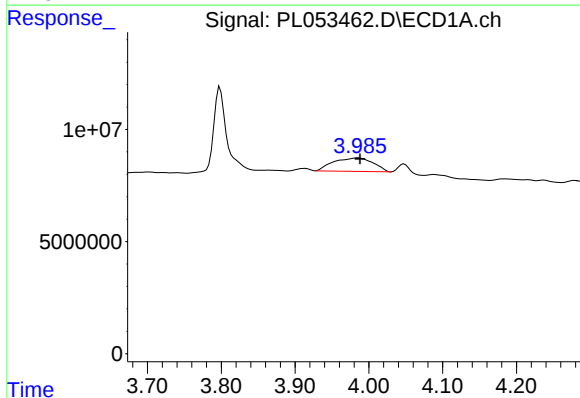


#2 alpha-BHC

R.T.: 3.985 min
Delta R.T.: -0.003 min
Response: 22345490
Conc: 1.28 ng/ml

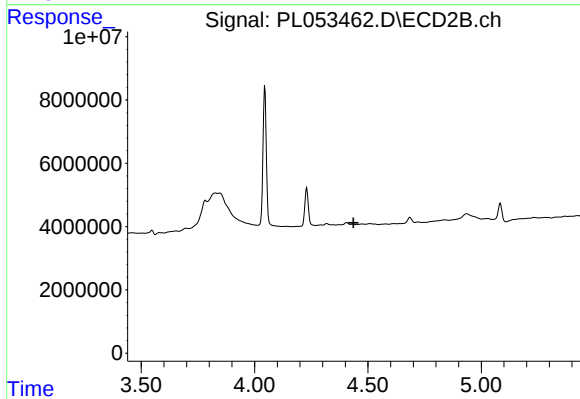

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.437 min
Response: 0
Conc: N.D.

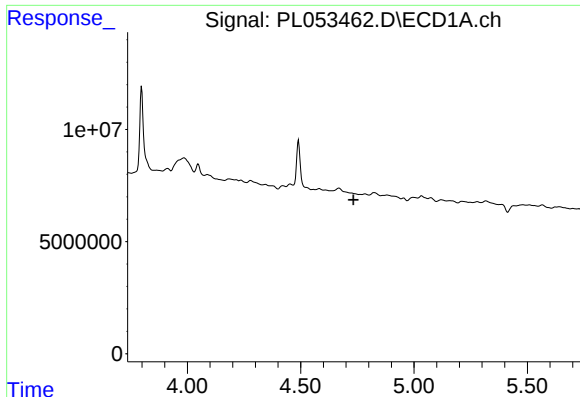

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

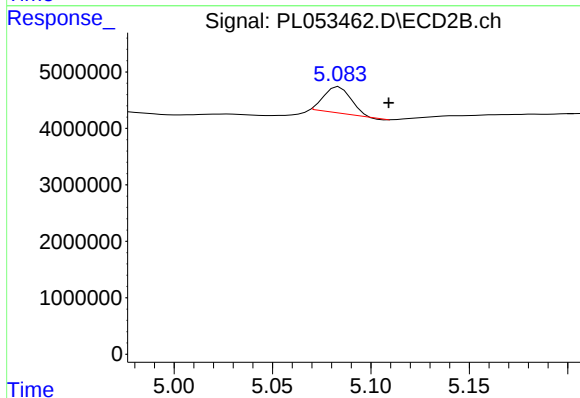


#7 delta-BHC

R.T.: 5.084 min
Delta R.T.: -0.025 min
Response: 4409717
Conc: 1.46 ng/ml

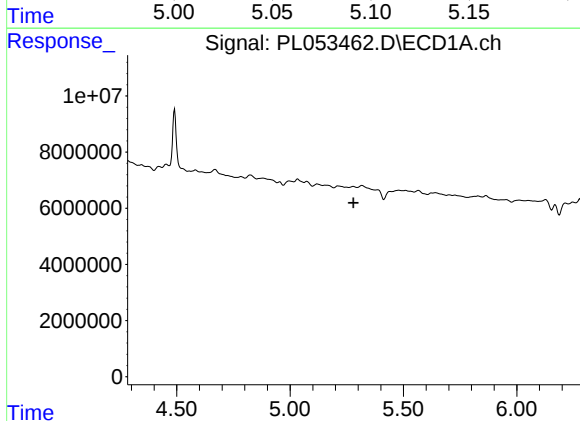


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

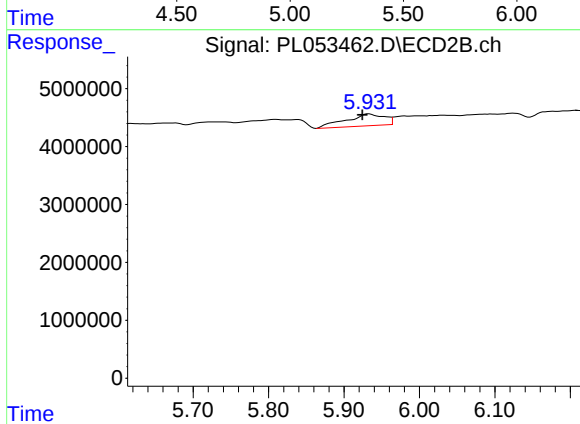

#8 Heptachlor epoxide


R.T.: 5.933 min
Delta R.T.: 0.008 min
Response: 7248260
Conc: 2.49 ng/ml

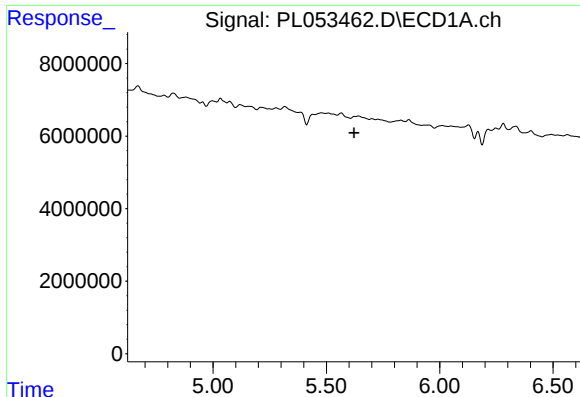

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

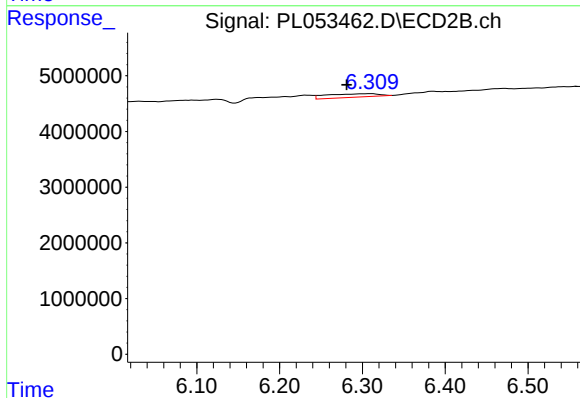


#9 Endosulfan I

R.T.: 6.310 min
Delta R.T.: 0.029 min
Response: 2746701
Conc: 1.01 ng/ml

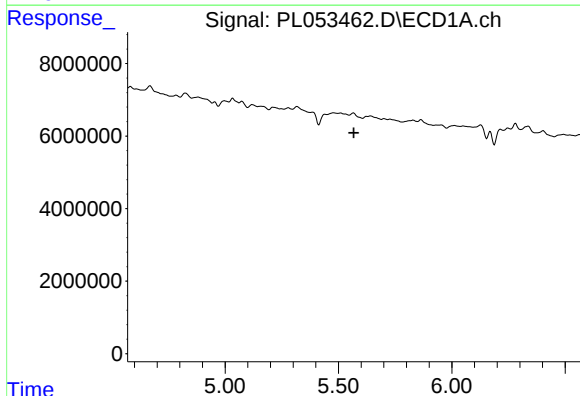


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

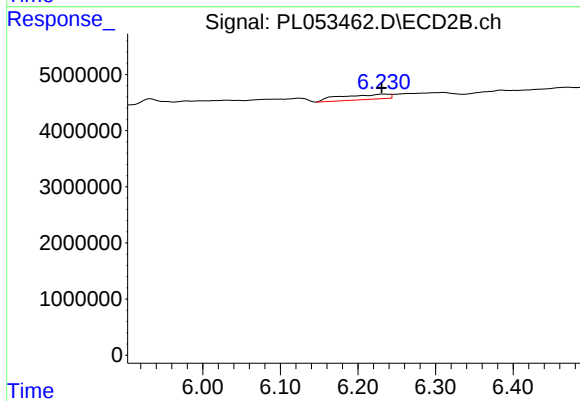

#11 alpha-Chlordane


R.T.: 6.232 min
Delta R.T.: 0.002 min
Response: 3889170
Conc: 1.33 ng/ml

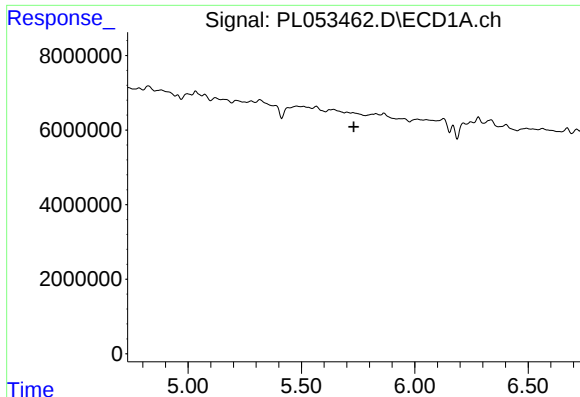

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

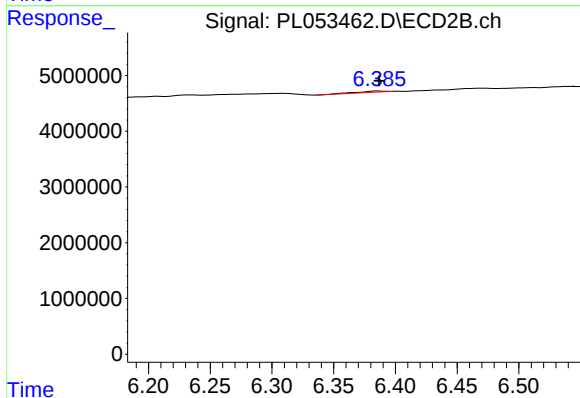


#12 4,4'-DDE

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 324907
Conc: 0.12 ng/ml

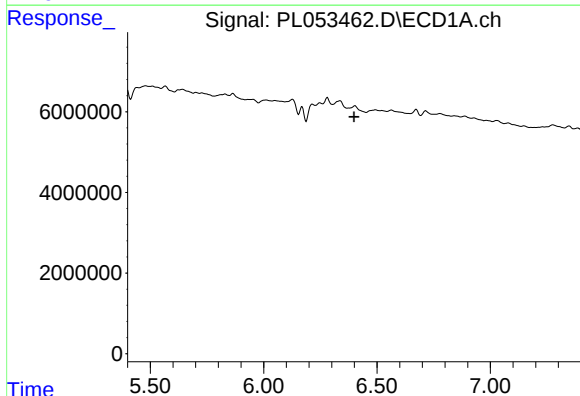


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

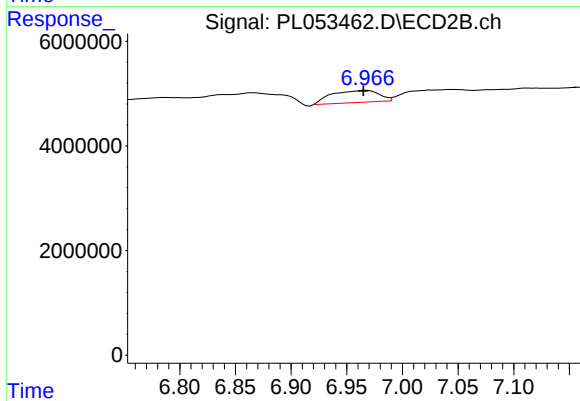

#15 Endosulfan II


R.T.: 6.968 min
Delta R.T.: 0.003 min
Response: 6786708
Conc: 2.66 ng/ml

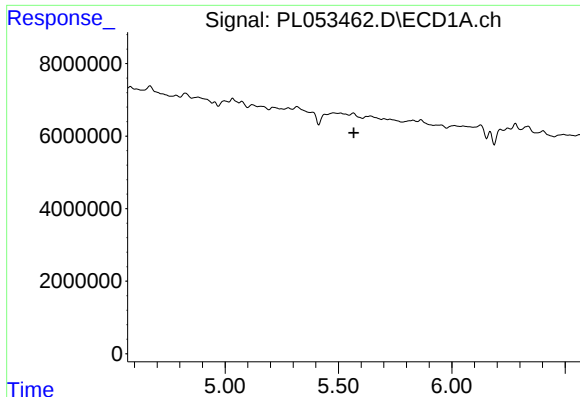

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

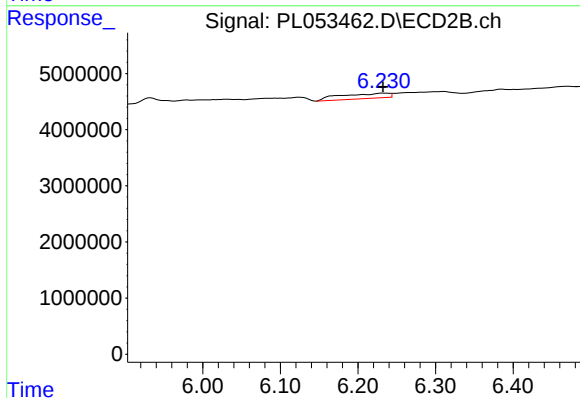


#26 Chlordane-4

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 3889170
Conc: 8.66 ng/ml

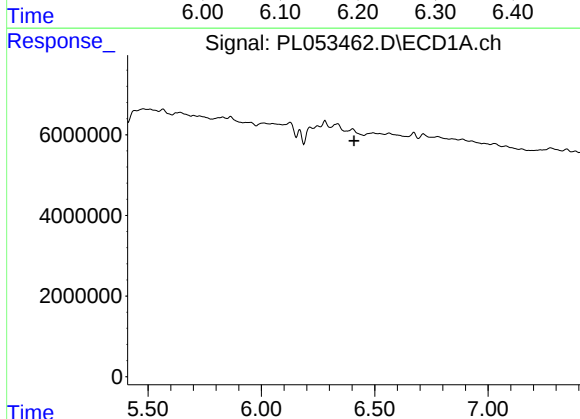


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

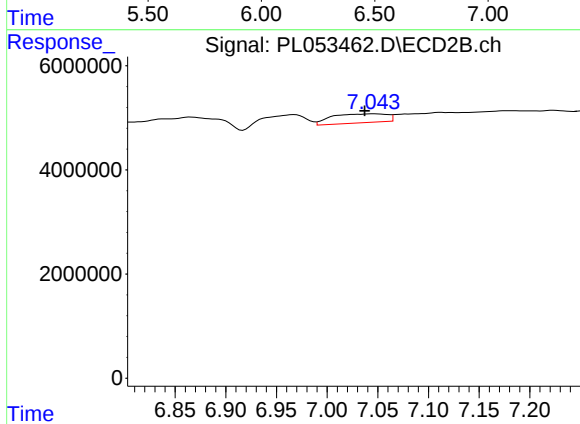

#27 Chlordane-5


R.T.: 7.045 min
Delta R.T.: 0.008 min
Response: 6550092
Conc: 85.68 ng/ml

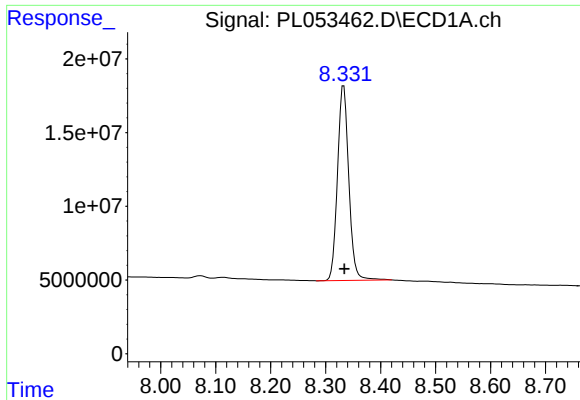

#28 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.001 min
Response: 189362030
Conc: 19.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

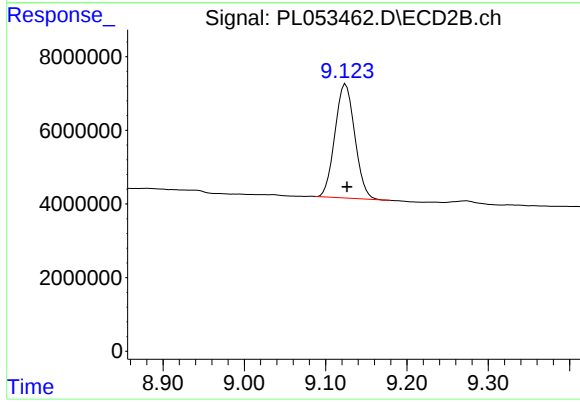

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.001 min
Response: 52387623
Conc: 18.60 ng/ml