

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 19:51
 Operator : SG\AJ
 Sample : K5394-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:03:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.045	164.3E6	39489913	15.162	15.781
28)	SA Decachlor...	8.332	9.126	168.9E6	48443766	17.218	17.203
Target Compounds							
2)	A alpha-BHC	3.982	0.000	19040043	0	1.092	N.D. #
7)	B delta-BHC	0.000	5.083f	0	2709611	N.D.	0.897 #
8)	B Heptachlo...	0.000	5.934	0	5357651	N.D.	1.837 #
9)	A Endosulfan I	0.000	6.308f	0	1853469	N.D.	0.684 #
11)	B alpha-Chl...	0.000	6.234	0	2580767	N.D.	0.884 #
12)	B 4,4'-DDE	0.000	6.391	0	497456	N.D.	0.177 #
15)	B Endosulfa...	0.000	6.968	0	5990010	N.D.	2.345 #
18)	B Endrin al...	0.000	7.111f	0	8818618	N.D.	4.014 #
26)	Chlordane-4	0.000	6.234	0	2580767	N.D.	5.749 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 19:51
Operator : SG\AJ
Sample : K5394-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:03:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

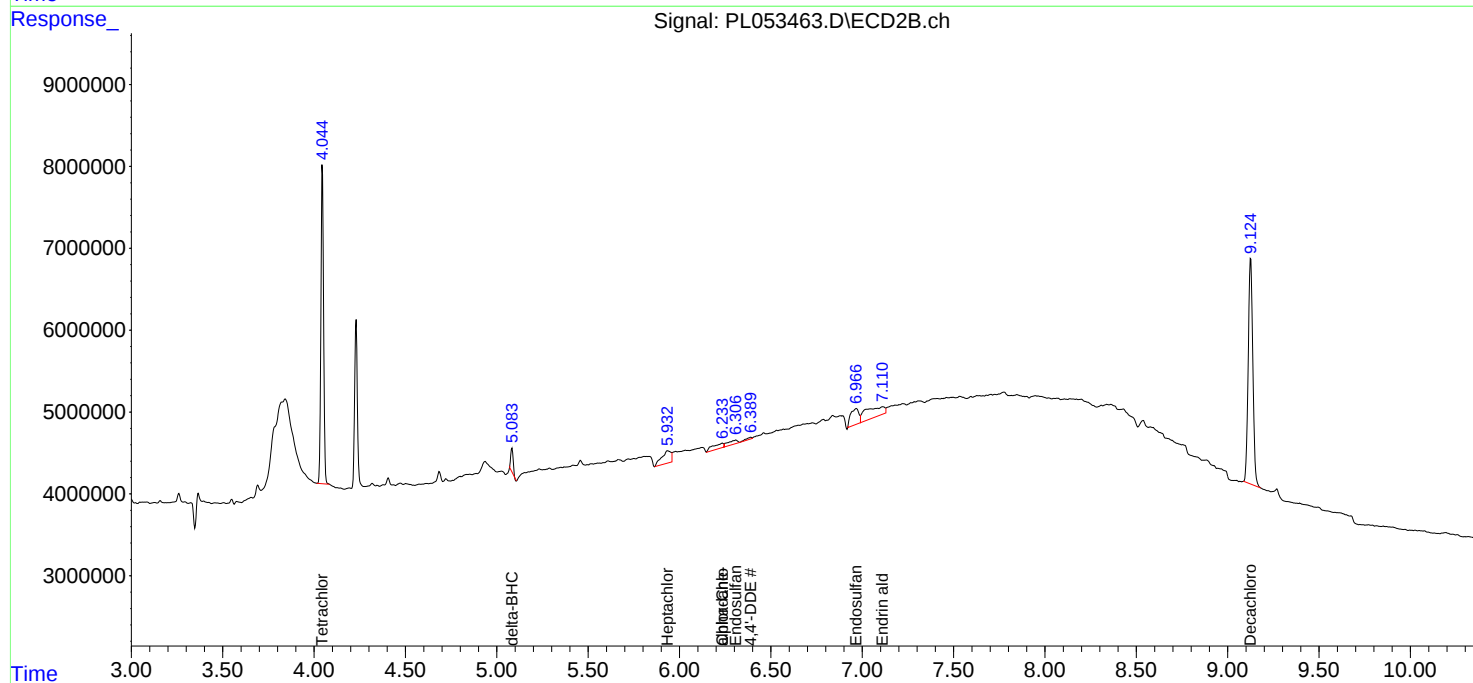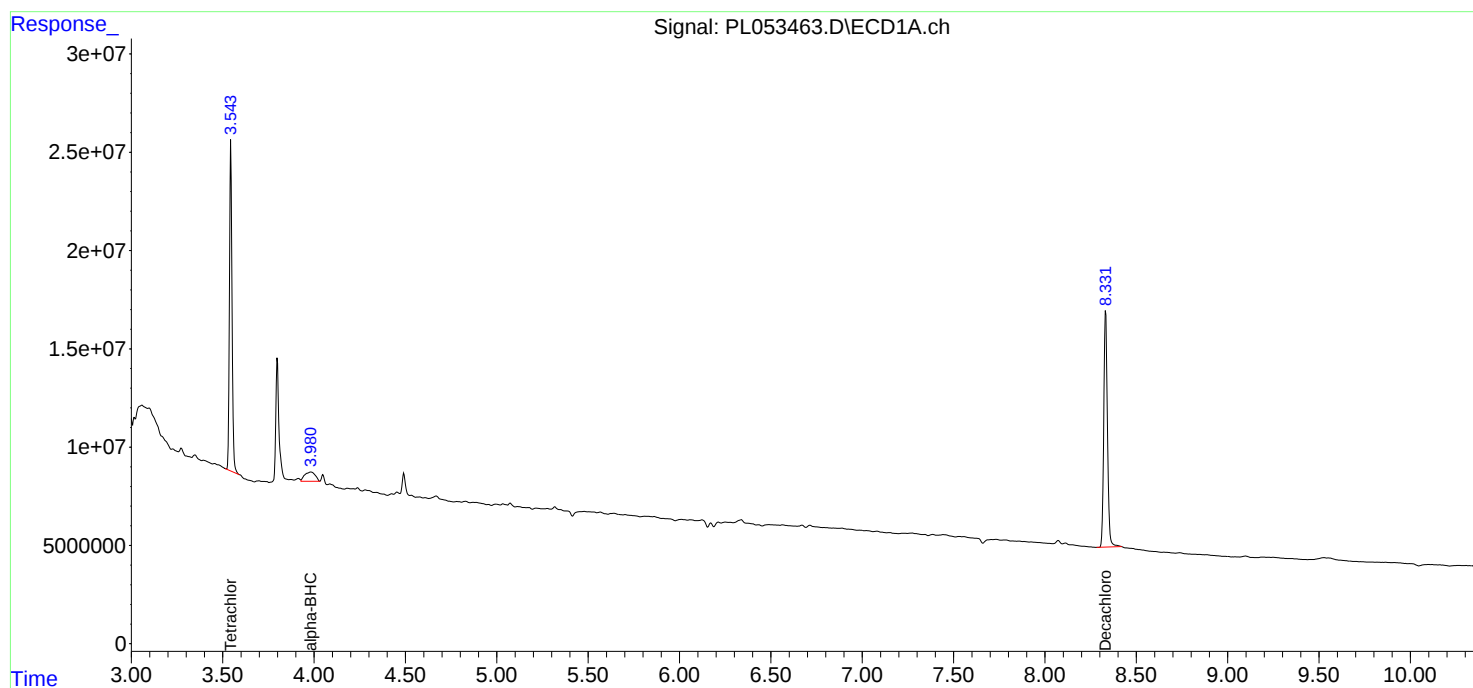


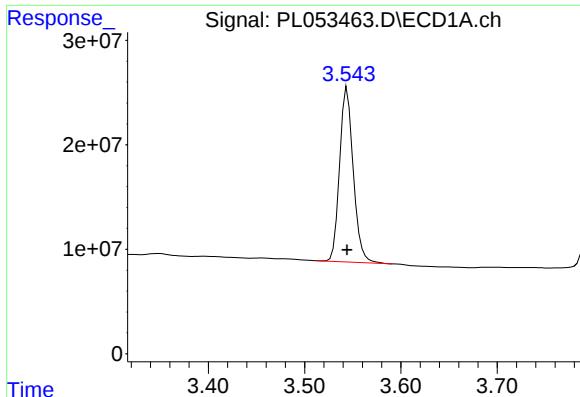

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 164349413
Conc: 15.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

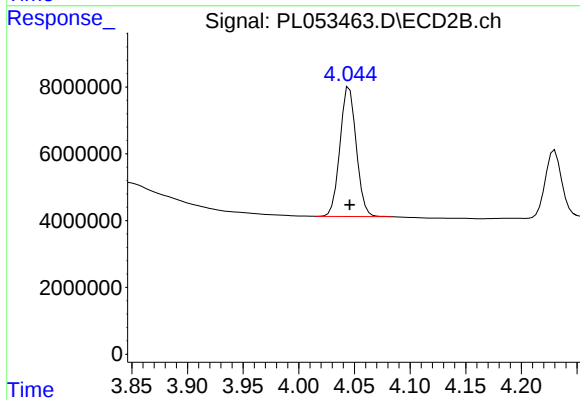


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 39489913
Conc: 15.78 ng/ml

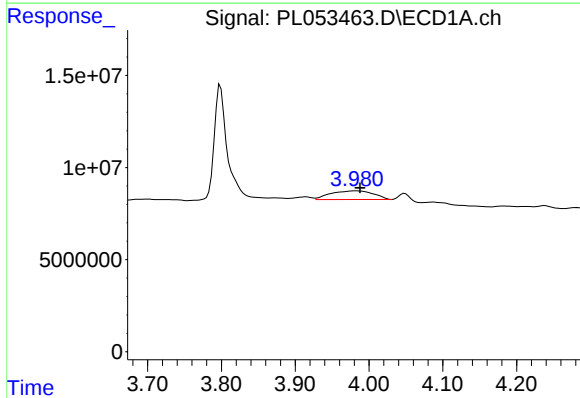


#2 alpha-BHC

R.T.: 3.982 min
Delta R.T.: -0.006 min
Response: 19040043
Conc: 1.09 ng/ml

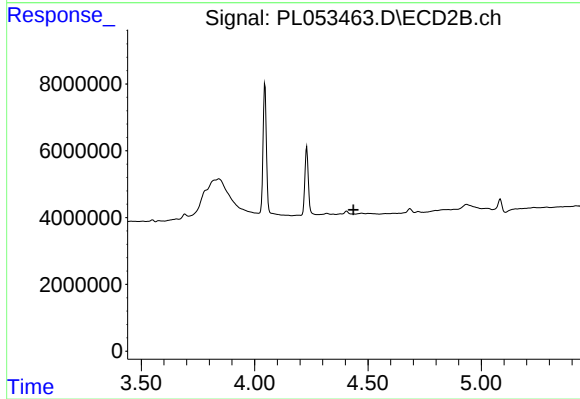

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.437 min
Response: 0
Conc: N.D.

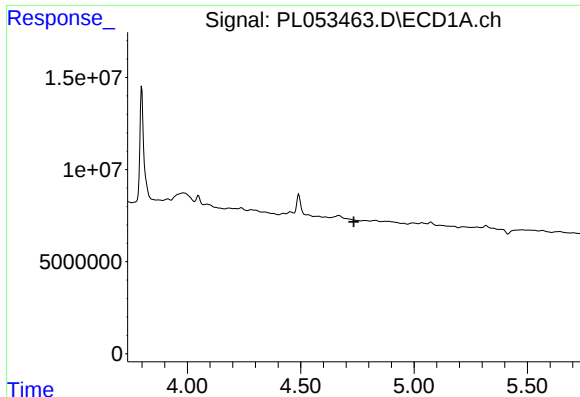

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

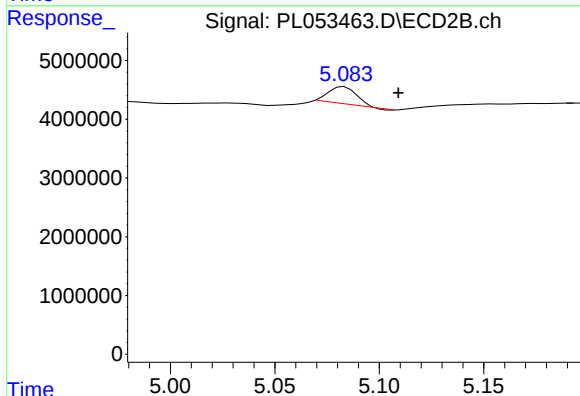


#7 delta-BHC

R.T.: 5.083 min
Delta R.T.: -0.026 min
Response: 2709611
Conc: 0.90 ng/ml

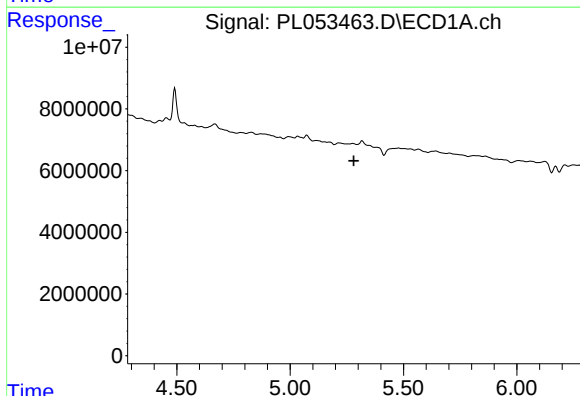


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

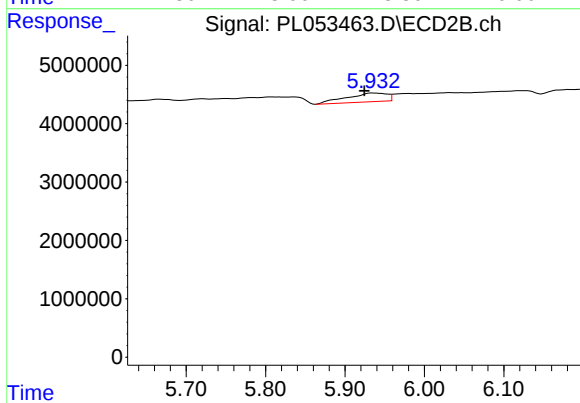

#8 Heptachlor epoxide


R.T.: 5.934 min
Delta R.T.: 0.009 min
Response: 5357651
Conc: 1.84 ng/ml

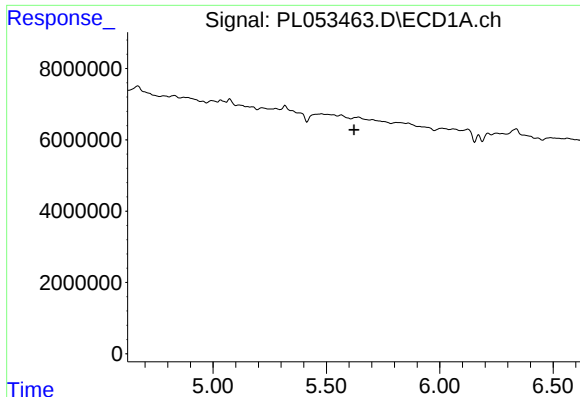

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

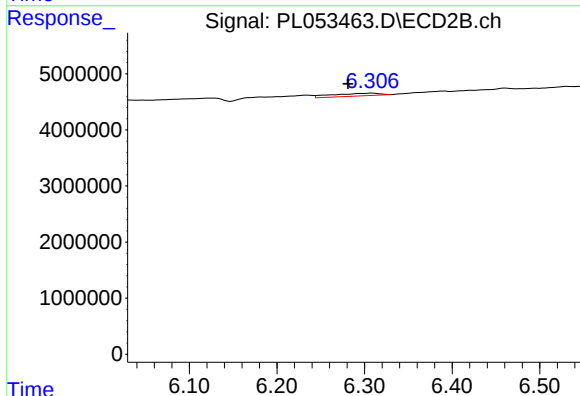


#9 Endosulfan I

R.T.: 6.308 min
Delta R.T.: 0.027 min
Response: 1853469
Conc: 0.68 ng/ml

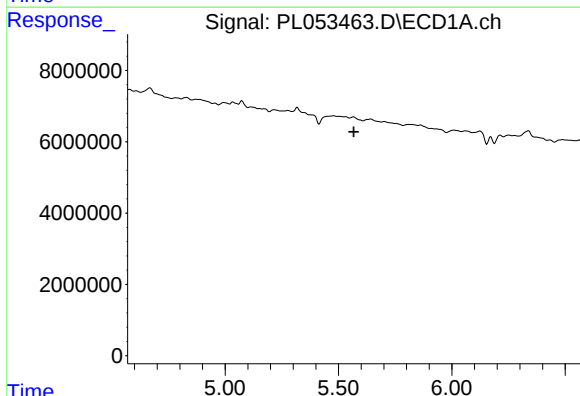


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

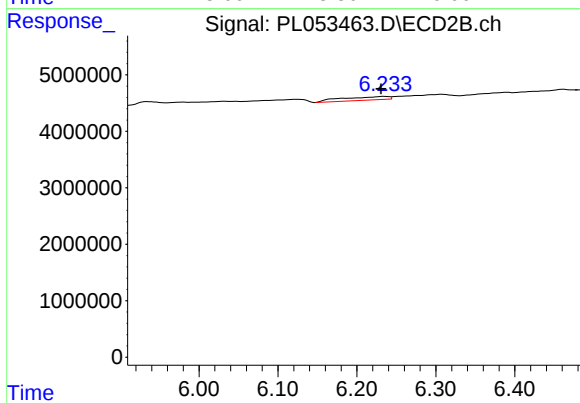

#11 alpha-Chlordane


R.T.: 6.234 min
Delta R.T.: 0.003 min
Response: 2580767
Conc: 0.88 ng/ml

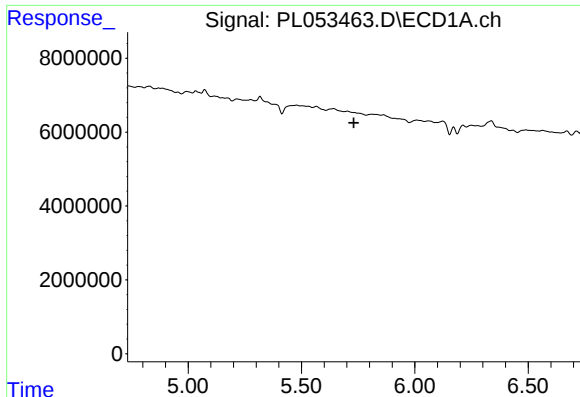

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

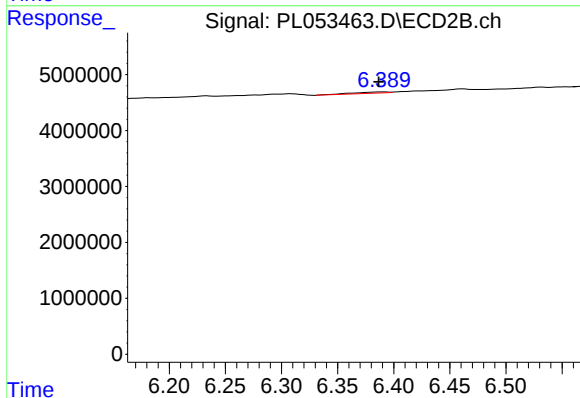


#12 4,4'-DDE

R.T.: 6.391 min
Delta R.T.: 0.004 min
Response: 497456
Conc: 0.18 ng/ml

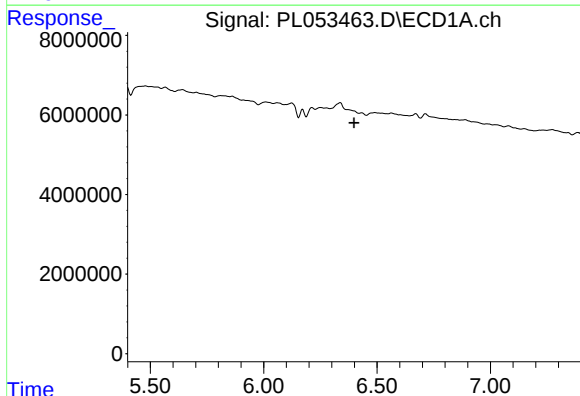


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

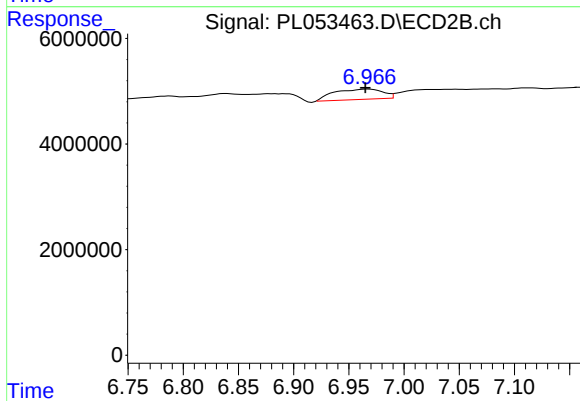

#15 Endosulfan II


R.T.: 6.968 min
Delta R.T.: 0.003 min
Response: 5990010
Conc: 2.34 ng/ml

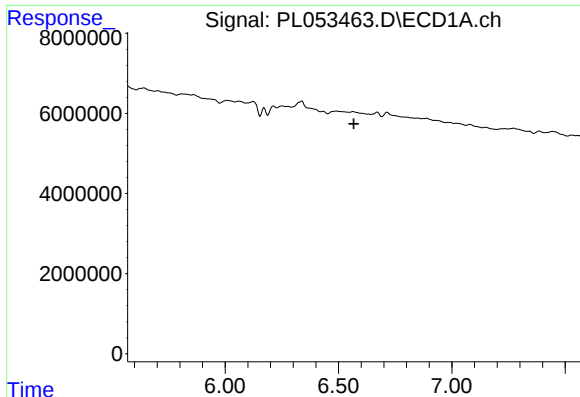

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

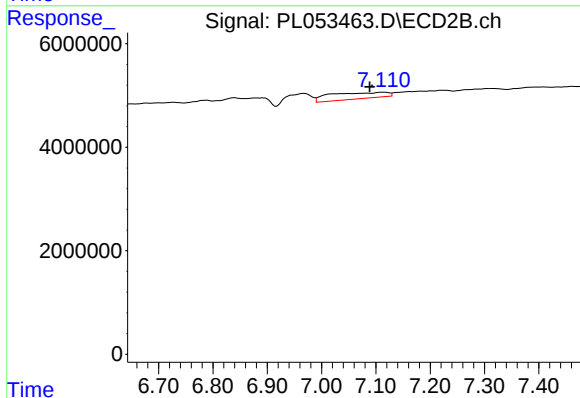


#18 Endrin aldehyde

R.T.: 7.111 min
Delta R.T.: 0.022 min
Response: 8818618
Conc: 4.01 ng/ml

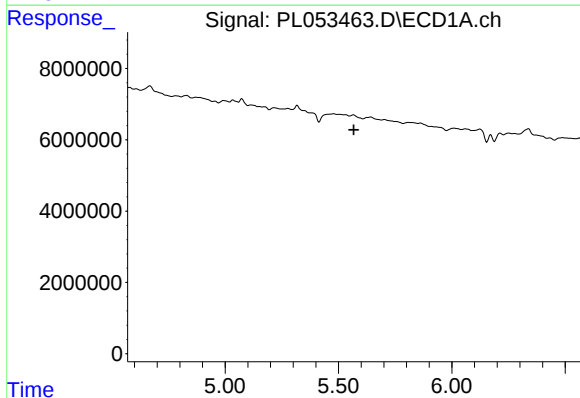


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

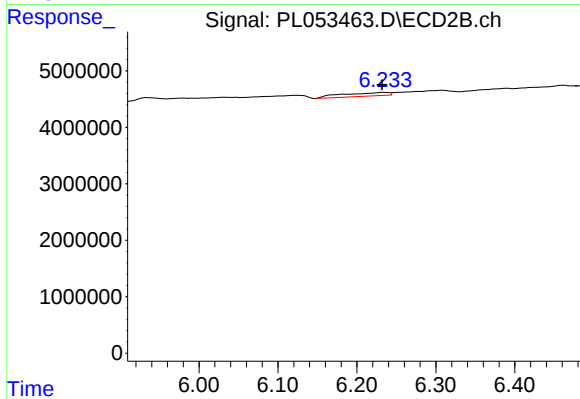

#26 Chlordane-4


R.T.: 6.234 min
Delta R.T.: 0.002 min
Response: 2580767
Conc: 5.75 ng/ml

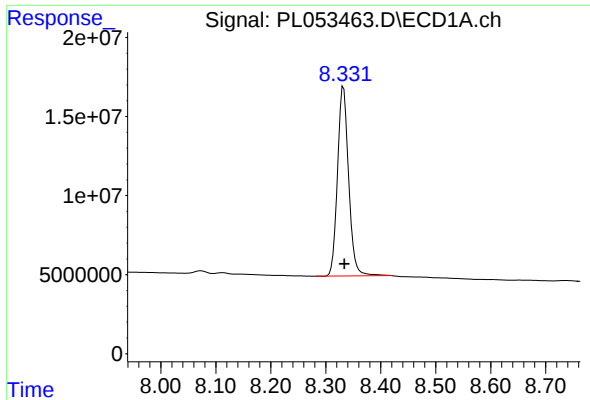

#28 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.002 min
Response: 168936856
Conc: 17.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

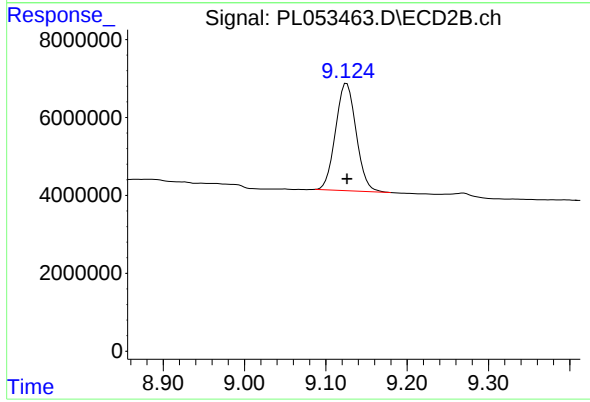

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 48443766
Conc: 17.20 ng/ml