

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 12:37
 Operator : SG\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 13:18:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:17:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.046	905.0E6	172.5E6	78.798	79.159
28)	SA Decachlor...	8.335	9.126	662.6E6	191.1E6	77.780	75.772
Target Compounds							
23)	Chlordane-1	4.429	5.044	267.5E6	62019911	799.134	797.828
24)	Chlordane-2	4.934	5.512	286.1E6	71865282	779.036	789.452
25)	Chlordane-3	5.510	6.159	904.0E6	278.0E6	804.470	822.473
26)	Chlordane-4	5.568	6.233	735.0E6	336.8E6	804.993	813.078
27)	Chlordane-5	6.410	7.038	271.6E6	57782578	800.205	808.185



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 12:37
Operator : SG\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 13:18:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:17:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

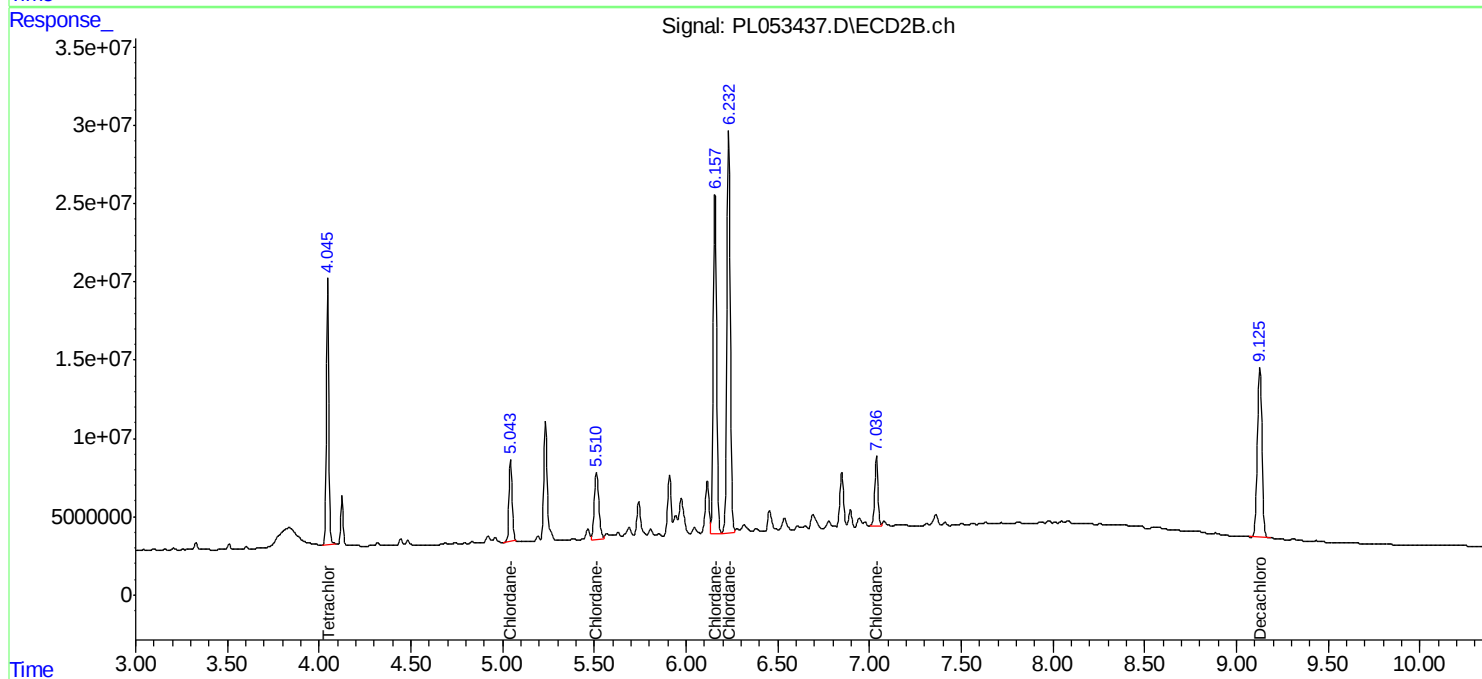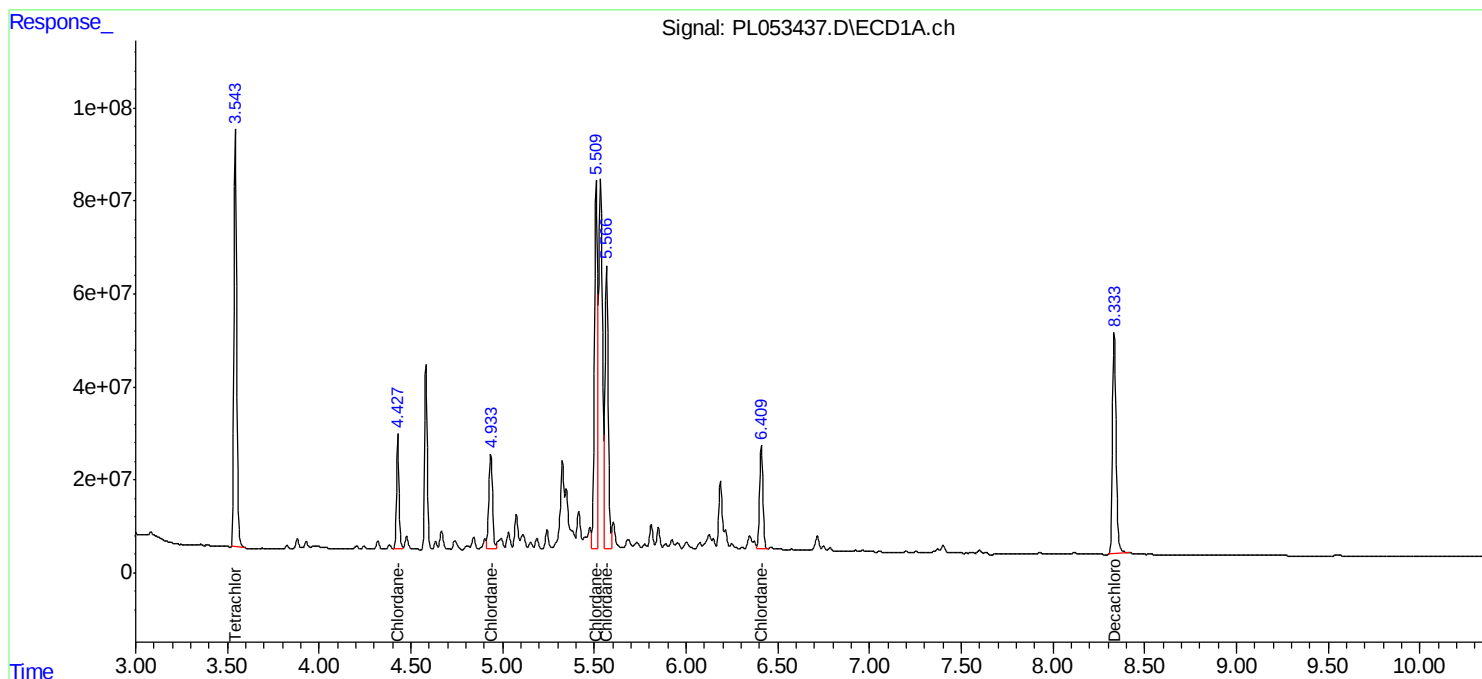


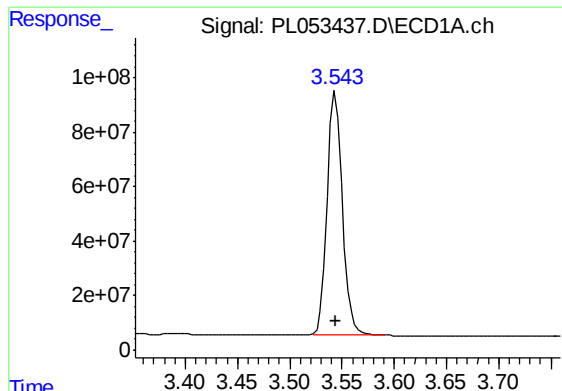

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 905027117
Conc: 78.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

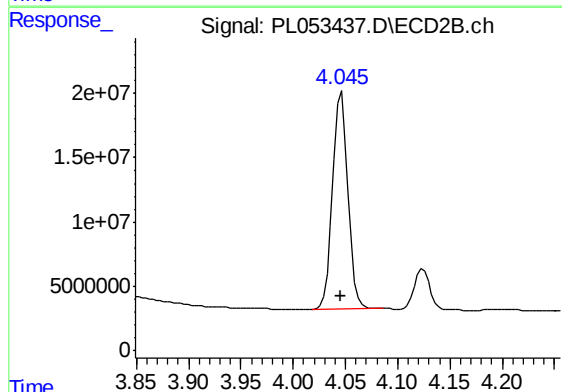


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 172457904
Conc: 79.16 ng/ml

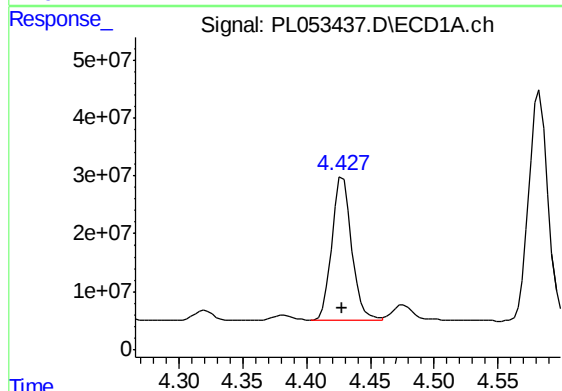


#23 Chlordane-1

R.T.: 4.429 min
Delta R.T.: 0.000 min
Response: 267502839
Conc: 799.13 ng/ml

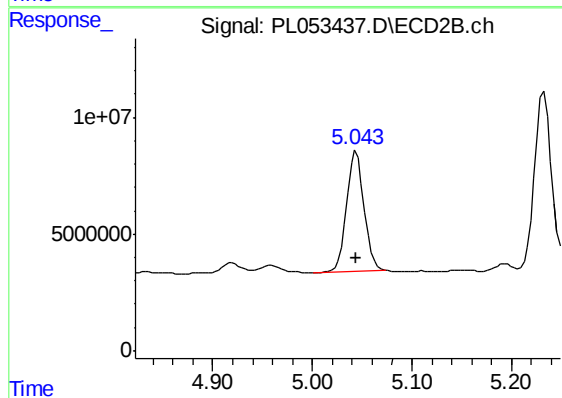

#23 Chlordane-1


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 62019911
Conc: 797.83 ng/ml

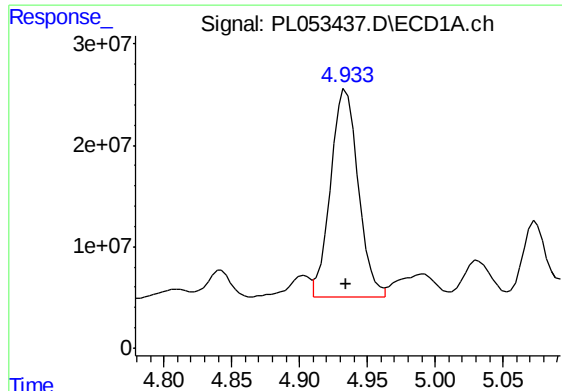

#24 Chlordane-2


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 286137664
Conc: 779.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

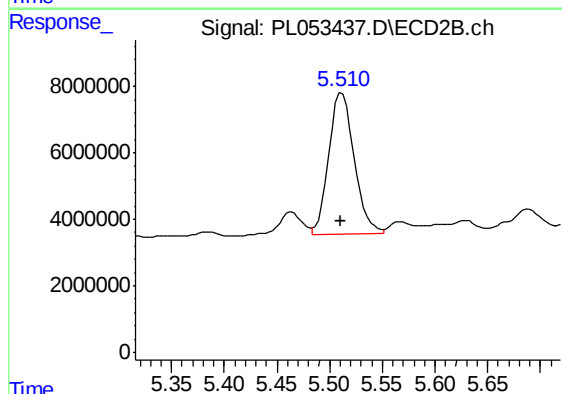


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.001 min
Response: 71865282
Conc: 789.45 ng/ml

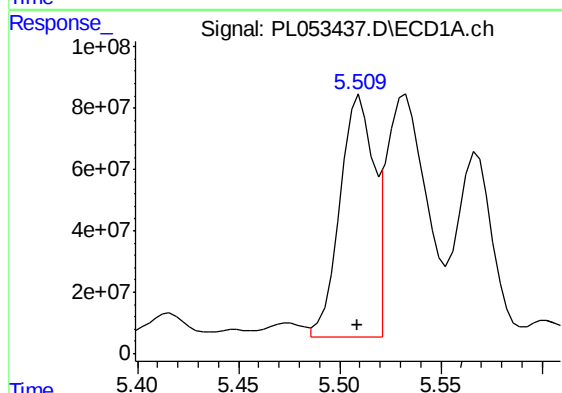


#25 Chlordane-3

R.T.: 5.510 min
Delta R.T.: 0.001 min
Response: 904045804
Conc: 804.47 ng/ml

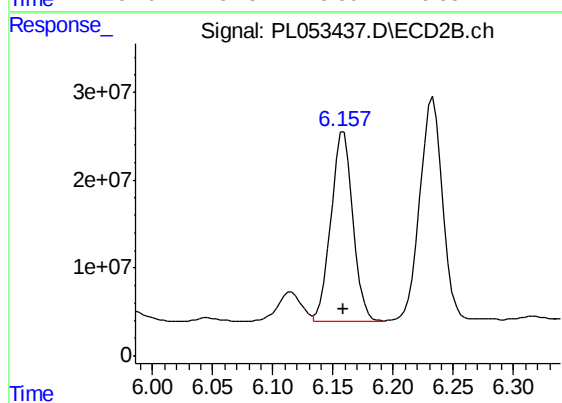

#25 Chlordane-3


R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 278016442
Conc: 822.47 ng/ml

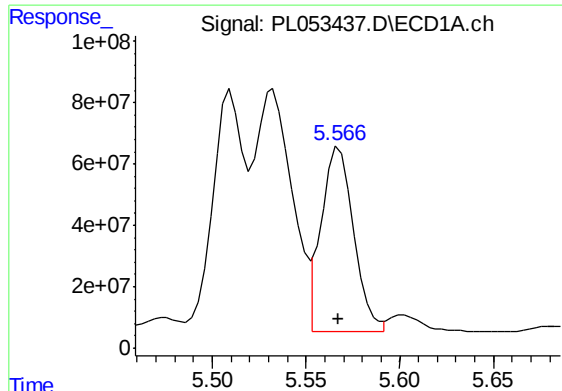

#26 Chlordane-4


R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 734999697
Conc: 804.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

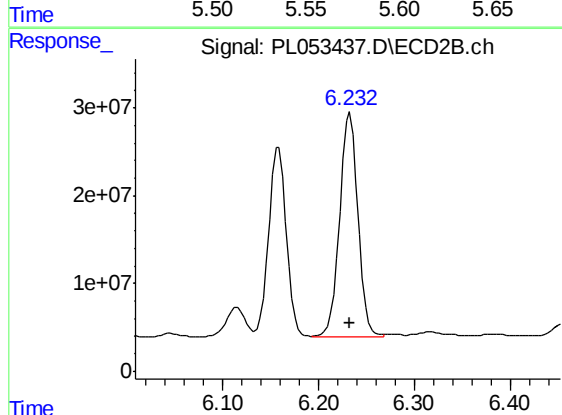


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 336812460
Conc: 813.08 ng/ml

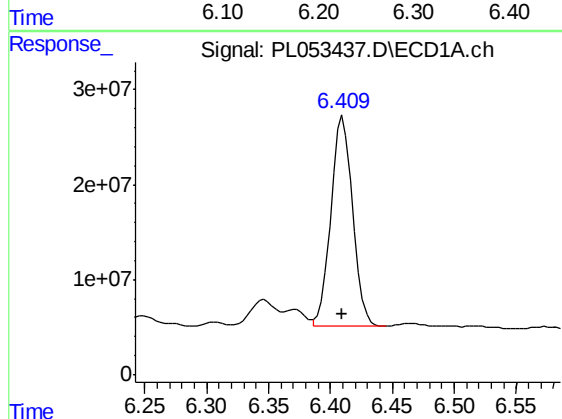


#27 Chlordane-5

R.T.: 6.410 min
Delta R.T.: 0.001 min
Response: 271606067
Conc: 800.21 ng/ml

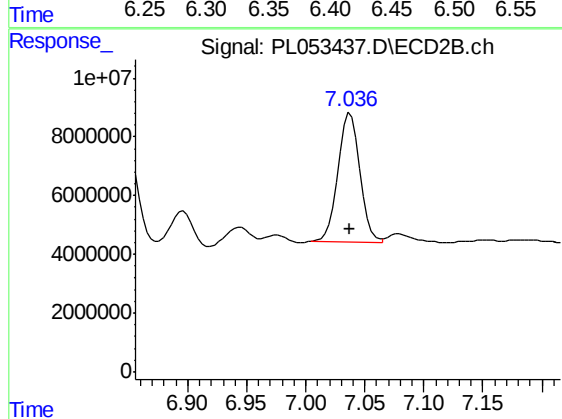

#27 Chlordane-5


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 57782578
Conc: 808.19 ng/ml

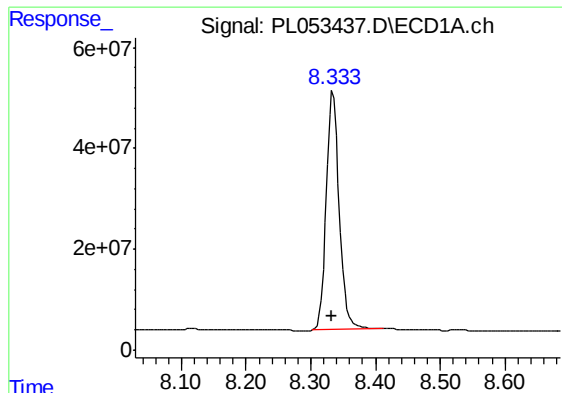

#28 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: 0.001 min
Response: 662559293
Conc: 77.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

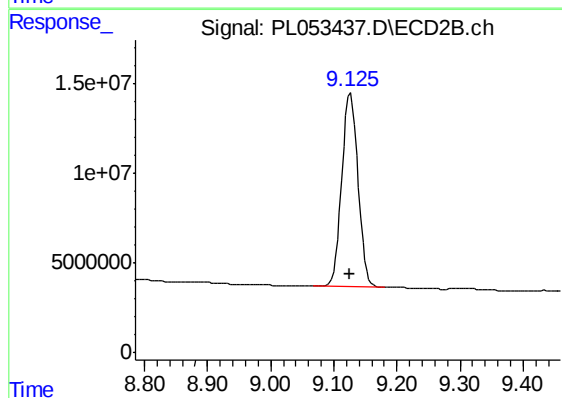

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 191126820
Conc: 75.77 ng/ml