

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 12:51
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 13:17:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:17:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.046	574.3E6	108.9E6	50.000	50.000
28)	SA Decachlor...	8.333	9.126	425.9E6	126.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.428	5.043	167.4E6	38867951	500.000	500.000
24)	Chlordane-2	4.934	5.510	183.6E6	45515938	500.000	500.000
25)	Chlordane-3	5.509	6.158	561.9E6	169.0E6	500.000	500.000
26)	Chlordane-4	5.568	6.232	456.5E6	207.1E6	500.000	500.000
27)	Chlordane-5	6.409	7.037	169.7E6	35748344	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 12:51
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 13:17:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:17:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

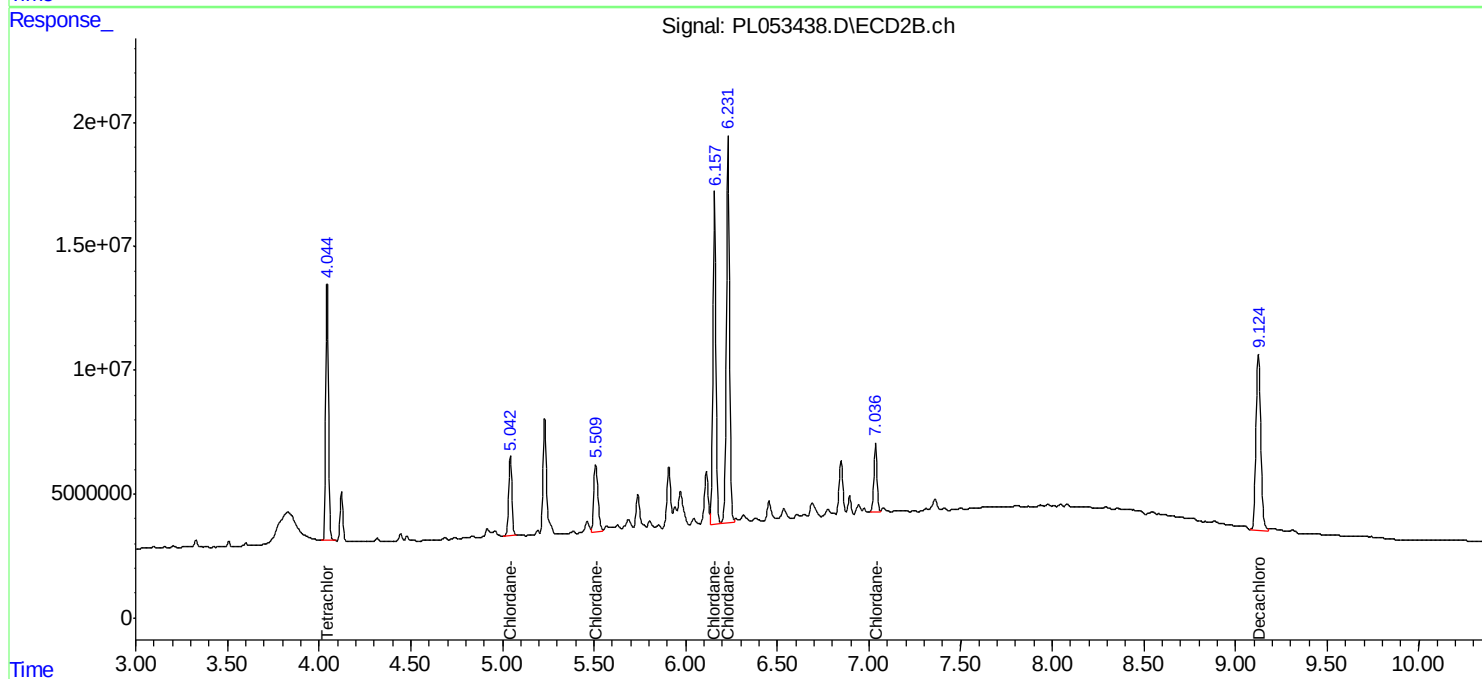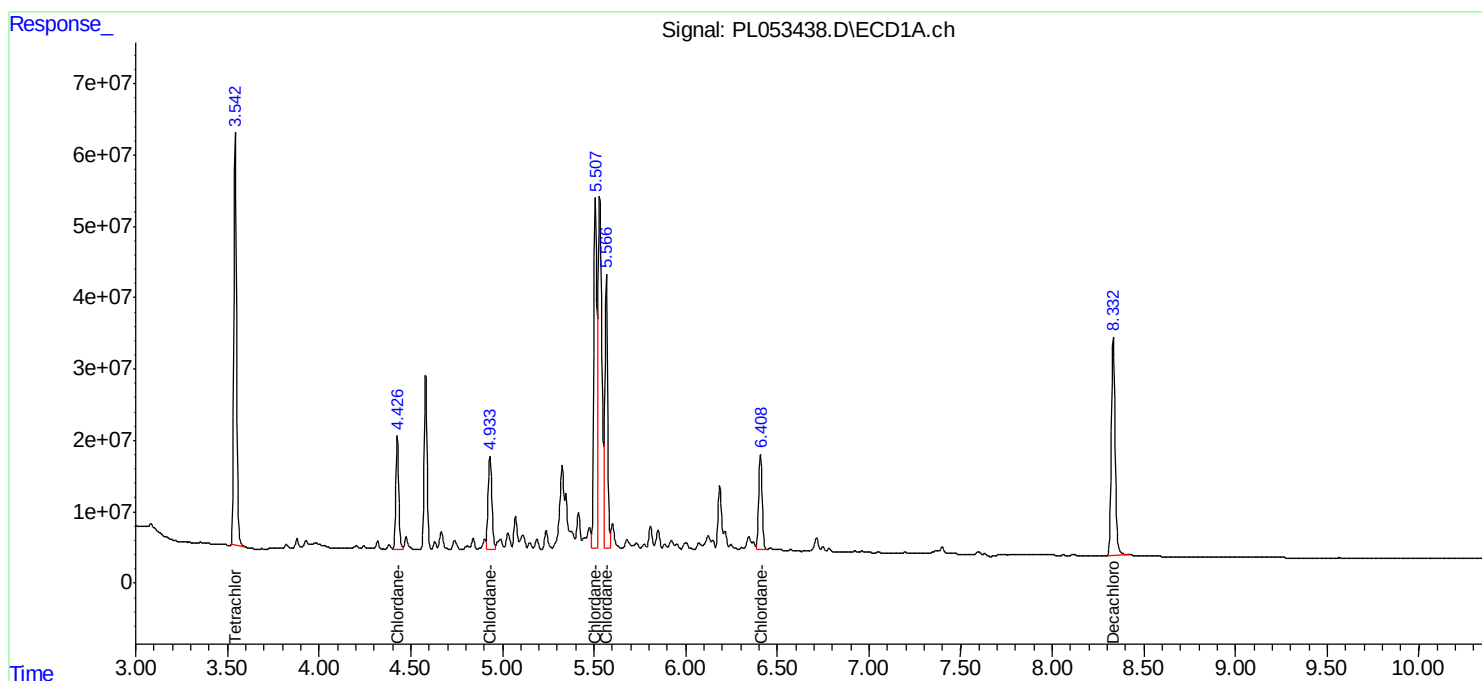


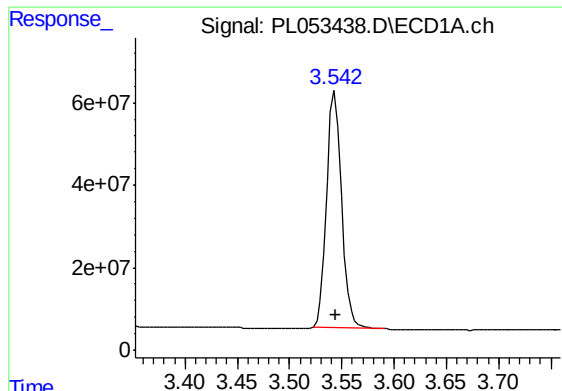

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 574268968
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

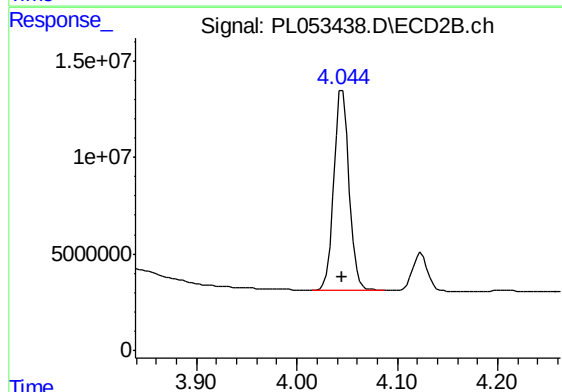


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 108931497
Conc: 50.00 ng/ml

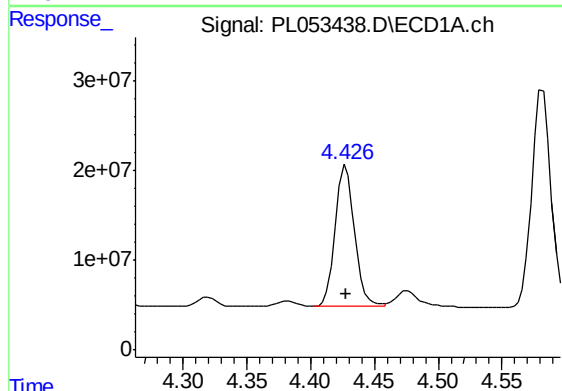


#23 Chlordane-1

R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 167370430
Conc: 500.00 ng/ml

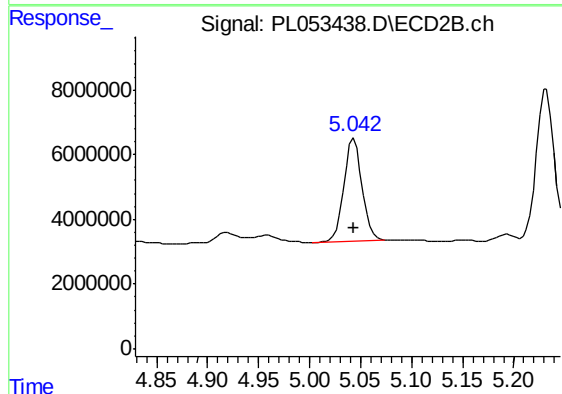

#23 Chlordane-1


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 38867951
Conc: 500.00 ng/ml

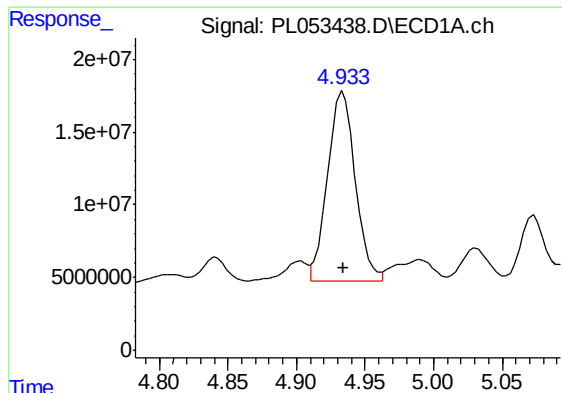

#24 Chlordane-2


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 183648628
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

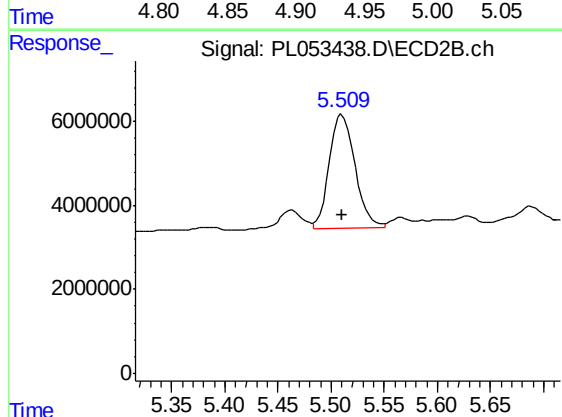


#24 Chlordane-2

R.T.: 5.510 min
Delta R.T.: 0.000 min
Response: 45515938
Conc: 500.00 ng/ml

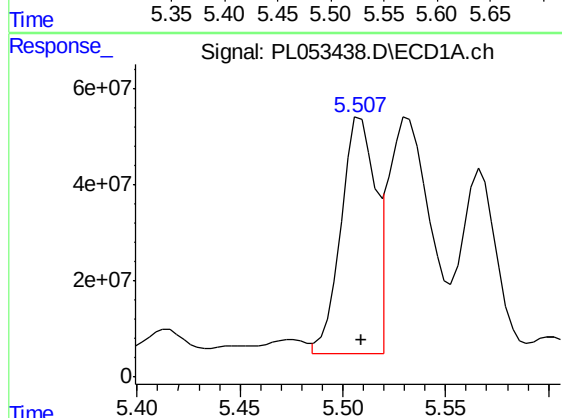


#25 Chlordane-3

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 561889154
Conc: 500.00 ng/ml

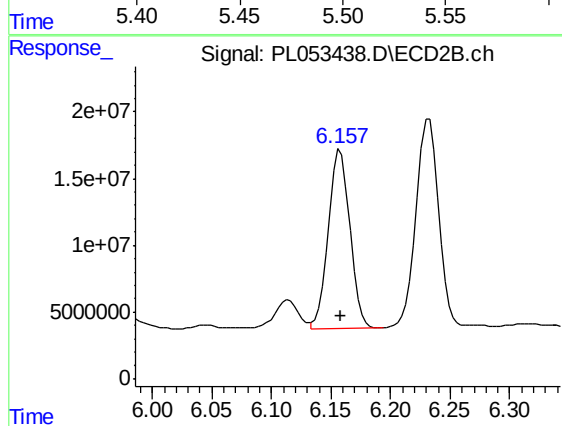

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 169012490
Conc: 500.00 ng/ml

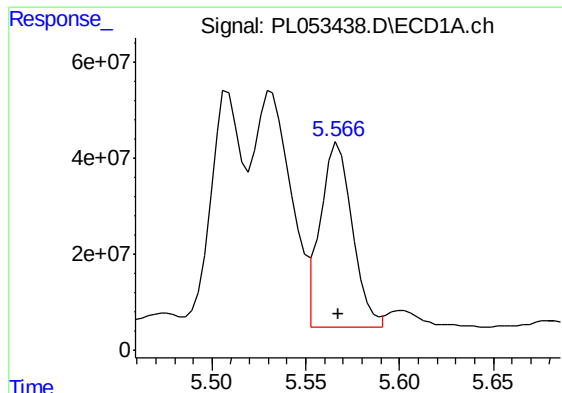

#26 Chlordane-4


R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 456525790
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

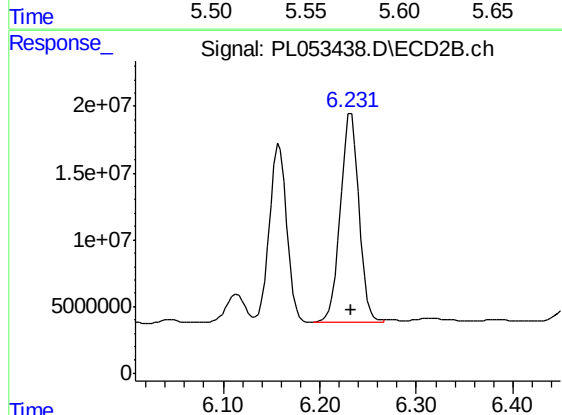


#26 Chlordane-4

R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 207121829
Conc: 500.00 ng/ml

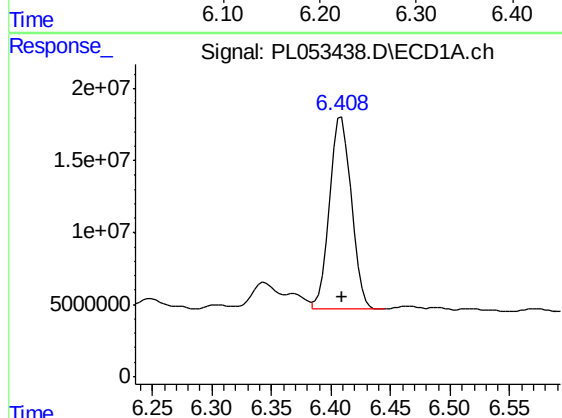


#27 Chlordane-5

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 169710220
Conc: 500.00 ng/ml

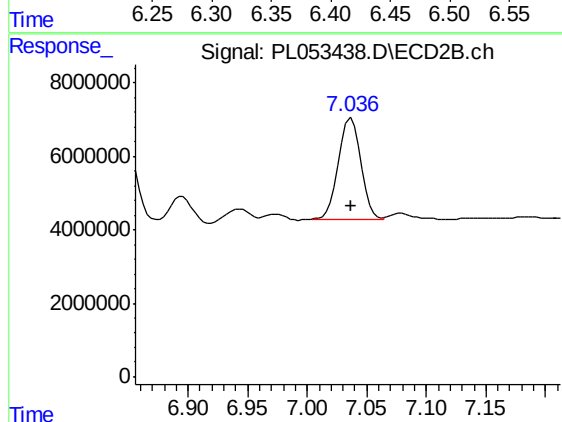

#27 Chlordane-5


R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 35748344
Conc: 500.00 ng/ml

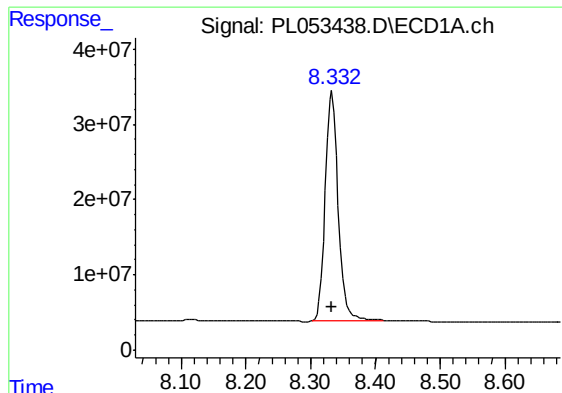

#28 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: 0.000 min
Response: 425918299
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

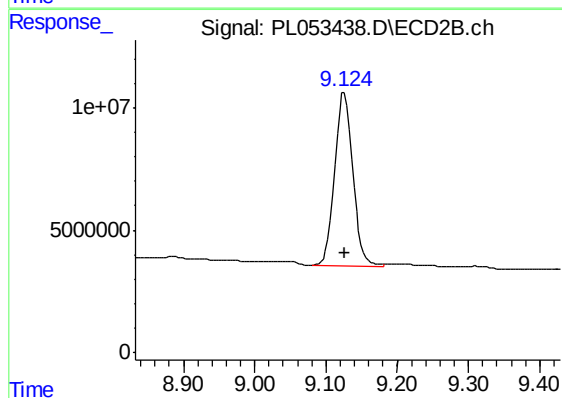

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 126119342
Conc: 50.00 ng/ml