

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2019 16:06
 Operator : SG\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL101919CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 00:04:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.046	578.2E6	109.1E6	53.340	43.607
28)	SA Decachlor...	8.333	9.126	438.8E6	122.2E6	44.724	43.396
Target Compounds							
23)	Chlordane-1	4.428	5.044	168.5E6	38636139	475.155	460.685
24)	Chlordane-2	4.934	5.511	183.8E6	45474187	476.991	462.976
25)	Chlordane-3	5.509	6.158	556.7E6	170.8E6	482.997	467.736
26)	Chlordane-4	5.568	6.233	457.6E6	209.0E6	488.103	465.573
27)	Chlordane-5	6.409	7.038	172.2E6	38383759	471.114	502.088



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2019 16:06
Operator : SG\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL101919CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 00:04:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

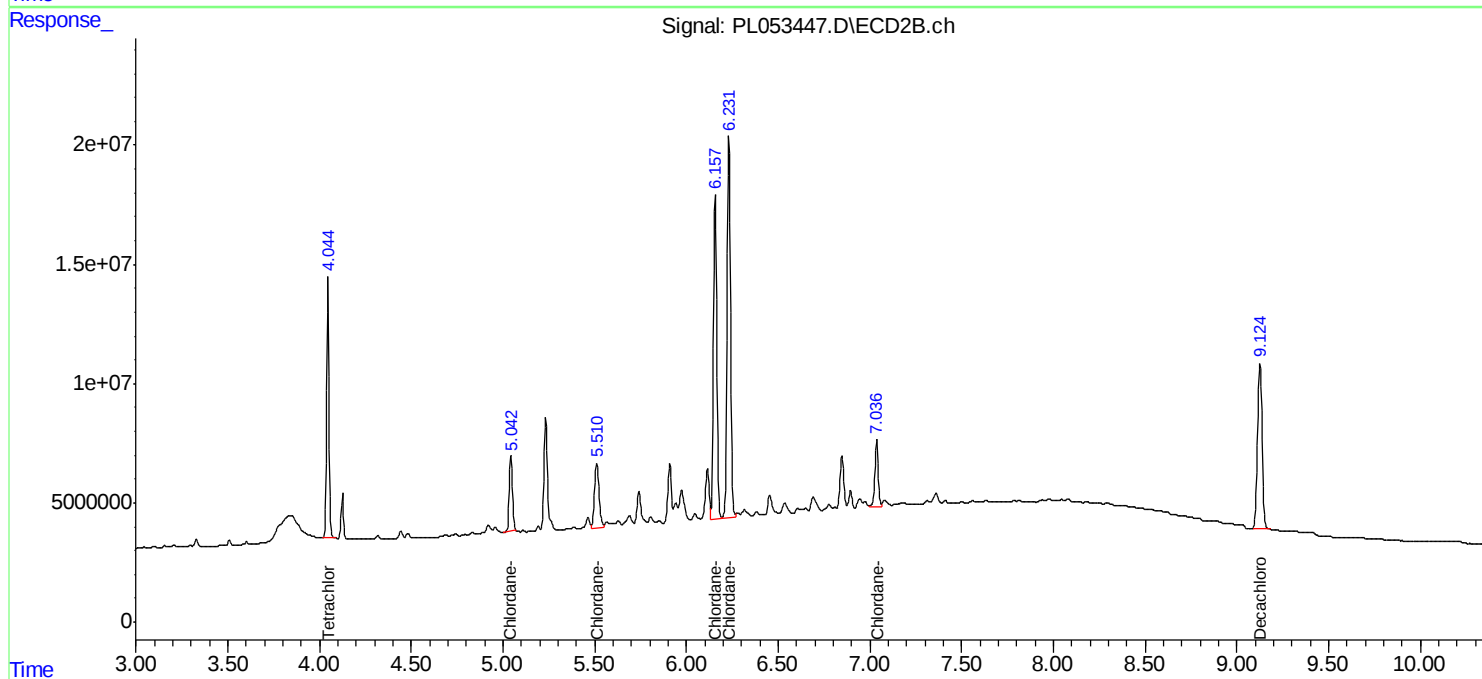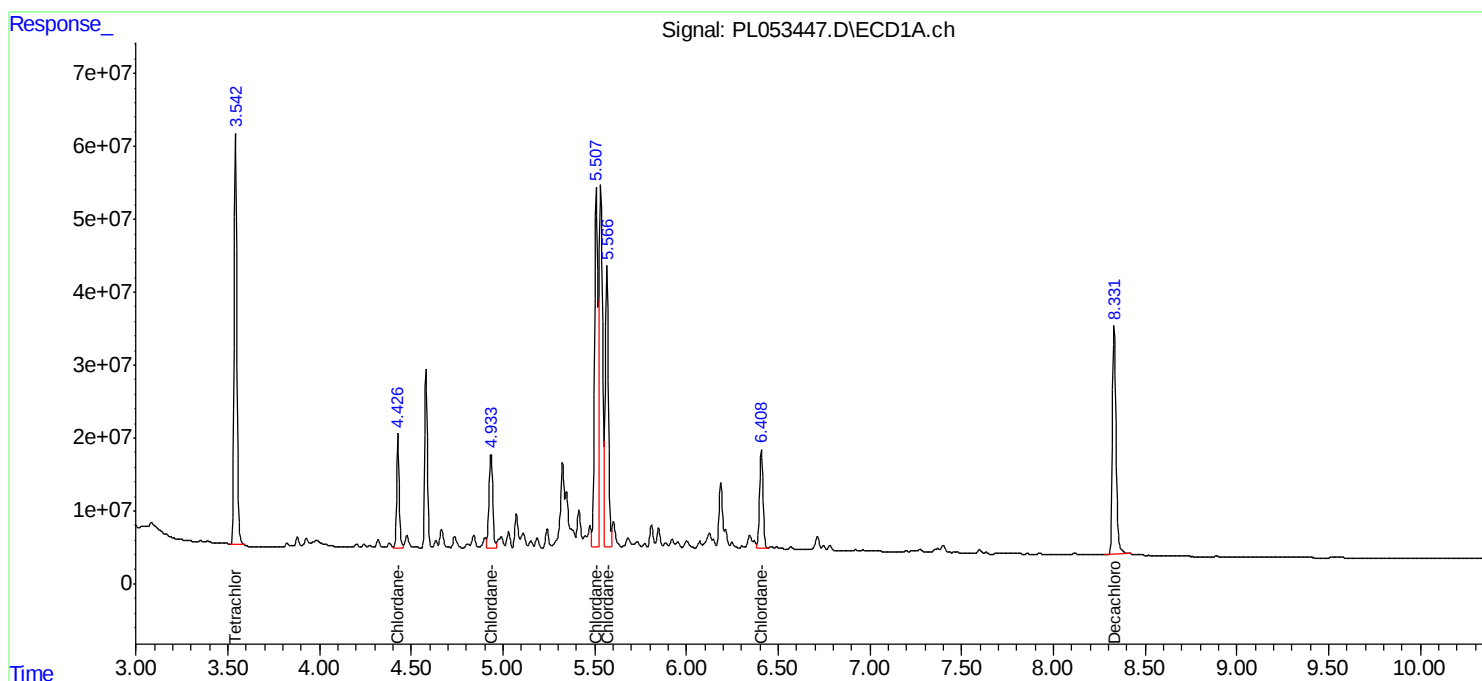


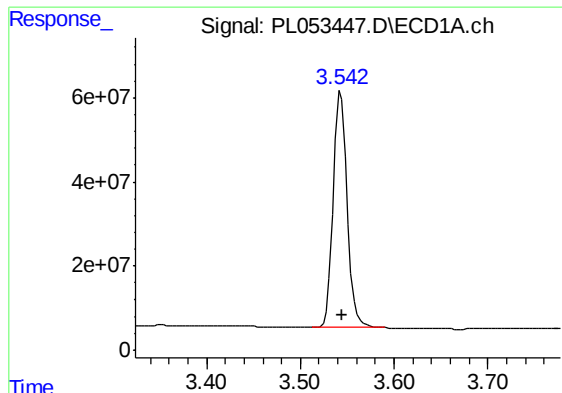

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 578171240
Conc: 53.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101919CHLOR

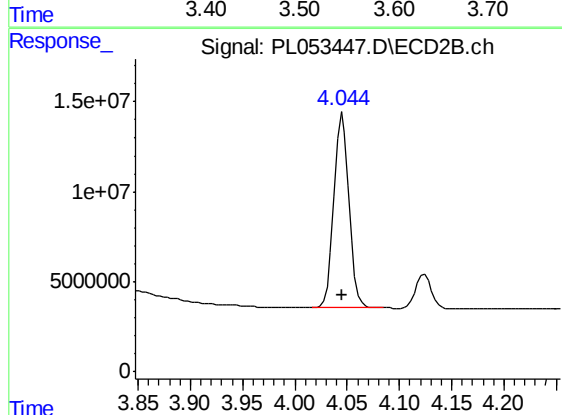


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 109122339
Conc: 43.61 ng/ml

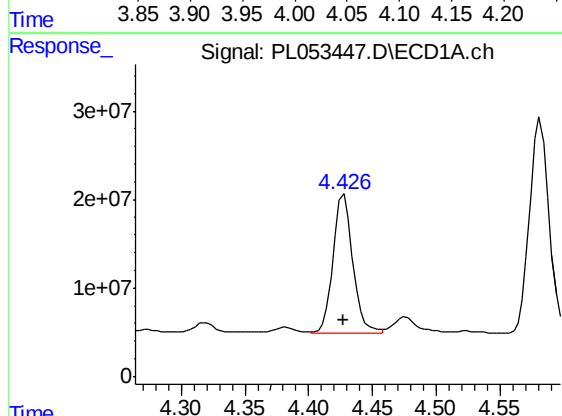


#23 Chlordane-1

R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 168523685
Conc: 475.15 ng/ml

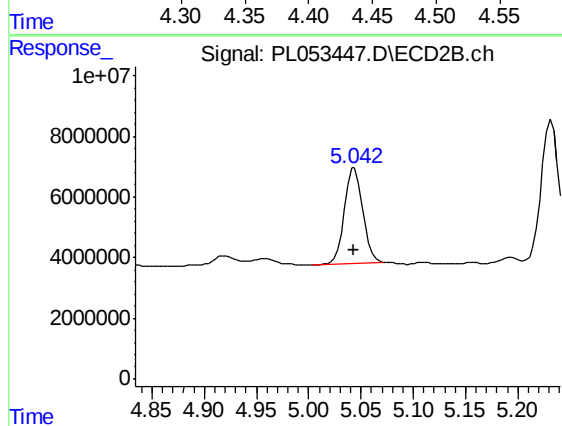

#23 Chlordane-1


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 38636139
Conc: 460.69 ng/ml

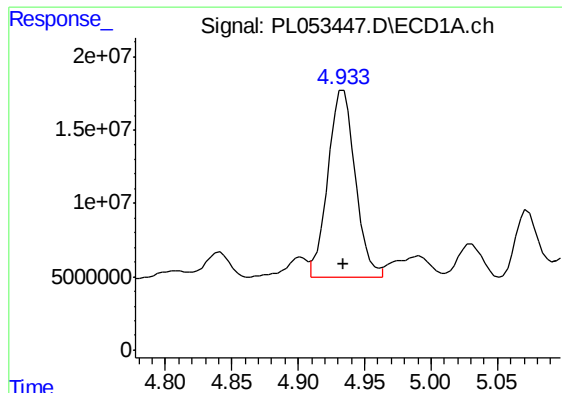

#24 Chlordane-2


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 183792011
Conc: 476.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101919CHLOR

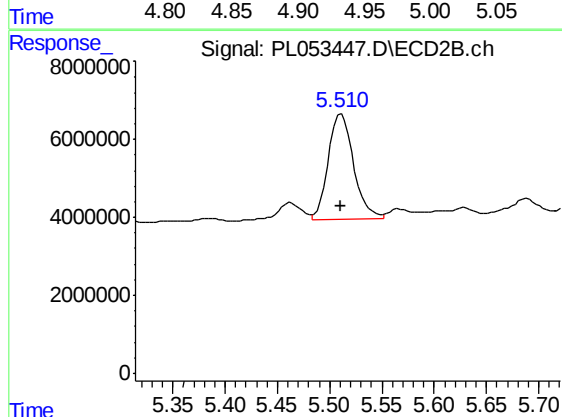


#24 Chlordane-2

R.T.: 5.511 min
Delta R.T.: 0.000 min
Response: 45474187
Conc: 462.98 ng/ml

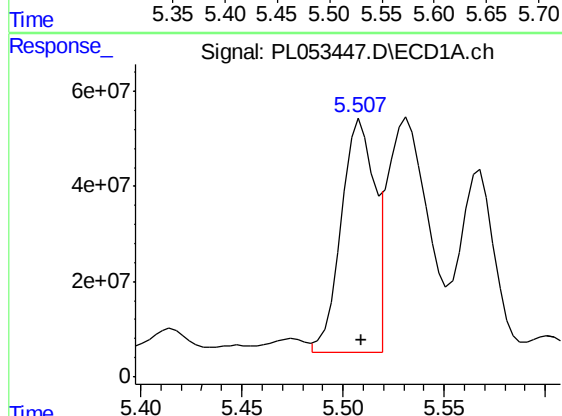


#25 Chlordane-3

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 556744203
Conc: 483.00 ng/ml

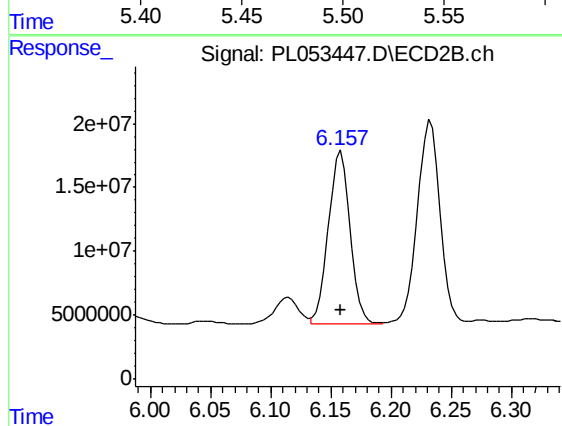

#25 Chlordane-3


R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 170831429
Conc: 467.74 ng/ml

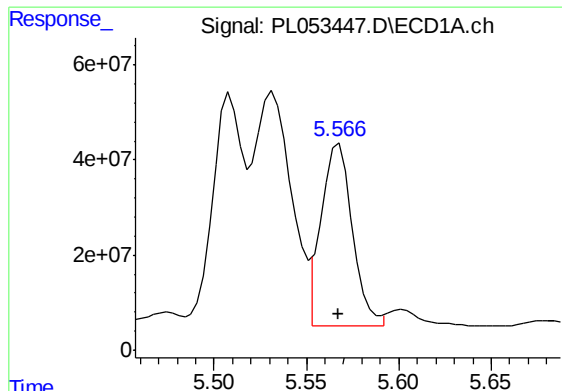

#26 Chlordane-4


R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 457572692
Conc: 488.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101919CHLOR

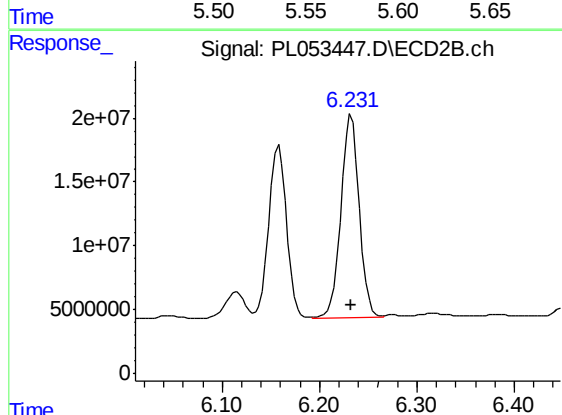


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 209012757
Conc: 465.57 ng/ml

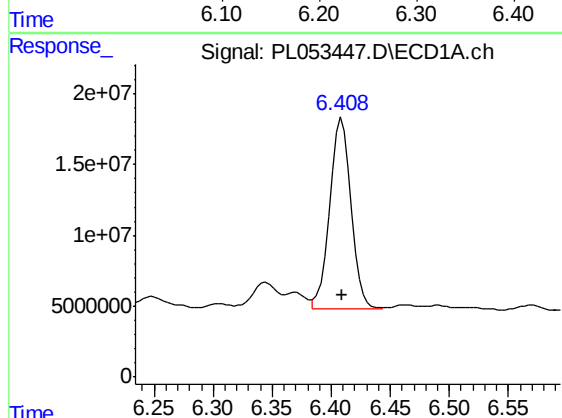


#27 Chlordane-5

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 172212997
Conc: 471.11 ng/ml

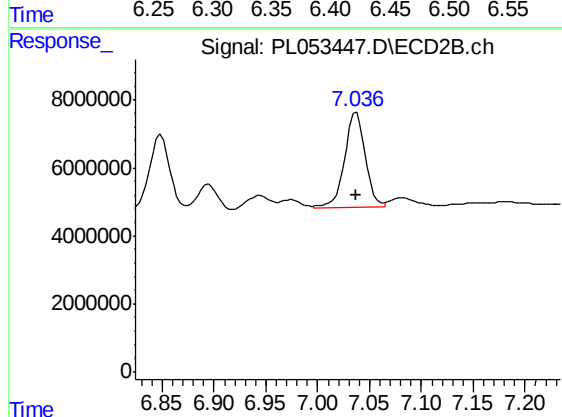

#27 Chlordane-5


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 38383759
Conc: 502.09 ng/ml

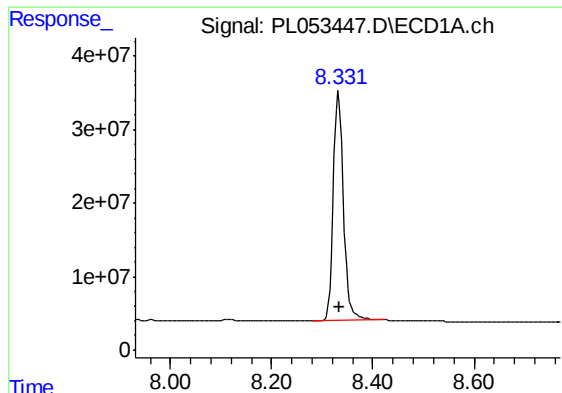

#28 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.001 min
Response: 438808669
Conc: 44.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL101919CHLOR

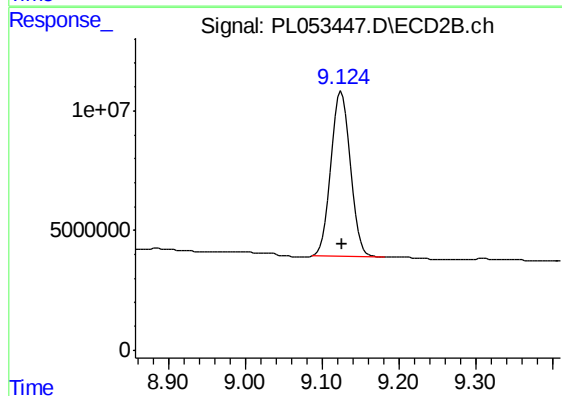

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 122203868
Conc: 43.40 ng/ml