

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
 Data File : PL053482.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2019 00:16
 Operator : SG\AJ
 Sample : K5420-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:44:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	4.046	198.7E6	47506827	18.333	18.985
28)	SA Decachlor...	8.331	9.125	149.4E6	43201230	15.224	15.341
Target Compounds							
15)	B Endosulfa...	6.407	6.977	454.5E6	132.2E6	40.656	51.763 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101919\
Data File : PL053482.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2019 00:16
Operator : SG\AJ
Sample : K5420-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:44:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

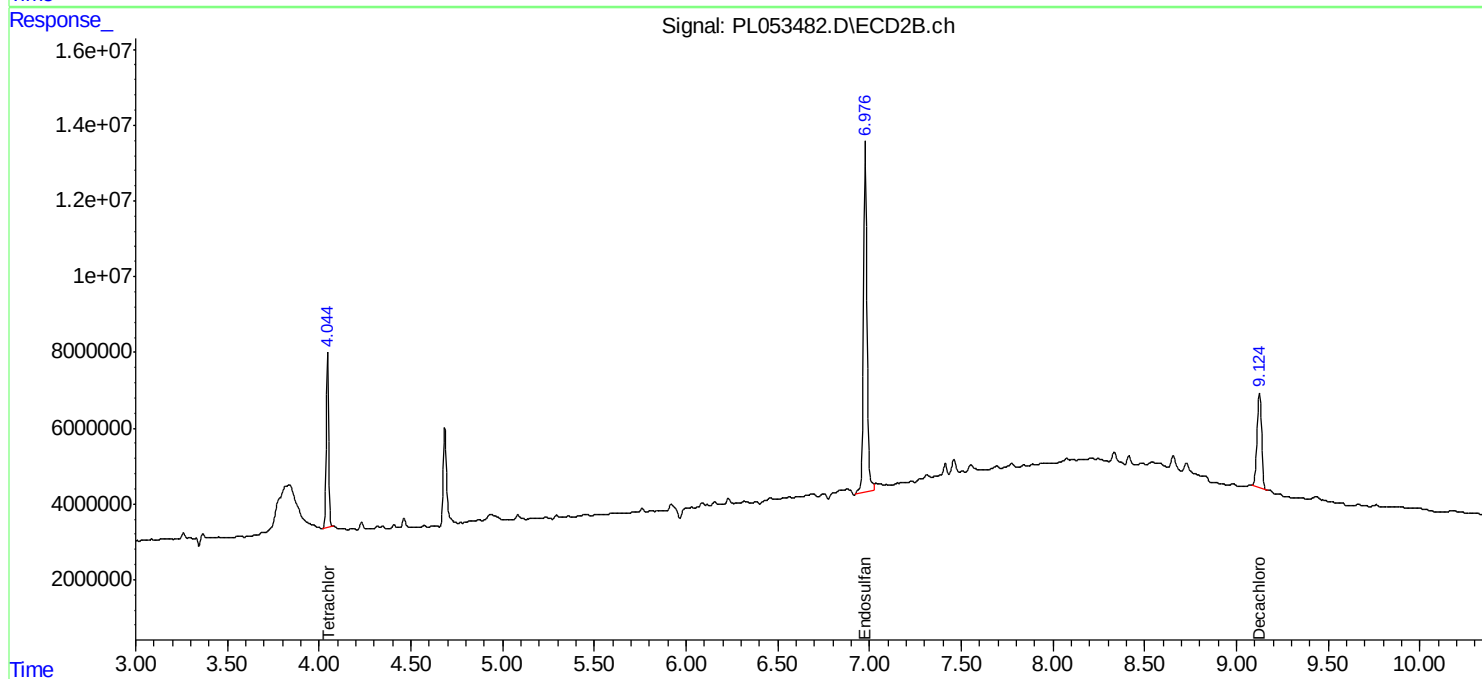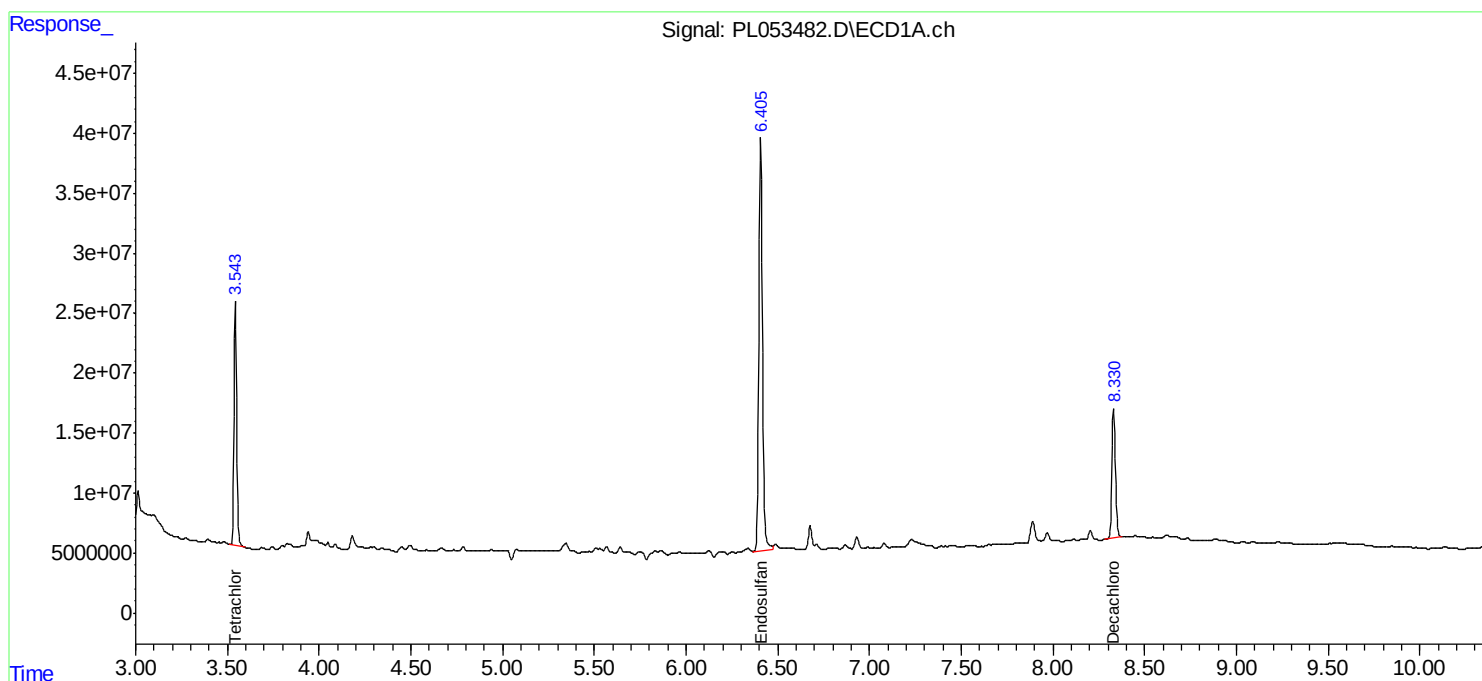


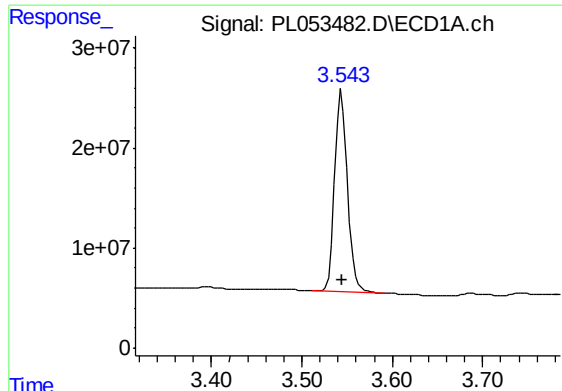

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 198721076
Conc: 18.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

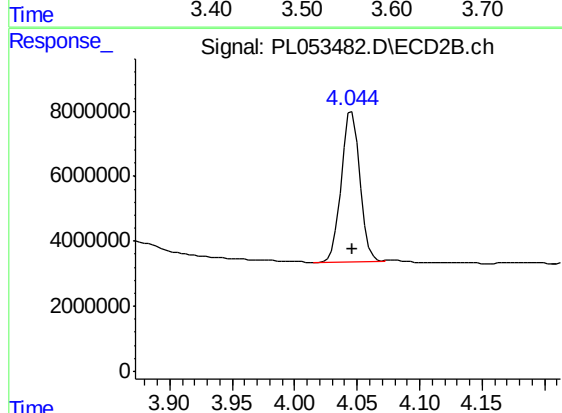


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 47506827
Conc: 18.98 ng/ml

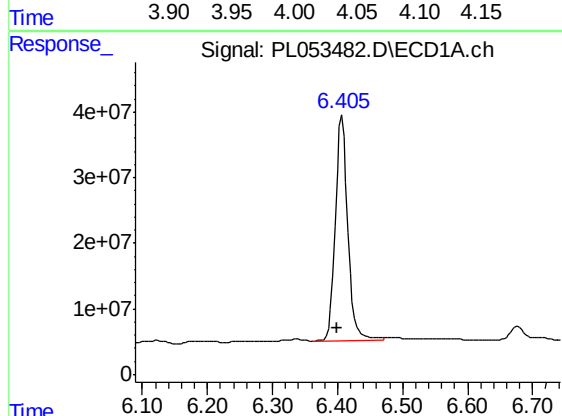


#15 Endosulfan II

R.T.: 6.407 min
Delta R.T.: 0.008 min
Response: 454548646
Conc: 40.66 ng/ml

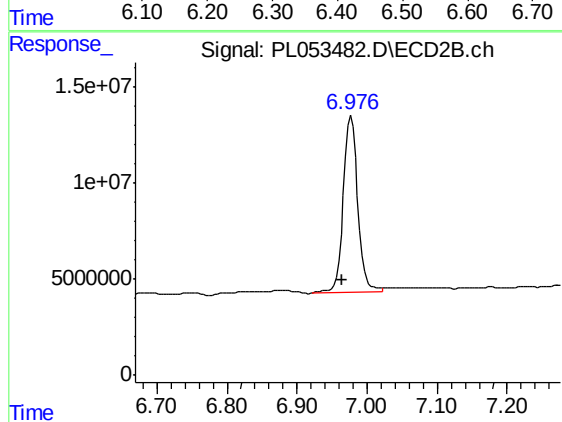

#15 Endosulfan II


R.T.: 6.977 min
Delta R.T.: 0.012 min
Response: 132227015
Conc: 51.76 ng/ml

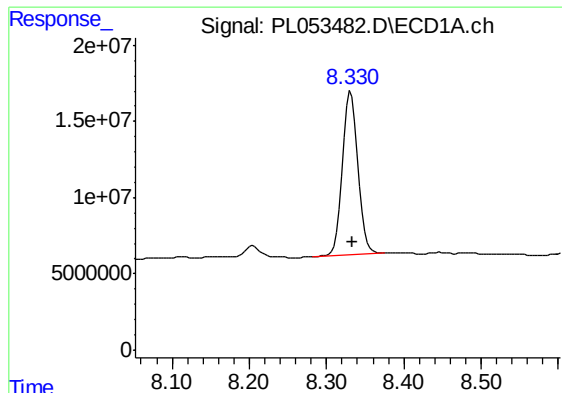

#28 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.003 min
Response: 149376034
Conc: 15.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

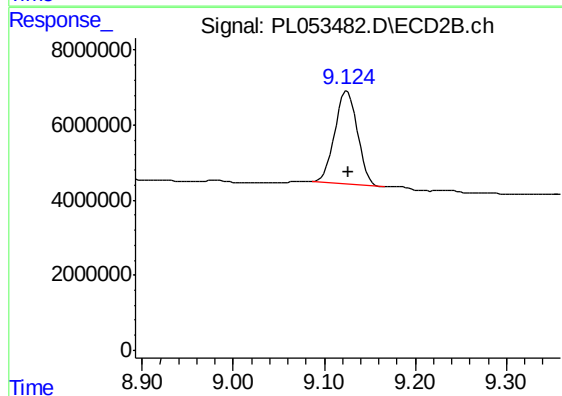

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: -0.001 min
Response: 43201230
Conc: 15.34 ng/ml