

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL101920\  
 Data File : PL062418.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Oct 2020 10:11  
 Operator : DD\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 20 07:02:03 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL101920.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Oct 20 07:00:50 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |       |         |   |       |        |
|------------------|--------------|--------|-------|---------|---|-------|--------|
| 18) B            | Endrin al... | 6.381  | 0.000 | 2670033 | 0 | 1.881 | N.D. # |
| 22)              | Mirex        | 7.275f | 0.000 | 1067435 | 0 | 0.727 | N.D. # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL101920\  
Data File : PL062418.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Oct 2020 10:11  
Operator : DD\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 20 07:02:03 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL101920.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 20 07:00:50 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

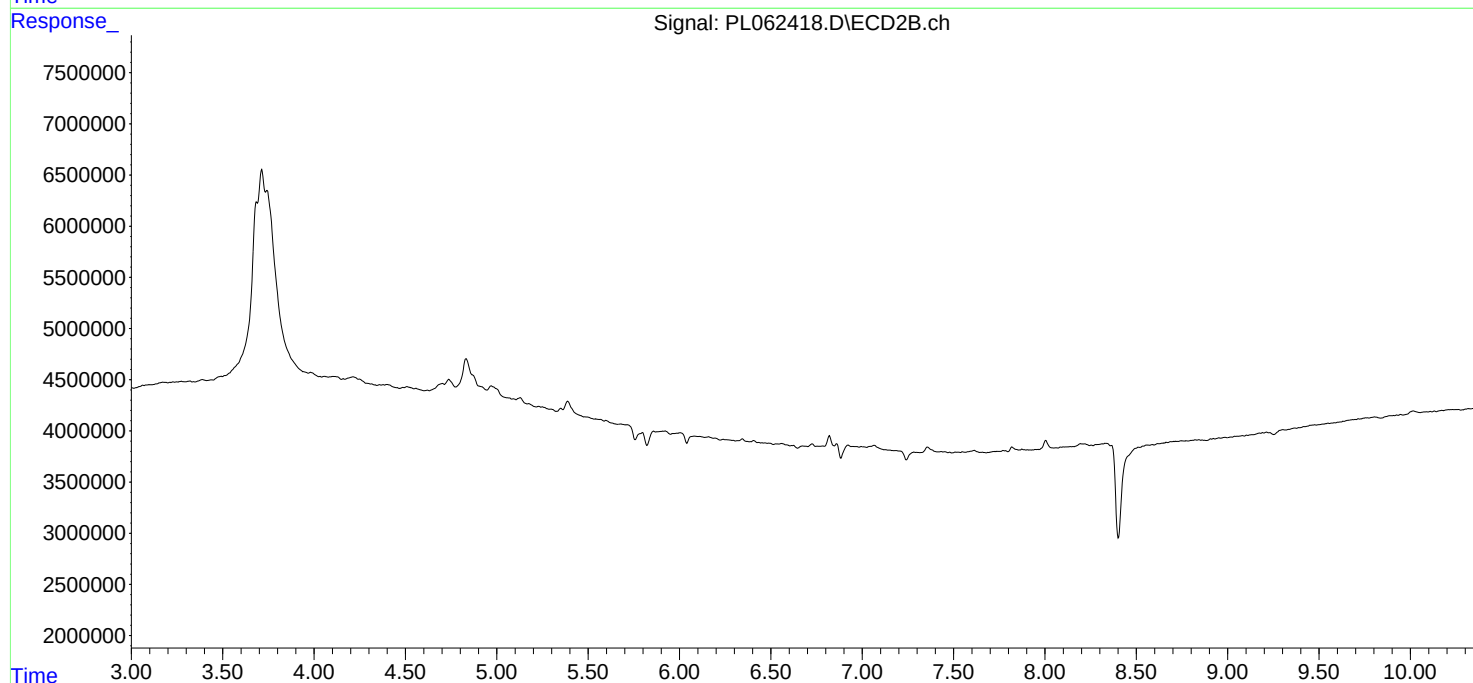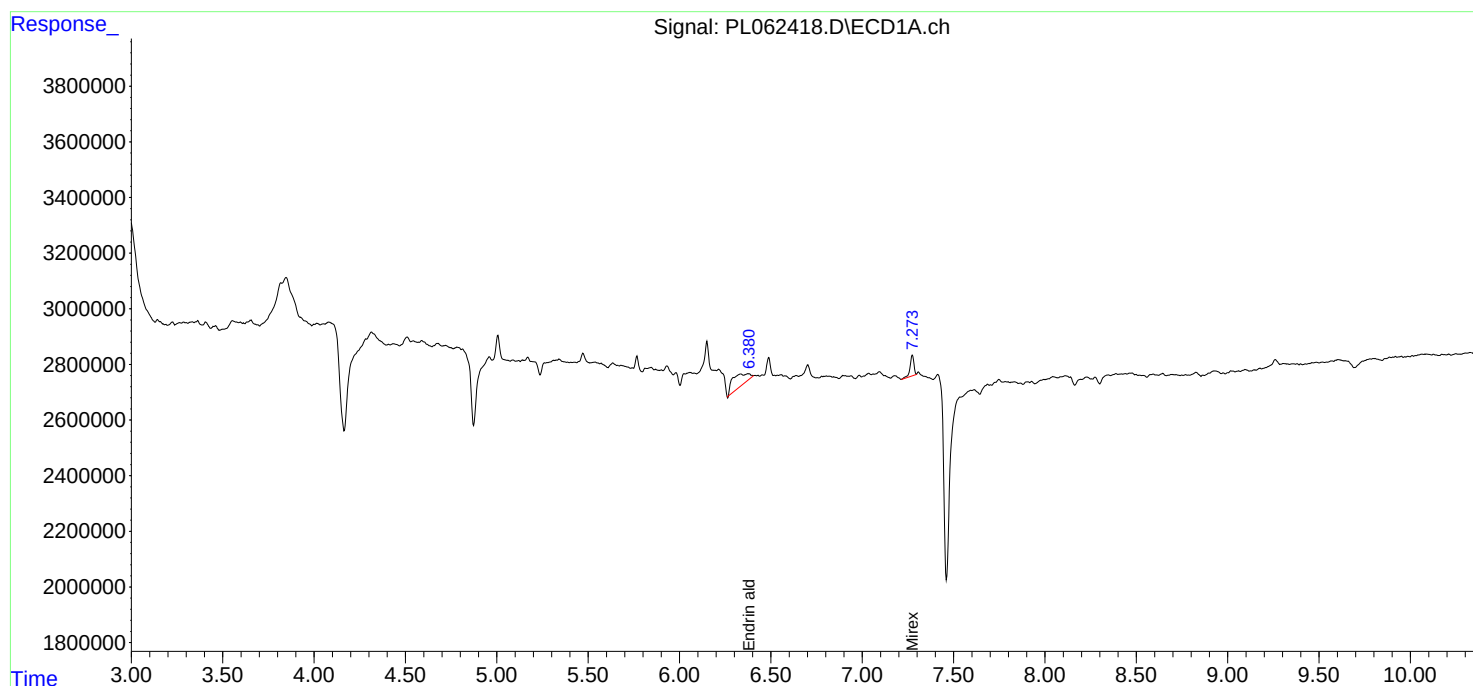


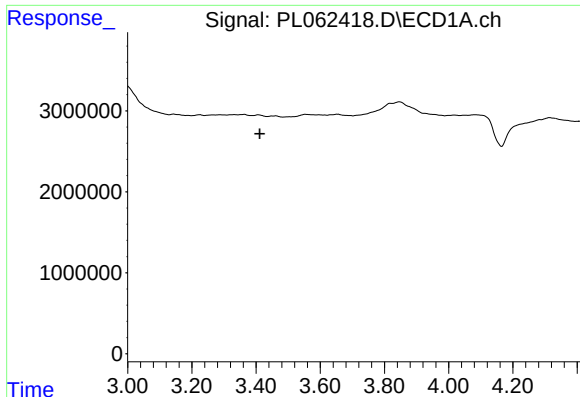

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.411 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

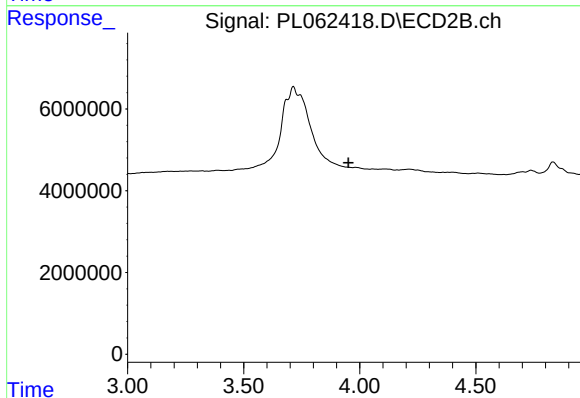


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.951 min  
Response: 0  
Conc: N.D.

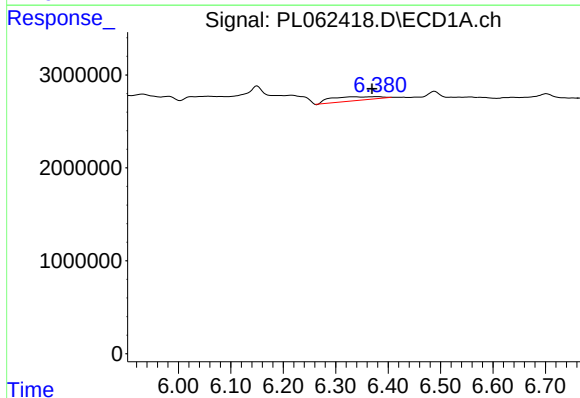


#18 Endrin aldehyde

R.T.: 6.381 min  
Delta R.T.: 0.012 min  
Response: 2670033  
Conc: 1.88 ng/ml

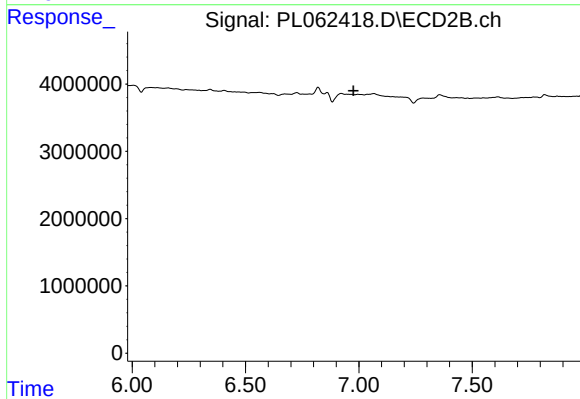

#18 Endrin aldehyde


R.T.: 0.000 min  
Exp R.T. : 6.976 min  
Response: 0  
Conc: N.D.

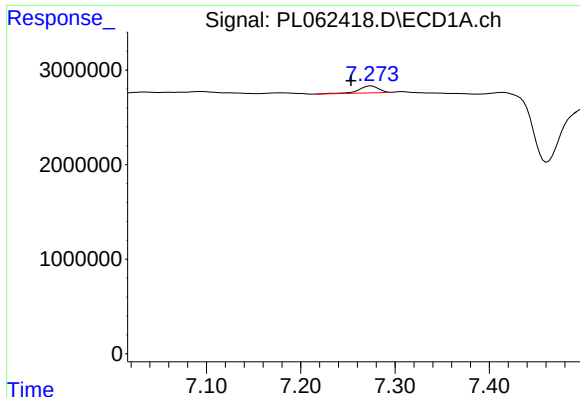

#22 Mirex


R.T.: 7.275 min  
Delta R.T.: 0.021 min  
Response: 1067435  
Conc: 0.73 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

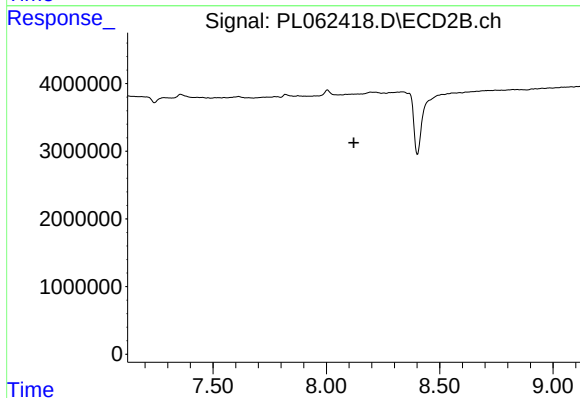


#22 Mirex

R.T.: 0.000 min  
Exp R.T. : 8.121 min  
Response: 0  
Conc: N.D.

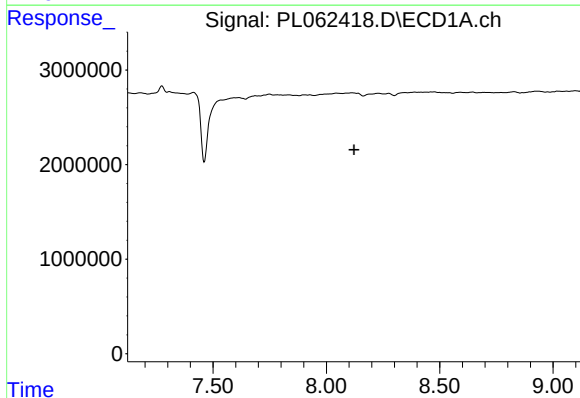

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.122 min  
Response: 0  
Conc: N.D.

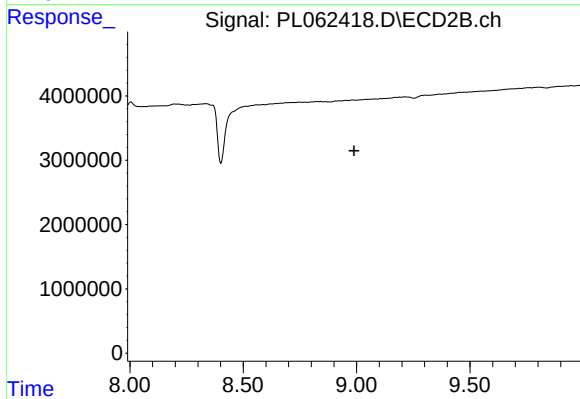

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.989 min  
Response: 0  
Conc: N.D.