

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101920\
 Data File : PL062423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 13:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 07:03:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	38004172	51381172	22.058	22.307
28)	SA Decachlor...	8.122	8.989	39912445	44829429	22.738	22.608
Target Compounds							
23)	Chlordane-1	4.296f	0.000	1349731	0	26.249	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101920\
Data File : PL062423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 13:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 07:03:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

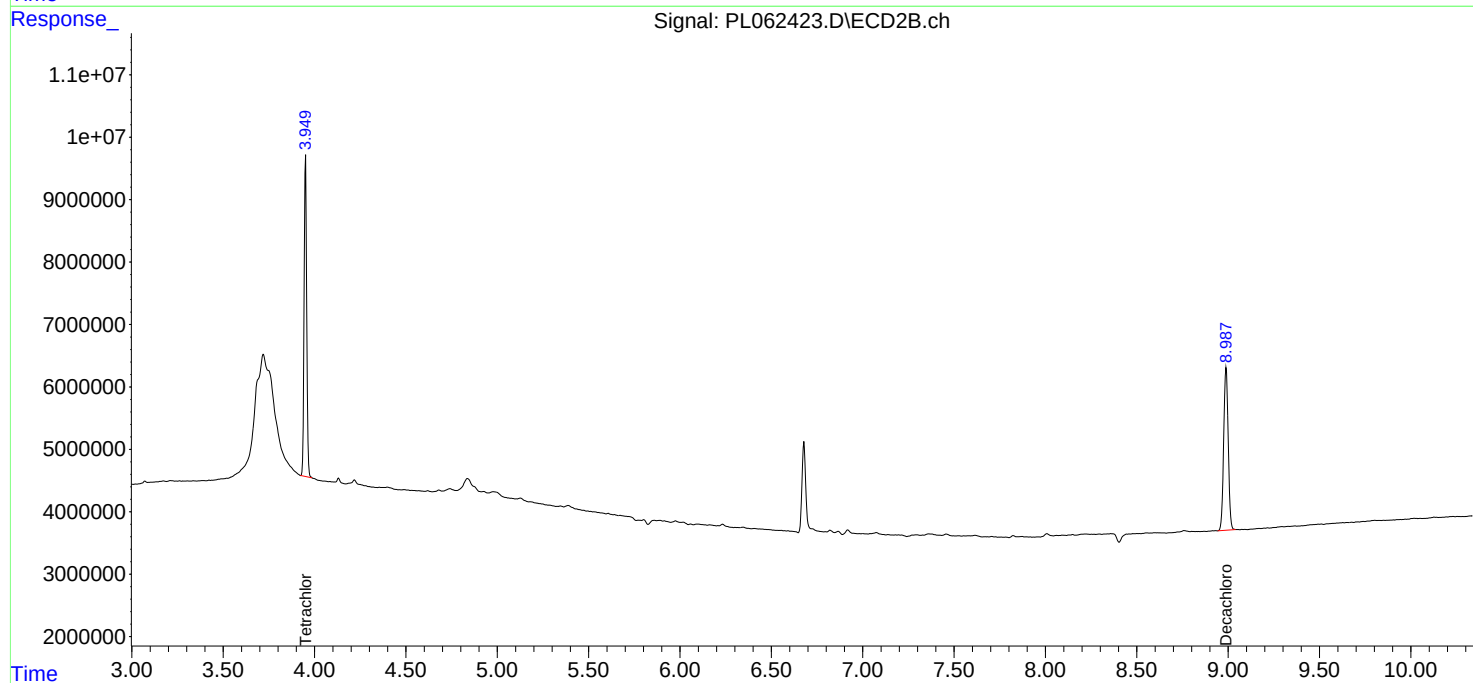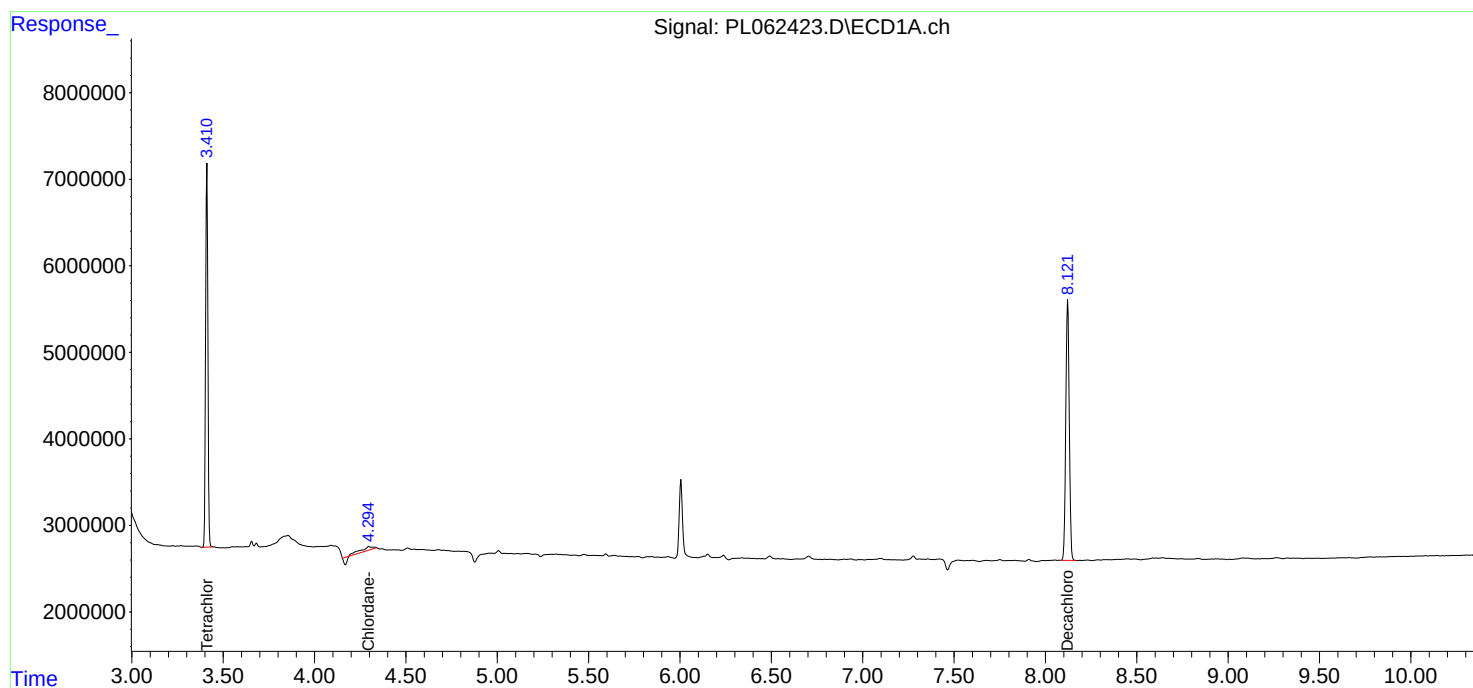


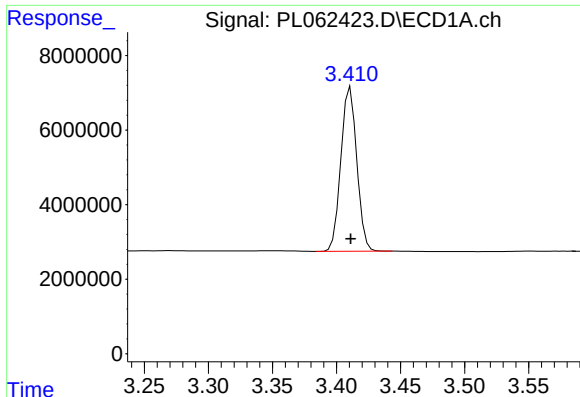

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 38004172
Conc: 22.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

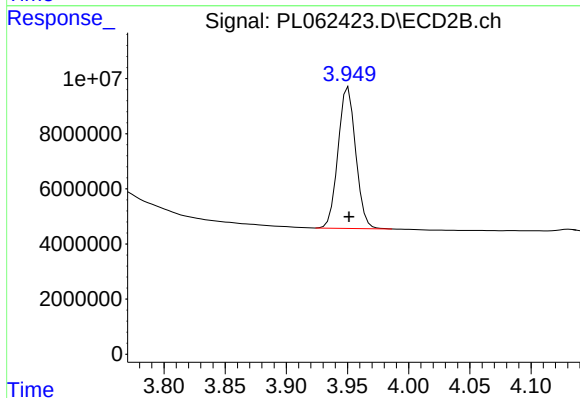


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 51381172
Conc: 22.31 ng/ml

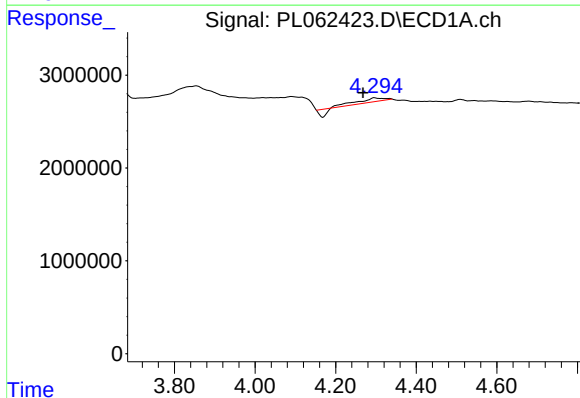


#23 Chlordane-1

R.T.: 4.296 min
Delta R.T.: 0.029 min
Response: 1349731
Conc: 26.25 ng/ml

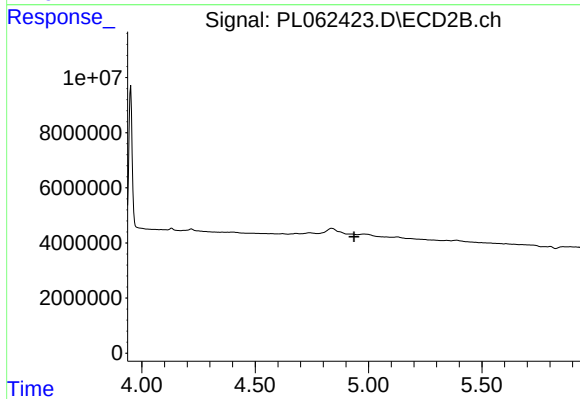

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.937 min
Response: 0
Conc: N.D.

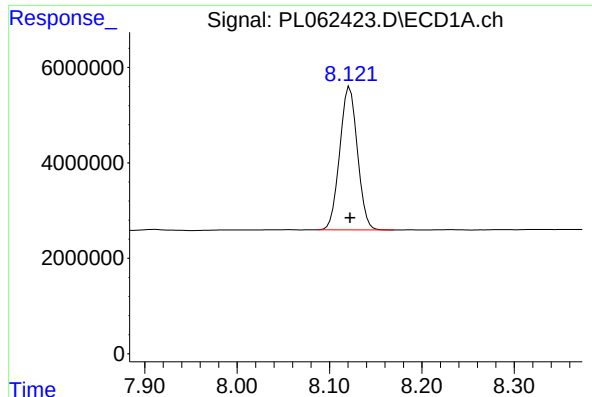

#28 Decachlorobiphenyl

R.T.: 8.122 min
Delta R.T.: 0.000 min
Response: 39912445
Conc: 22.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

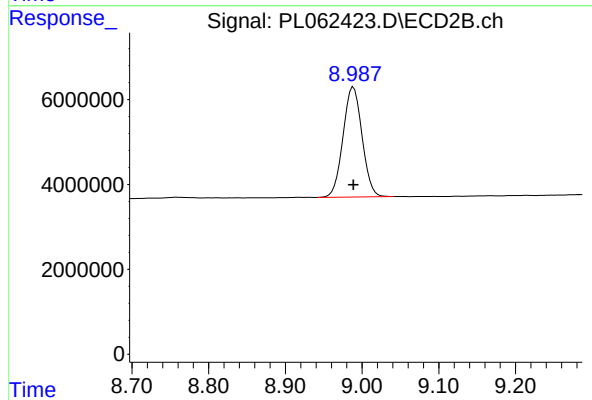

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 44829429
Conc: 22.61 ng/ml