

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL101920\  
 Data File : PL062423.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Oct 2020 13:44  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 20 07:03:02 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL101920.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Oct 20 07:00:50 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.411  | 3.951 | 38004172 | 51381172 | 22.058 | 22.307 |
| 28)                         | SA Decachlor... | 8.122  | 8.989 | 39912445 | 44829429 | 22.738 | 22.608 |
| Target Compounds            |                 |        |       |          |          |        |        |
| 23)                         | Chlordane-1     | 4.296f | 0.000 | 1349731  | 0        | 26.249 | N.D. # |
| -----                       |                 |        |       |          |          |        |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL101920\  
Data File : PL062423.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Oct 2020 13:44  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 20 07:03:02 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL101920.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 20 07:00:50 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

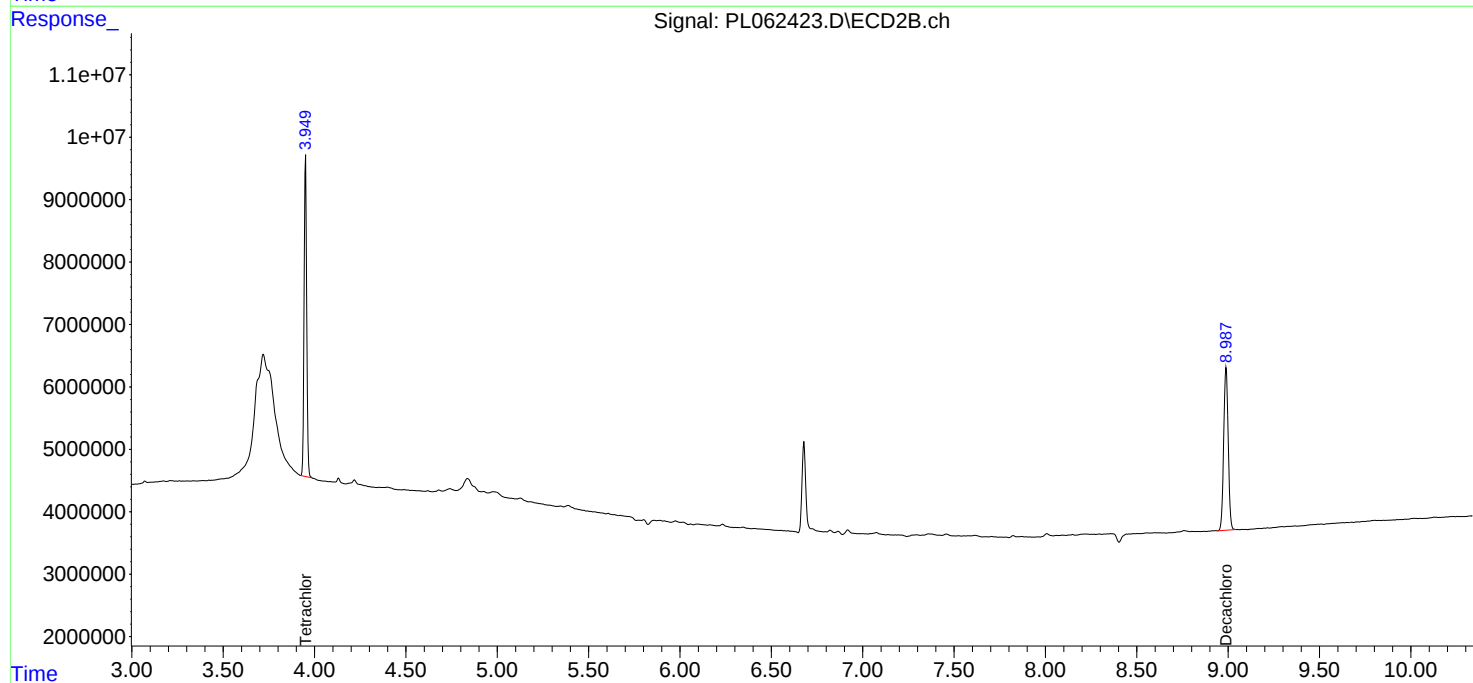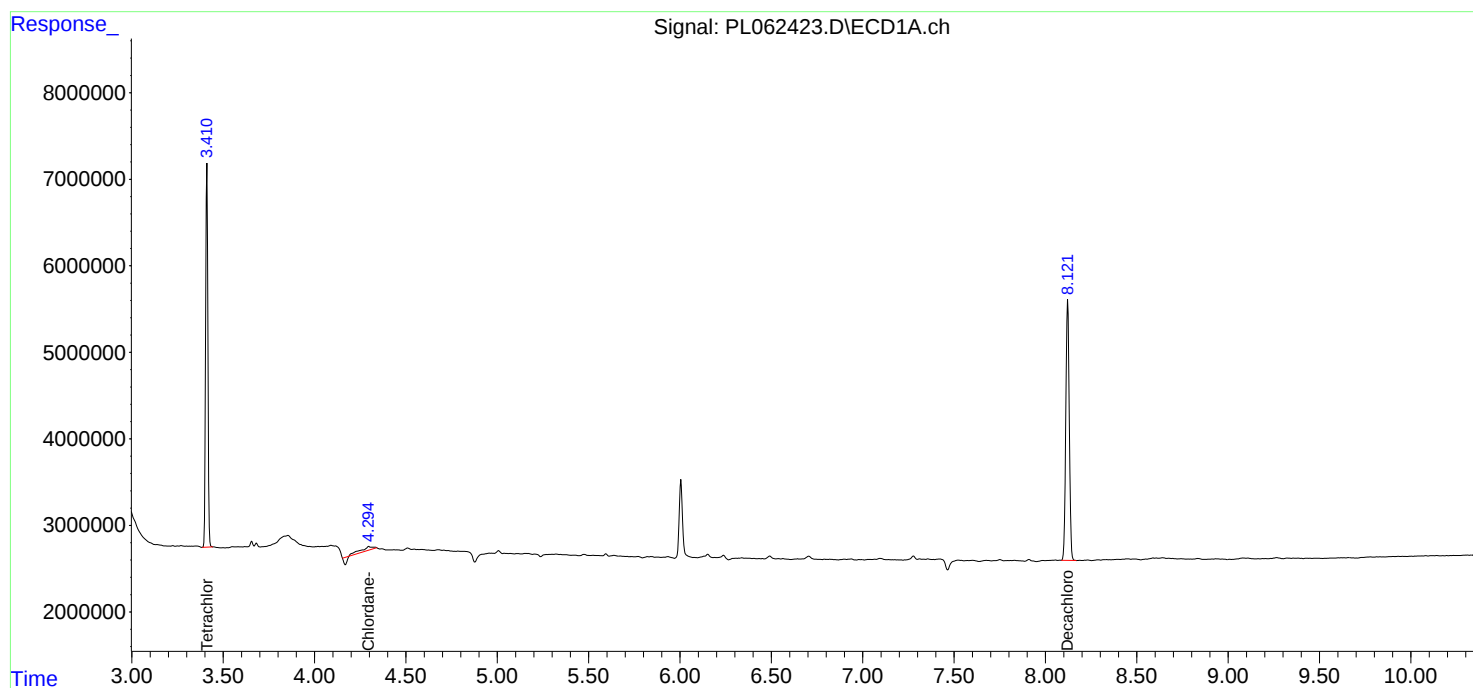


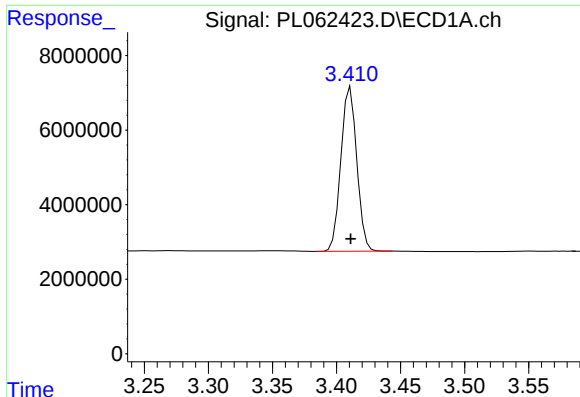

#1 Tetrachloro-m-xylene


R.T.: 3.411 min  
Delta R.T.: 0.000 min  
Response: 38004172  
Conc: 22.06 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

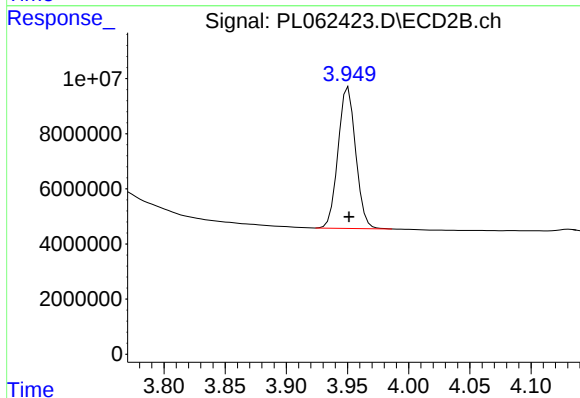


#1 Tetrachloro-m-xylene

R.T.: 3.951 min  
Delta R.T.: 0.000 min  
Response: 51381172  
Conc: 22.31 ng/ml

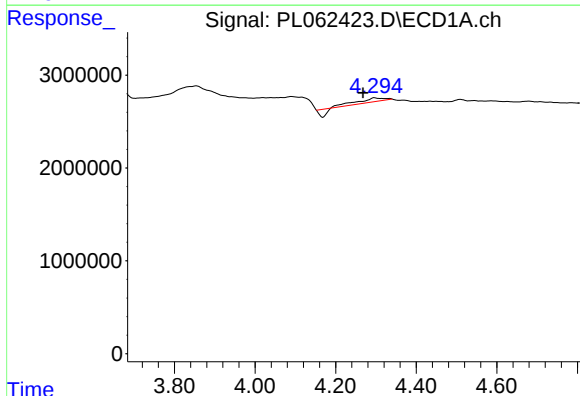


#23 Chlordane-1

R.T.: 4.296 min  
Delta R.T.: 0.029 min  
Response: 1349731  
Conc: 26.25 ng/ml

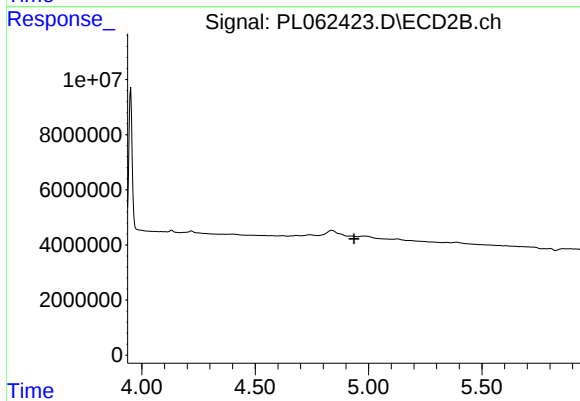

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T.: 4.937 min  
Response: 0  
Conc: N.D.

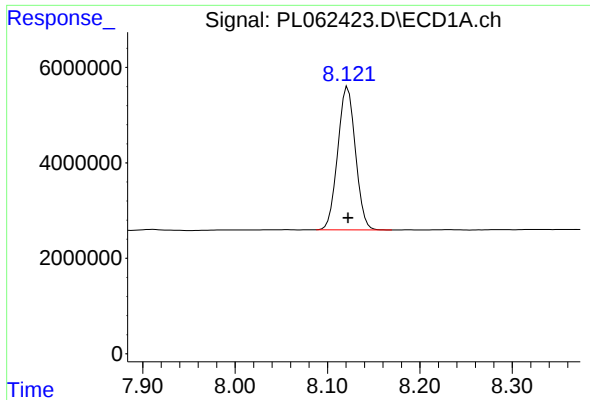

#28 Decachlorobiphenyl

R.T.: 8.122 min  
Delta R.T.: 0.000 min  
Response: 39912445  
Conc: 22.74 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
I.BLK

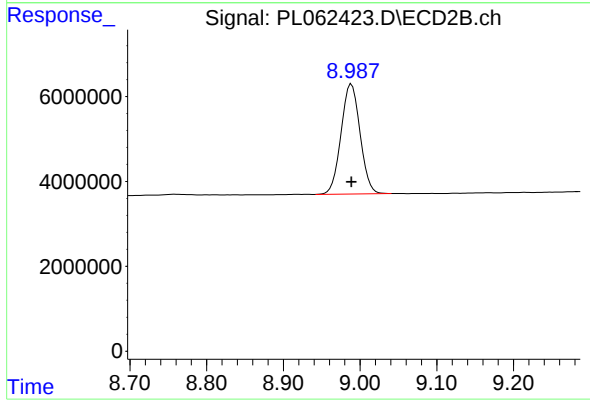

#28 Decachlorobiphenyl

R.T.: 8.989 min  
Delta R.T.: 0.000 min  
Response: 44829429  
Conc: 22.61 ng/ml