

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101920\
 Data File : PL062425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 14:12
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 07:03:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	46854157	62166164	27.194	26.990
28)	SA Decachlor...	8.121	8.990	47487441	53628156	27.053	27.046
Target Compounds							
7)	B delta-BHC	0.000	4.984f	0	2299901	N.D.	0.881 #
9)	A Endosulfan I	5.436	6.169	20874302	30654331	12.759	12.680
10)	B gamma-Chl...	5.326	6.048	23412513	30892356	13.294	12.197
12)	B 4,4'-DDE	5.548	6.279	40853806	61014300	25.289	25.108
13)	MA Dieldrin	5.676	6.426	44016221	62386883	25.601	25.432
19)	B Endosulfa...	6.581	7.199	40958885	51579529	25.491	25.134
20)	A Methoxychlor	6.841	7.526	110.0E6	139.1E6	129.576	125.357
21)	B Endrin ke...	7.066	7.668	48136374	54276248	25.994	25.505
22)	Mirex	7.277f	0.000	3651832	0	2.487	N.D. #
23)	Chlordane-1	4.269	0.000	772936	0	15.032	N.D. #
25)	Chlordane-3	5.326	6.048	23412513	30892356	160.278	101.609 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101920\
Data File : PL062425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 14:12
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 07:03:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

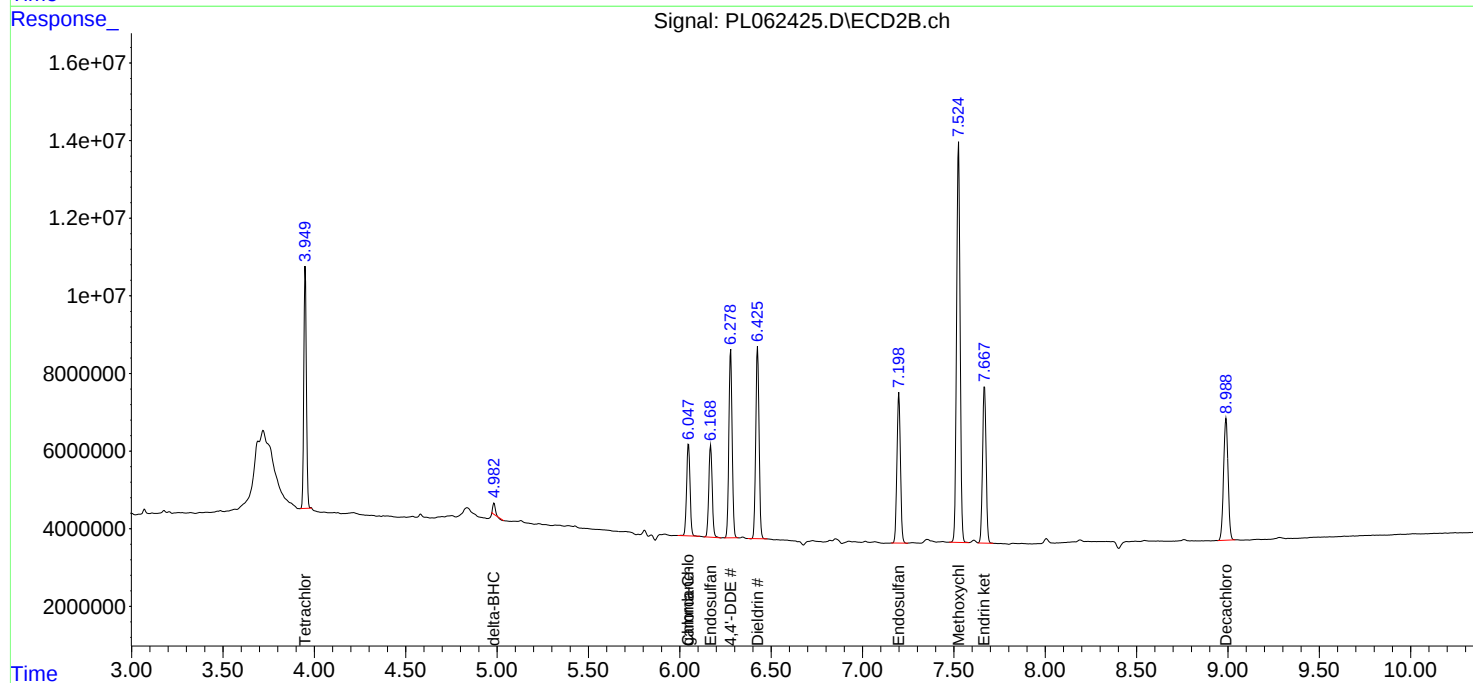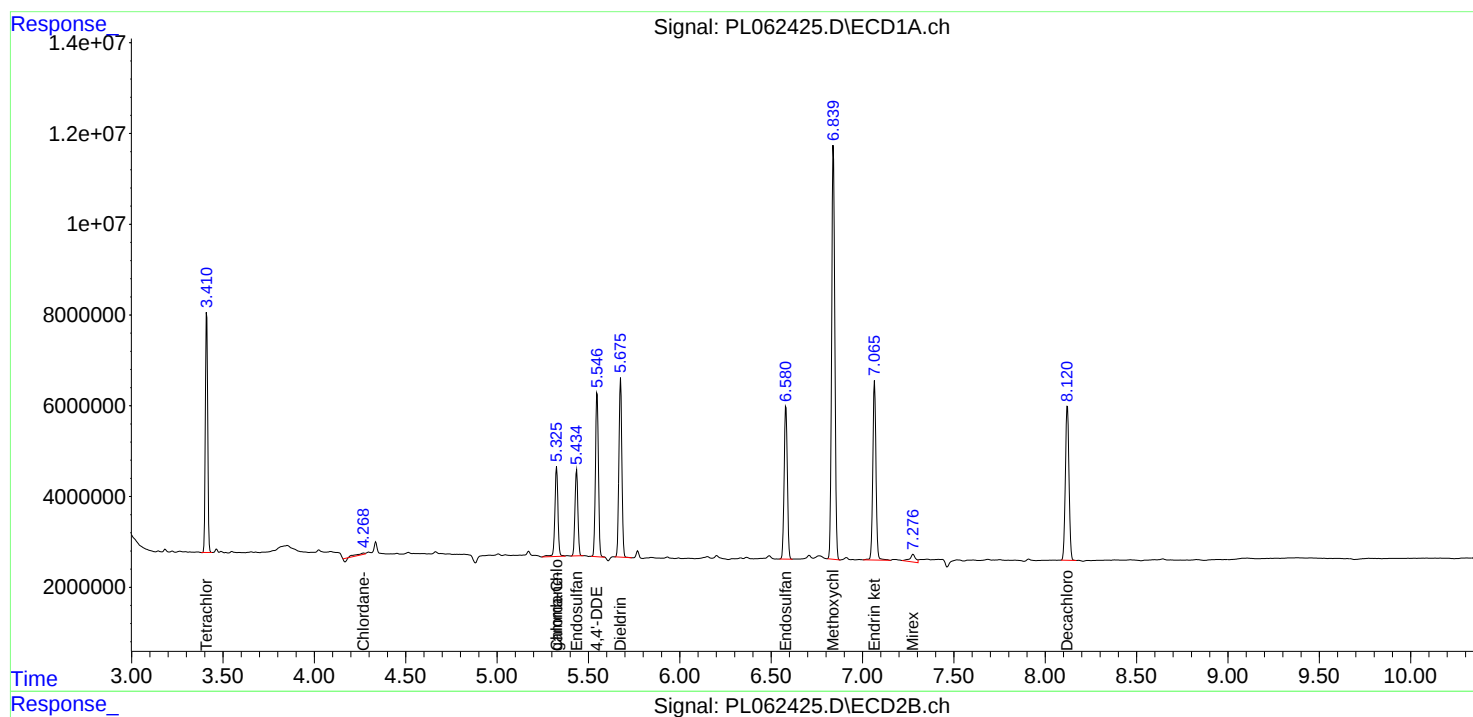


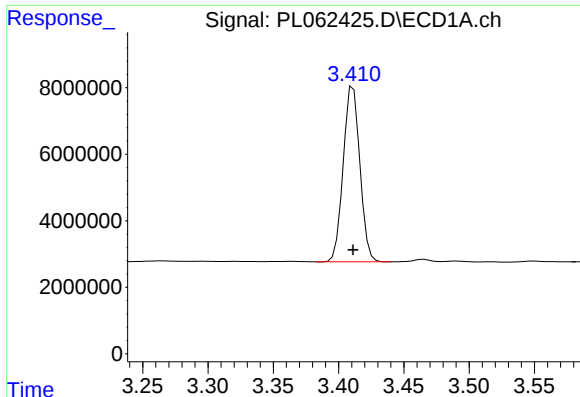

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 46854157
Conc: 27.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

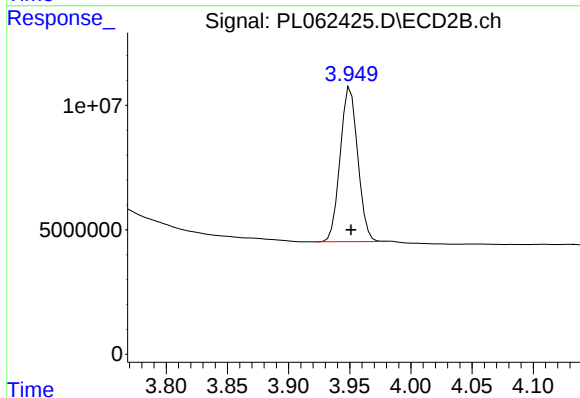


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 62166164
Conc: 26.99 ng/ml

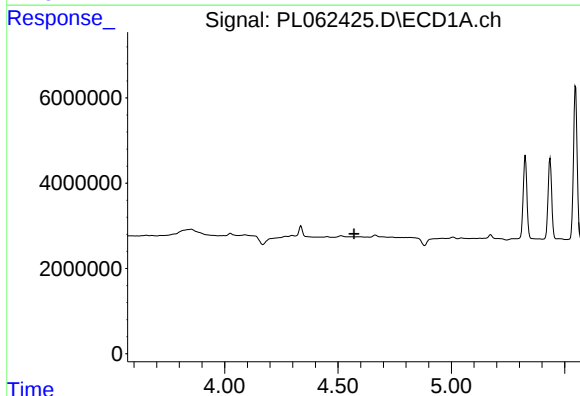


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

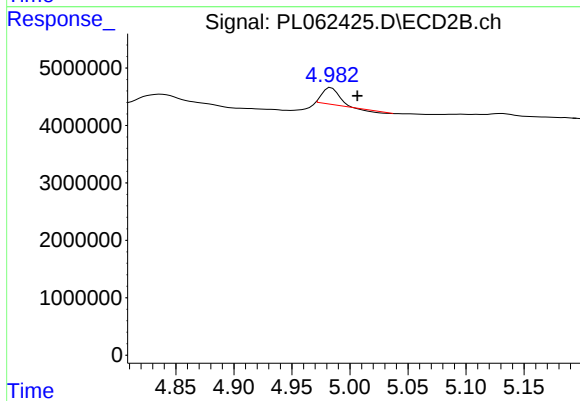

#7 delta-BHC


R.T.: 4.984 min
Delta R.T.: -0.023 min
Response: 2299901
Conc: 0.88 ng/ml

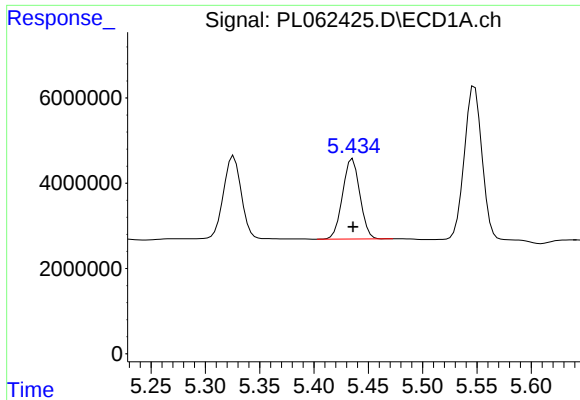

#9 Endosulfan I


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 20874302
Conc: 12.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

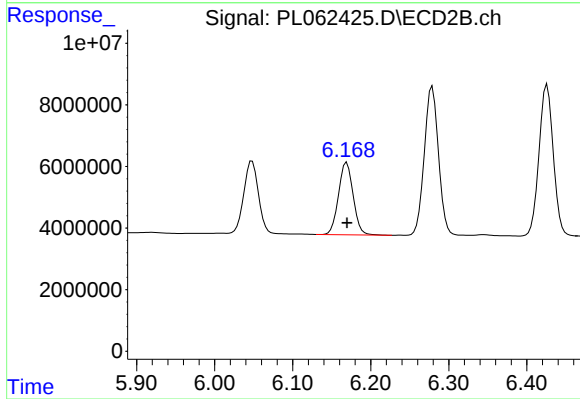


#9 Endosulfan I

R.T.: 6.169 min
Delta R.T.: 0.000 min
Response: 30654331
Conc: 12.68 ng/ml

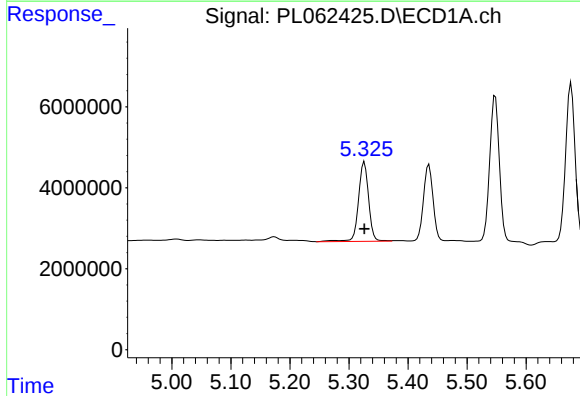


#10 gamma-Chlordane

R.T.: 5.326 min
Delta R.T.: 0.000 min
Response: 23412513
Conc: 13.29 ng/ml

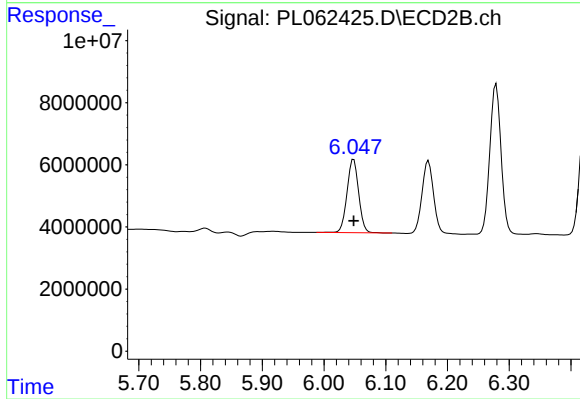

#10 gamma-Chlordane


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 30892356
Conc: 12.20 ng/ml

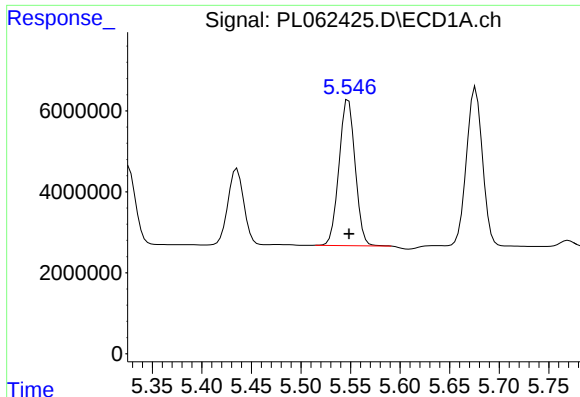

#12 4,4'-DDE


R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 40853806
Conc: 25.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

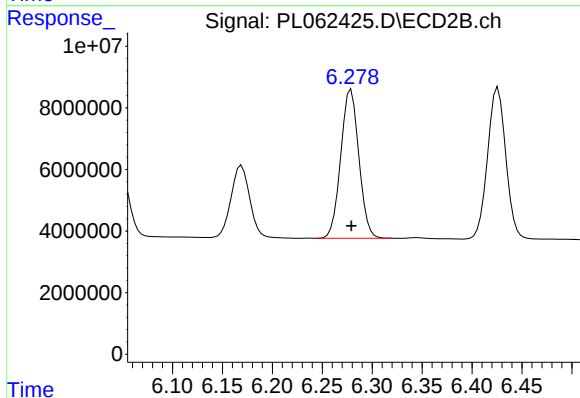


#12 4,4'-DDE

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 61014300
Conc: 25.11 ng/ml

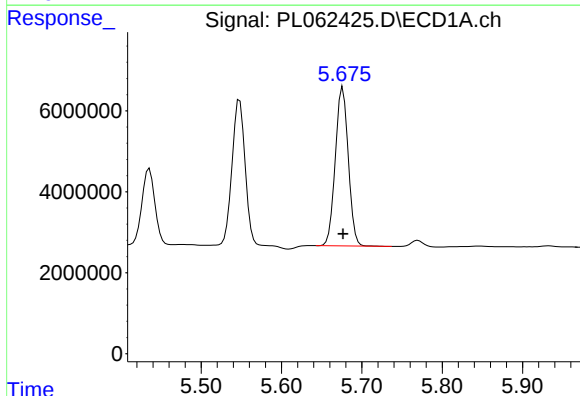


#13 Dieldrin

R.T.: 5.676 min
Delta R.T.: 0.000 min
Response: 44016221
Conc: 25.60 ng/ml

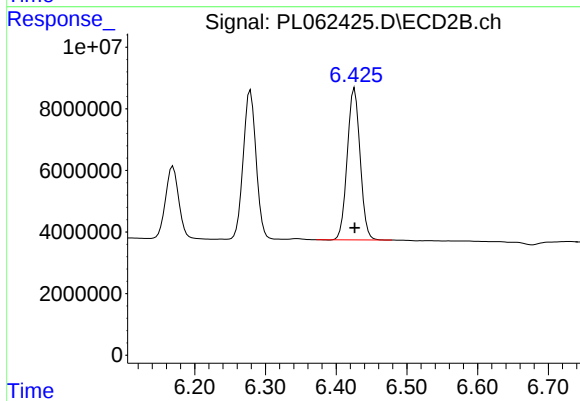

#13 Dieldrin


R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 62386883
Conc: 25.43 ng/ml

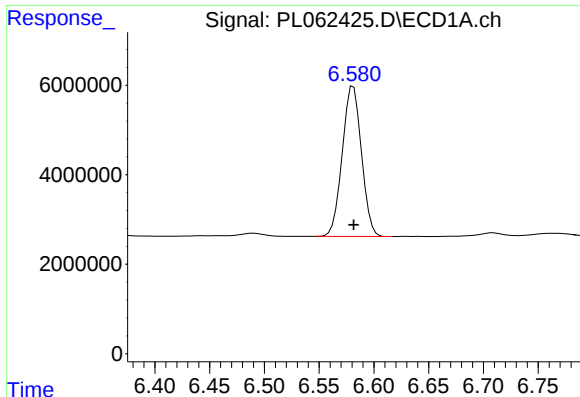

#19 Endosulfan Sulfate


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 40958885
Conc: 25.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

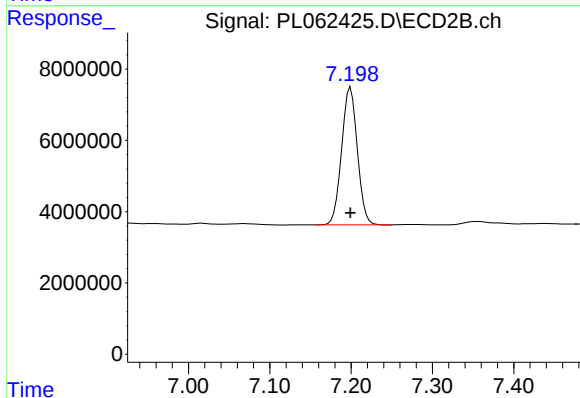


#19 Endosulfan Sulfate

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 51579529
Conc: 25.13 ng/ml

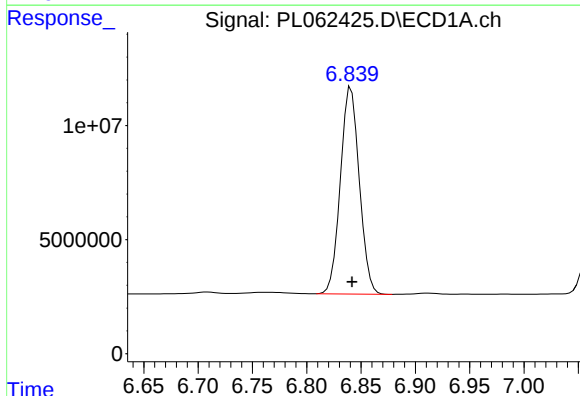


#20 Methoxychlor

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 109950459
Conc: 129.58 ng/ml

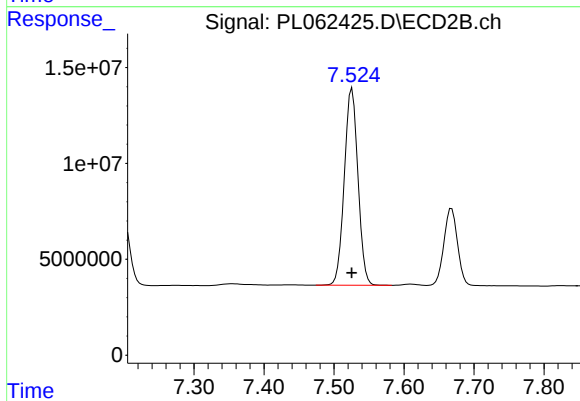

#20 Methoxychlor


R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 139057536
Conc: 125.36 ng/ml

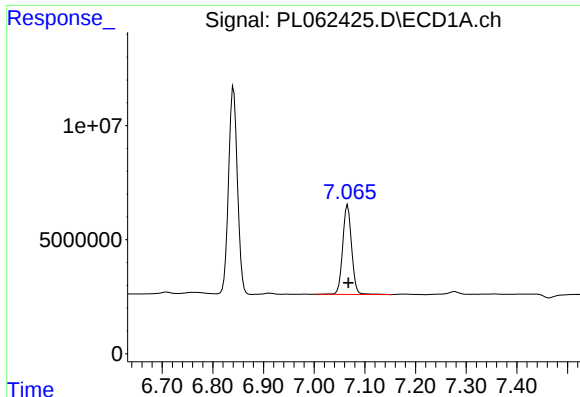

#21 Endrin ketone


R.T.: 7.066 min
Delta R.T.: -0.001 min
Response: 48136374
Conc: 25.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

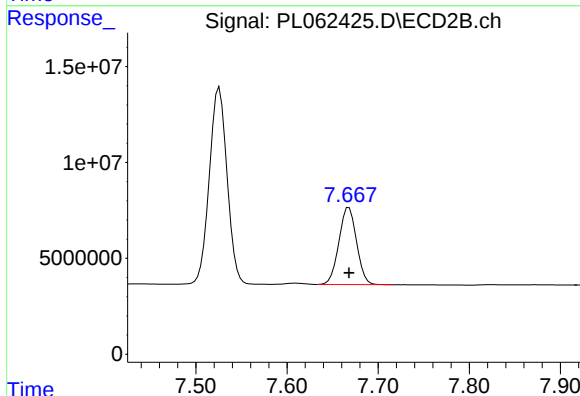


#21 Endrin ketone

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 54276248
Conc: 25.51 ng/ml

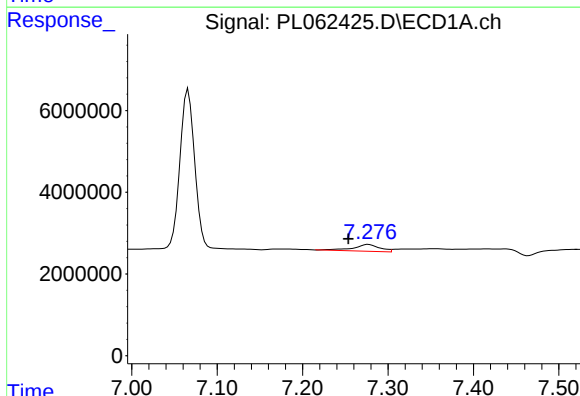


#22 Mirex

R.T.: 7.277 min
Delta R.T.: 0.024 min
Response: 3651832
Conc: 2.49 ng/ml

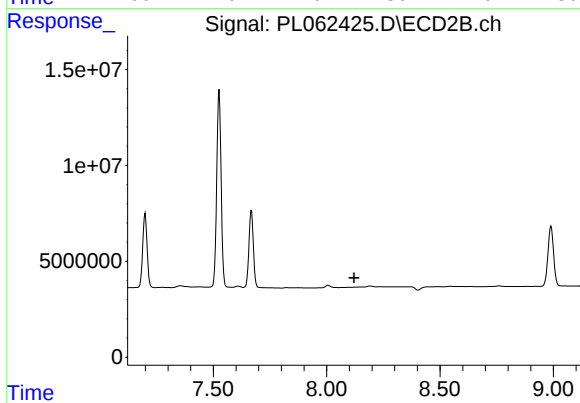

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

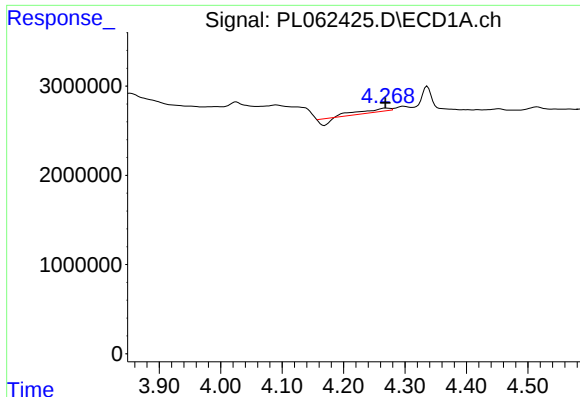

#23 Chlordane-1


R.T.: 4.269 min
Delta R.T.: 0.001 min
Response: 772936
Conc: 15.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

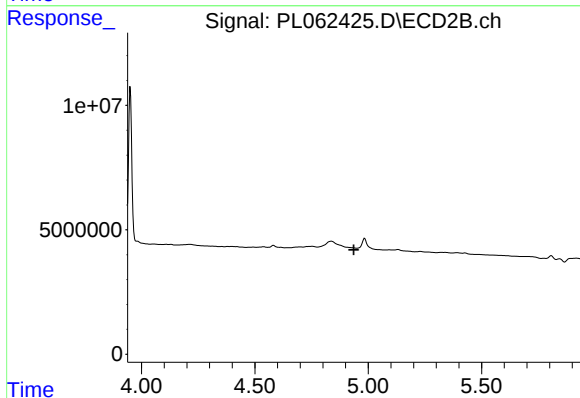


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.937 min
Response: 0
Conc: N.D.

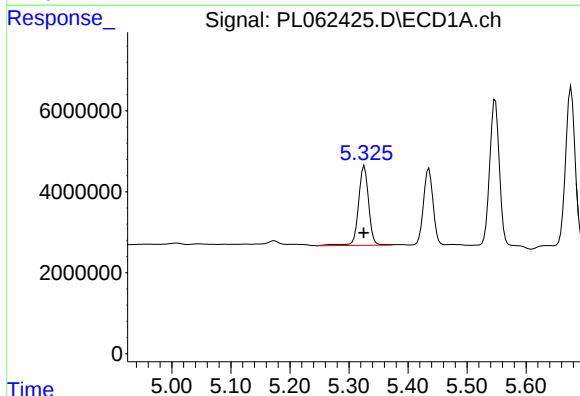


#25 Chlordane-3

R.T.: 5.326 min
Delta R.T.: 0.000 min
Response: 23412513
Conc: 160.28 ng/ml

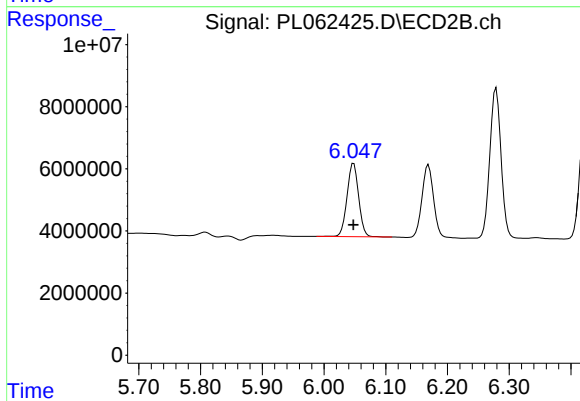

#25 Chlordane-3


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 30892356
Conc: 101.61 ng/ml

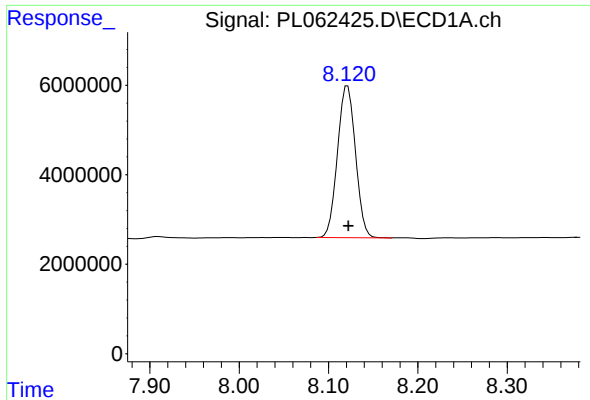

#28 Decachlorobiphenyl

R.T.: 8.121 min
Delta R.T.: 0.000 min
Response: 47487441
Conc: 27.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

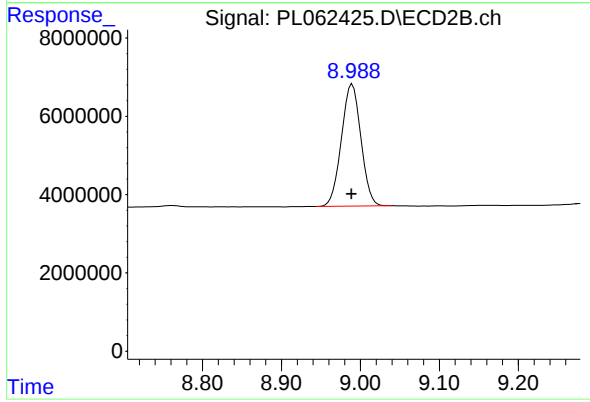

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 53628156
Conc: 27.05 ng/ml