

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101920\
 Data File : PL062431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2020 15:38
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 06:54:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 06:54:17 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	93232330	107.9E6	50.000	50.000
28)	SA Decachlor...	8.121	8.989	81732505	93707301	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.268	4.937	25710492	37958760	500.000	500.000
24)	Chlordane-2	4.763	5.403	30651515	41668203	500.000	500.000
25)	Chlordane-3	5.325	6.047	73037110	152.0E6	500.000	500.000
26)	Chlordane-4	5.383	6.121	61976805	184.9E6	500.000	500.000
27)	Chlordane-5	6.210	6.923	25889723	30642788	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101920\
Data File : PL062431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2020 15:38
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 06:54:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 06:54:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

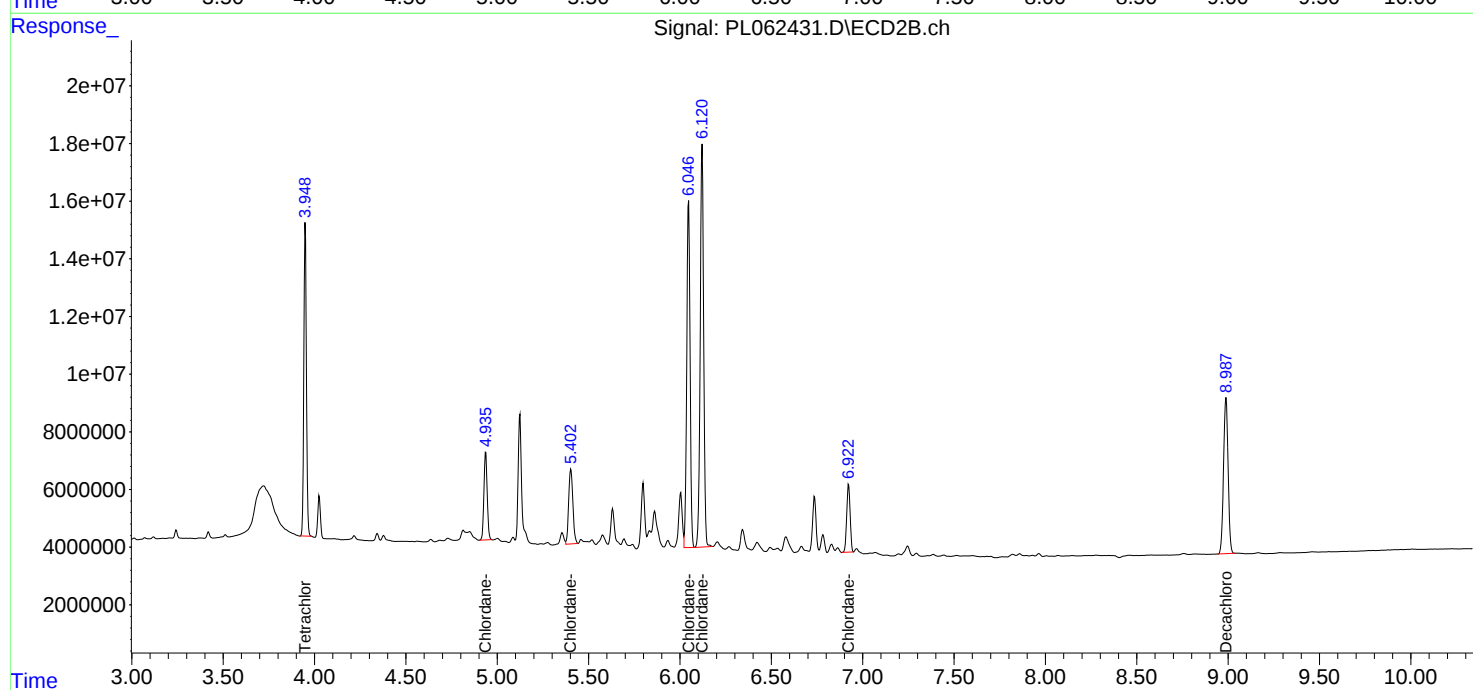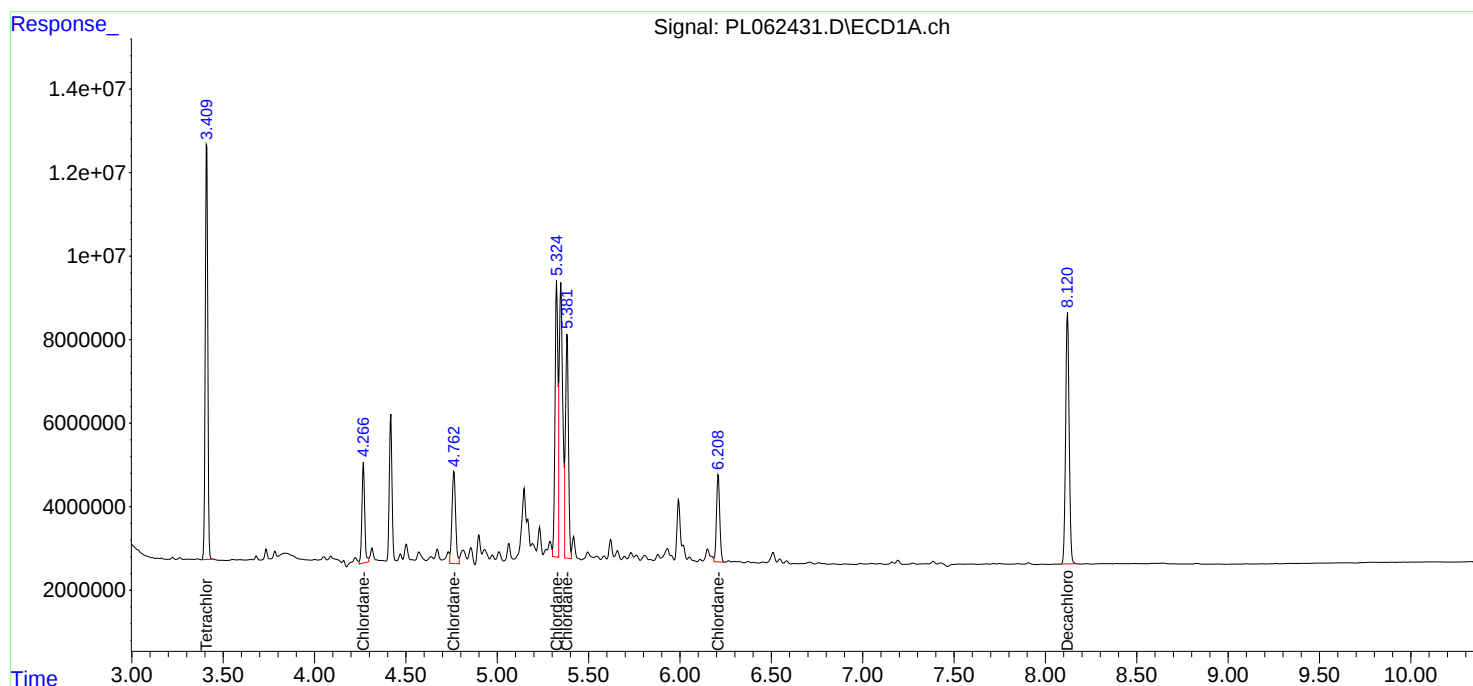


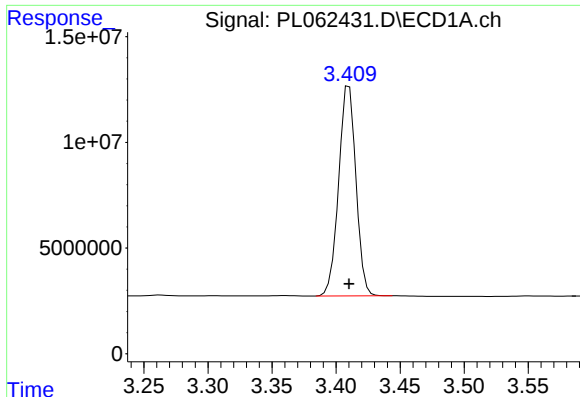

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 93232330
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

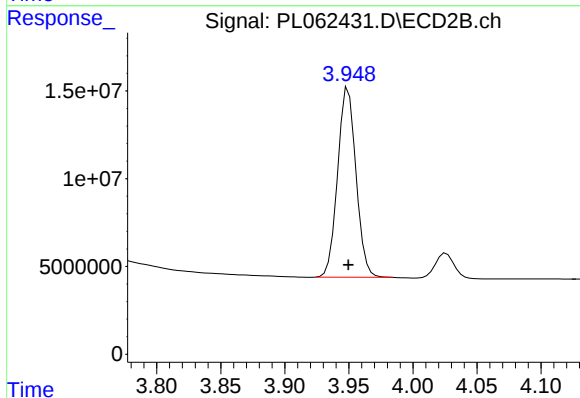


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 107872328
Conc: 50.00 ng/ml

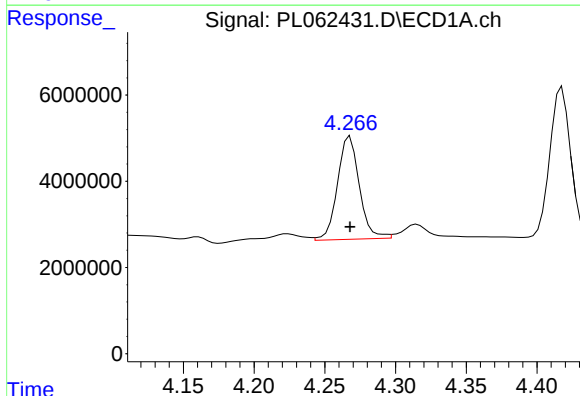


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 25710492
Conc: 500.00 ng/ml

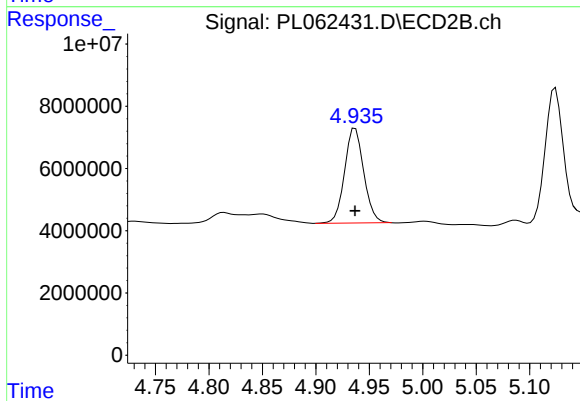

#23 Chlordane-1


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 37958760
Conc: 500.00 ng/ml

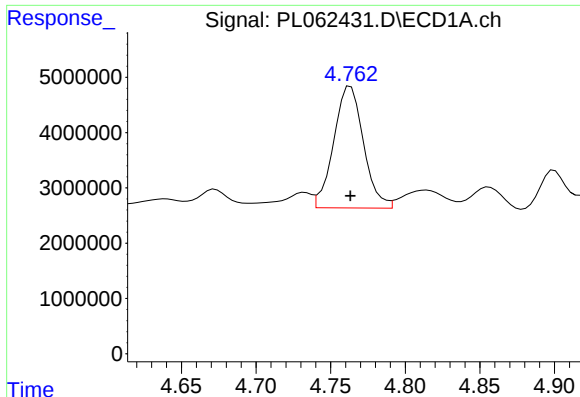

#24 Chlordane-2


R.T.: 4.763 min
Delta R.T.: 0.000 min
Response: 30651515
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

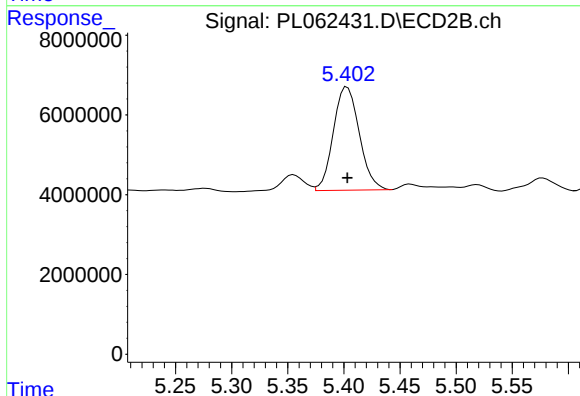


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 41668203
Conc: 500.00 ng/ml

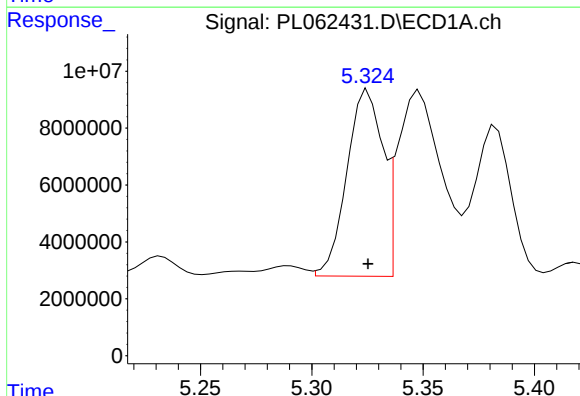


#25 Chlordane-3

R.T.: 5.325 min
Delta R.T.: 0.000 min
Response: 73037110
Conc: 500.00 ng/ml

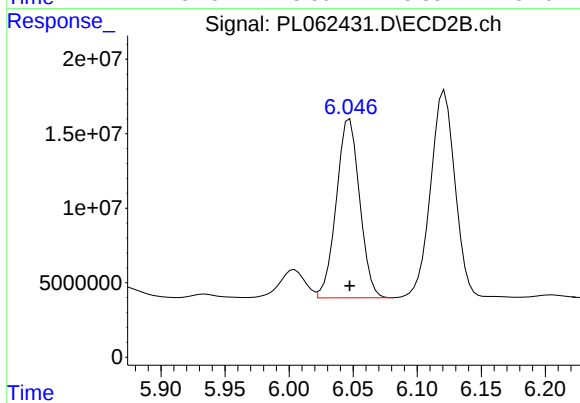

#25 Chlordane-3


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 152015524
Conc: 500.00 ng/ml

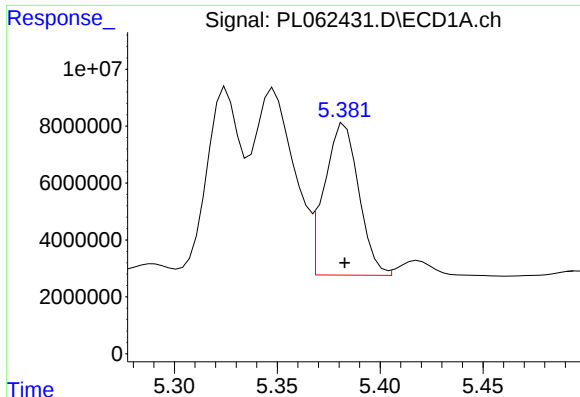

#26 Chlordane-4


R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 61976805
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

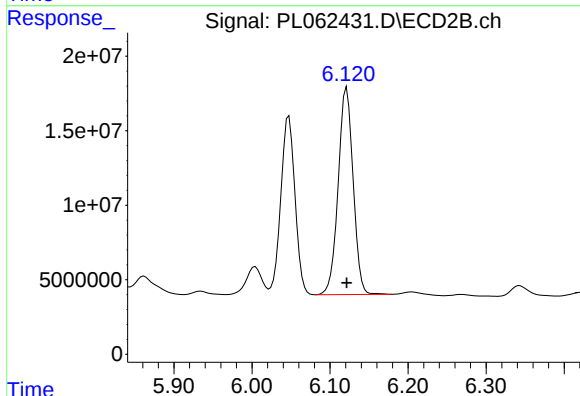


#26 Chlordane-4

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 184882324
Conc: 500.00 ng/ml

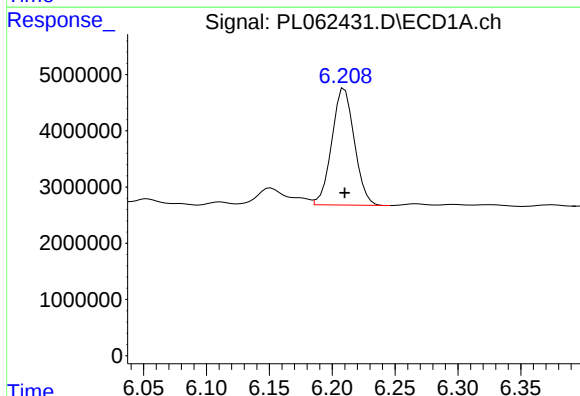


#27 Chlordane-5

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 25889723
Conc: 500.00 ng/ml

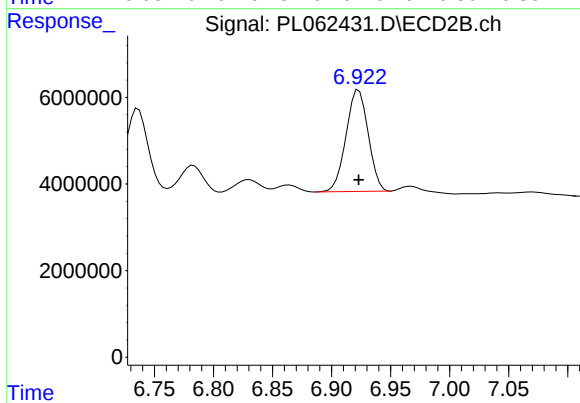

#27 Chlordane-5


R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 30642788
Conc: 500.00 ng/ml

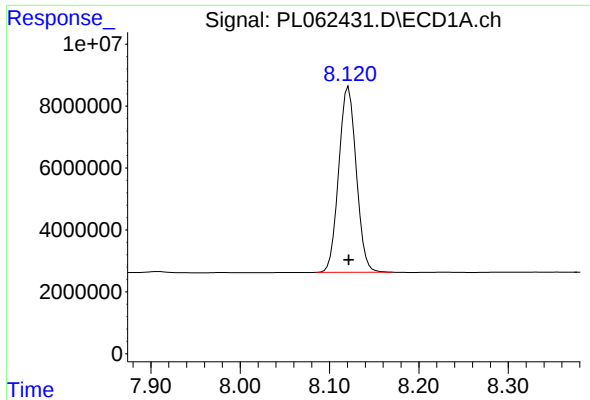

#28 Decachlorobiphenyl

R.T.: 8.121 min
Delta R.T.: 0.000 min
Response: 81732505
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

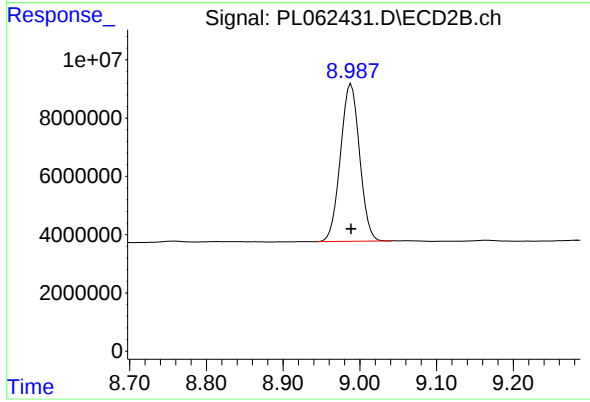

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 93707301
Conc: 50.00 ng/ml