

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101921\
 Data File : PL070421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2021 17:34
 Operator : AR\AJ
 Sample : M4271-01 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-101821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 04:47:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.624	5.581	946509	2174683	1.892	1.644
28) SA Decachlor...	10.390	11.503	1421039	2071543	2.054	1.712
Target Compounds						
12) B 4,4'-DDE	7.624	8.583	938883	1725584	1.475	1.114
17) MA 4,4'-DDT	8.469	9.443	323570	647874	0.529	0.496


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL101921\
Data File : PL070421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2021 17:34
Operator : AR\AJ
Sample : M4271-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
OK-01-101821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 04:47:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

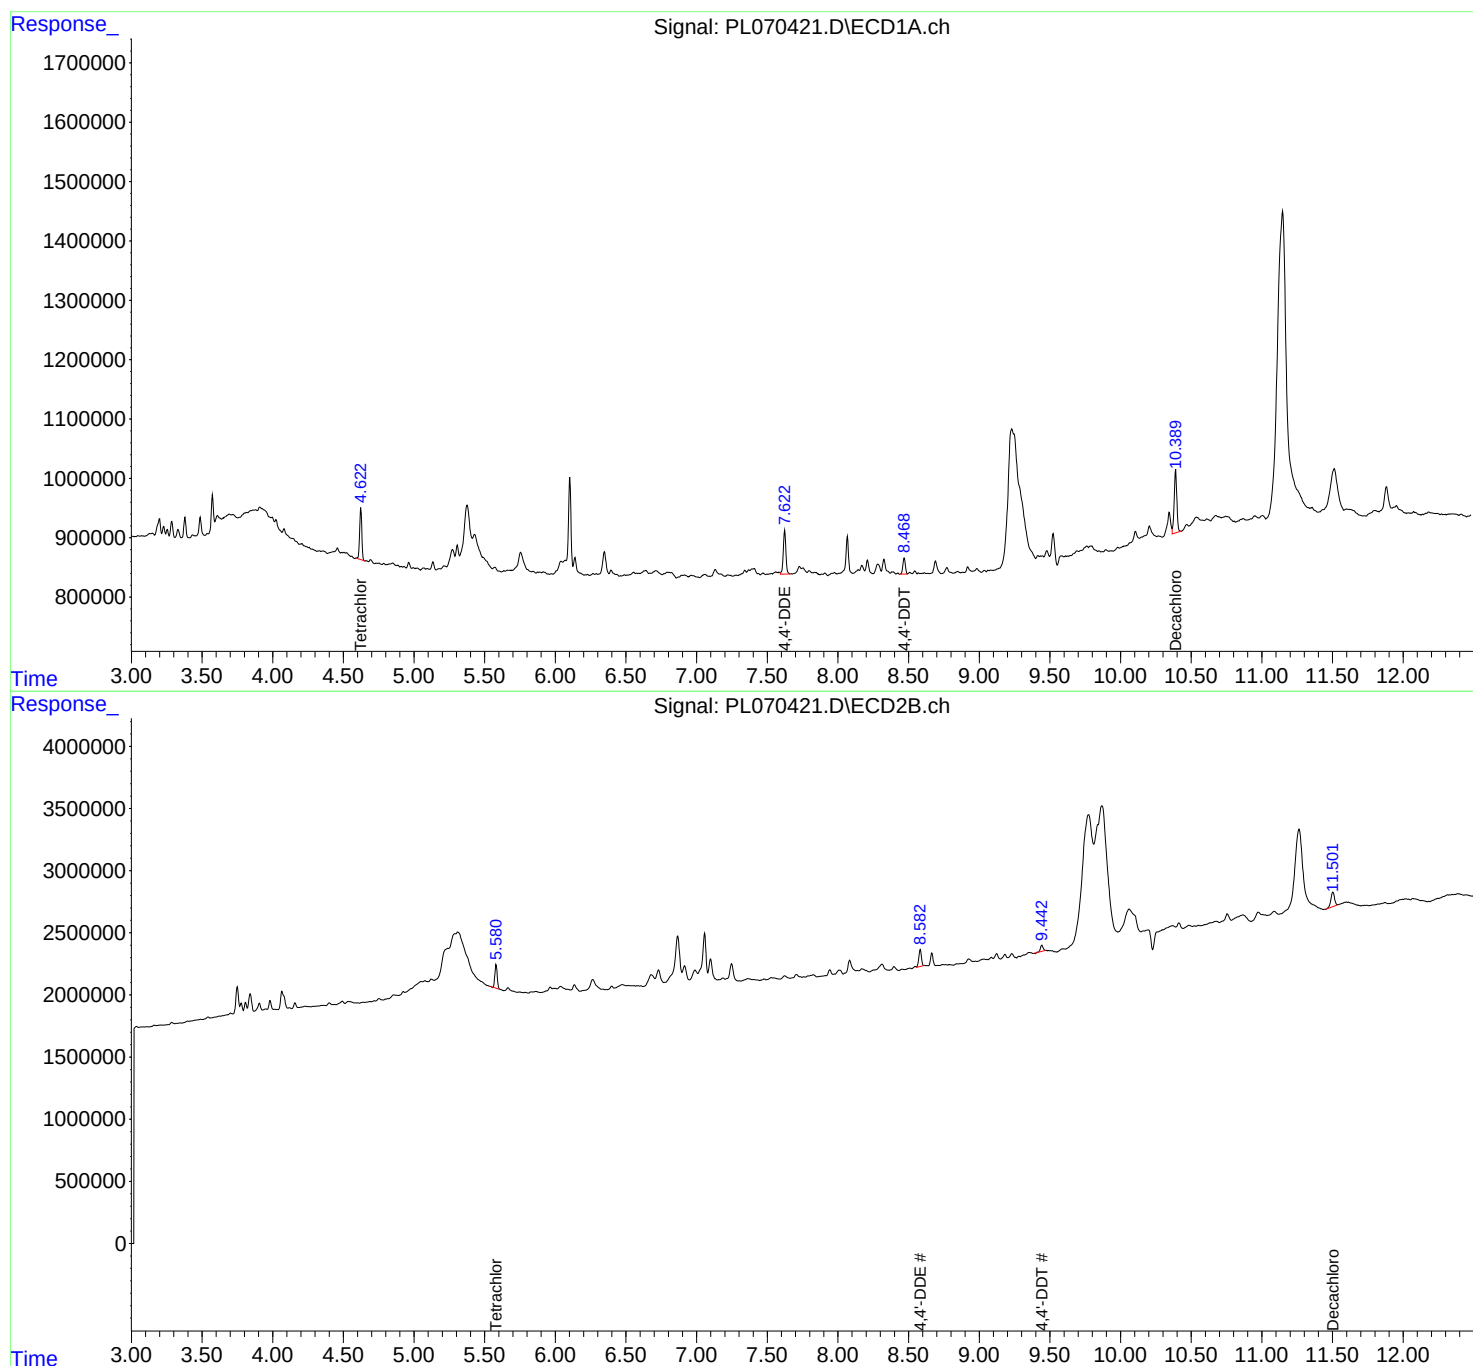


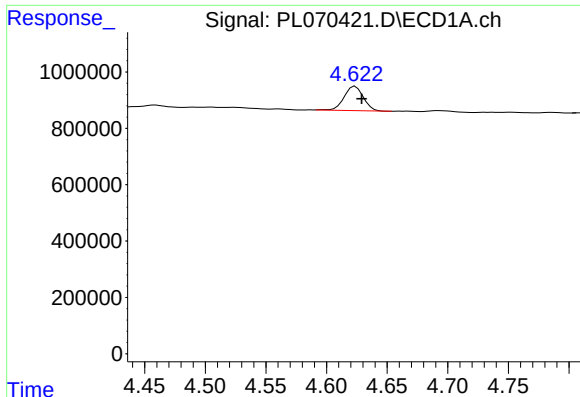

#1 Tetrachloro-m-xylene


R.T.: 4.624 min
Delta R.T.: -0.005 min
Response: 946509
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-101821

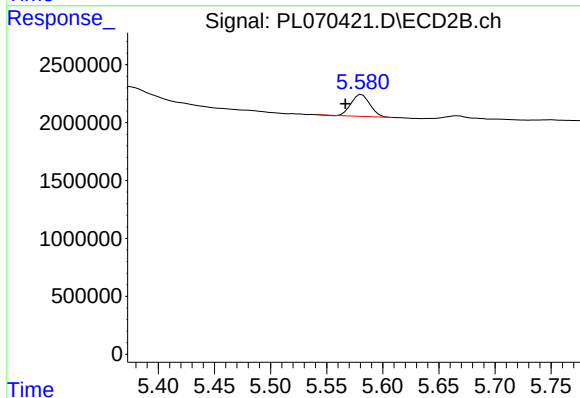


#1 Tetrachloro-m-xylene

R.T.: 5.581 min
Delta R.T.: 0.015 min
Response: 2174683
Conc: 1.64 ng/ml

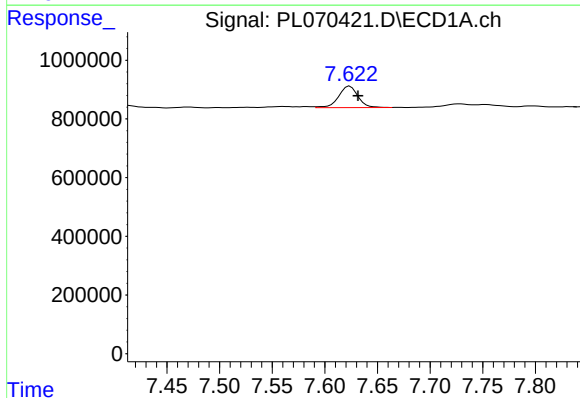


#12 4,4'-DDE

R.T.: 7.624 min
Delta R.T.: -0.008 min
Response: 938883
Conc: 1.48 ng/ml

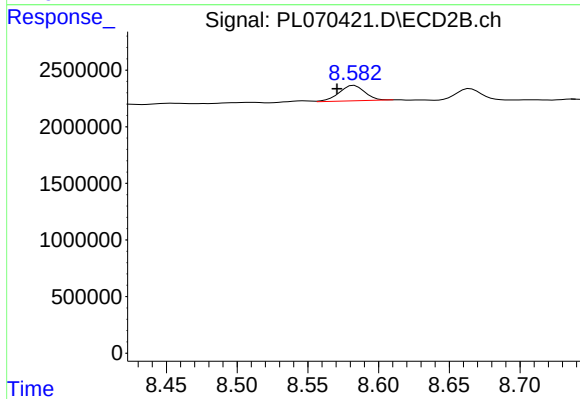

#12 4,4'-DDE


R.T.: 8.583 min
Delta R.T.: 0.012 min
Response: 1725584
Conc: 1.11 ng/ml

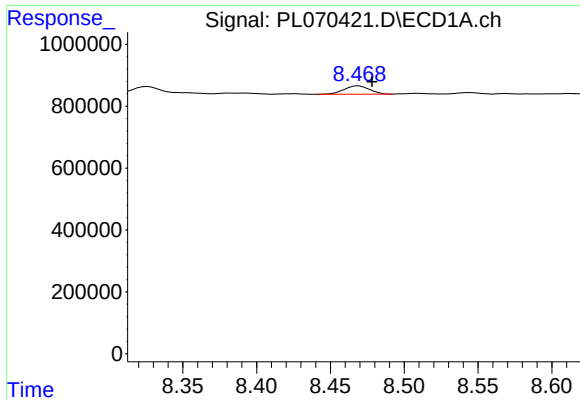

#17 4,4'-DDT


R.T.: 8.469 min
Delta R.T.: -0.009 min
Response: 323570
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-101821

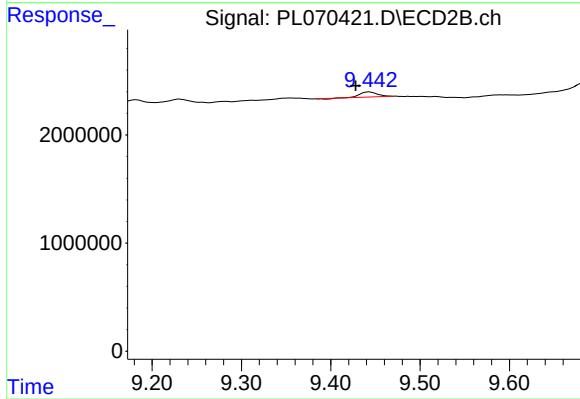


#17 4,4'-DDT

R.T.: 9.443 min
Delta R.T.: 0.015 min
Response: 647874
Conc: 0.50 ng/ml

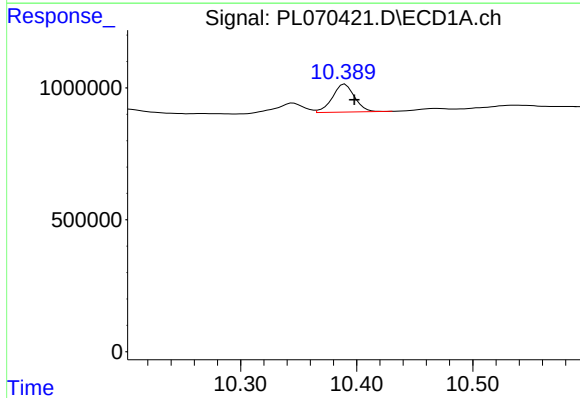

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.008 min
Response: 1421039
Conc: 2.05 ng/ml

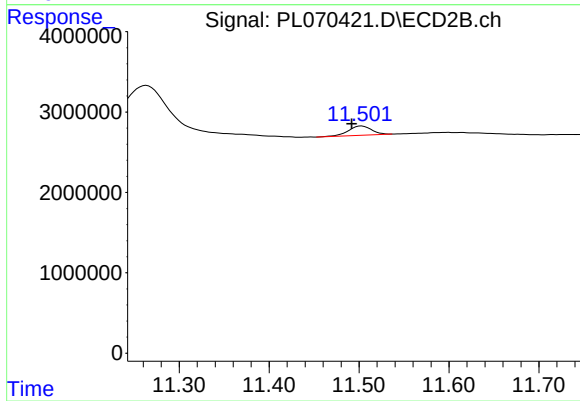

#28 Decachlorobiphenyl

R.T.: 11.503 min
Delta R.T.: 0.011 min
Response: 2071543
Conc: 1.71 ng/ml