

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
 Data File : PL062441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2020 13:54
 Operator : DD\AJ
 Sample : L4454-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:47:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	25801931	33550406	14.975	14.566
28)	SA Decachlor...	8.123	8.990	27641733	31389459	15.747	15.830
Target Compounds							
9)	A Endosulfan I	5.453f	0.000	1263928	0	0.773	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
Data File : PL062441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2020 13:54
Operator : DD\AJ
Sample : L4454-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TEST-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:47:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

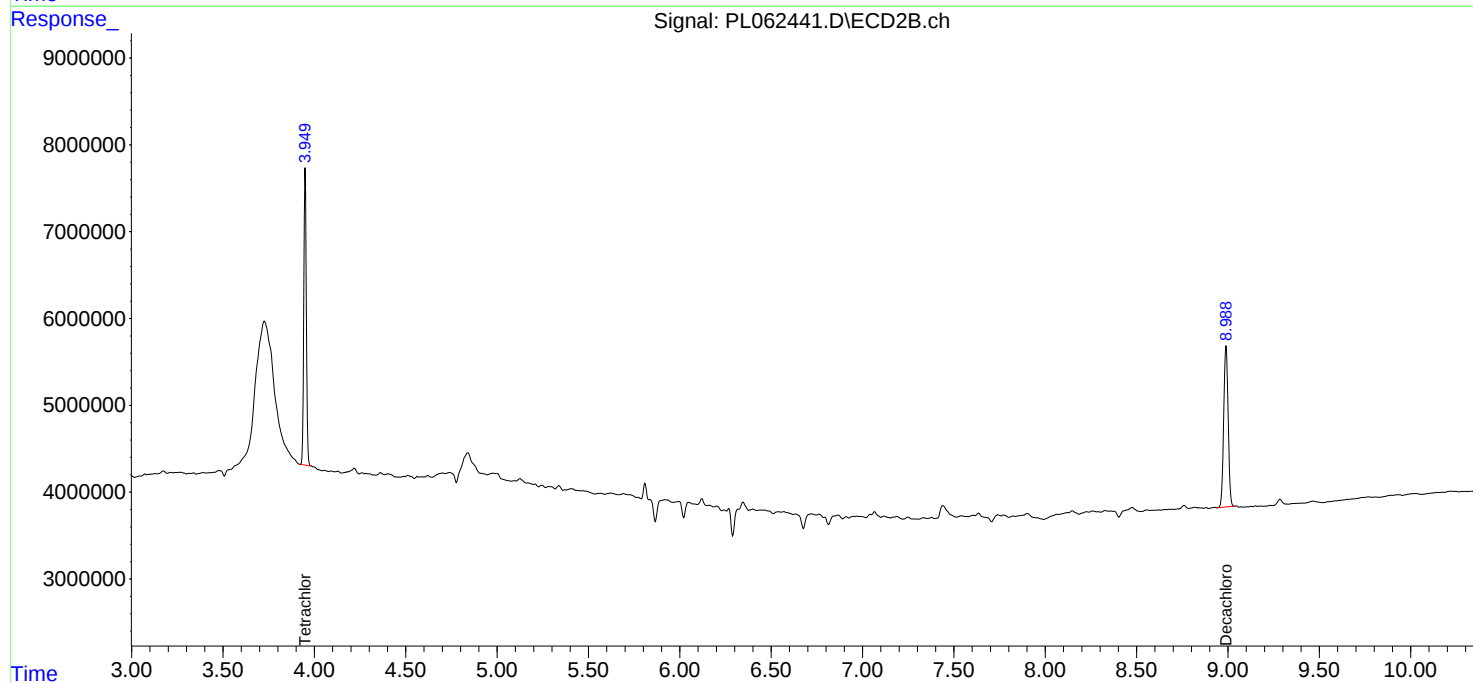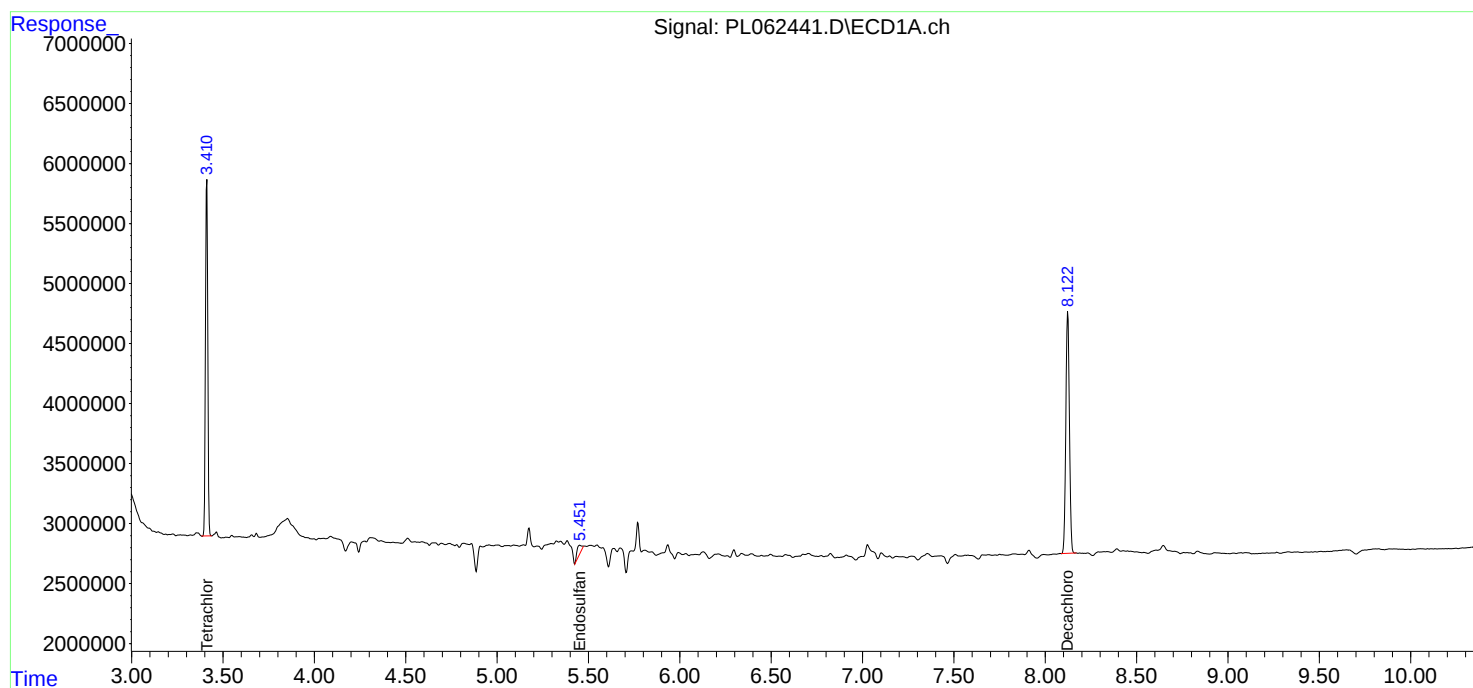


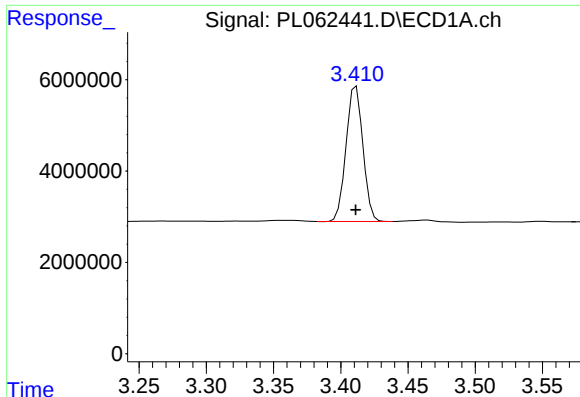

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 25801931
Conc: 14.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT

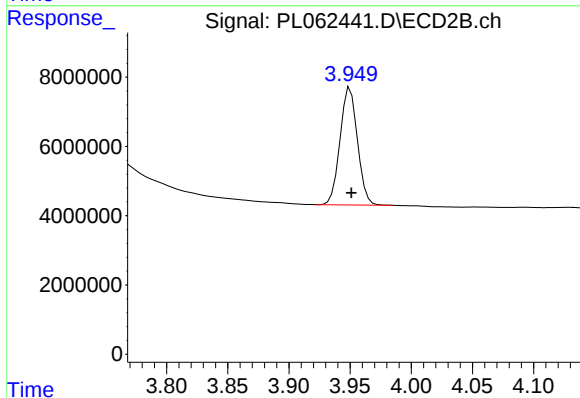


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 33550406
Conc: 14.57 ng/ml

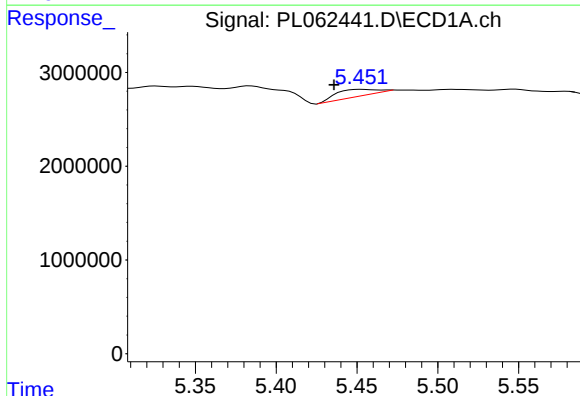


#9 Endosulfan I

R.T.: 5.453 min
Delta R.T.: 0.017 min
Response: 1263928
Conc: 0.77 ng/ml

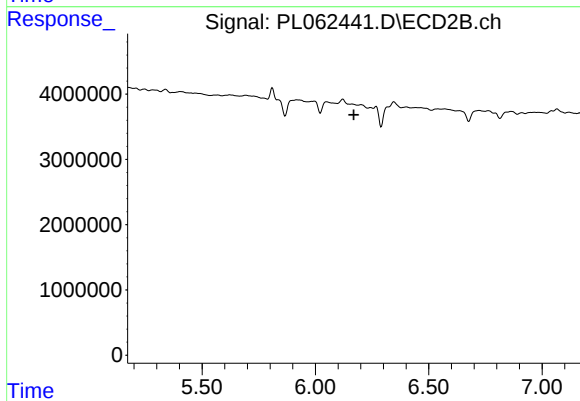

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

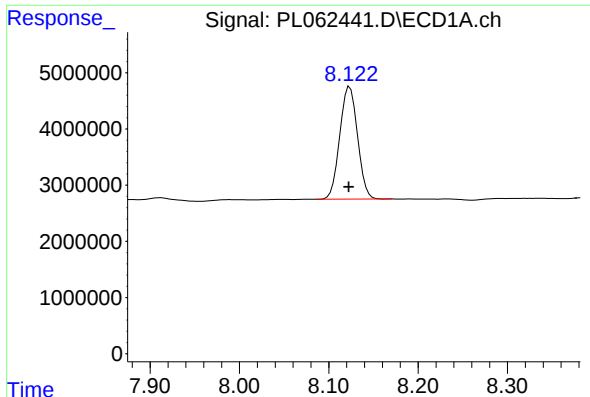

#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: 0.001 min
Response: 27641733
Conc: 15.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TEST-PIT

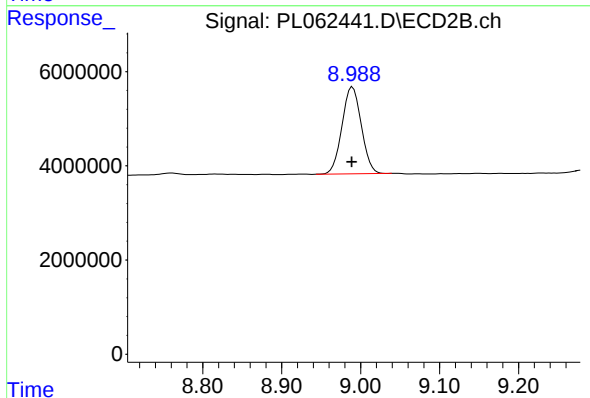

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 31389459
Conc: 15.83 ng/ml