

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
 Data File : PL062451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2020 16:21
 Operator : DD\AJ
 Sample : L4222-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-03-101920

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:48:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	31736802	42233758	18.420	18.336
28)	SA Decachlor...	8.126	8.988	34594432	39172535	19.708	19.755
Target Compounds							
7)	B delta-BHC	0.000	4.982f	0	186361	N.D.	0.071 #
23)	Chlordane-1	4.274	0.000	937698	0	18.236	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
Data File : PL062451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2020 16:21
Operator : DD\AJ
Sample : L4222-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-03-101920

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:48:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

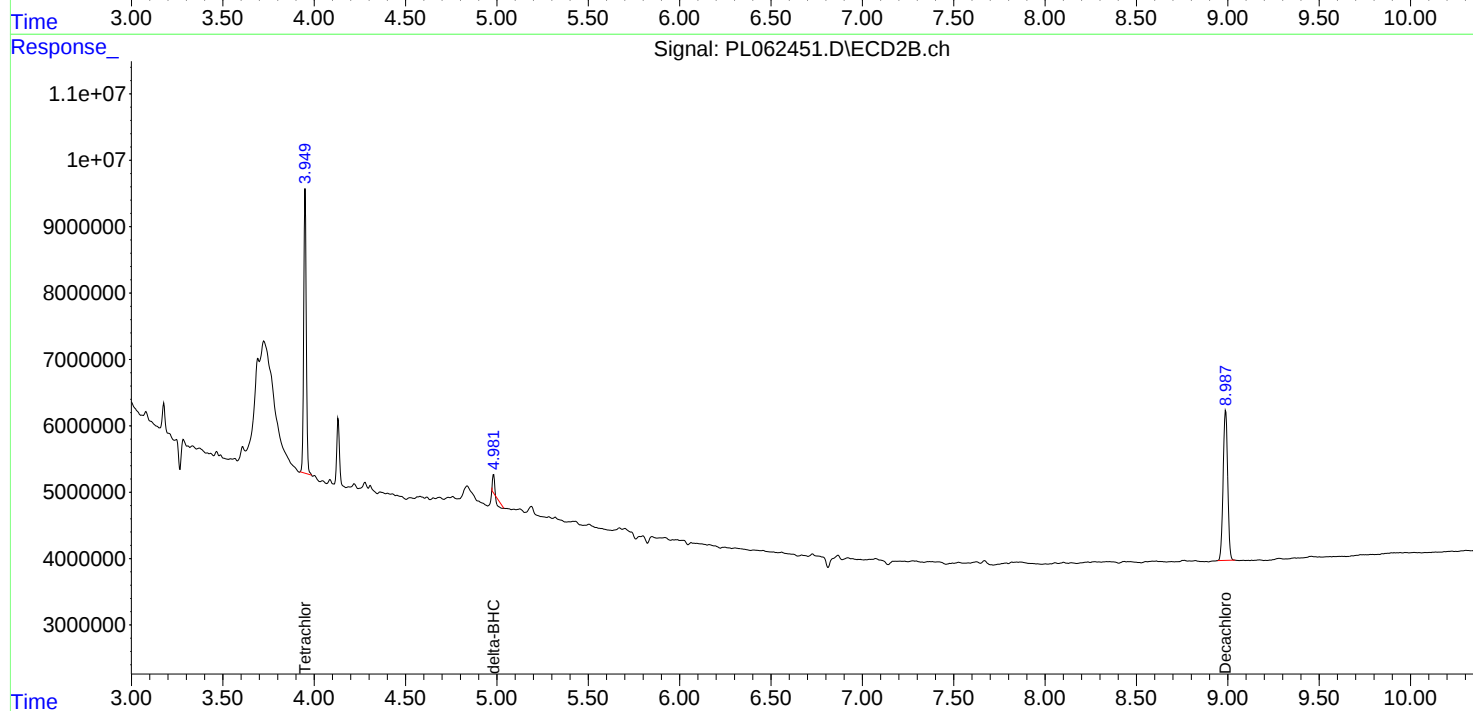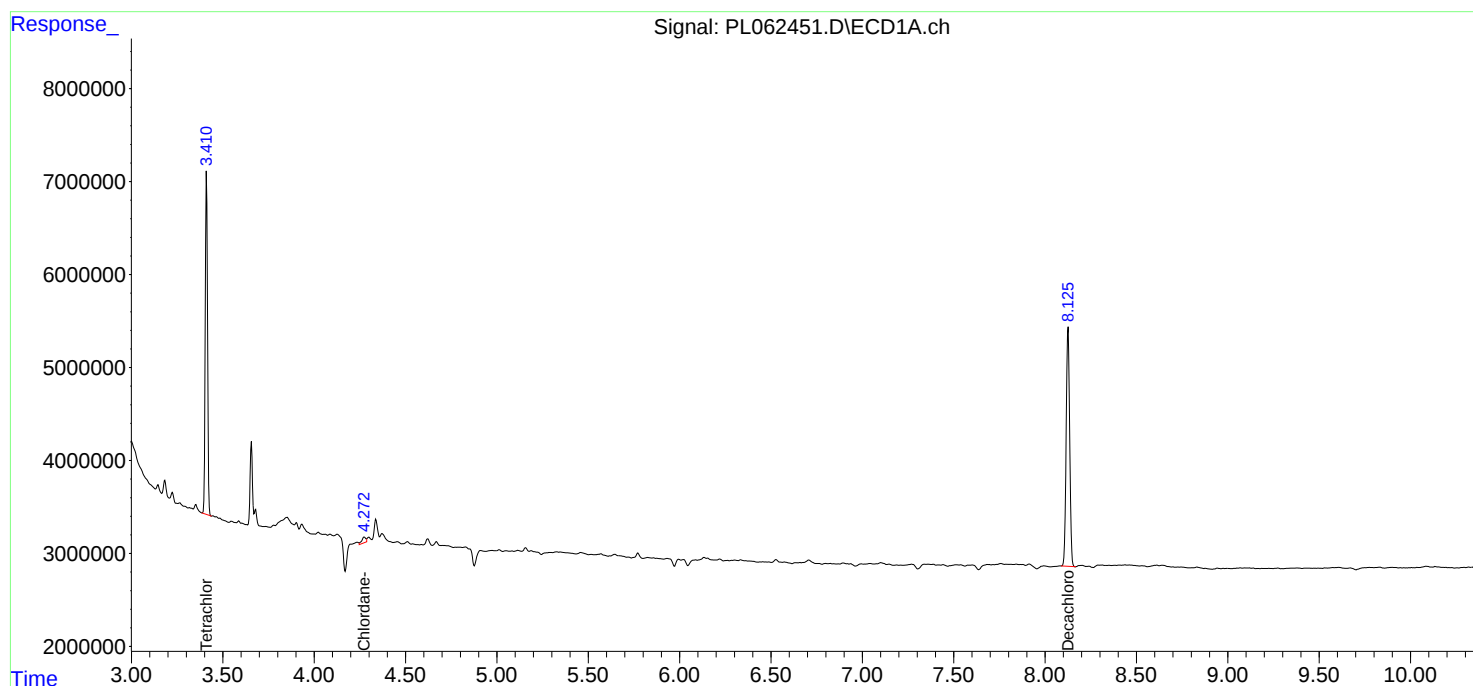


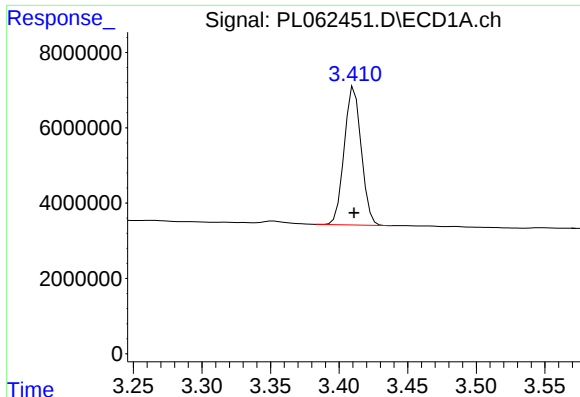

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 31736802
Conc: 18.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-03-101920

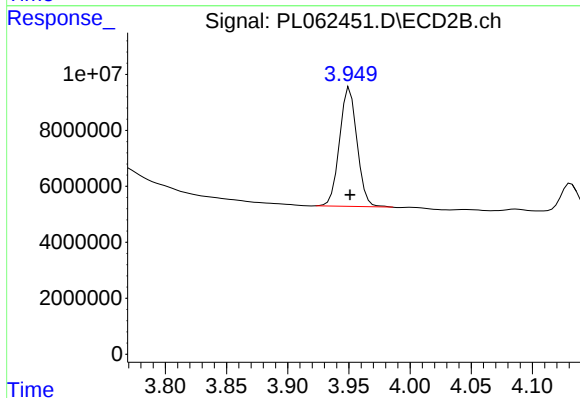


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 42233758
Conc: 18.34 ng/ml

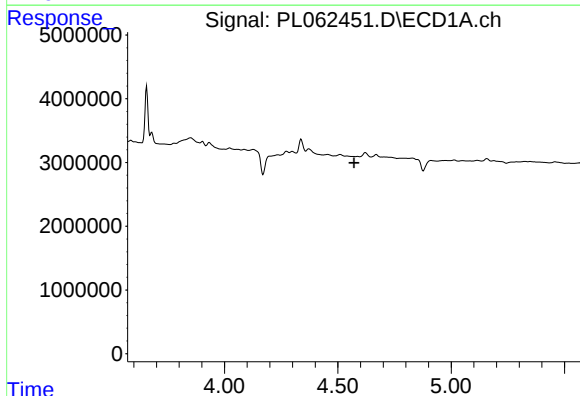


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

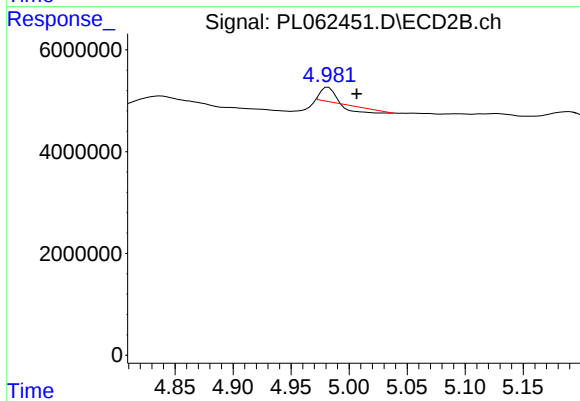

#7 delta-BHC


R.T.: 4.982 min
Delta R.T.: -0.024 min
Response: 186361
Conc: 0.07 ng/ml

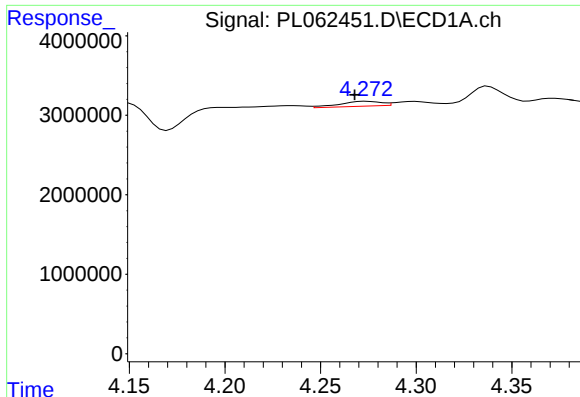

#23 Chlordane-1


R.T.: 4.274 min
Delta R.T.: 0.006 min
Response: 937698
Conc: 18.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-03-101920

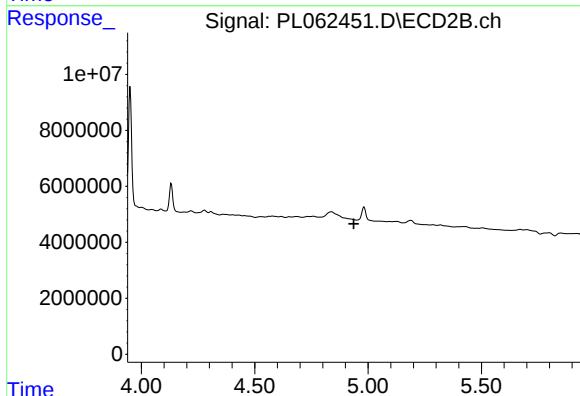


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.937 min
Response: 0
Conc: N.D.

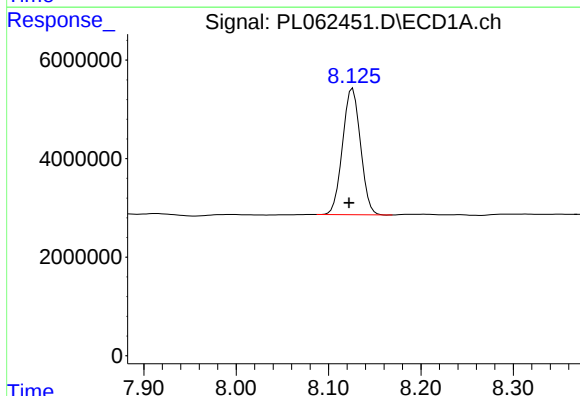

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.004 min
Response: 34594432
Conc: 19.71 ng/ml

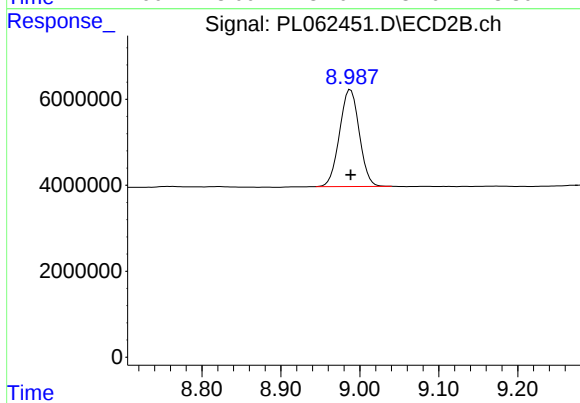

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 39172535
Conc: 19.76 ng/ml