

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
 Data File : PL062455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2020 17:18
 Operator : DD\AJ
 Sample : L4457-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SUTTON-PR-2152-SED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:49:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	36694335	48937620	21.297	21.246
28)	SA Decachlor...	8.126	8.989	34432518	38484357	19.616	19.408
Target Compounds							
23)	Chlordane-1	4.274	0.000	867303	0	16.867	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
Data File : PL062455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2020 17:18
Operator : DD\AJ
Sample : L4457-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SUTTON-PR-2152-SED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:49:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

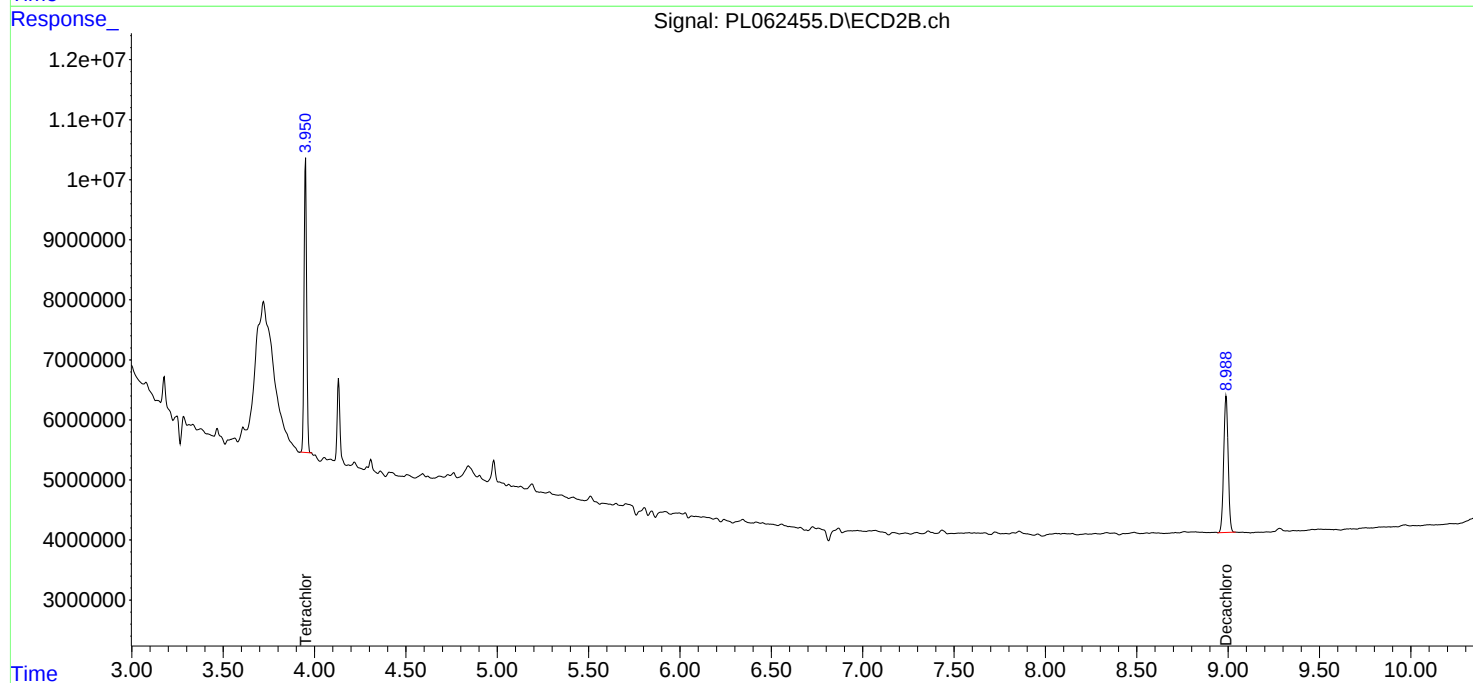


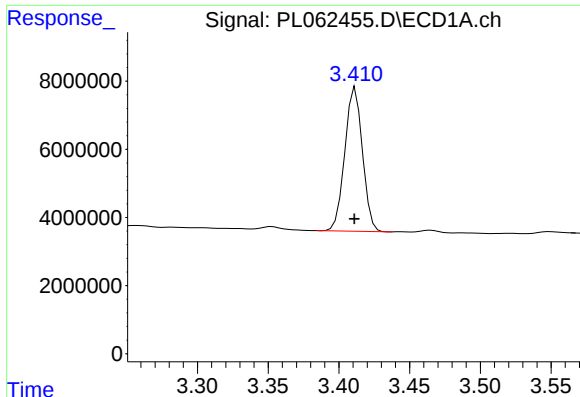

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 36694335
Conc: 21.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
SUTTON-PR-2152-SED

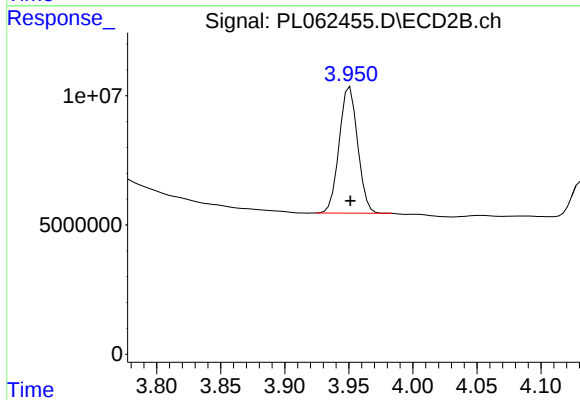


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 48937620
Conc: 21.25 ng/ml

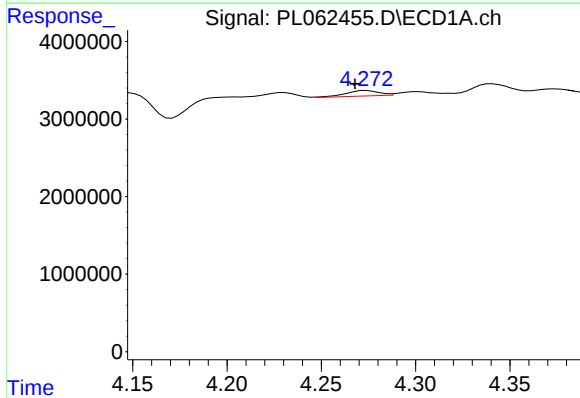


#23 Chlordane-1

R.T.: 4.274 min
Delta R.T.: 0.006 min
Response: 867303
Conc: 16.87 ng/ml

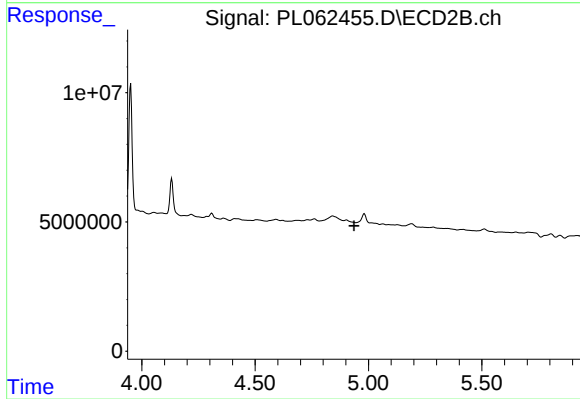

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.937 min
Response: 0
Conc: N.D.

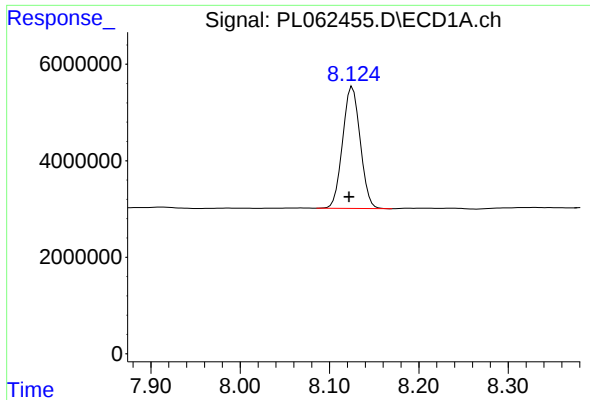

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.003 min
Response: 34432518
Conc: 19.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
SUTTON-PR-2152-SED

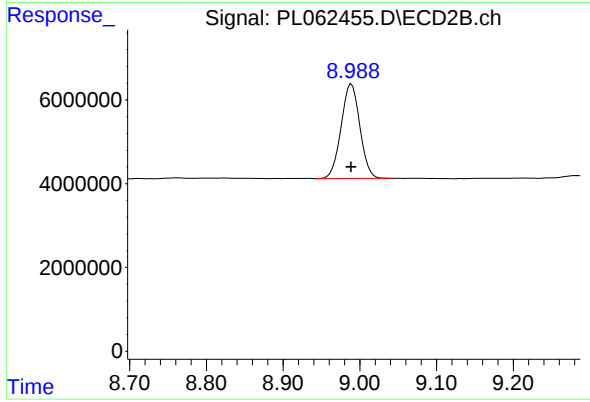

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 38484357
Conc: 19.41 ng/ml