

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
 Data File : PL062462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2020 18:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:50:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:00:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.952	35579296	44035266	20.650	19.118
28)	SA Decachlor...	8.127	8.990	23034472	23950643	13.123	12.079
Target Compounds							
20)	A Methoxychlor	6.870f	0.000	1220510	0	1.438	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102020\
Data File : PL062462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2020 18:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:50:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:00:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

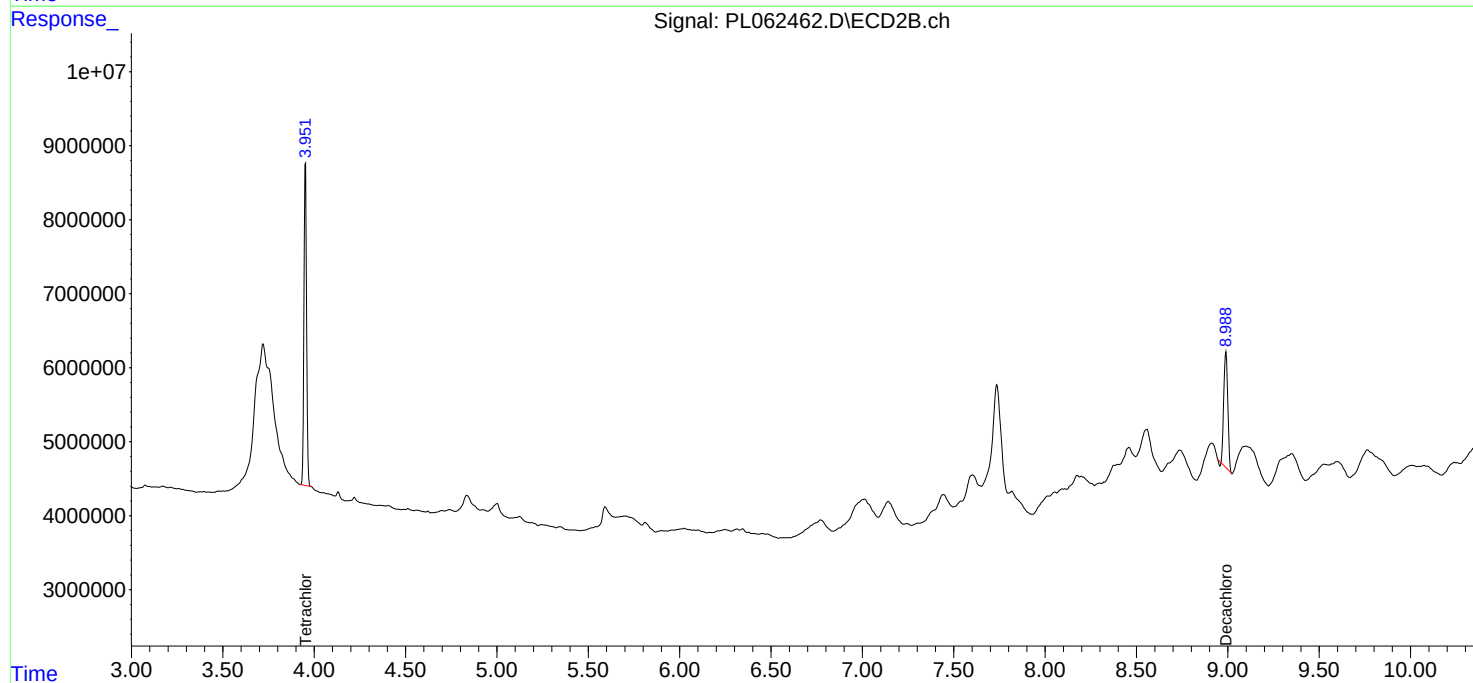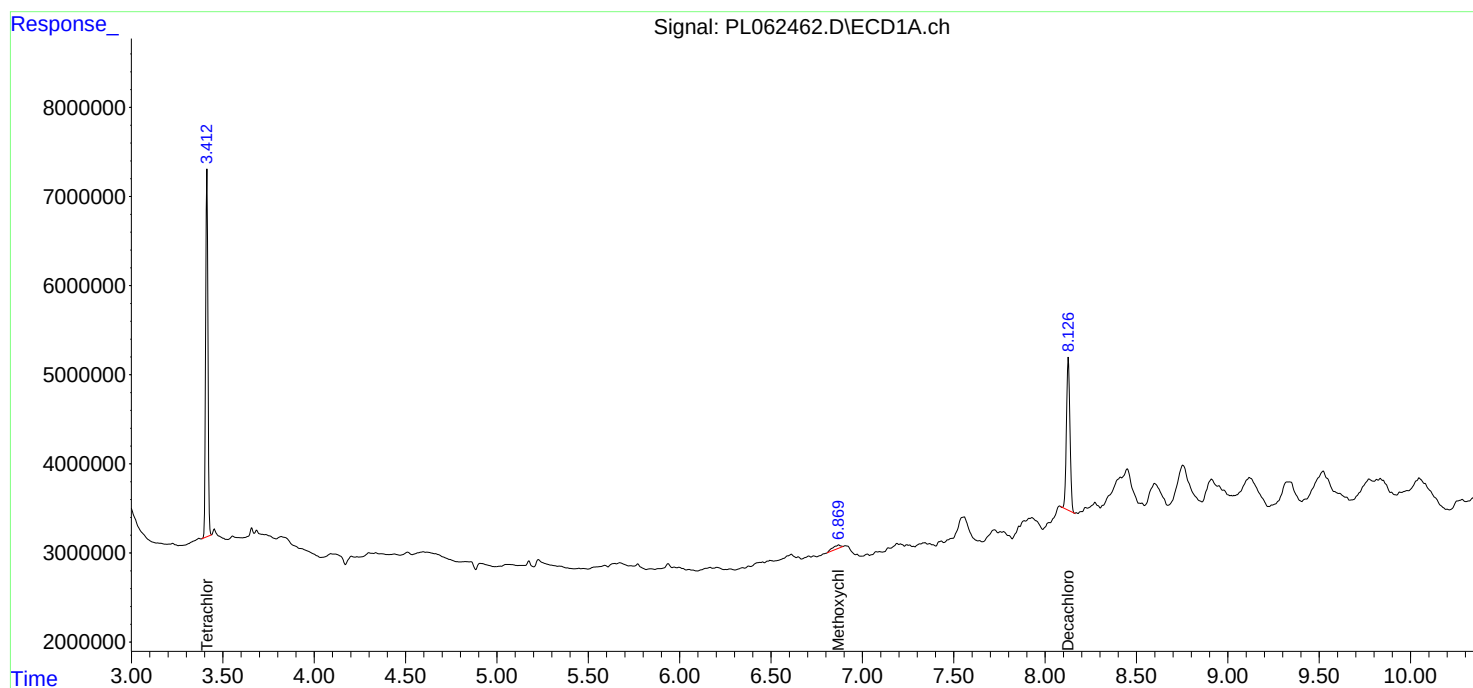


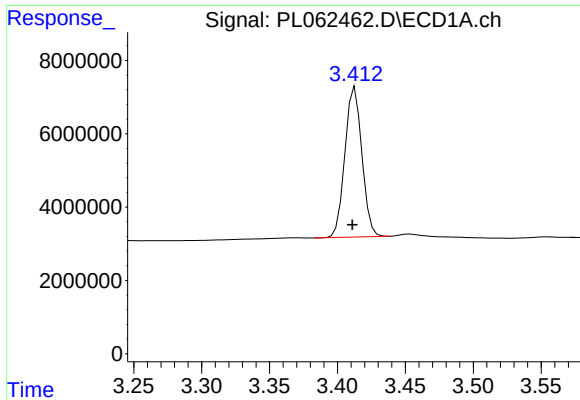

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.002 min
Response: 35579296
Conc: 20.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

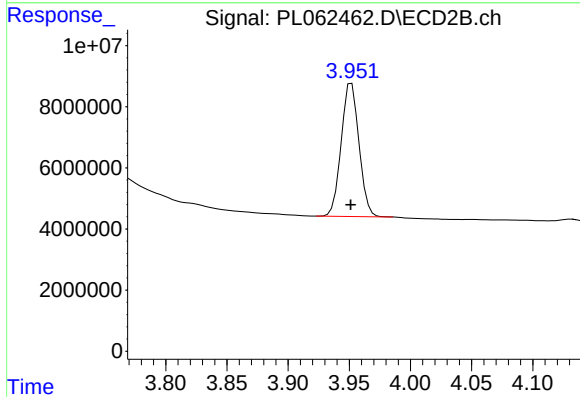


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 44035266
Conc: 19.12 ng/ml

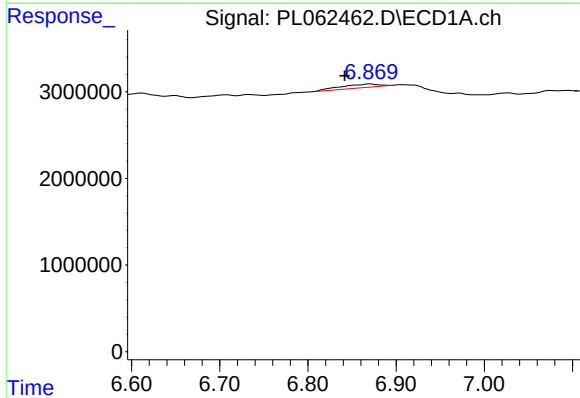


#20 Methoxychlor

R.T.: 6.870 min
Delta R.T.: 0.029 min
Response: 1220510
Conc: 1.44 ng/ml

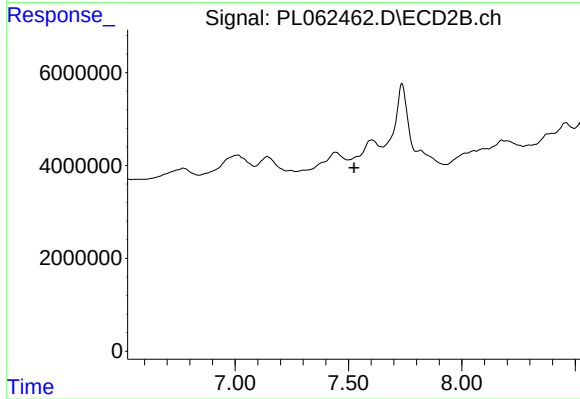

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.525 min
Response: 0
Conc: N.D.

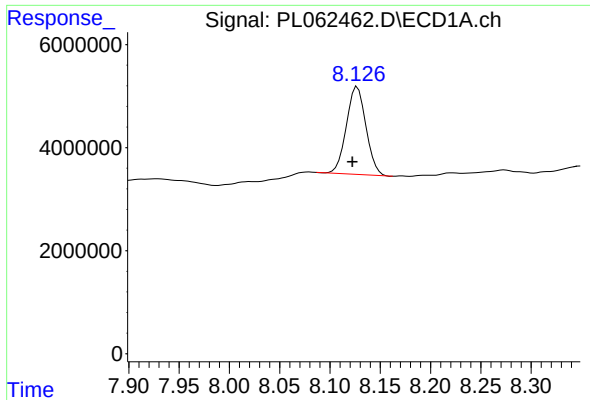

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.005 min
Response: 23034472
Conc: 13.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

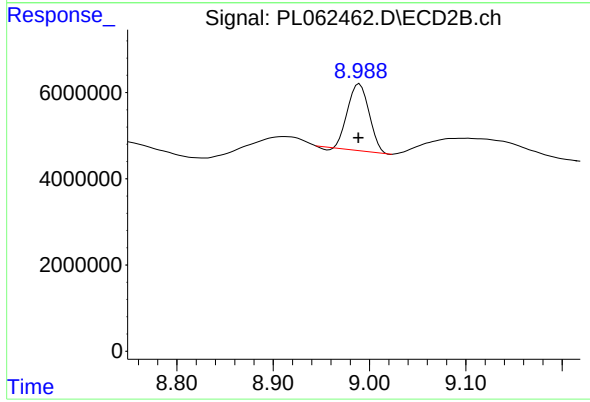

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 23950643
Conc: 12.08 ng/ml