

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102021\
 Data File : PL070435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 16:16
 Operator : AR\AJ
 Sample : M4285-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:50:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.625	5.564	10147857	26032589	20.280	19.682
28)	SA Decachlor...	10.392	11.489	13553909	24010399	19.587	19.840
Target Compounds							
2)	A alpha-BHC	5.308f	0.000	1572284	0	2.124	N.D. #
10)	B gamma-Chl...	7.343	8.299	1054016	3204111	1.455	2.003 #
11)	B alpha-Chl...	7.413	8.382	1477468	5099184	2.029	3.233 #
15)	B Endosulfa...	8.363	9.214	379651	850600	0.598	0.712
21)	B Endrin ke...	0.000	10.086	0	1502406	N.D.	1.123 #
25)	Chlordane-3	7.343	8.299	1054016	3204111	15.406	15.129
26)	Chlordane-4	7.413	8.382	1477468	5099184	20.217	20.063
27)	Chlordane-5	8.363	0.000	379651	0	19.089	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102021\
Data File : PL070435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 16:16
Operator : AR\AJ
Sample : M4285-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:50:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

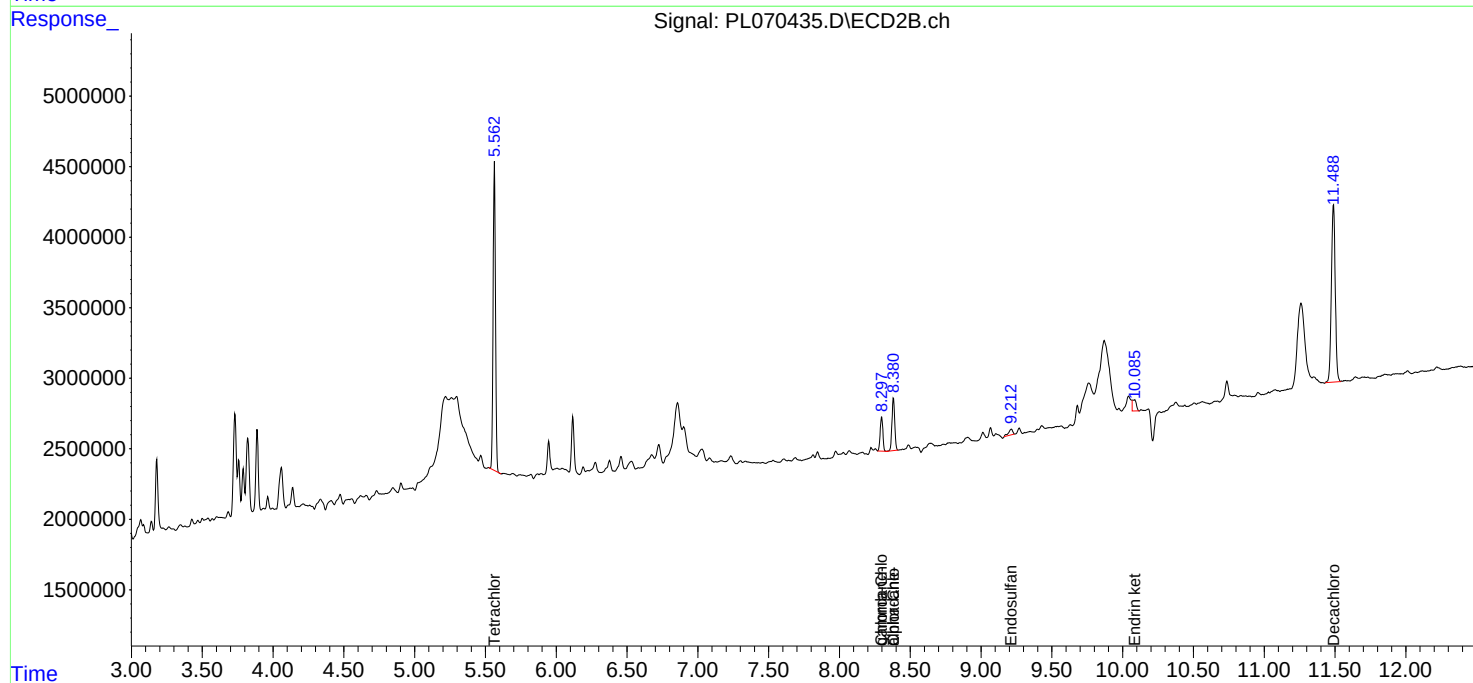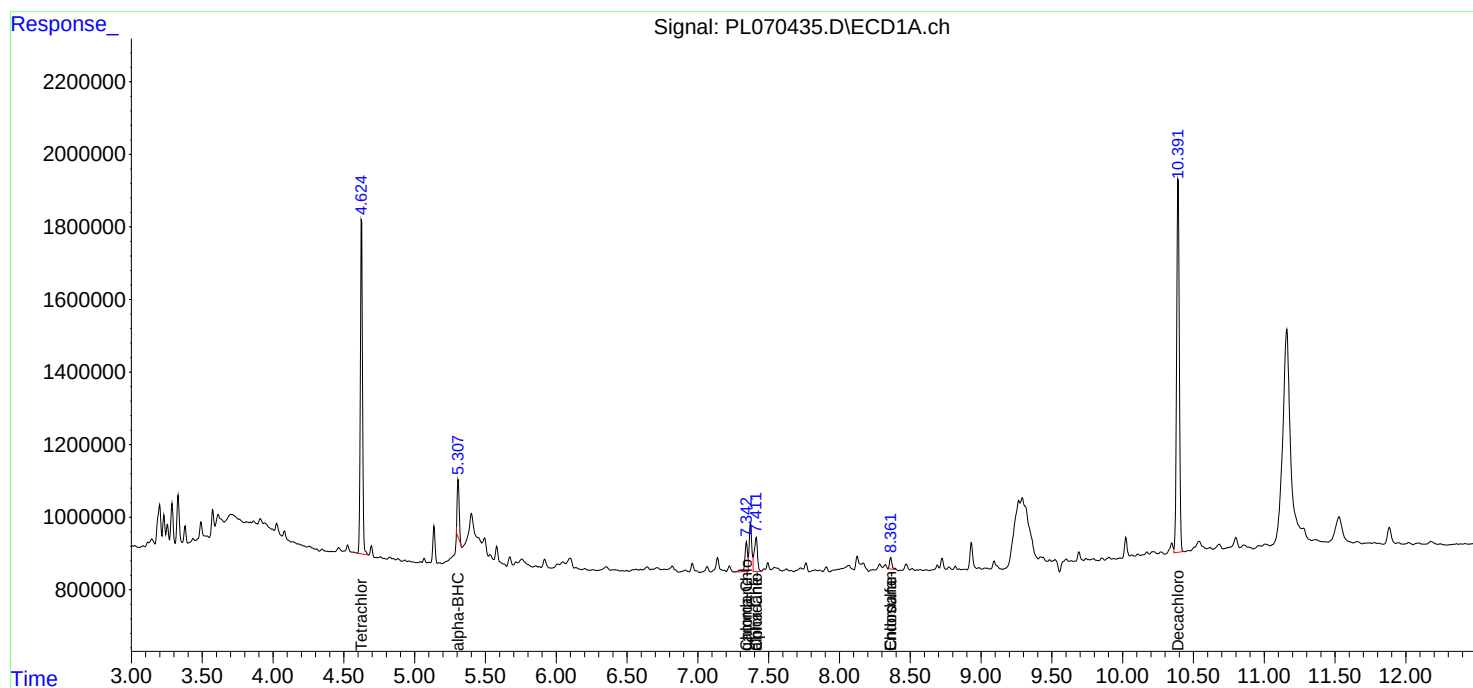


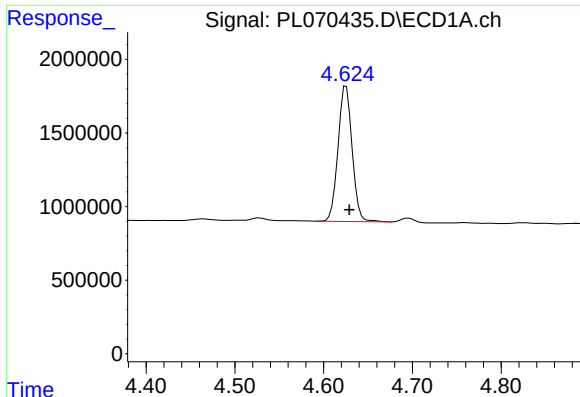

#1 Tetrachloro-m-xylene


R.T.: 4.625 min
Delta R.T.: -0.004 min
Response: 10147857
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

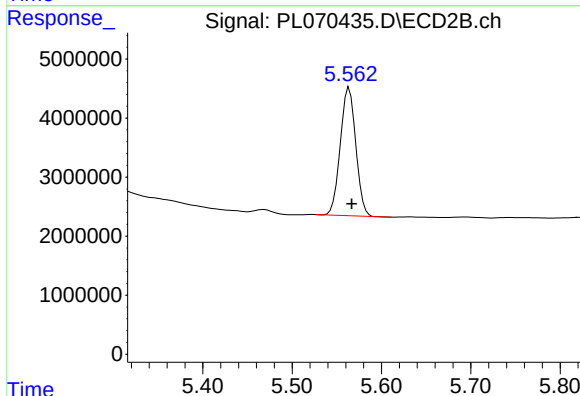


#1 Tetrachloro-m-xylene

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 26032589
Conc: 19.68 ng/ml

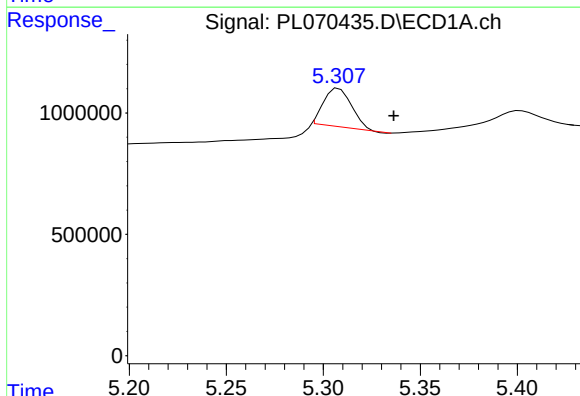


#2 alpha-BHC

R.T.: 5.308 min
Delta R.T.: -0.028 min
Response: 1572284
Conc: 2.12 ng/ml

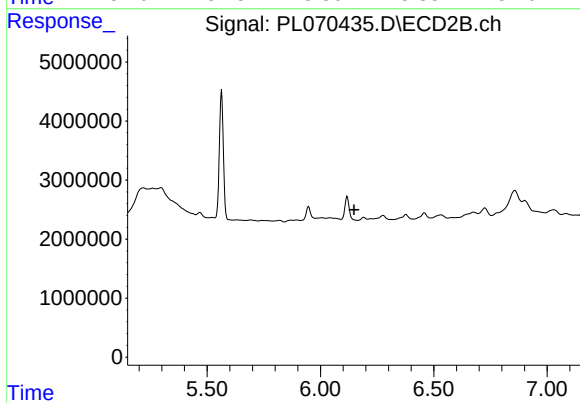

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

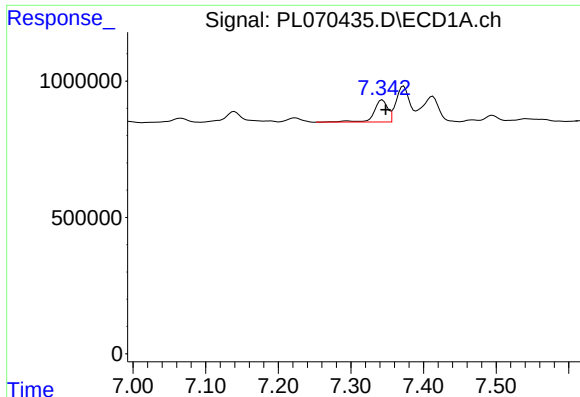

#10 gamma-Chlordane


R.T.: 7.343 min
Delta R.T.: -0.005 min
Response: 1054016
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

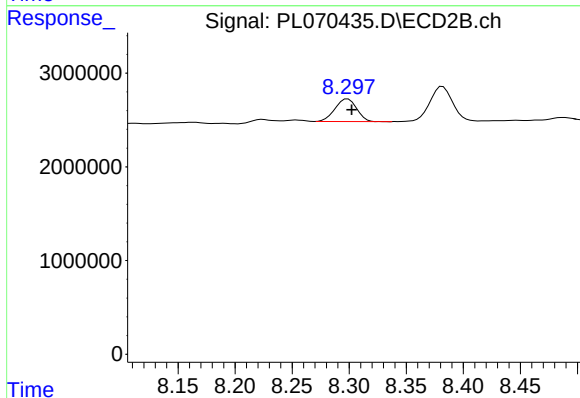


#10 gamma-Chlordane

R.T.: 8.299 min
Delta R.T.: -0.003 min
Response: 3204111
Conc: 2.00 ng/ml

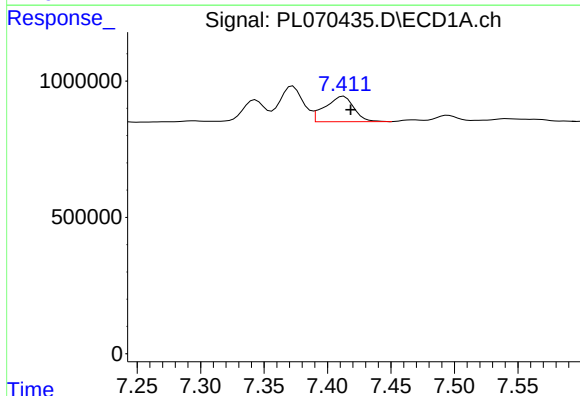


#11 alpha-Chlordane

R.T.: 7.413 min
Delta R.T.: -0.006 min
Response: 1477468
Conc: 2.03 ng/ml

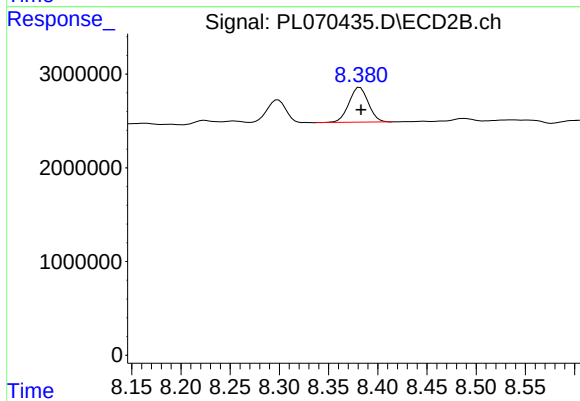

#11 alpha-Chlordane


R.T.: 8.382 min
Delta R.T.: -0.001 min
Response: 5099184
Conc: 3.23 ng/ml

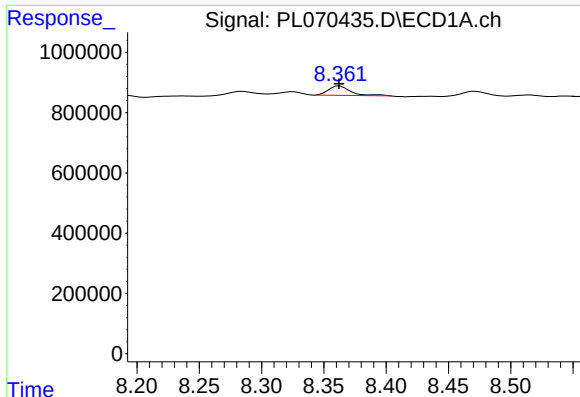

#15 Endosulfan II


R.T.: 8.363 min
Delta R.T.: 0.000 min
Response: 379651
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

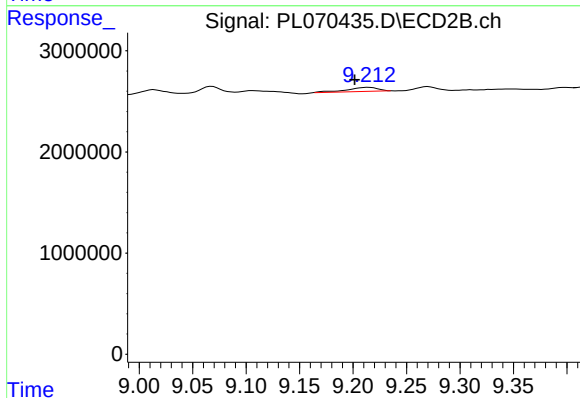


#15 Endosulfan II

R.T.: 9.214 min
Delta R.T.: 0.013 min
Response: 850600
Conc: 0.71 ng/ml

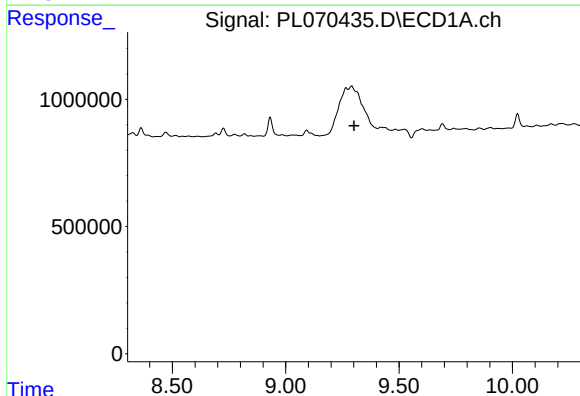


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.301 min
Response: 0
Conc: N.D.

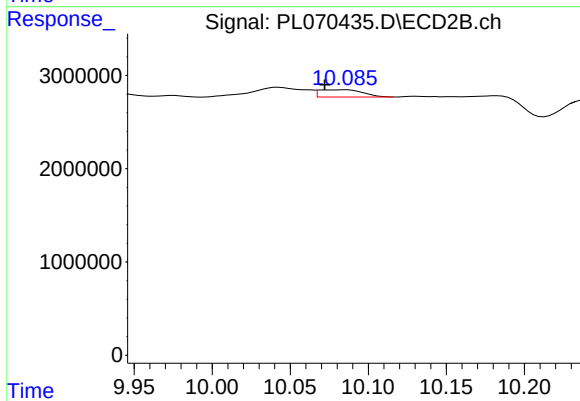

#21 Endrin ketone


R.T.: 10.086 min
Delta R.T.: 0.014 min
Response: 1502406
Conc: 1.12 ng/ml

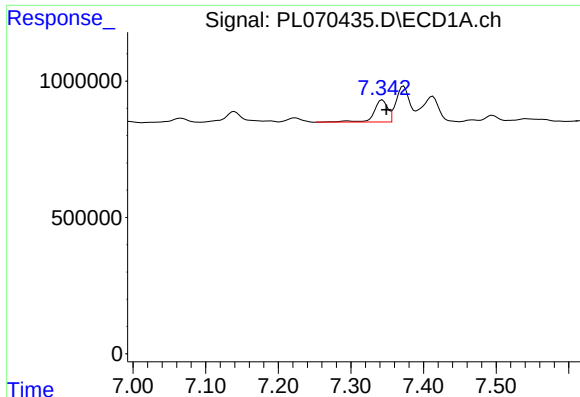

#25 Chlordane-3


R.T.: 7.343 min
Delta R.T.: -0.006 min
Response: 1054016
Conc: 15.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

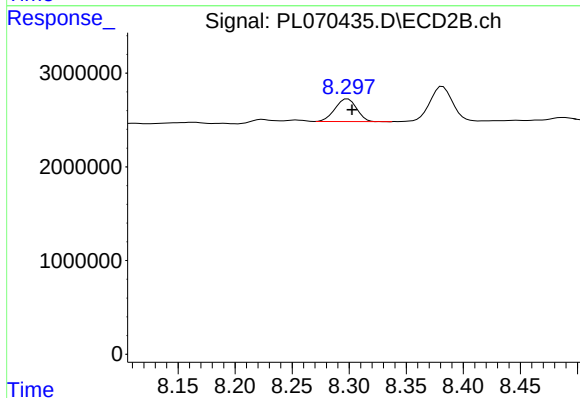


#25 Chlordane-3

R.T.: 8.299 min
Delta R.T.: -0.004 min
Response: 3204111
Conc: 15.13 ng/ml

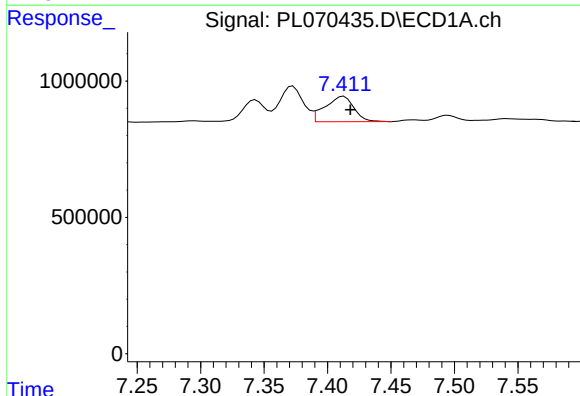


#26 Chlordane-4

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 1477468
Conc: 20.22 ng/ml

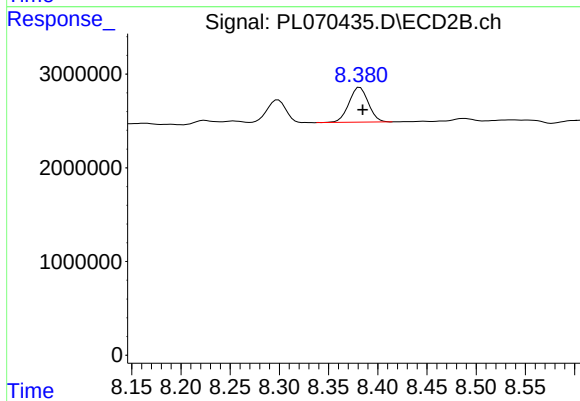

#26 Chlordane-4


R.T.: 8.382 min
Delta R.T.: -0.003 min
Response: 5099184
Conc: 20.06 ng/ml

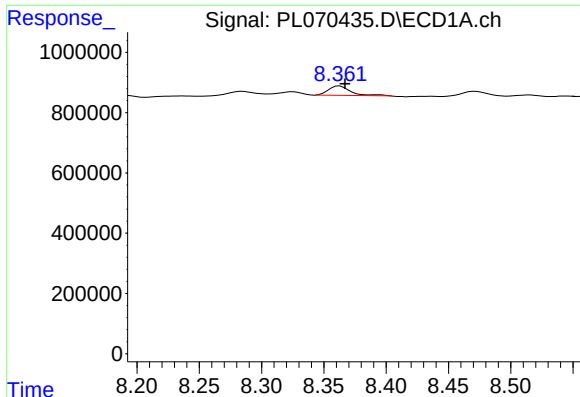

#27 Chlordane-5


R.T.: 8.363 min
Delta R.T.: -0.004 min
Response: 379651
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

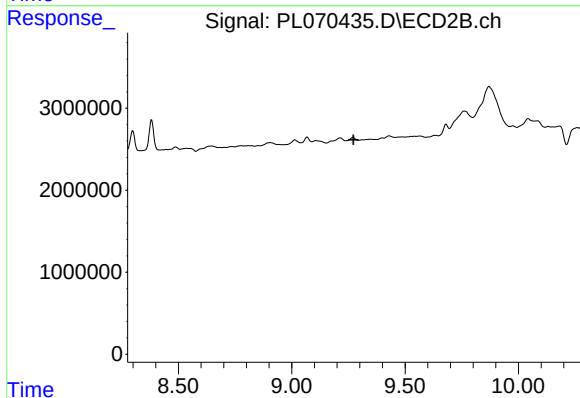


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.273 min
Response: 0
Conc: N.D.

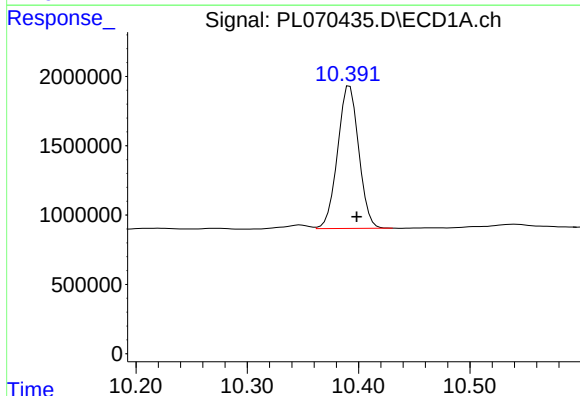

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.006 min
Response: 13553909
Conc: 19.59 ng/ml

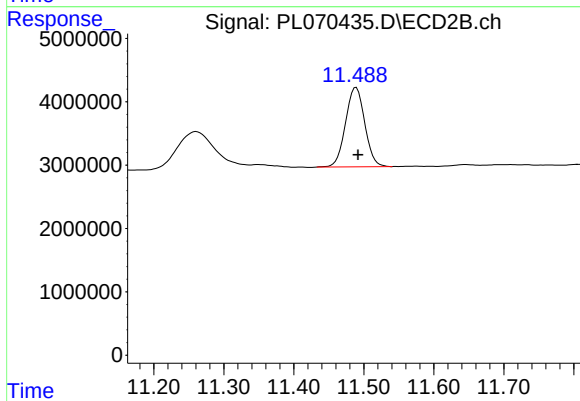

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.003 min
Response: 24010399
Conc: 19.84 ng/ml