

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102021\
 Data File : PL070430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 14:52
 Operator : AR\AJ
 Sample : M4280-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2081

Manual Integrations
 APPROVED

mohammad
 10/21/2021 1:41:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:48:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.629	5.565	7695829	19733766	15.380	14.920
28)	SA Decachlor...	10.395	11.490	12457142	20839893	18.002	17.221
Target Compounds							
12)	B 4,4'-DDE	7.627	8.569	2070105	4665345	3.253m	3.012
17)	MA 4,4'-DDT	8.475	9.427	1101591	2356179	1.801	1.803

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102021\
Data File : PL070430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 14:52
Operator : AR\AJ
Sample : M4280-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
2081


Manual Integrations
APPROVED

mohammad
10/21/2021 1:41:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:48:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

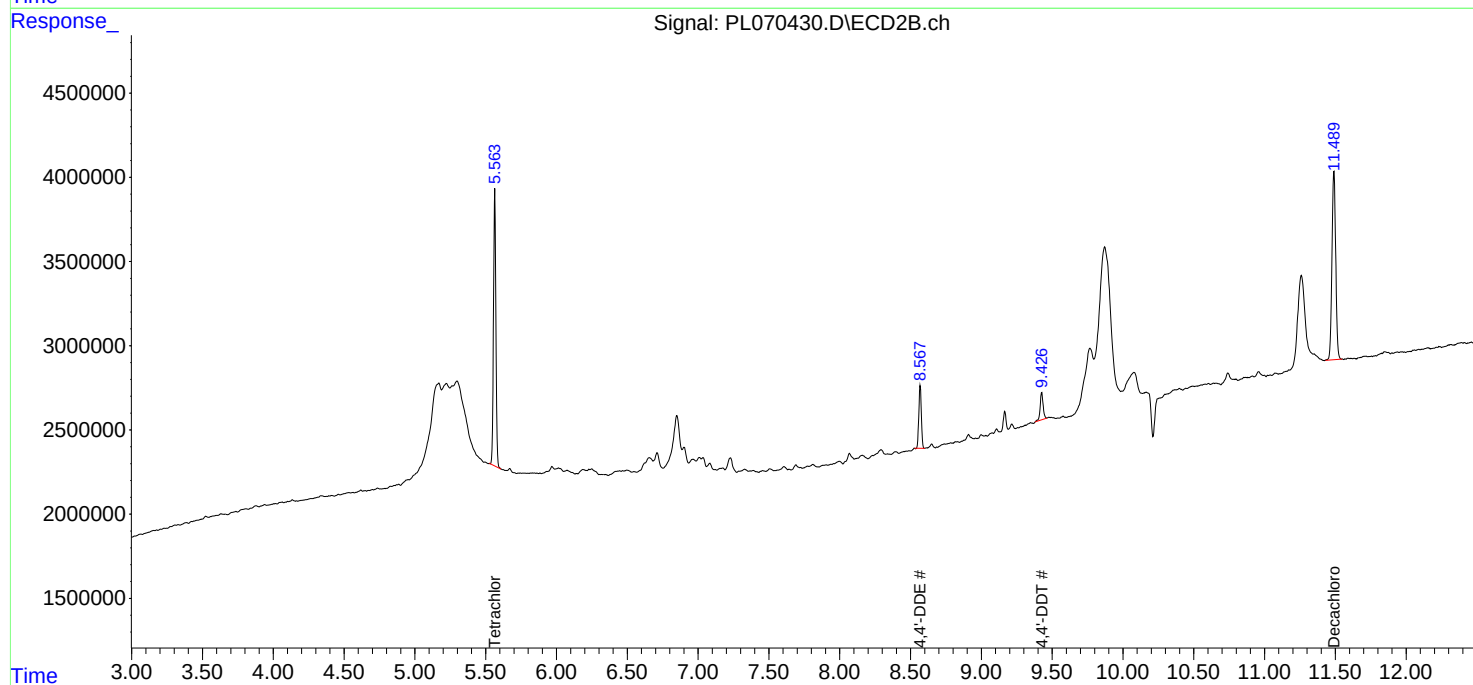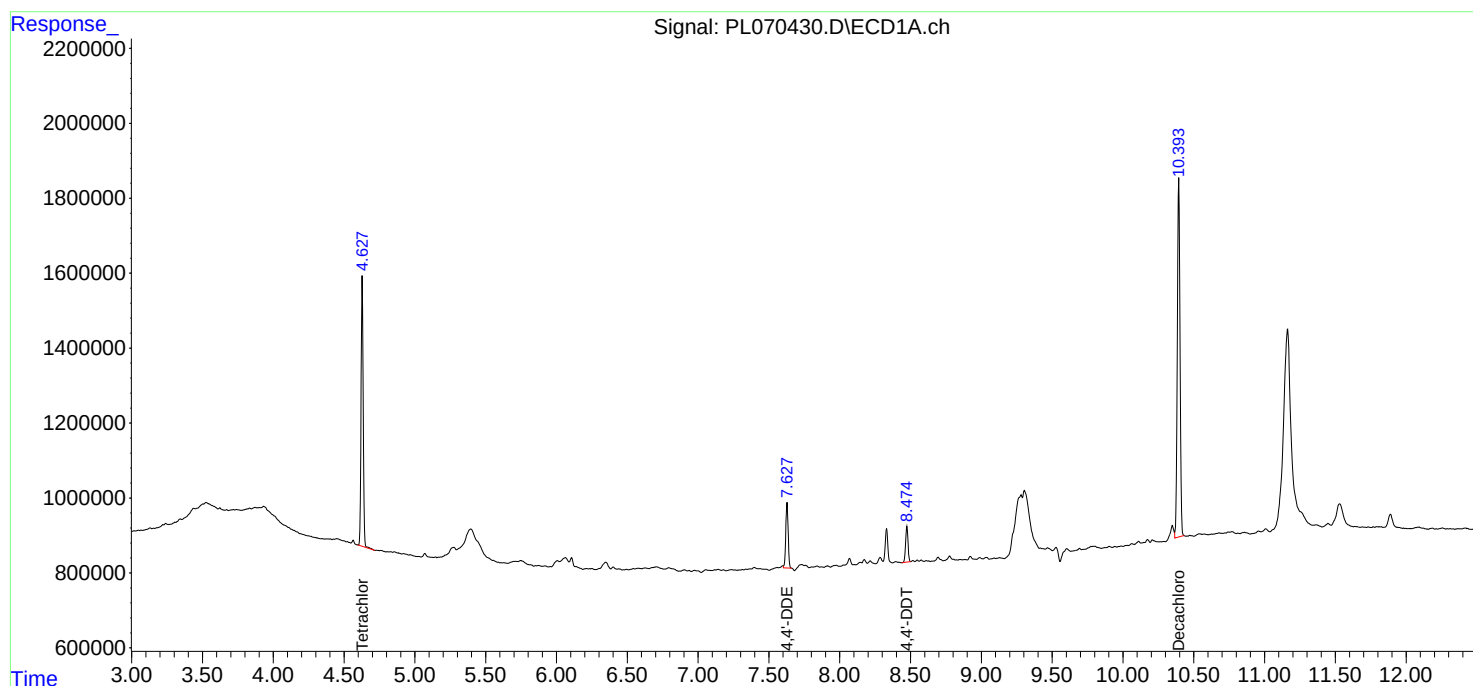

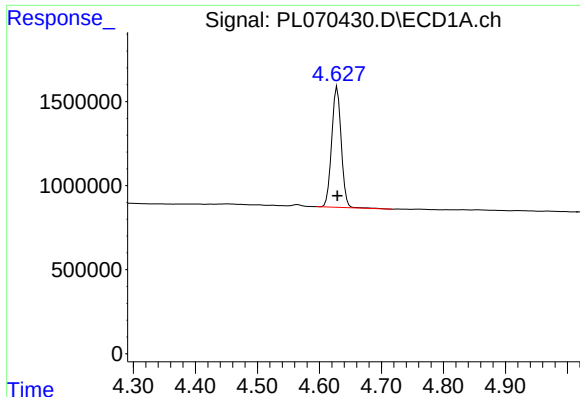


#1 Tetrachloro-m-xylene

R.T.: 4.629 min
Delta R.T.: 0.000 min
Response: 7695829
Conc: 15.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
2081


Manual Integrations
APPROVED

mohammad
10/21/2021 1:41:09 PM

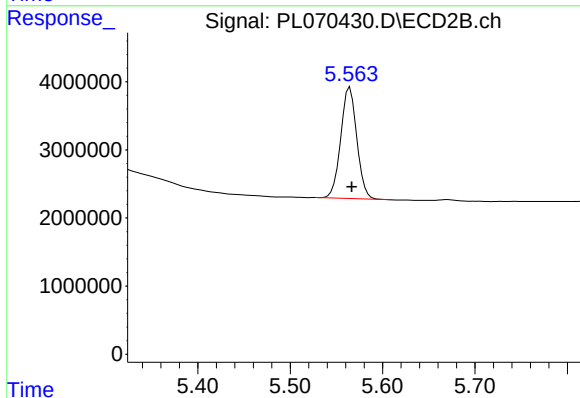


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 19733766
Conc: 14.92 ng/ml

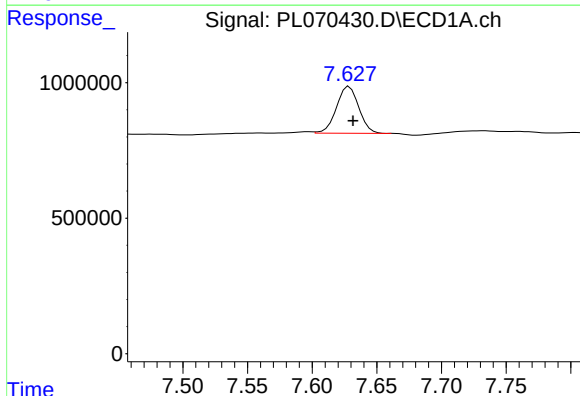


#12 4,4'-DDE

R.T.: 7.627 min
Delta R.T.: -0.004 min
Response: 2070105
Conc: 3.25 ng/ml m

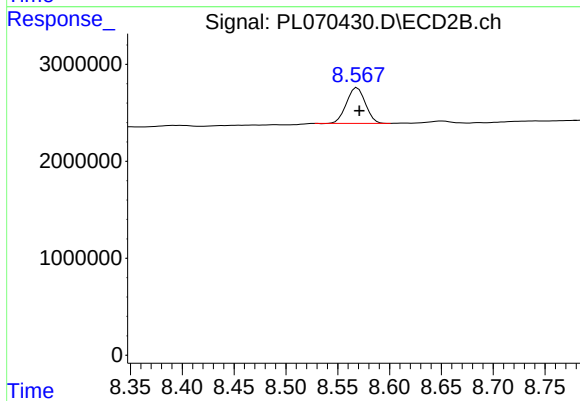

#12 4,4'-DDE

R.T.: 8.569 min
Delta R.T.: -0.002 min
Response: 4665345
Conc: 3.01 ng/ml

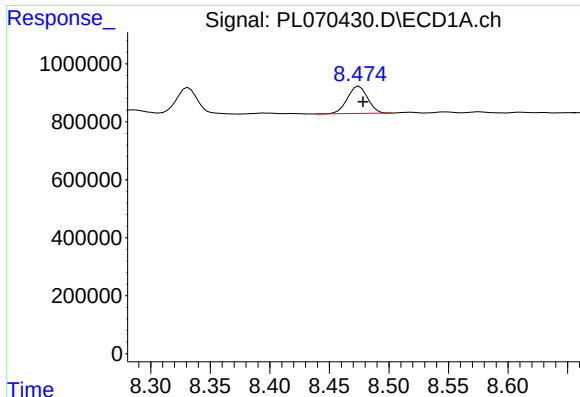


#17 4,4'-DDT

R.T.: 8.475 min
Delta R.T.: -0.003 min
Response: 1101591
Conc: 1.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
2081


Manual Integrations
APPROVED

mohammad
10/21/2021 1:41:09 PM

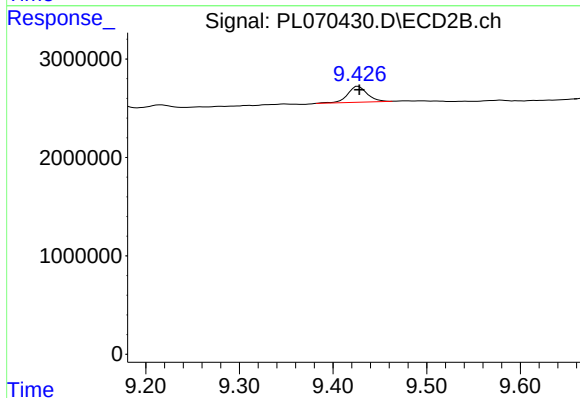


#17 4,4'-DDT

R.T.: 9.427 min
Delta R.T.: -0.001 min
Response: 2356179
Conc: 1.80 ng/ml

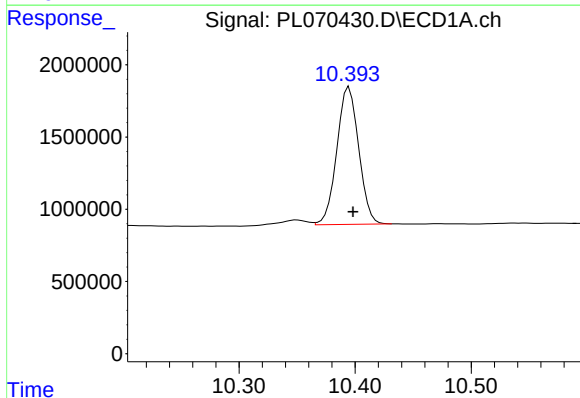

#28 Decachlorobiphenyl

R.T.: 10.395 min
Delta R.T.: -0.003 min
Response: 12457142
Conc: 18.00 ng/ml

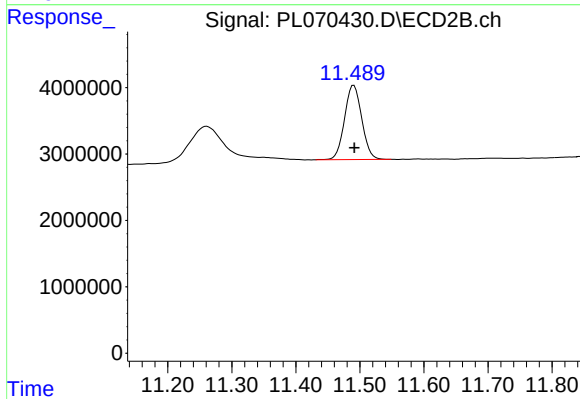

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: -0.001 min
Response: 20839893
Conc: 17.22 ng/ml