

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102021\
 Data File : PL070431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 15:09
 Operator : AR\AJ
 Sample : M4283-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-231

Manual Integrations
 APPROVED

mohammad
 10/21/2021 1:41:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:48:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.624	5.563	7326943	14712531	14.643m	11.124m
28) SA Decachlor...	10.393	11.489	9267504	15469889	13.393	12.783
Target Compounds						
10) B gamma-Chl...	7.342	8.299	1642624	3192794	2.268m	1.996m
11) B alpha-Chl...	7.412	8.379	1572076	3856771	2.158	2.445m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102021\
Data File : PL070431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 15:09
Operator : AR\AJ
Sample : M4283-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
VNJ-231


Manual Integrations
APPROVED

mohammad
10/21/2021 1:41:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:48:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

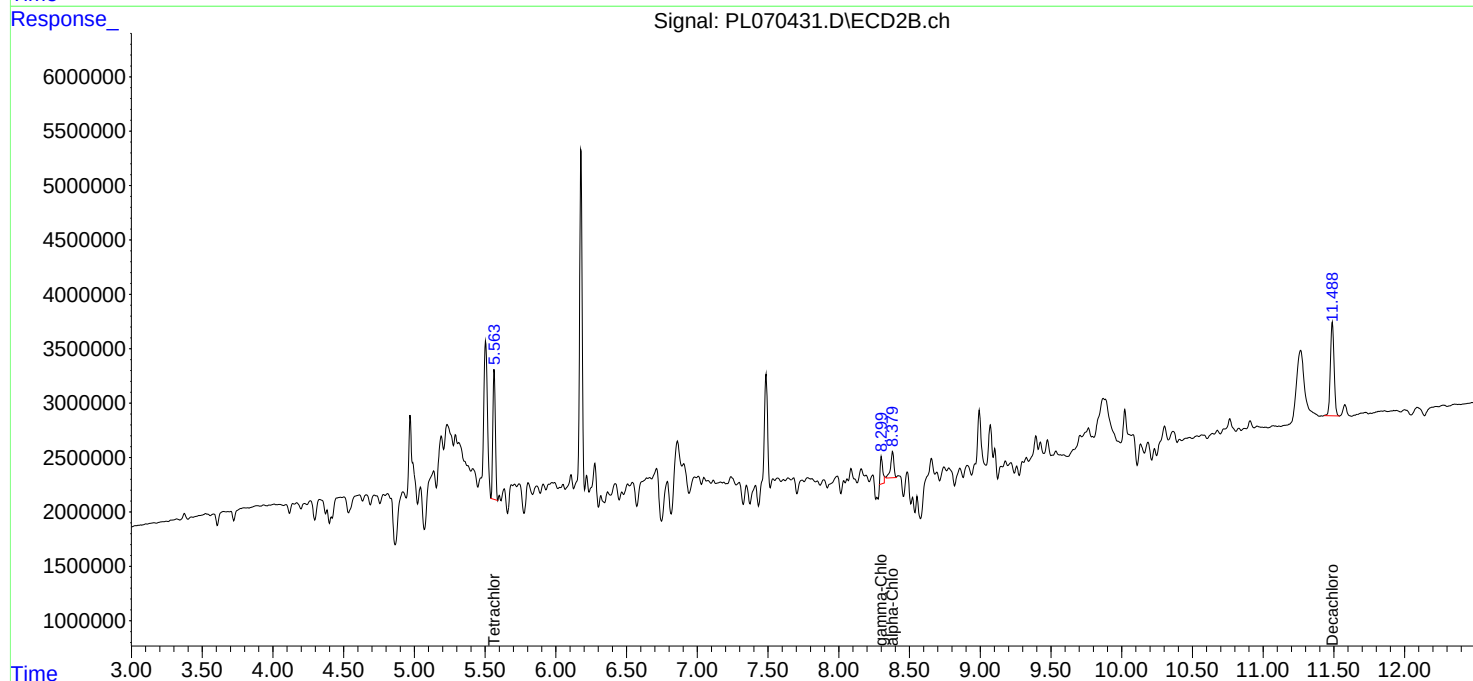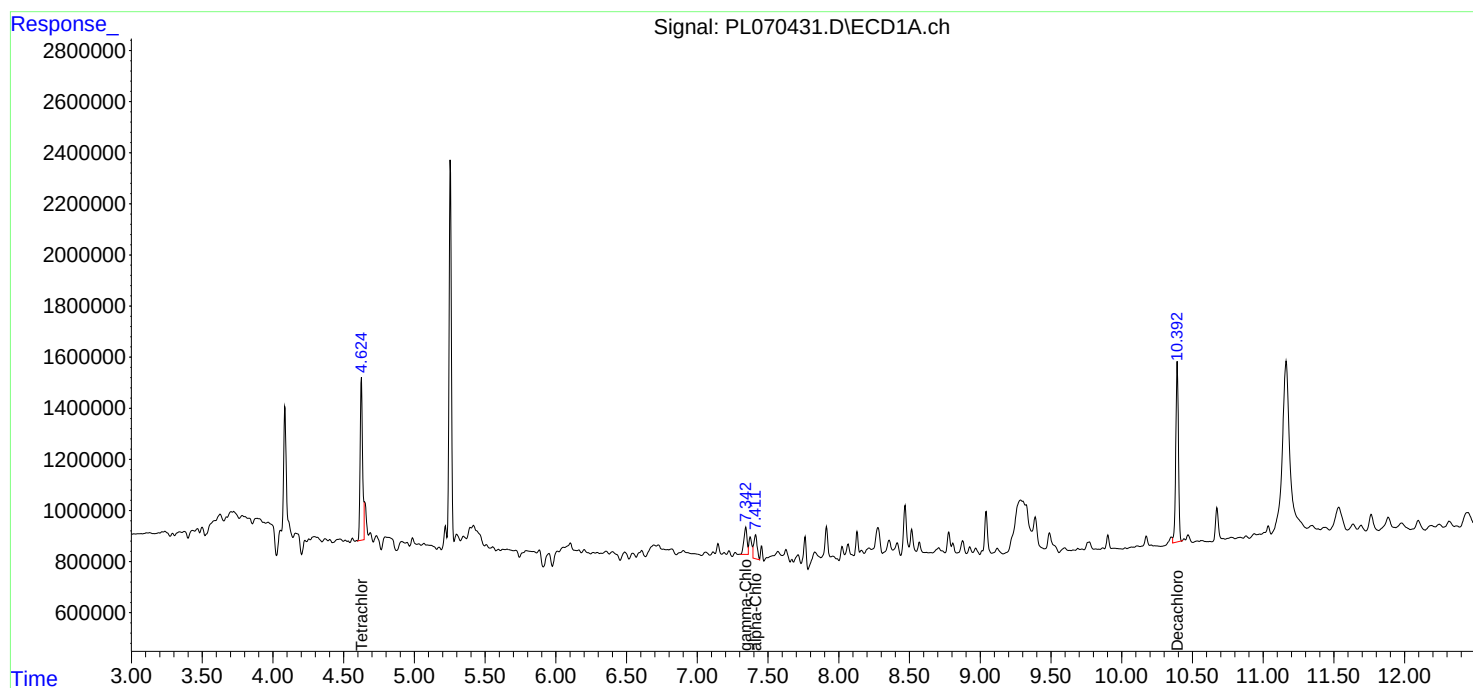

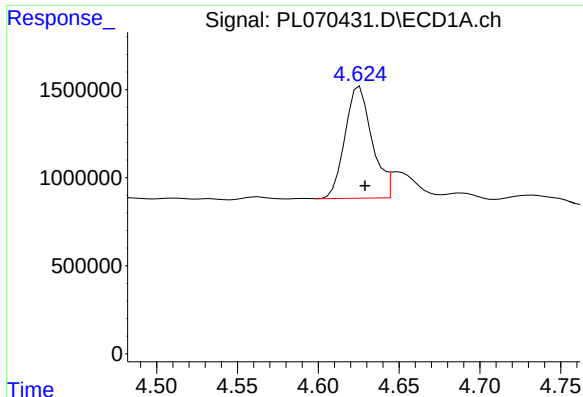


#1 Tetrachloro-m-xylene

R.T.: 4.624 min
Delta R.T.: -0.005 min
Response: 7326943
Conc: 14.64 ng/ml m

Instrument :
ECD_L
ClientSampleId :
VNJ-231


Manual Integrations
APPROVED

mohammad
10/21/2021 1:41:12 PM

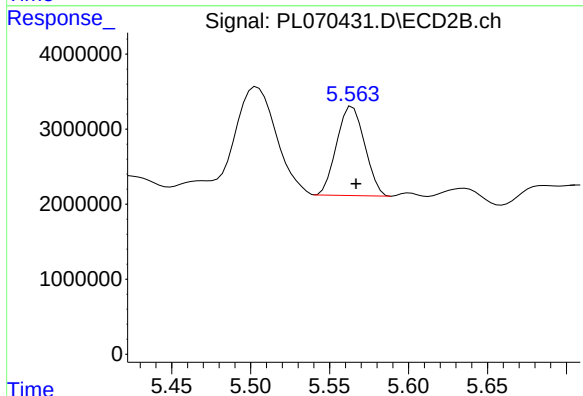


#1 Tetrachloro-m-xylene

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 14712531
Conc: 11.12 ng/ml m

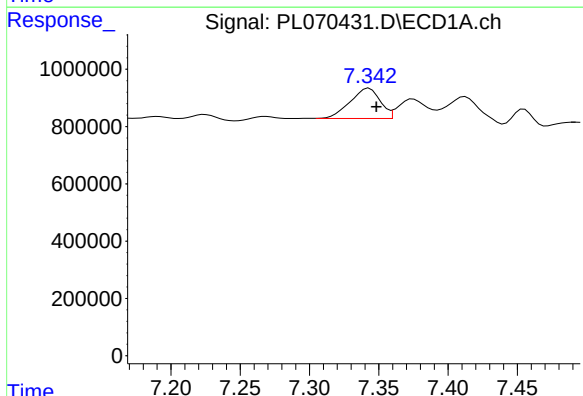


#10 gamma-Chlordane

R.T.: 7.342 min
Delta R.T.: -0.006 min
Response: 1642624
Conc: 2.27 ng/ml m

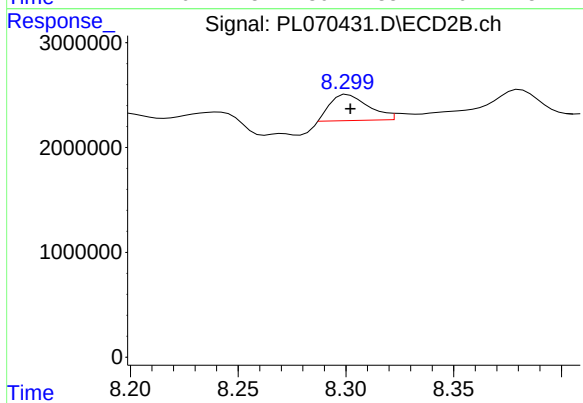

#10 gamma-Chlordane

R.T.: 8.299 min
Delta R.T.: -0.003 min
Response: 3192794
Conc: 2.00 ng/ml m

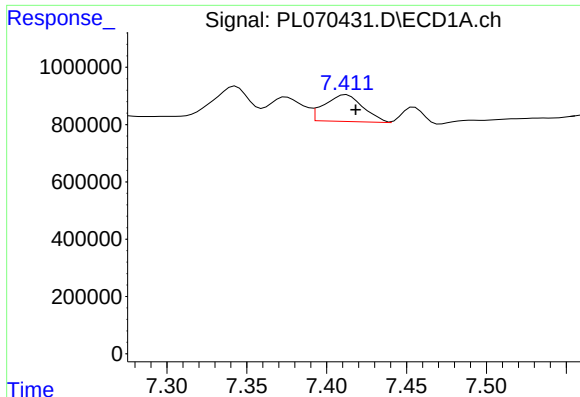


#11 alpha-Chlordane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 1572076
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-231


Manual Integrations
APPROVED

mohammad
10/21/2021 1:41:12 PM

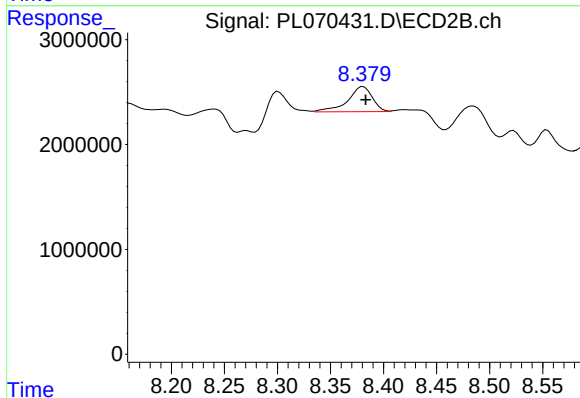


#11 alpha-Chlordane

R.T.: 8.379 min
Delta R.T.: -0.004 min
Response: 3856771
Conc: 2.45 ng/ml m

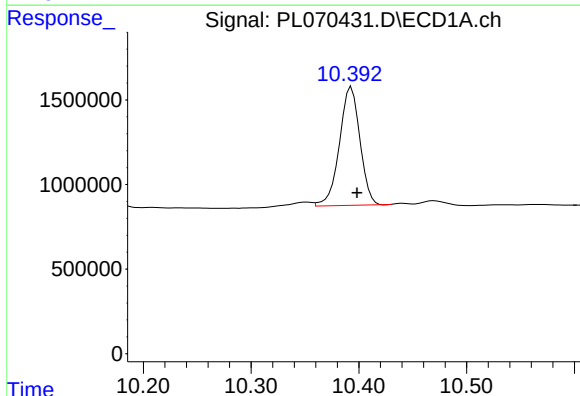

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: -0.005 min
Response: 9267504
Conc: 13.39 ng/ml

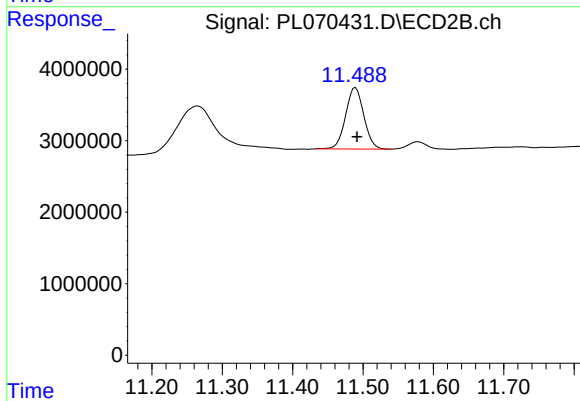

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.002 min
Response: 15469889
Conc: 12.78 ng/ml