

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102022\
 Data File : PL078427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 13:13
 Operator : AR\AJ
 Sample : N5133-03 (Sig #1); N5133-03RE (Sig #2)
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HAS-WATER-1013

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 13:57:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 15:30:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.619	25532701	41785601	15.450	15.808
28)	SA Decachlor...	8.908	7.717	15932014	24539599	10.320	11.289

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102022\
Data File : PL078427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 13:13
Operator : AR\AJ
Sample : N5133-03 (Sig #1); N5133-03RE (Sig #2)
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HAS-WATER-1013

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 13:57:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101222.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 15:30:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

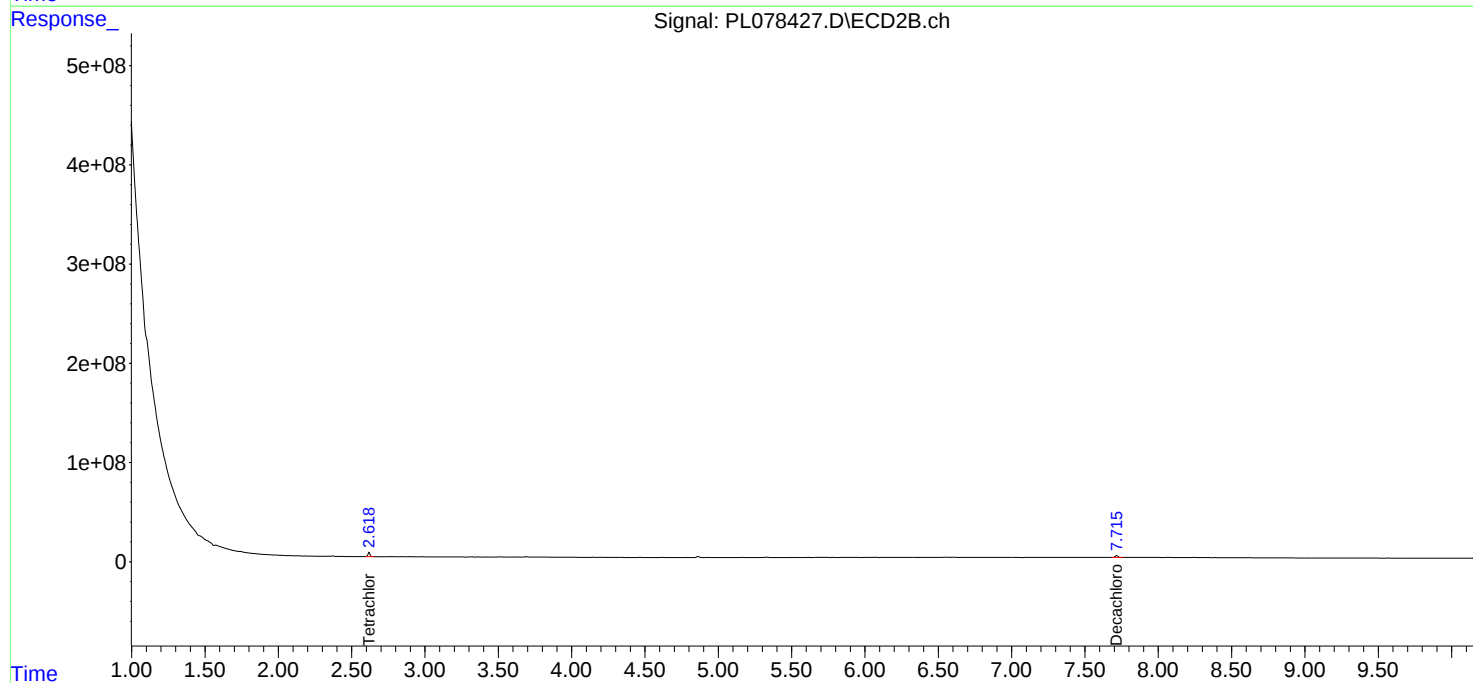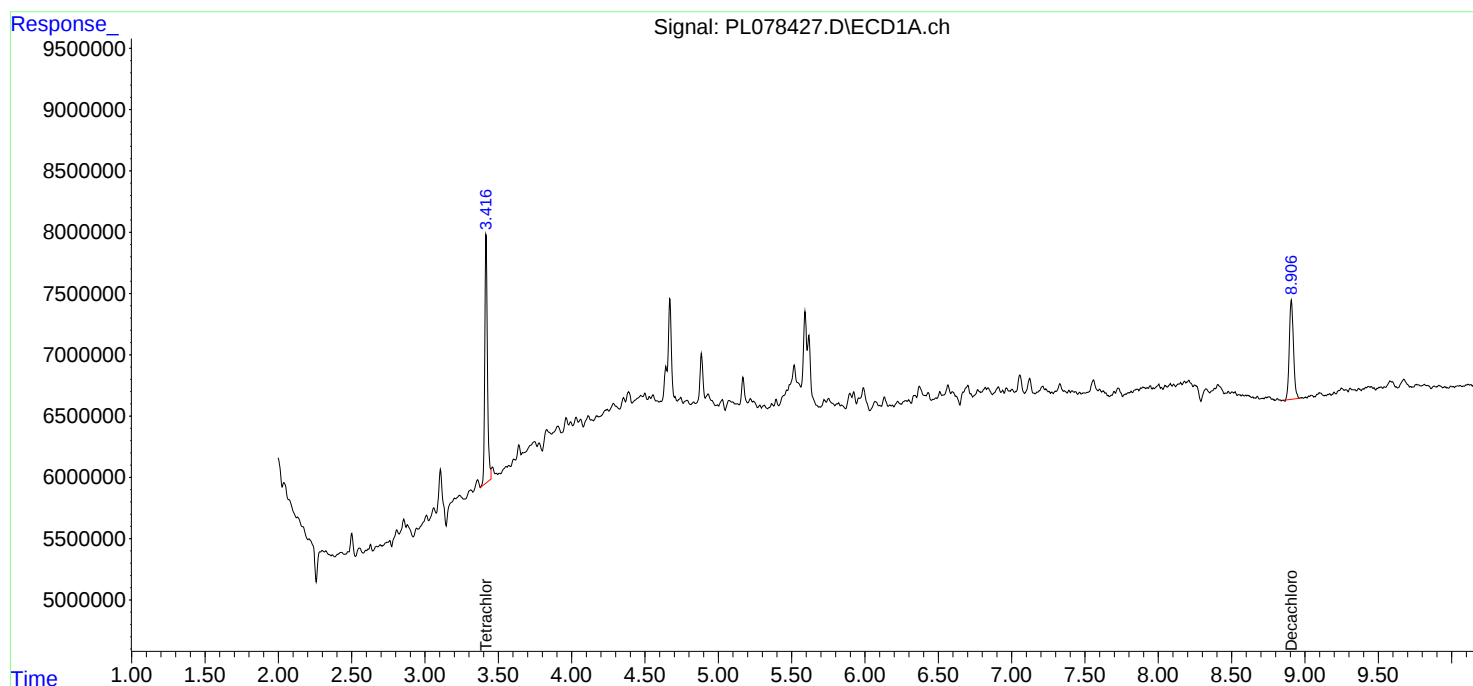


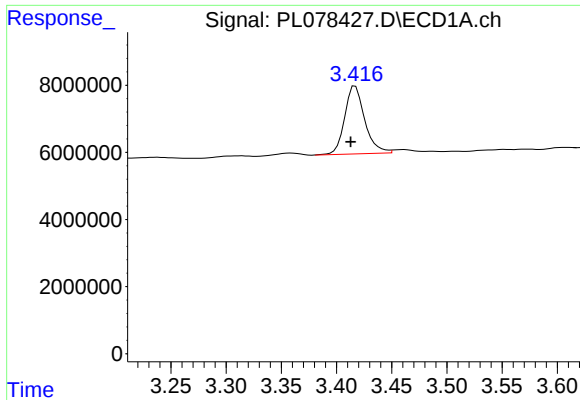

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.004 min
Response: 25532701
Conc: 15.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HAS-WATER-1013

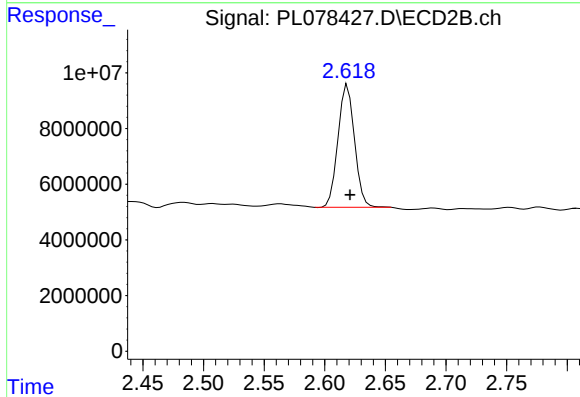


#1 Tetrachloro-m-xylene

R.T.: 2.619 min
Delta R.T.: -0.002 min
Response: 41785601
Conc: 15.81 ng/ml

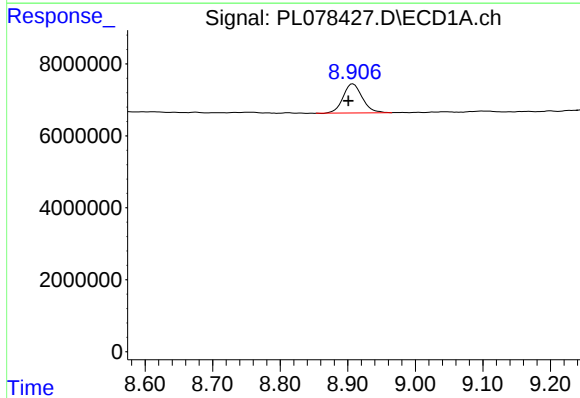

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.007 min
Response: 15932014
Conc: 10.32 ng/ml

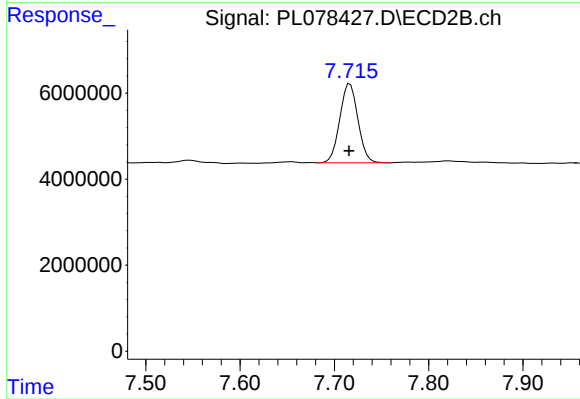

#28 Decachlorobiphenyl

R.T.: 7.717 min
Delta R.T.: 0.001 min
Response: 24539599
Conc: 11.29 ng/ml