

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102023\
 Data File : PL086062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 16:07
 Operator : AR\AJ
 Sample : 04957-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-F

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/23/2023
 Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 22:36:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.355	2.623	50062909	15810393	16.833m	16.926
2) SA Decachlor...	8.858	7.774	37901495	18084957	17.402	19.594
Target Compounds						
13) MA Dieldrin	6.156	5.198	3407467	1008680	1.037m	1.040

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102023\
Data File : PL086062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 16:07
Operator : AR\AJ
Sample : 04957-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MH-F


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/23/2023
Supervised By : Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 22:36:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

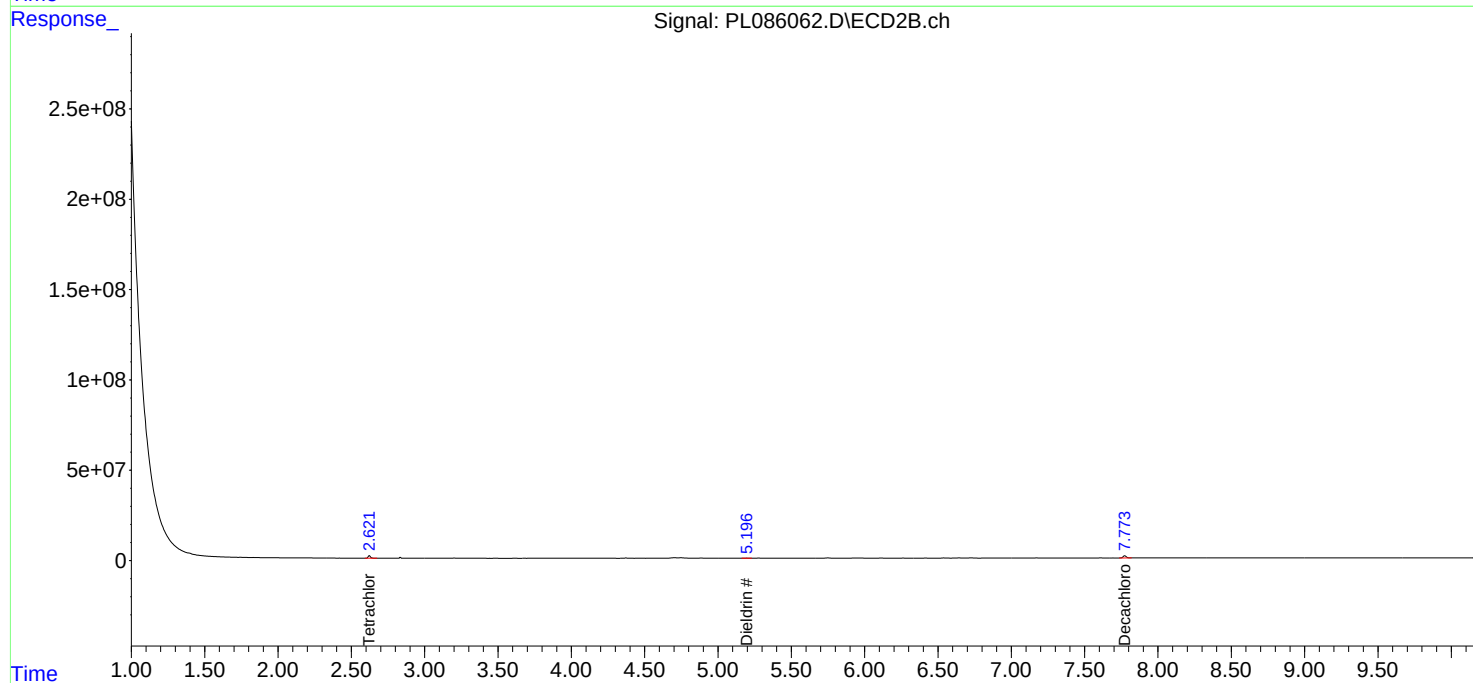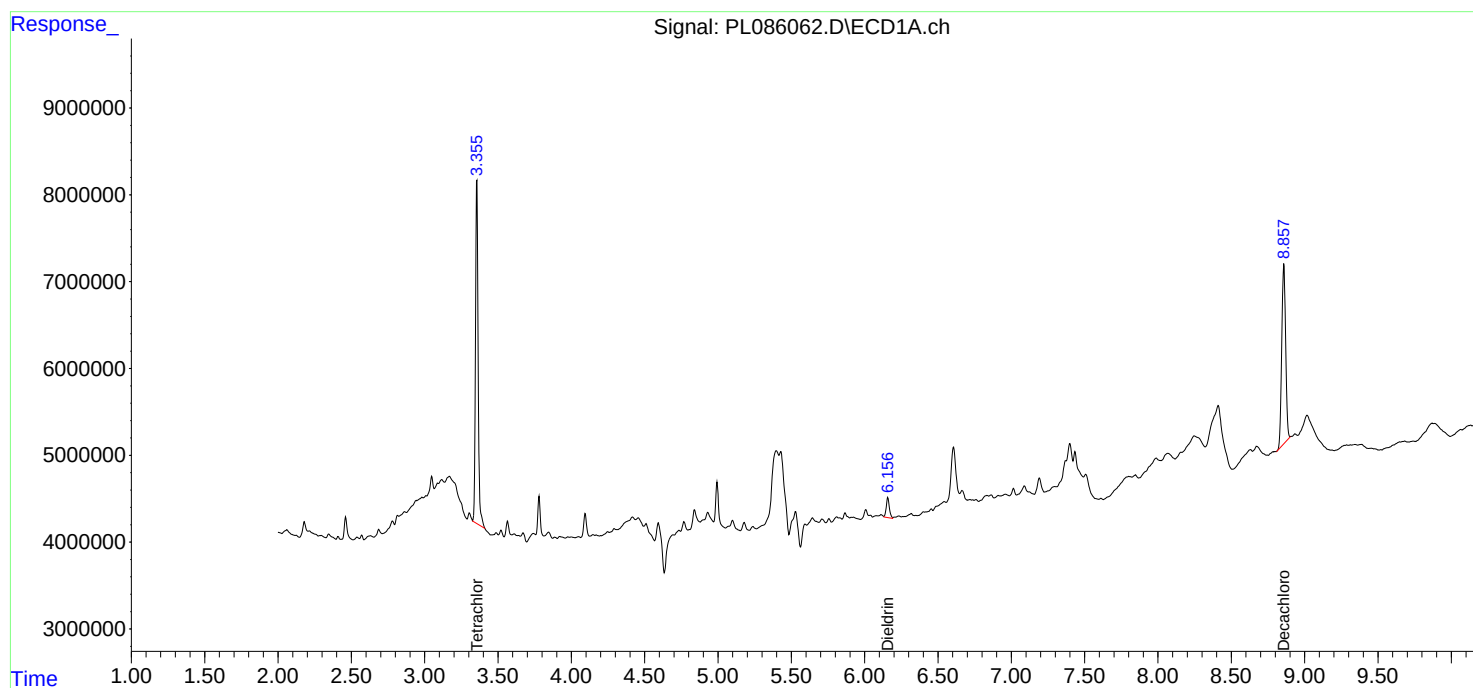

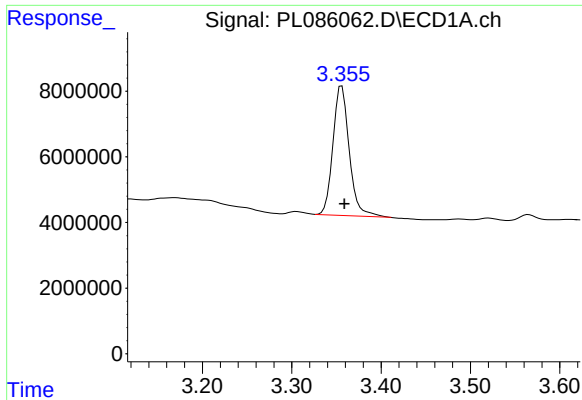


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.004 min
Response: 50062909
Conc: 16.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-F


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

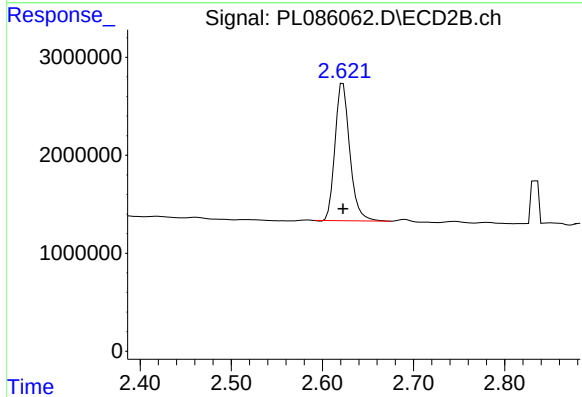


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 15810393
Conc: 16.93 ng/ml

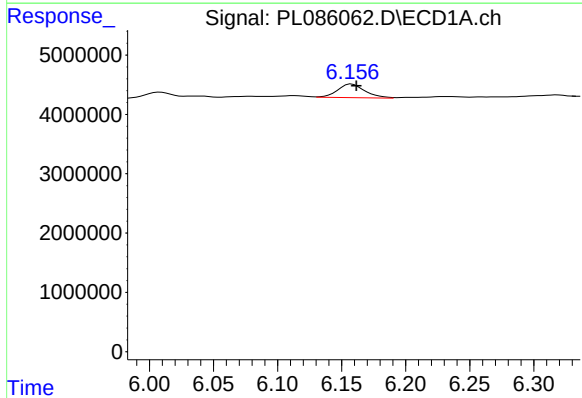


#13 Dieldrin

R.T.: 6.156 min
Delta R.T.: -0.005 min
Response: 3407467
Conc: 1.04 ng/ml m

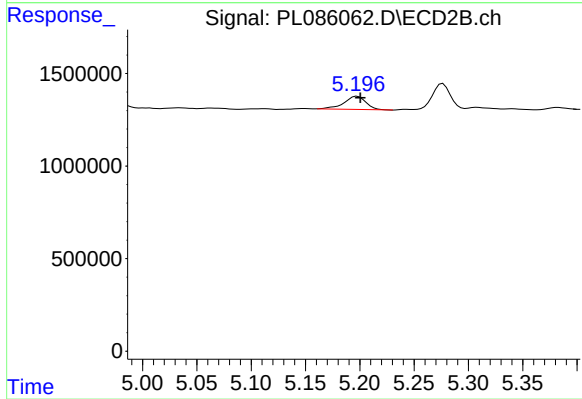

#13 Dieldrin

R.T.: 5.198 min
Delta R.T.: -0.003 min
Response: 1008680
Conc: 1.04 ng/ml

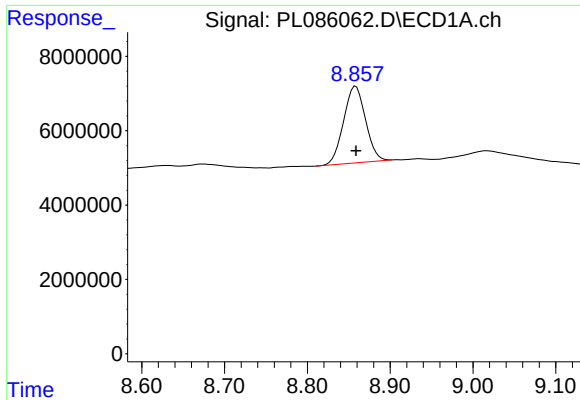


#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 37901495
Conc: 17.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-F

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

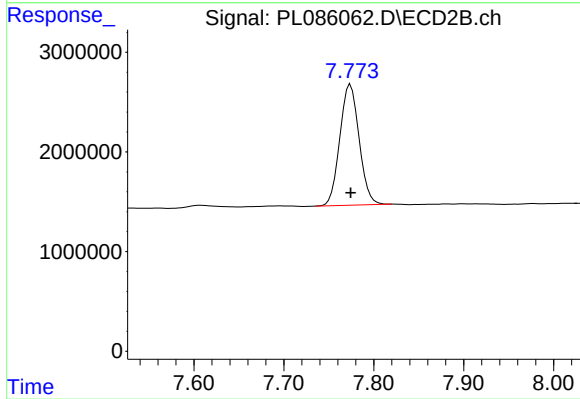

#28 Decachlorobiphenyl

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 18084957
Conc: 19.59 ng/ml