

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102119\
 Data File : PL053556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2019 22:50
 Operator : SG\AJ
 Sample : K5459-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:07:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	201.6E6	49265096	18.598	19.687
28)	SA Decachlor...	8.329	9.123	115.8E6	35521366	11.804	12.614
Target Compounds							
7)	B delta-BHC	0.000	5.104	0	1924330	N.D.	0.637 #
8)	B Heptachlo...	0.000	5.928	0	3198879	N.D.	1.097 #
11)	B alpha-Chl...	0.000	6.230	0	3029332	N.D.	1.038 #
15)	B Endosulfa...	0.000	6.972	0	7799408	N.D.	3.053 #
17)	MA 4,4'-DDT	0.000	7.151f	0	1362565	N.D.	0.589 #
19)	B Endosulfa...	0.000	7.308	0	1435769	N.D.	0.585 #
26)	Chlordane-4	0.000	6.230	0	3029332	N.D.	6.748 #
27)	Chlordane-5	0.000	7.039	0	3698574	N.D.	48.380 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102119\
Data File : PL053556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2019 22:50
Operator : SG\AJ
Sample : K5459-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:07:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

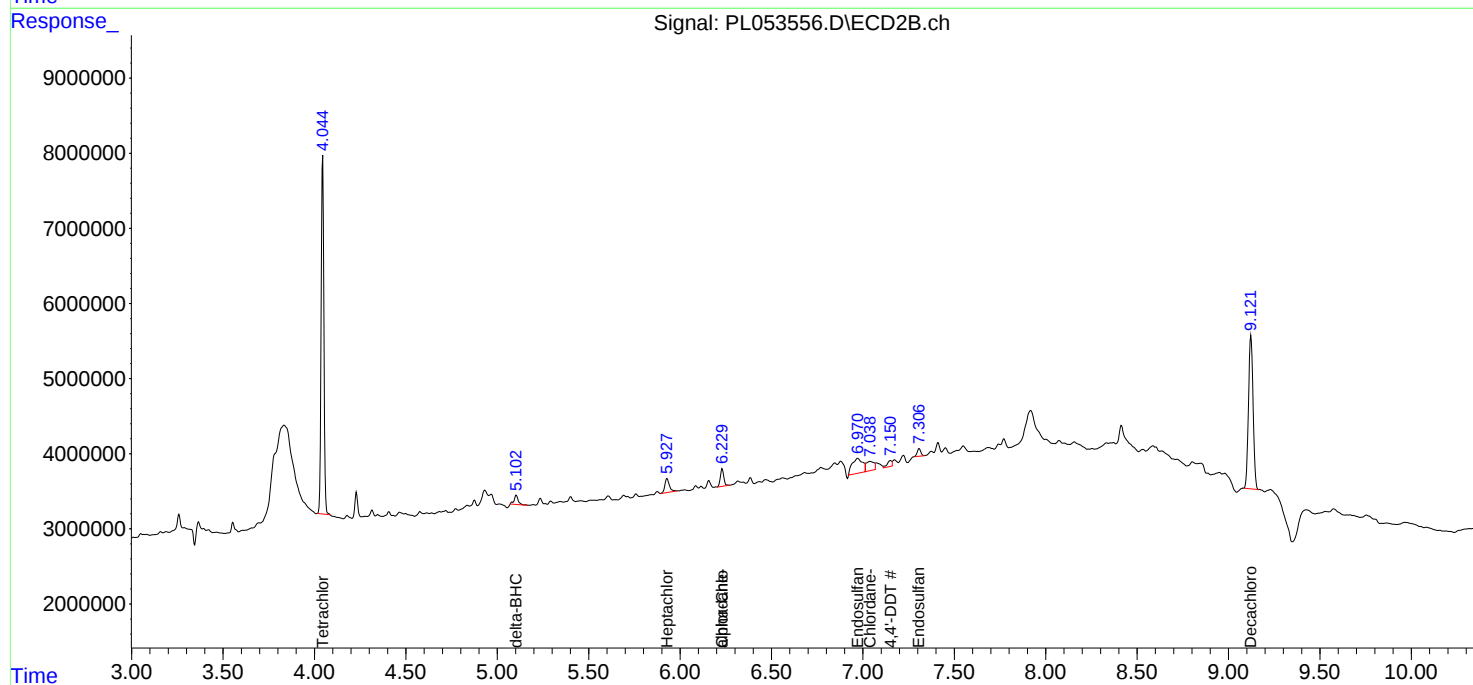


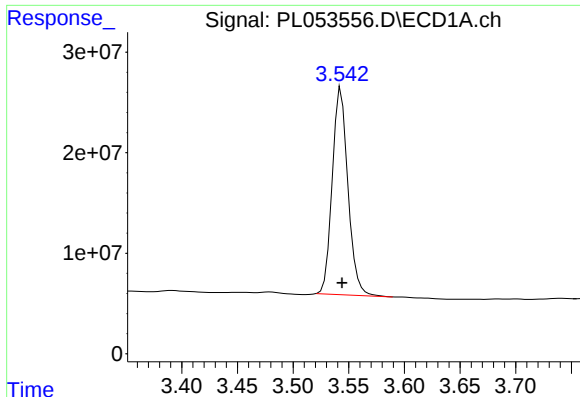

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 201587161
Conc: 18.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

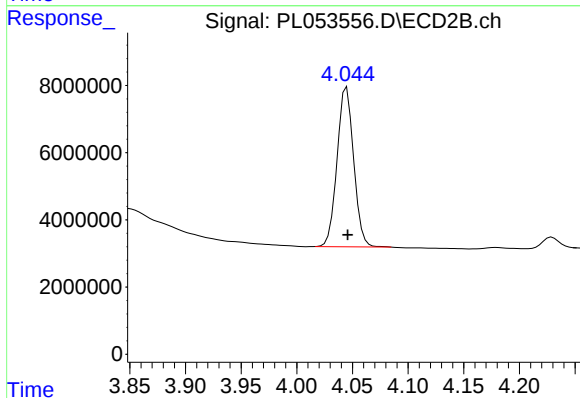


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 49265096
Conc: 19.69 ng/ml

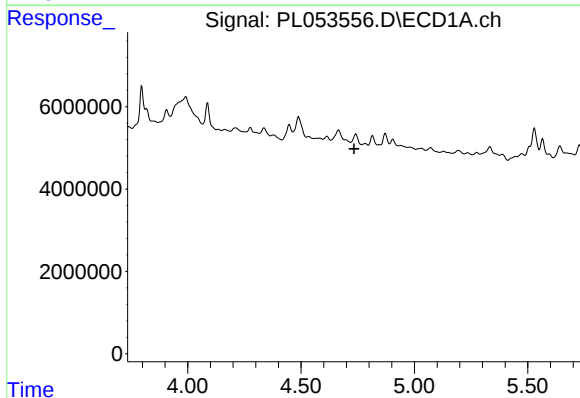


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.734 min
Response: 0
Conc: N.D.

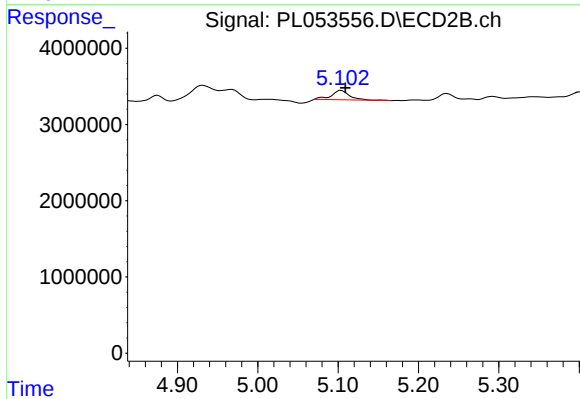

#7 delta-BHC


R.T.: 5.104 min
Delta R.T.: -0.005 min
Response: 1924330
Conc: 0.64 ng/ml

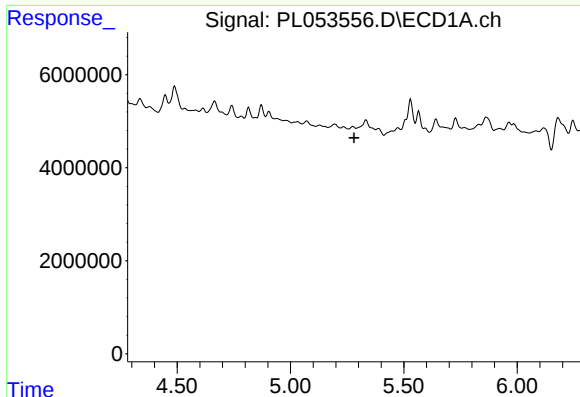

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

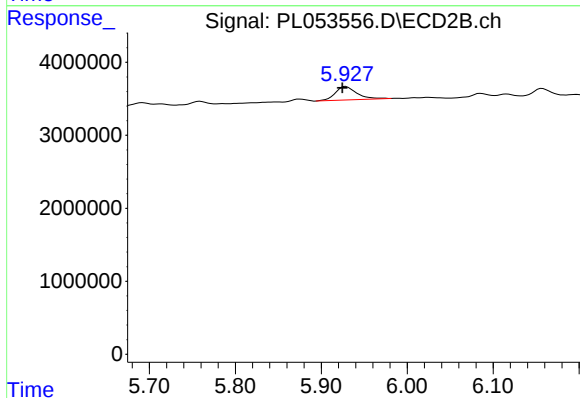


#8 Heptachlor epoxide

R.T.: 5.928 min
Delta R.T.: 0.004 min
Response: 3198879
Conc: 1.10 ng/ml

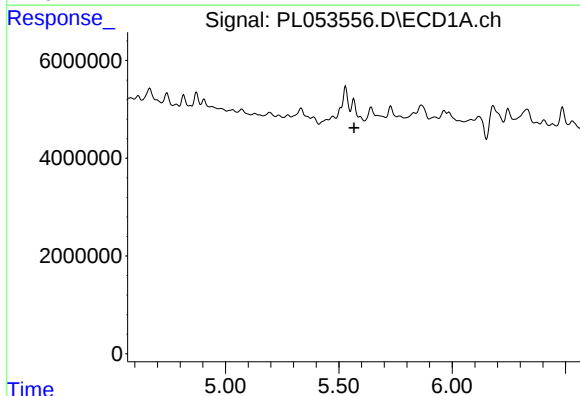


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

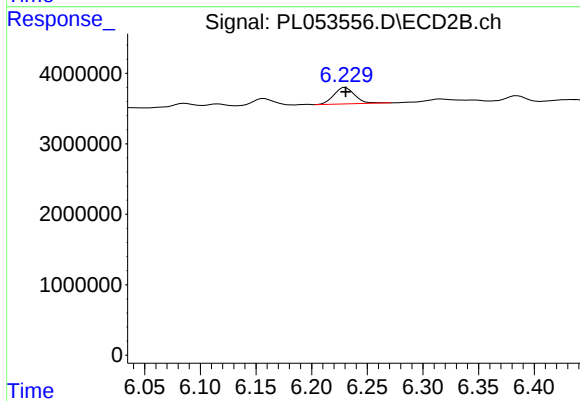

#11 alpha-Chlordane


R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 3029332
Conc: 1.04 ng/ml

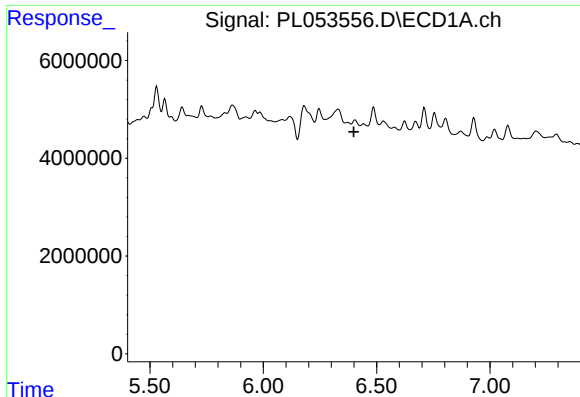

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

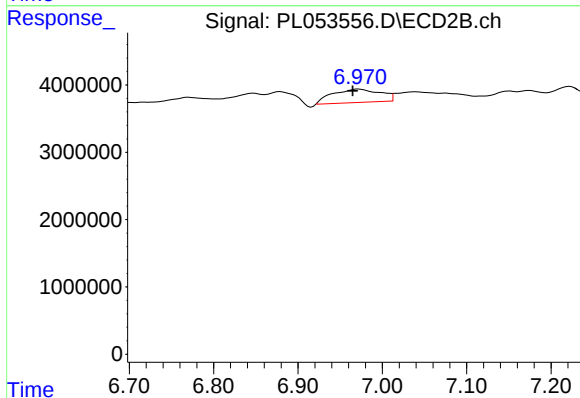


#15 Endosulfan II

R.T.: 6.972 min
Delta R.T.: 0.007 min
Response: 7799408
Conc: 3.05 ng/ml

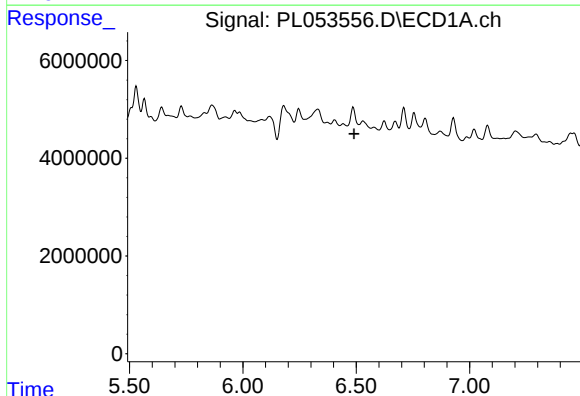


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

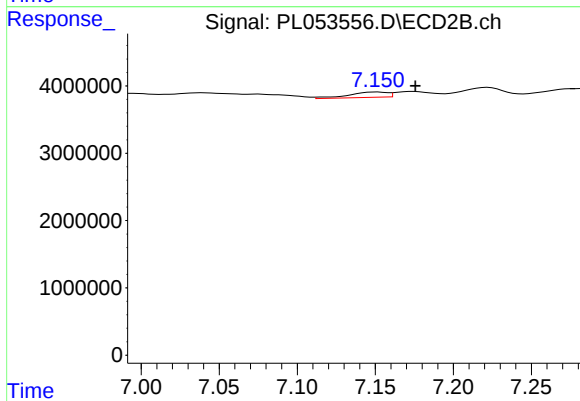

#17 4,4'-DDT


R.T.: 7.151 min
Delta R.T.: -0.025 min
Response: 1362565
Conc: 0.59 ng/ml

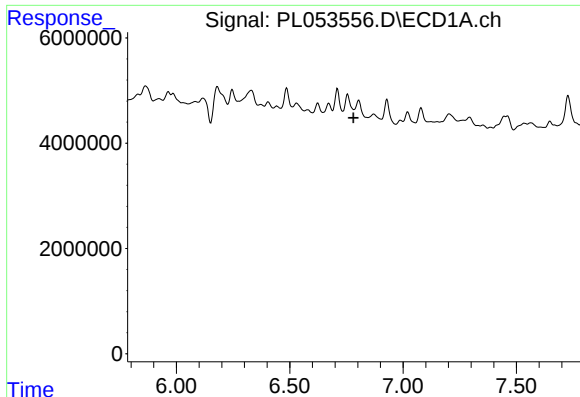

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.781 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

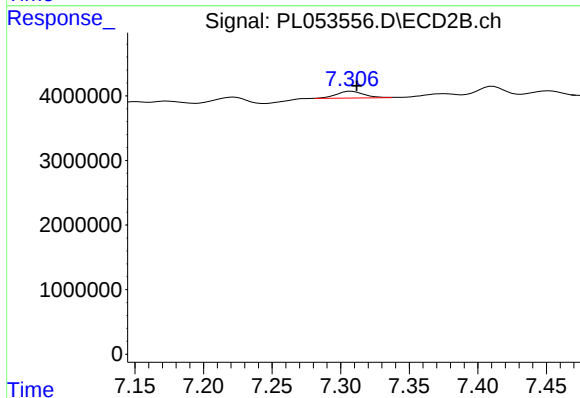


#19 Endosulfan Sulfate

R.T.: 7.308 min
Delta R.T.: -0.004 min
Response: 1435769
Conc: 0.59 ng/ml

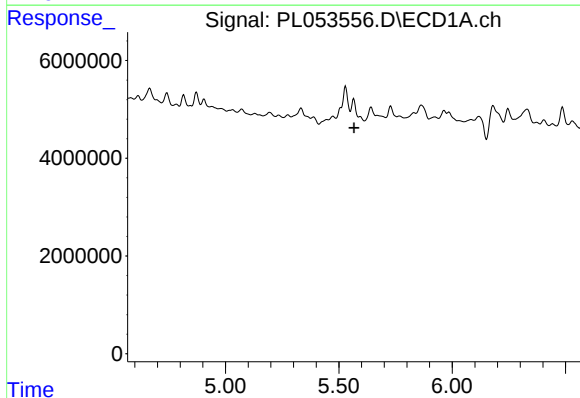


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.568 min
Response: 0
Conc: N.D.

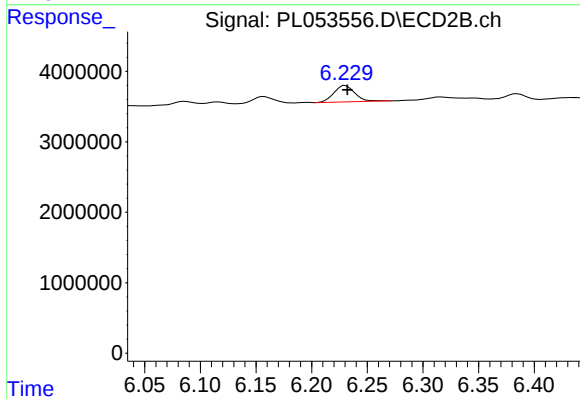

#26 Chlordane-4


R.T.: 6.230 min
Delta R.T.: -0.002 min
Response: 3029332
Conc: 6.75 ng/ml

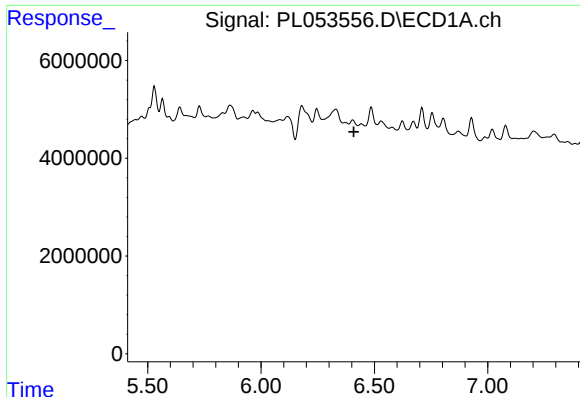

#27 Chloroform-5


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

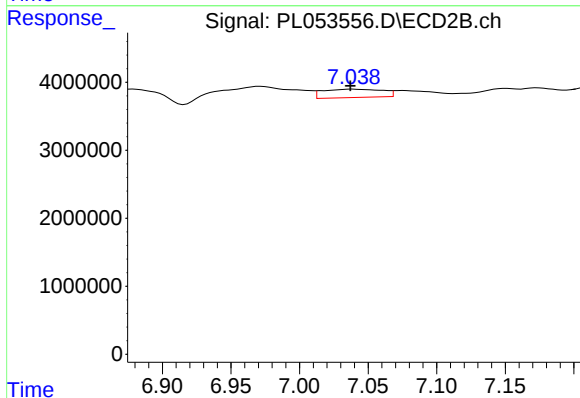


#27 Chloroform-5

R.T.: 7.039 min
Delta R.T.: 0.002 min
Response: 3698574
Conc: 48.38 ng/ml

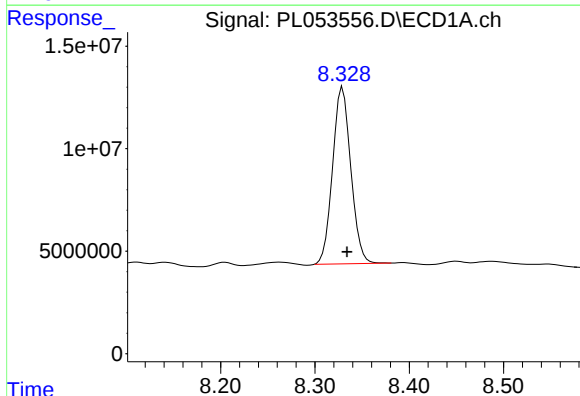

#28 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: -0.005 min
Response: 115813920
Conc: 11.80 ng/ml

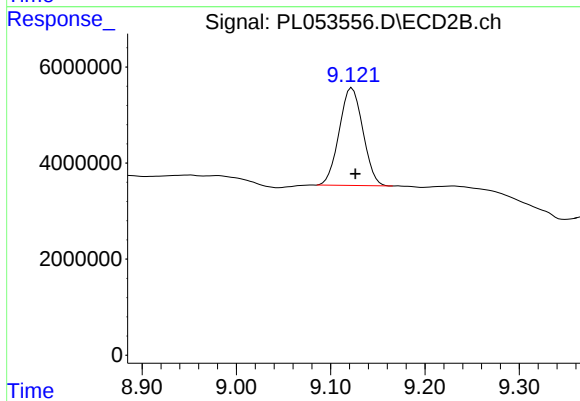

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.004 min
Response: 35521366
Conc: 12.61 ng/ml