

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102119\
 Data File : PL053536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2019 18:12
 Operator : SG\AJ
 Sample : K5146-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-101819

Manual Integrations
 APPROVED

Ankita
 10/22/2019 12:24:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:04:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.044	104.0E6	26245390	9.594	10.488
28)	SA Decachlor...	8.331	9.123	90701941	28931674	9.244	10.274
Target Compounds							
12)	B 4,4'-DDE	5.726	6.380	6907780	2311684	0.581m	0.821m#
17)	MA 4,4'-DDT	6.484	7.176	5166399	1189345	0.522m	0.514m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102119\
Data File : PL053536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2019 18:12
Operator : SG\AJ
Sample : K5146-08
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-101819


Manual Integrations
APPROVED

Ankita
10/22/2019 12:24:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:04:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

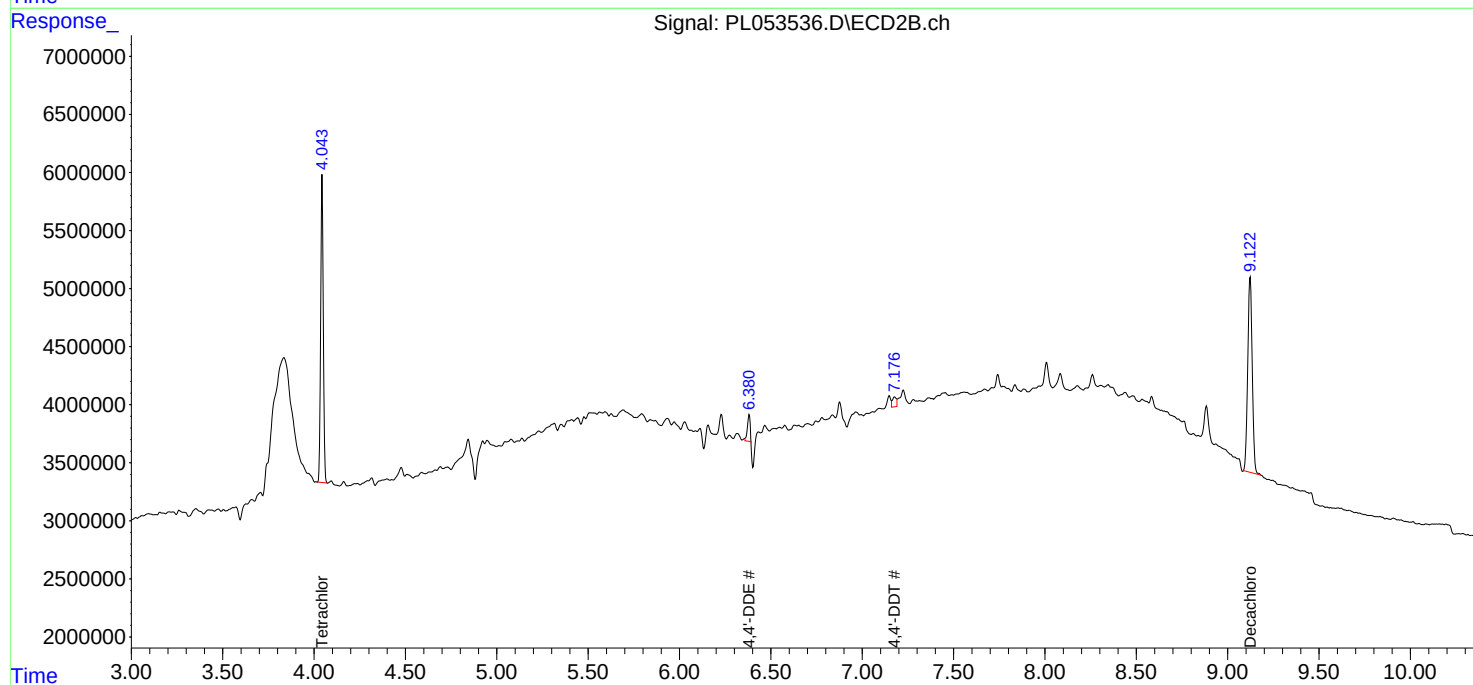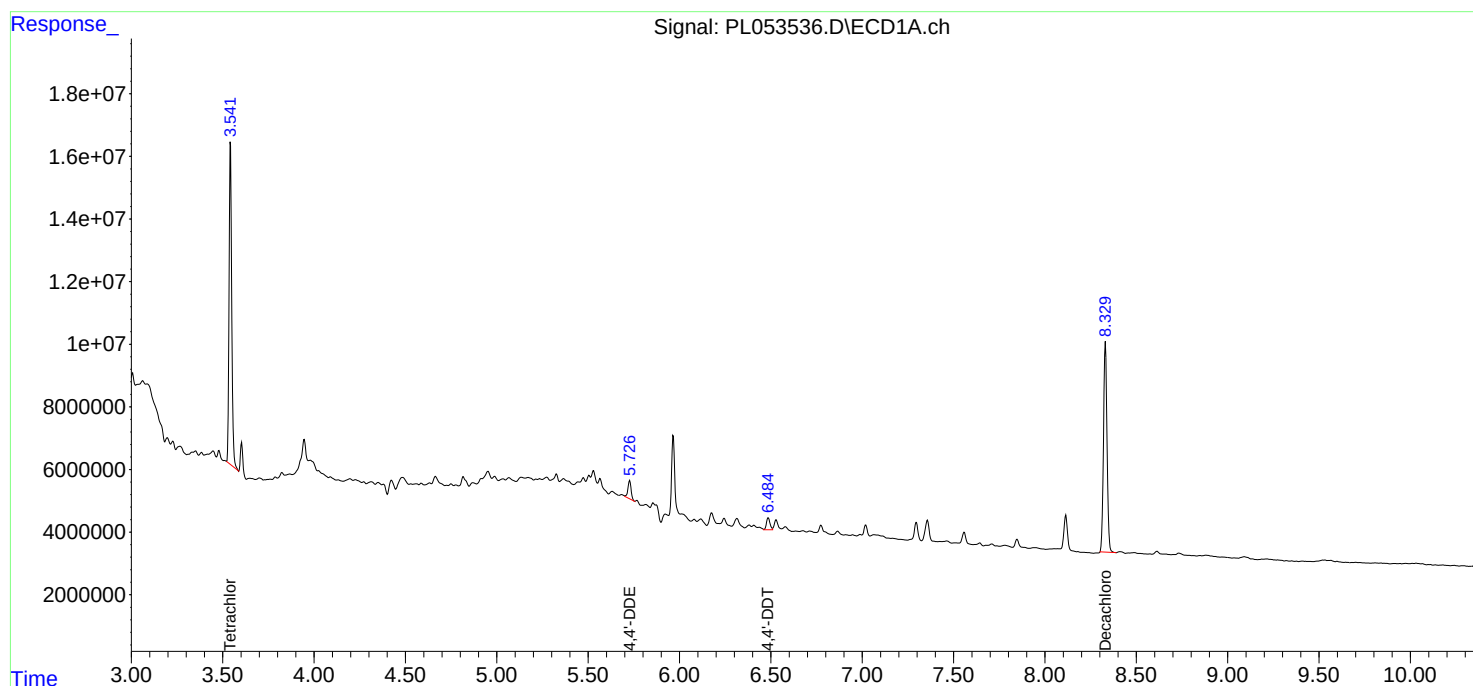

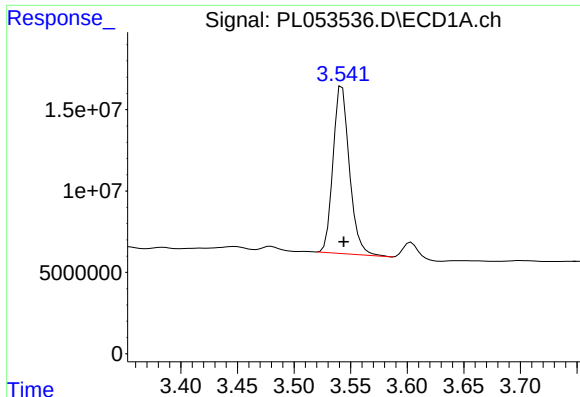


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 103996299
Conc: 9.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-101819


Manual Integrations
APPROVED

Ankita
10/22/2019 12:24:26 PM

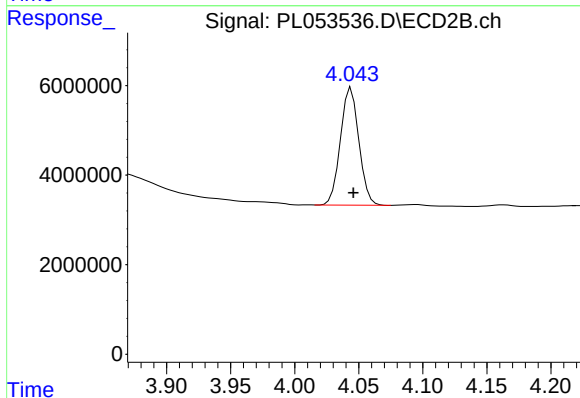


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 26245390
Conc: 10.49 ng/ml

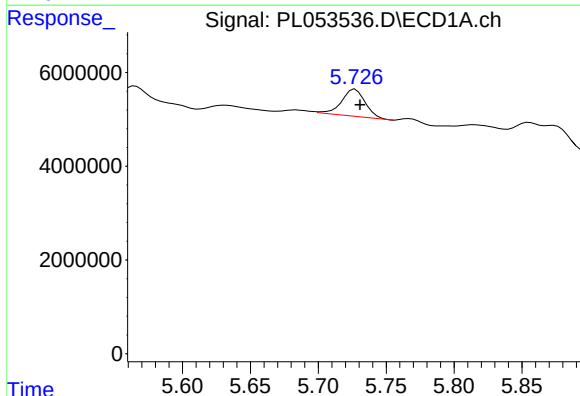


#12 4,4'-DDE

R.T.: 5.726 min
Delta R.T.: -0.005 min
Response: 6907780
Conc: 0.58 ng/ml m

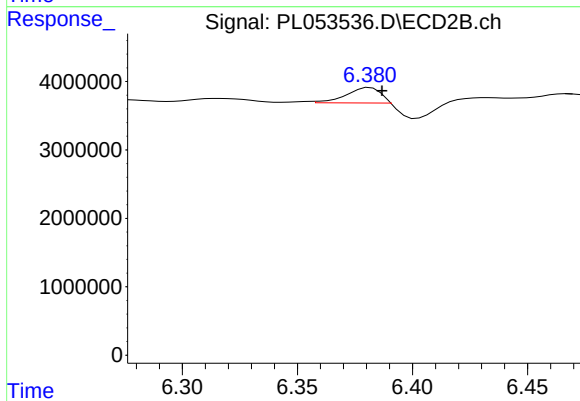

#12 4,4'-DDE

R.T.: 6.380 min
Delta R.T.: -0.006 min
Response: 2311684
Conc: 0.82 ng/ml m

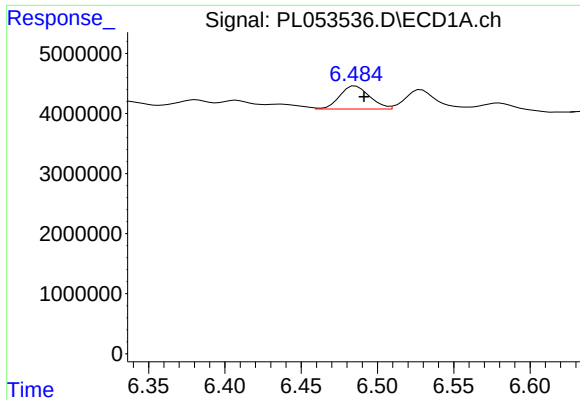


#17 4,4'-DDT

R.T.: 6.484 min
Delta R.T.: -0.007 min
Response: 5166399
Conc: 0.52 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-101819


Manual Integrations
APPROVED

Ankita
10/22/2019 12:24:26 PM

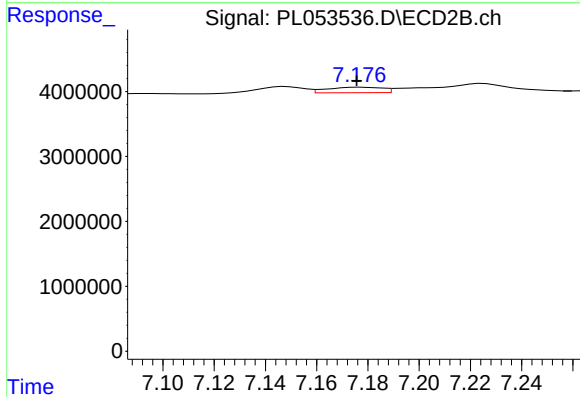


#17 4,4'-DDT

R.T.: 7.176 min
Delta R.T.: 0.000 min
Response: 1189345
Conc: 0.51 ng/ml m

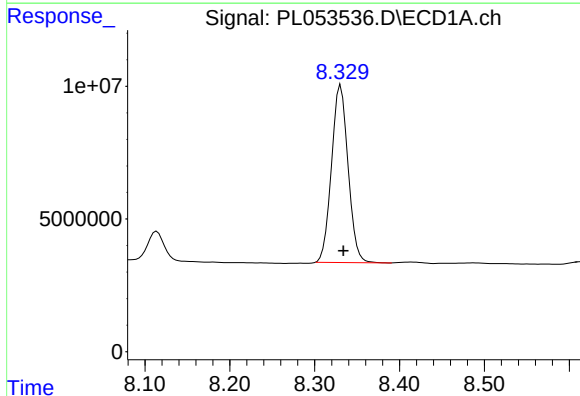

#28 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.003 min
Response: 90701941
Conc: 9.24 ng/ml

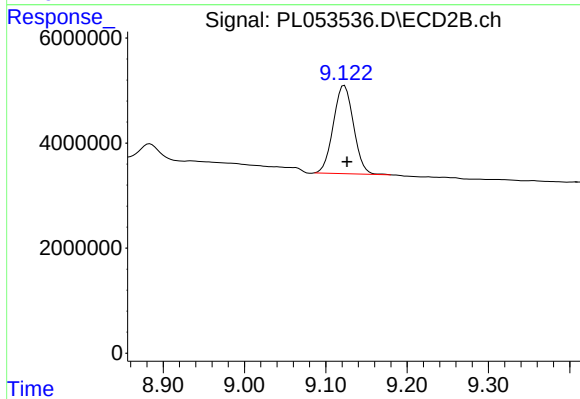

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 28931674
Conc: 10.27 ng/ml