

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 10:48
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 04:55:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
7) B	delta-BHC	4.546f	0.000	1292055	0	0.595	N.D. #
8) B	Heptachlo...	0.000	5.808	0	23480076	N.D.	7.250 #
9) A	Endosulfan I	0.000	6.163	0	5049417	N.D.	1.601 #
14) MA	Endrin	5.934	0.000	1145206	0	0.688	N.D. #
15) B	Endosulfa...	0.000	6.866	0	3233655	N.D.	1.131 #
22)	Mirex	7.279f	0.000	2038034	0	1.438	N.D. #
24)	Chlordane-2	0.000	5.388f	0	6016149	N.D.	55.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 10:48
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 04:55:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

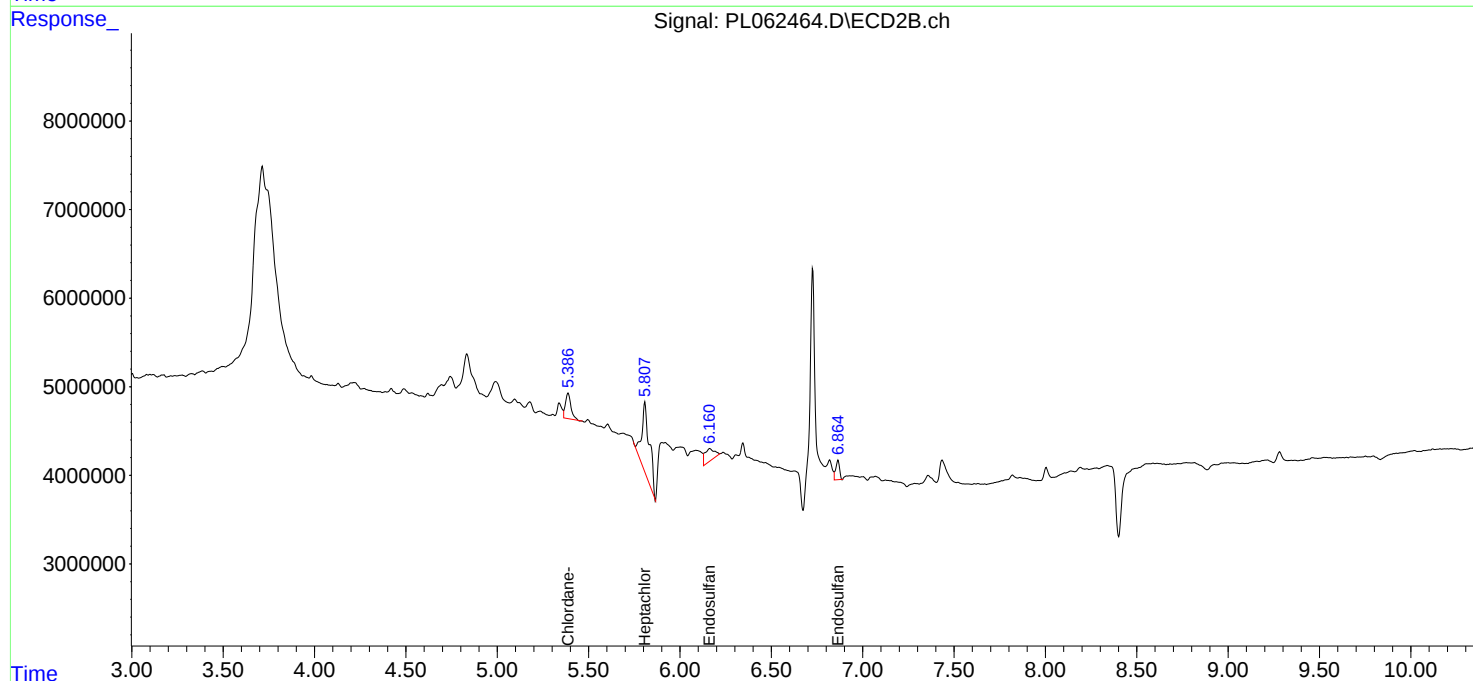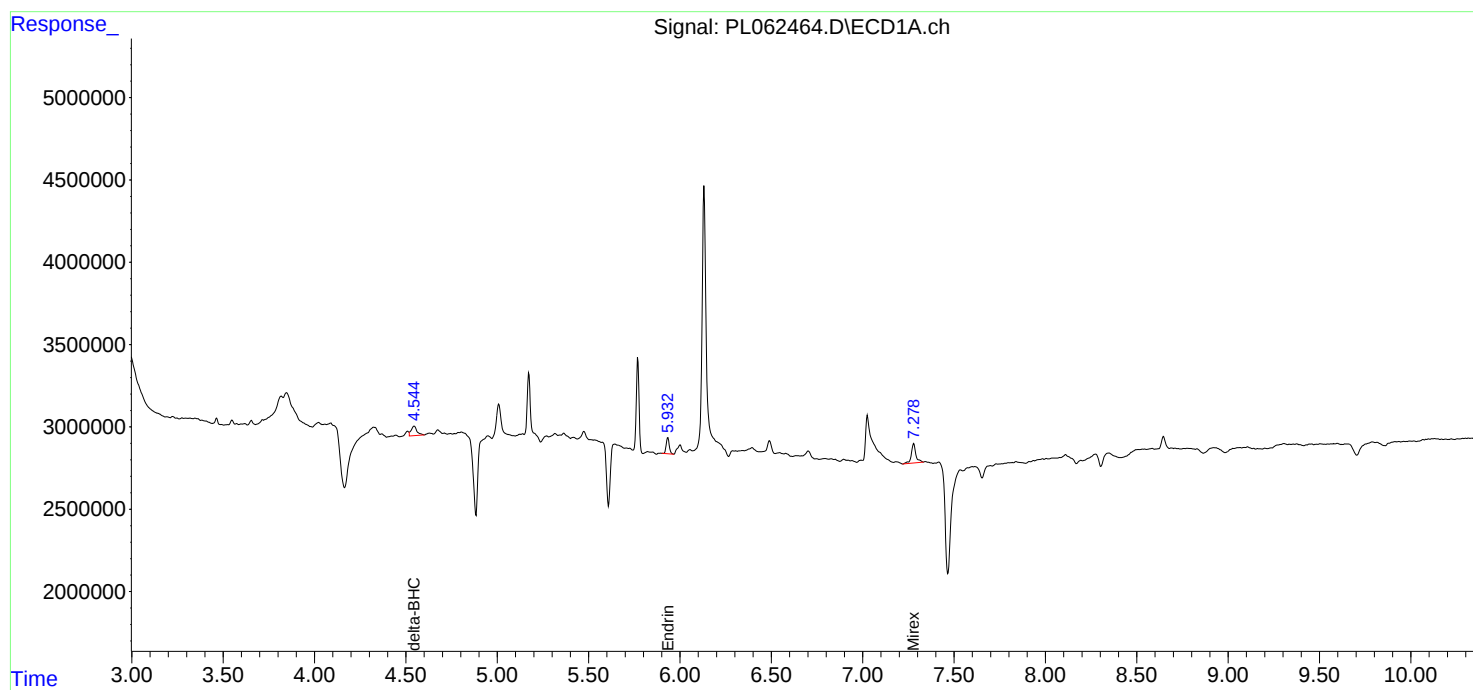


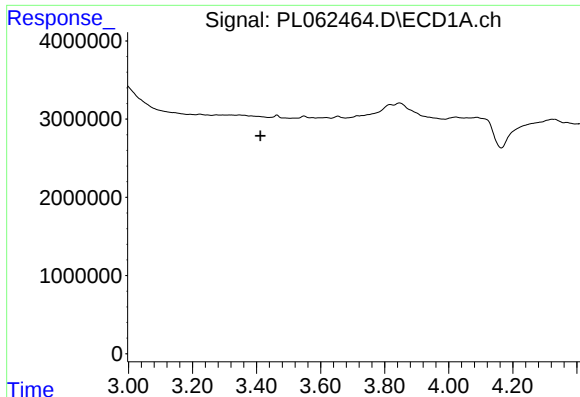

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

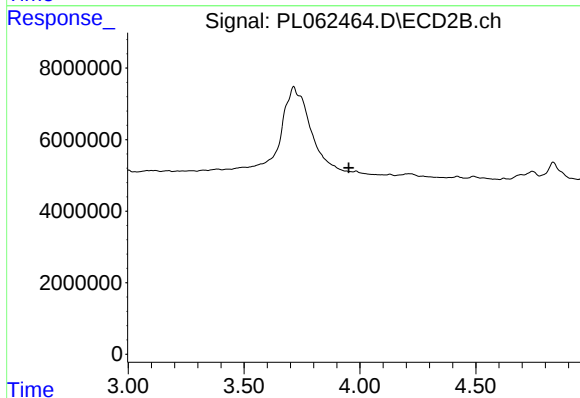


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.952 min
Response: 0
Conc: N.D.

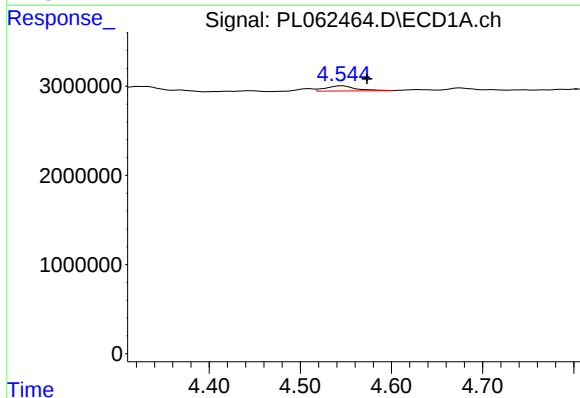


#7 delta-BHC

R.T.: 4.546 min
Delta R.T.: -0.027 min
Response: 1292055
Conc: 0.59 ng/ml

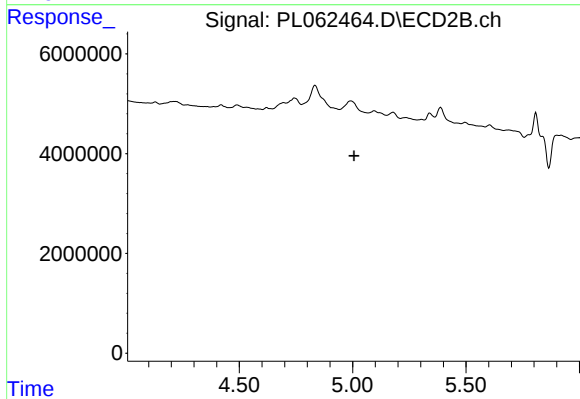

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 5.007 min
Response: 0
Conc: N.D.

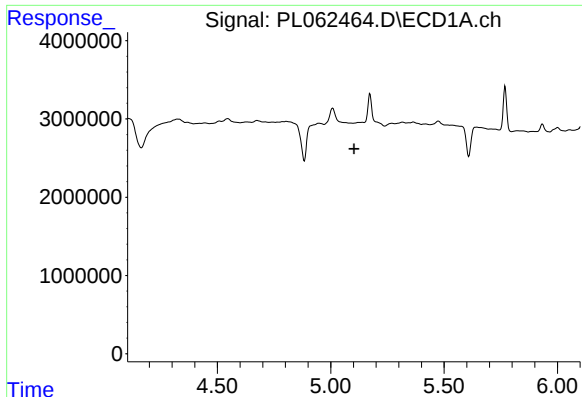

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

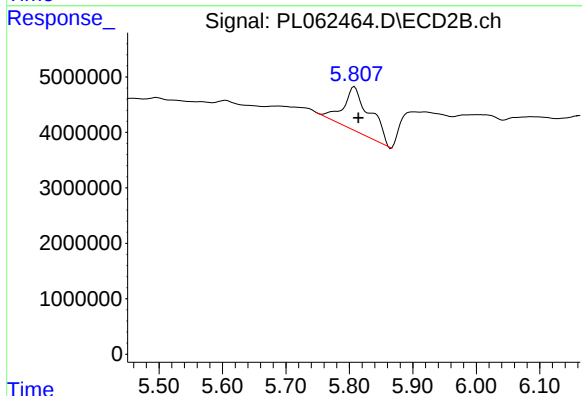


#8 Heptachlor epoxide

R.T.: 5.808 min
Delta R.T.: -0.007 min
Response: 23480076
Conc: 7.25 ng/ml

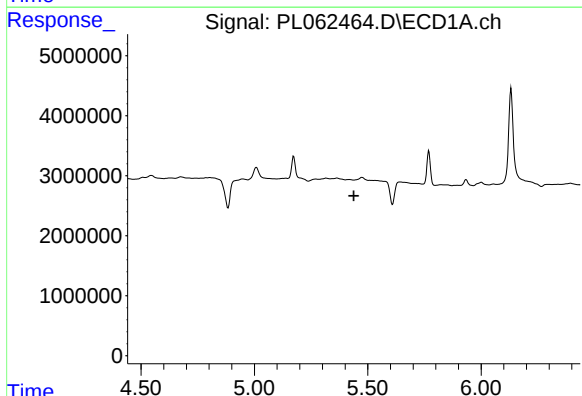


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.438 min
Response: 0
Conc: N.D.

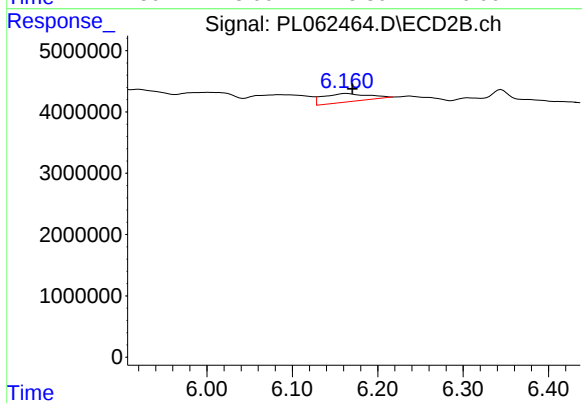

#9 Endosulfan I


R.T.: 6.163 min
Delta R.T.: -0.007 min
Response: 5049417
Conc: 1.60 ng/ml

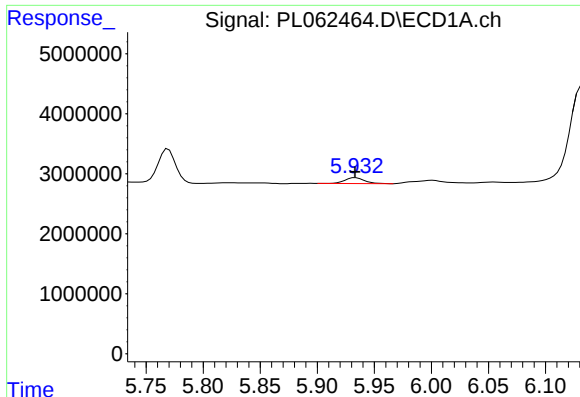

#14 Endrin


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 1145206
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

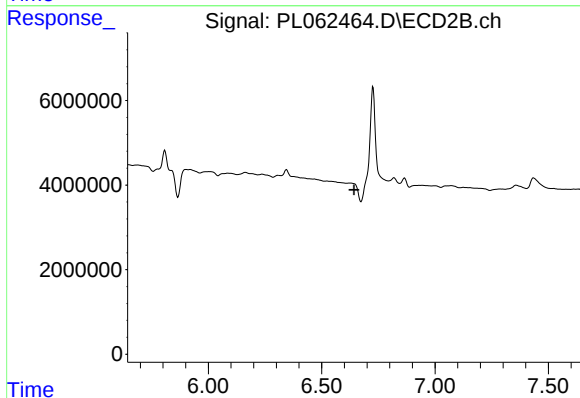


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

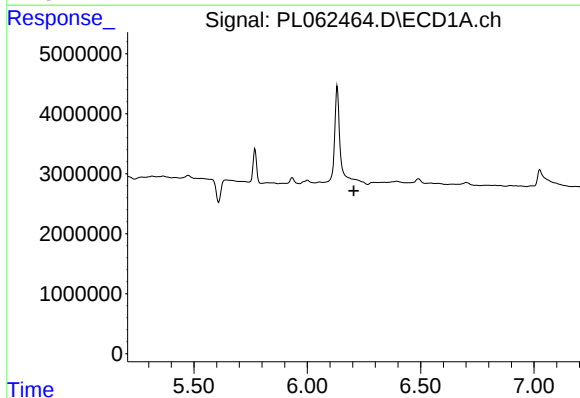


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

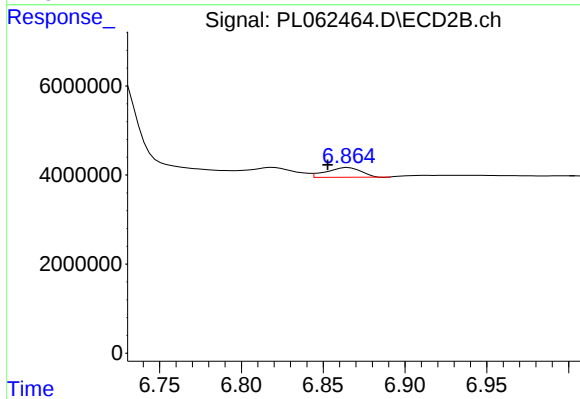

#15 Endosulfan II


R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 3233655
Conc: 1.13 ng/ml

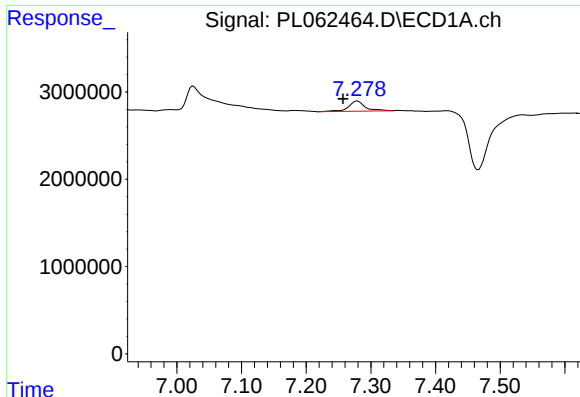

#22 Mirex


R.T.: 7.279 min
Delta R.T.: 0.022 min
Response: 2038034
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

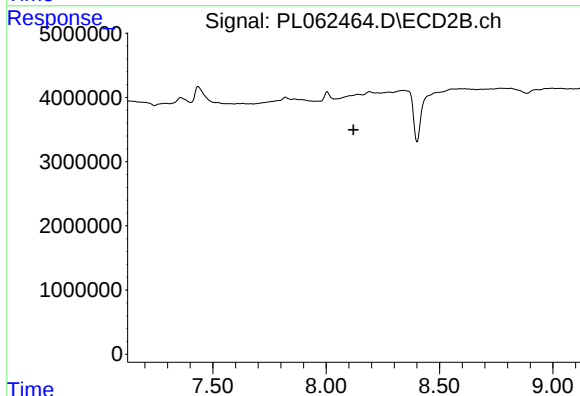


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

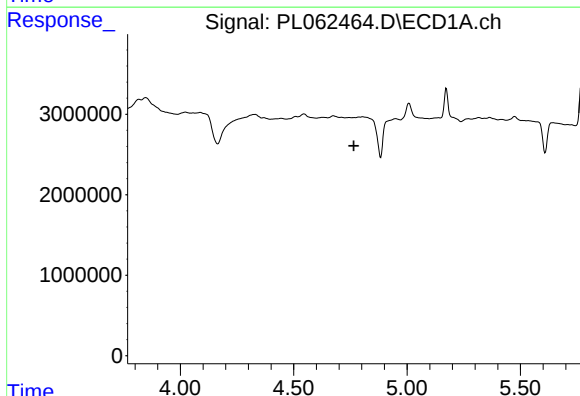


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

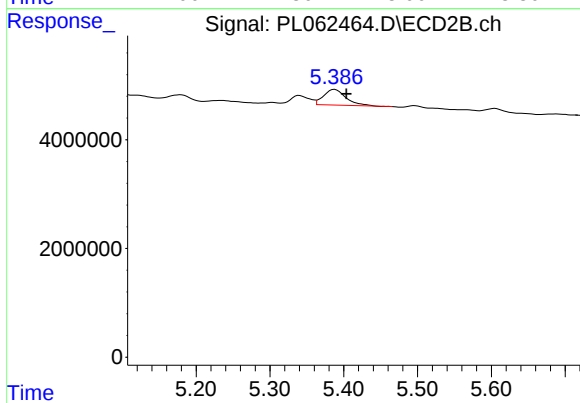

#24 Chlordane-2


R.T.: 5.388 min
Delta R.T.: -0.016 min
Response: 6016149
Conc: 55.18 ng/ml

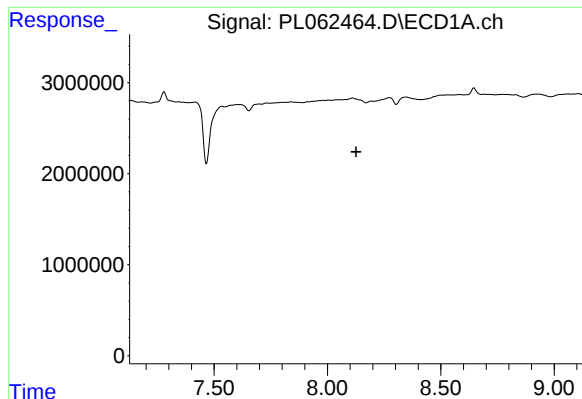

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

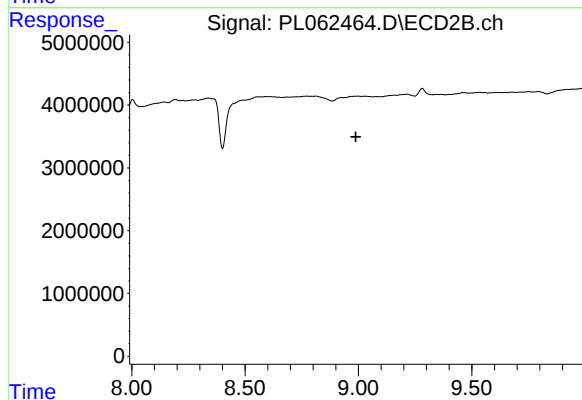

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.989 min
Response: 0
Conc: N.D.