

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 11:30
 Operator : DD\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 04:55:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	88270092	156.6E6	51.317	53.272
28)	SA Decachlor...	8.127	8.989	78302454	103.1E6	48.808	49.238
Target Compounds							
2)	A alpha-BHC	3.844	4.338	130.8E6	238.2E6	51.318	53.608
3)	MA gamma-BHC...	4.123	4.620	117.8E6	221.9E6	50.828	53.139
4)	MA Heptachlor	4.420	5.126	109.4E6	205.3E6	50.996	51.474
5)	MB Aldrin	4.664	5.429	97236350	192.4E6	50.943	53.160
6)	B beta-BHC	4.372	4.791	47792498	94105880	50.034	49.976
7)	B delta-BHC	4.573	5.006	111.5E6	172.4E6	51.314	49.264
8)	B Heptachlo...	5.103	5.814	92487021	180.7E6	50.689	55.799
9)	A Endosulfan I	5.438	6.170	84558685	164.7E6	50.585	52.233
10)	B gamma-Chl...	5.328	6.048	91194343	190.6E6	50.619	56.617
11)	B alpha-Chl...	5.386	6.120	90541850	177.7E6	50.085	52.749
12)	B 4,4'-DDE	5.551	6.279	85629781	163.3E6	51.757	50.689
13)	MA Dieldrin	5.678	6.426	90500850	158.6E6	51.218	49.555
14)	MA Endrin	5.933	6.643	86647364	135.2E6	52.079	48.455
15)	B Endosulfa...	6.205	6.852	82964453	131.2E6	50.323	45.911
16)	A 4,4'-DDD	6.062	6.768	72348816	124.8E6	51.148	48.758
17)	MA 4,4'-DDT	6.302	7.066	71747860	110.6E6	53.761	49.245
18)	B Endrin al...	6.372	6.976	72036739	105.2E6	49.609	46.119
19)	B Endosulfa...	6.585	7.199	81381809	114.5E6	49.315	47.715
20)	A Methoxychlor	6.845	7.525	42740154	58523909	49.623	47.368
21)	B Endrin ke...	7.071	7.667	84609956	113.3E6	46.927	47.808
22)	Mirex	7.257	8.122	68305320	84630212	48.181	49.663
23)	Chlordane-1	4.298f	0.000	2233590	0	43.329	N.D. #
24)	Chlordane-2	0.000	5.429f	0	192.4E6	N.D.	1764.653 #
25)	Chlordane-3	5.328	6.048	91194343	190.6E6	595.540	471.837
26)	Chlordane-4	5.386	6.120	90541850	177.7E6	695.082	366.942 #
27)	Chlordane-5	6.205	0.000	82964453	0	1719.626	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 11:30
Operator : DD\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 04:55:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

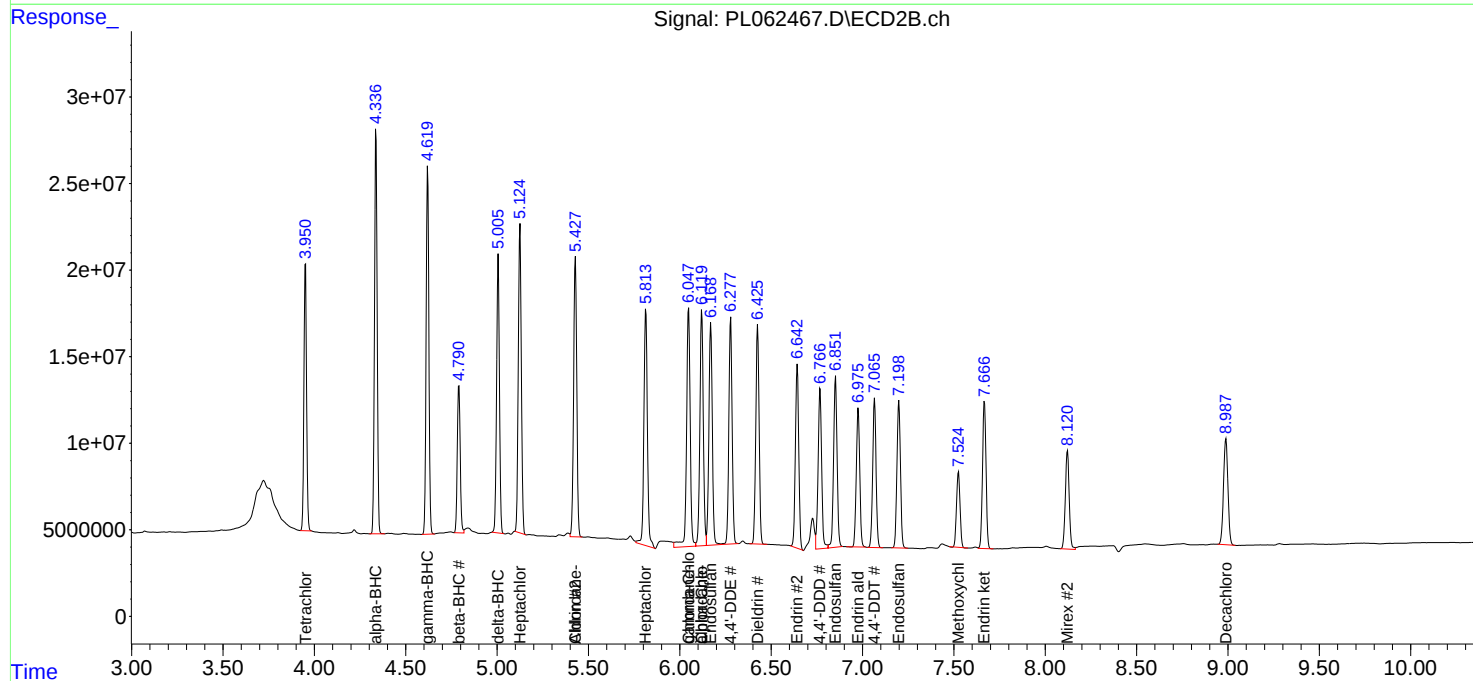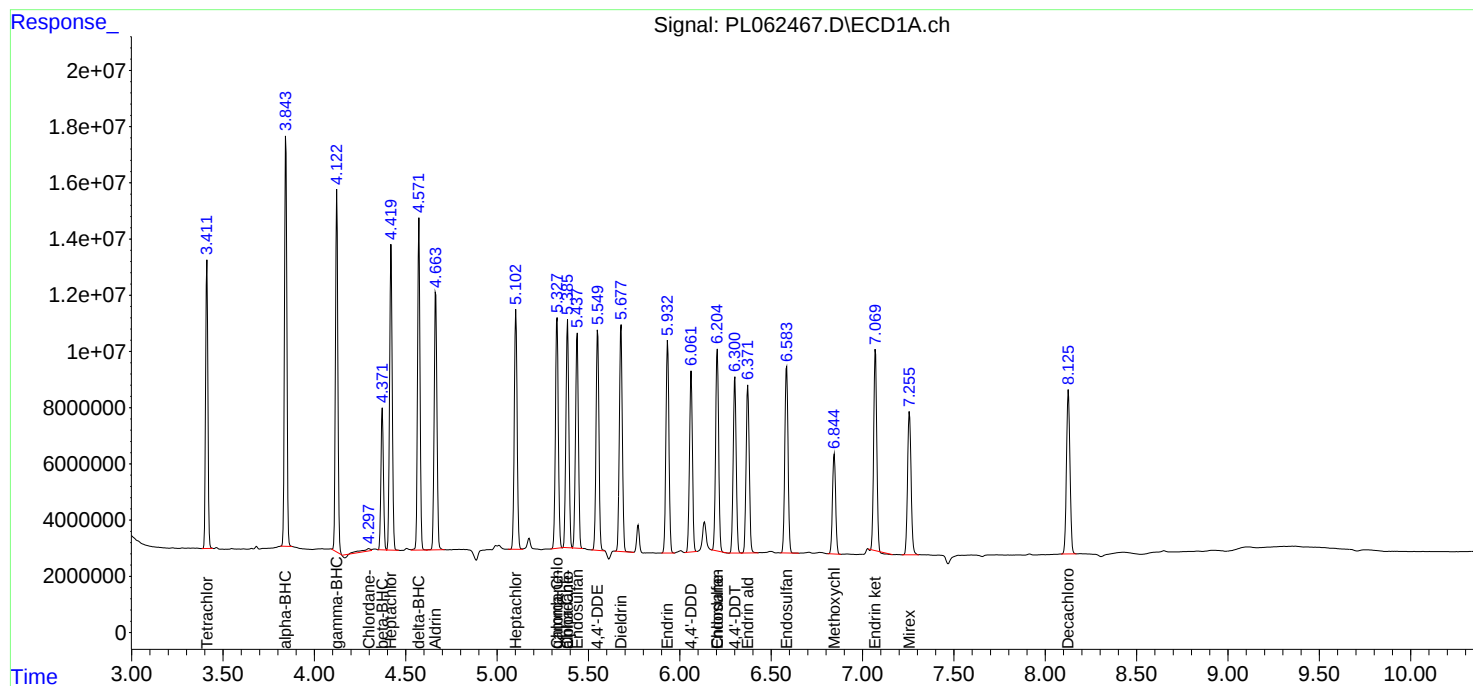


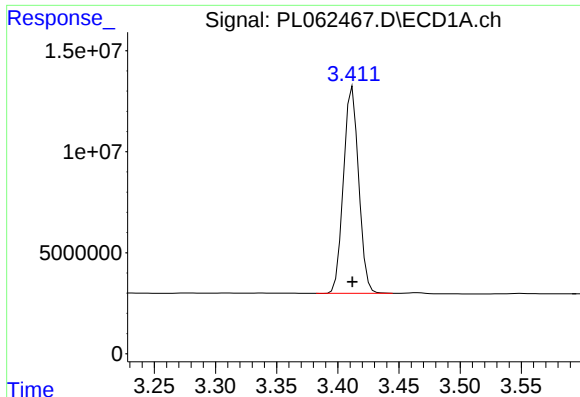

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 88270092
Conc: 51.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

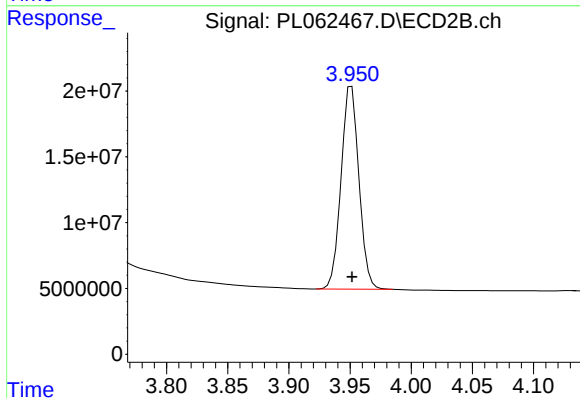


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 156552384
Conc: 53.27 ng/ml

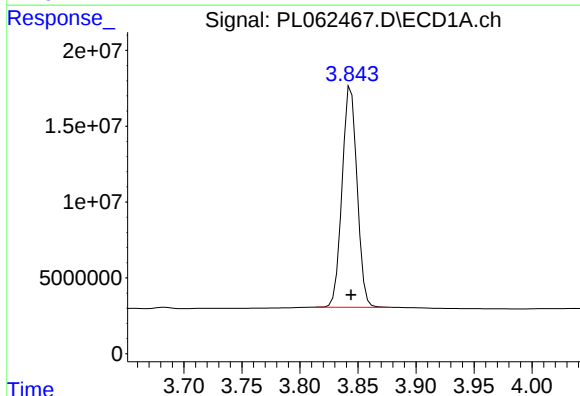


#2 alpha-BHC

R.T.: 3.844 min
Delta R.T.: 0.000 min
Response: 130844616
Conc: 51.32 ng/ml

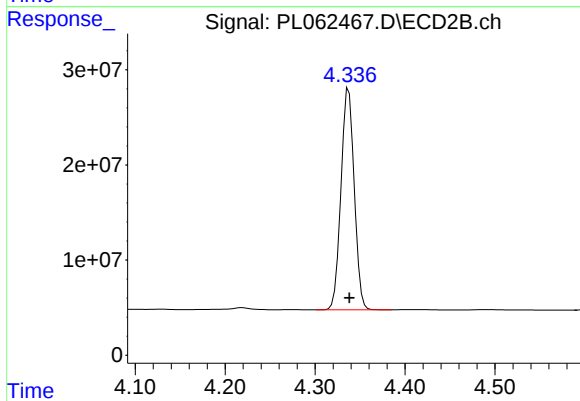

#2 alpha-BHC


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 238190878
Conc: 53.61 ng/ml

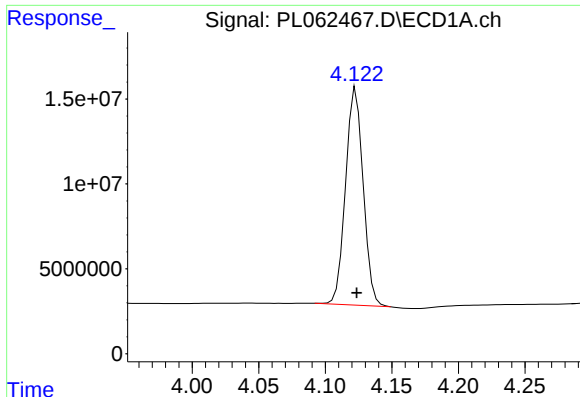

#3 gamma-BHC (Lindane)


R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 117753077
Conc: 50.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

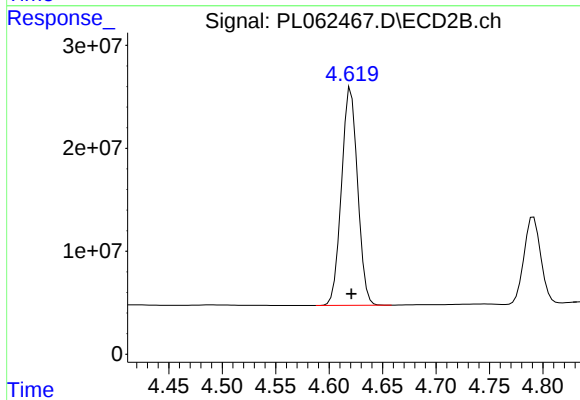


#3 gamma-BHC (Lindane)

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 221895345
Conc: 53.14 ng/ml

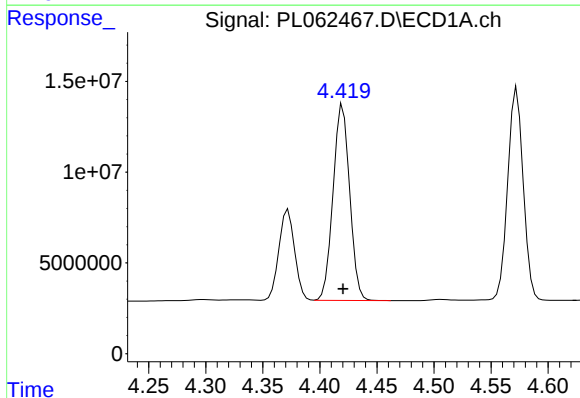


#4 Heptachlor

R.T.: 4.420 min
Delta R.T.: 0.000 min
Response: 109427753
Conc: 51.00 ng/ml

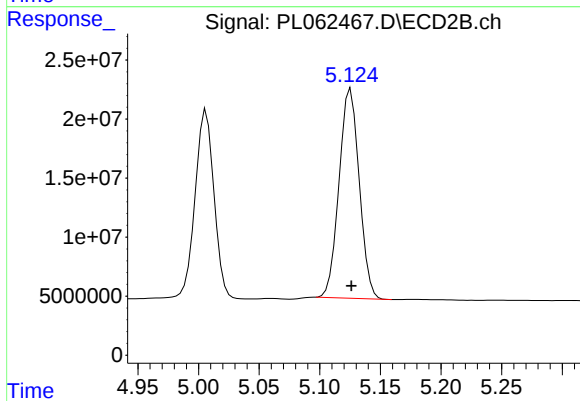

#4 Heptachlor


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 205274437
Conc: 51.47 ng/ml

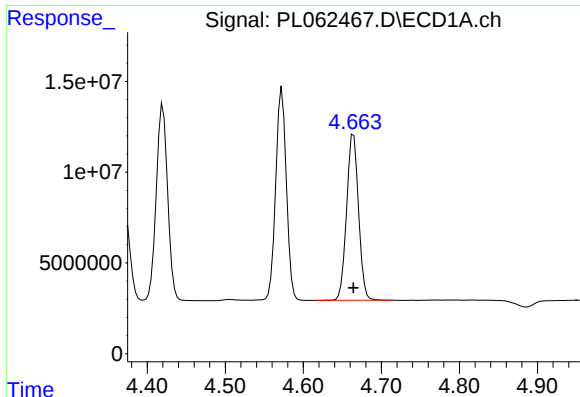

#5 Aldrin


R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 97236350
Conc: 50.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

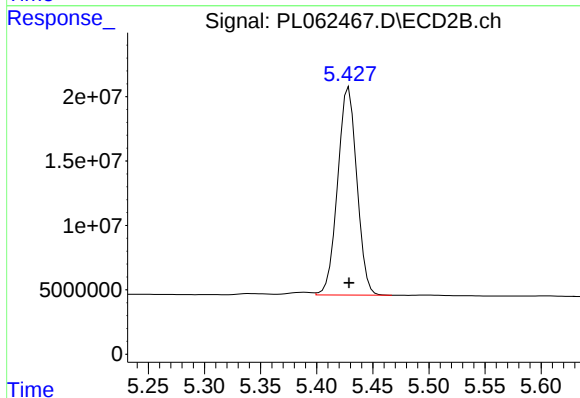


#5 Aldrin

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 192410662
Conc: 53.16 ng/ml

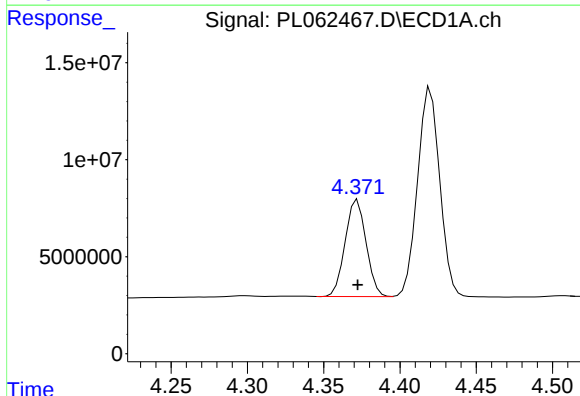


#6 beta-BHC

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 47792498
Conc: 50.03 ng/ml

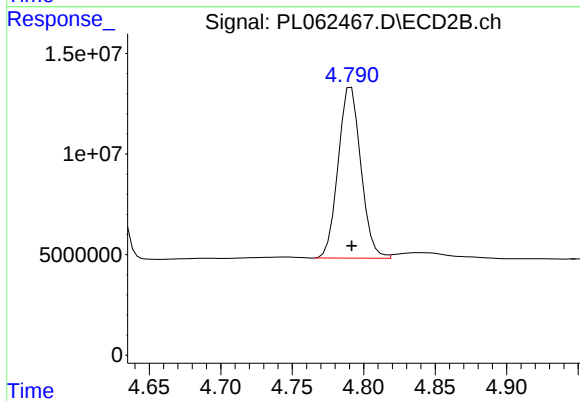

#6 beta-BHC


R.T.: 4.791 min
Delta R.T.: 0.000 min
Response: 94105880
Conc: 49.98 ng/ml

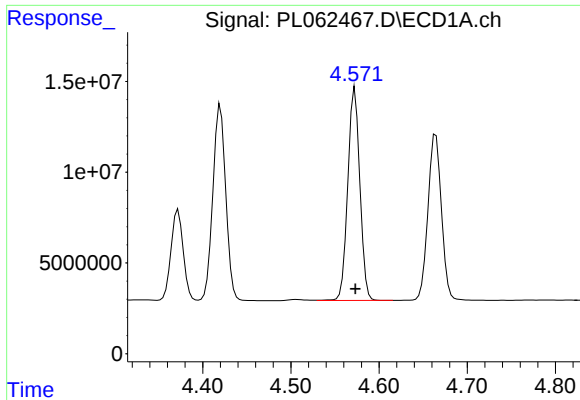

#7 delta-BHC


R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 111517551
Conc: 51.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

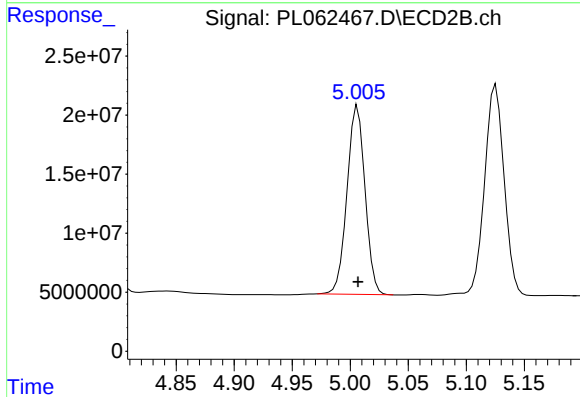


#7 delta-BHC

R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 172397348
Conc: 49.26 ng/ml

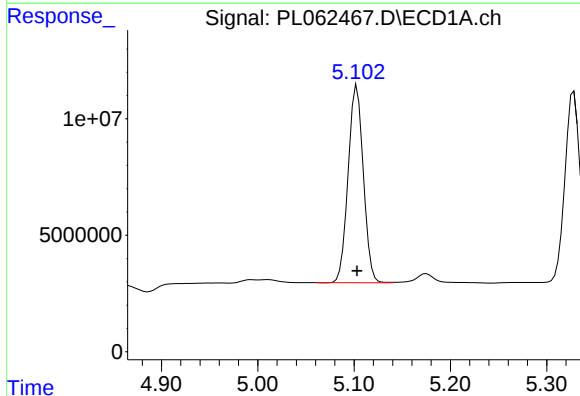


#8 Heptachlor epoxide

R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 92487021
Conc: 50.69 ng/ml

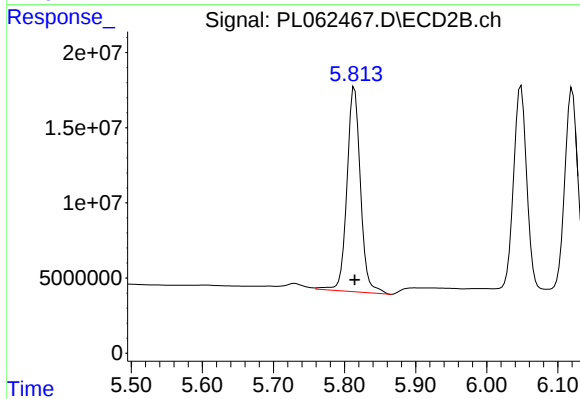

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 180710088
Conc: 55.80 ng/ml

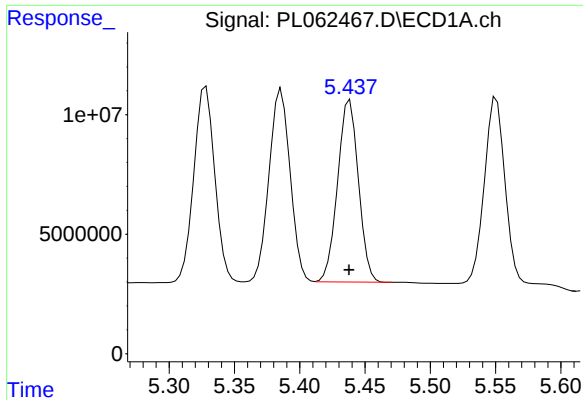

#9 Endosulfan I


R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 84558685
Conc: 50.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

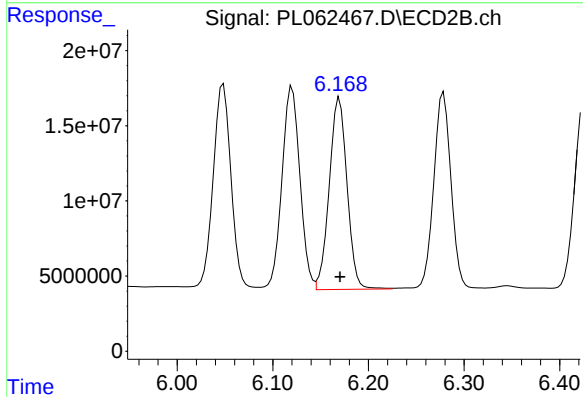


#9 Endosulfan I

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 164734132
Conc: 52.23 ng/ml

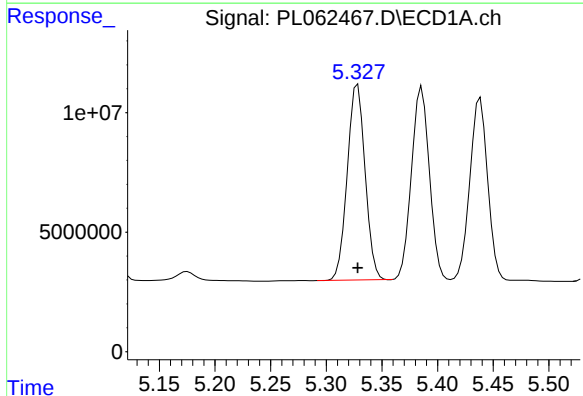


#10 gamma-Chlordane

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 91194343
Conc: 50.62 ng/ml

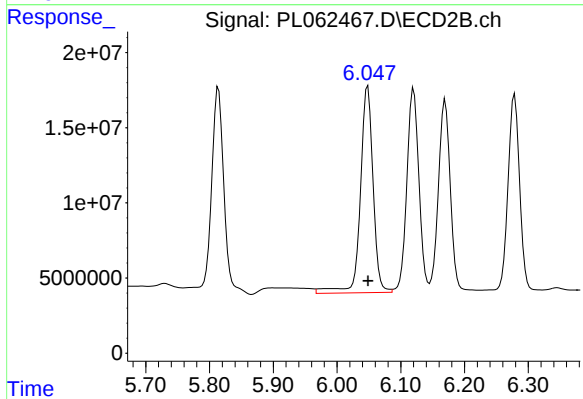

#10 gamma-Chlordane


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 190594385
Conc: 56.62 ng/ml

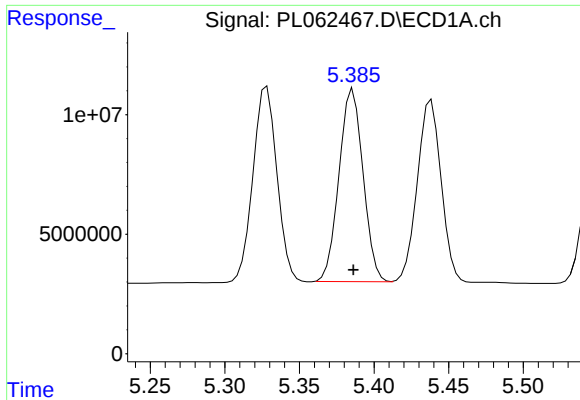

#11 alpha-Chlordane


R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 90541850
Conc: 50.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

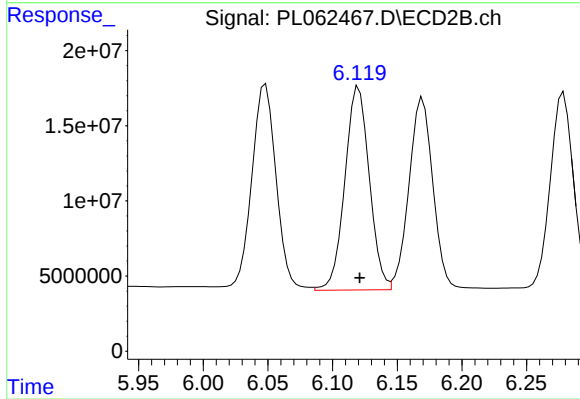


#11 alpha-Chlordane

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 177705226
Conc: 52.75 ng/ml

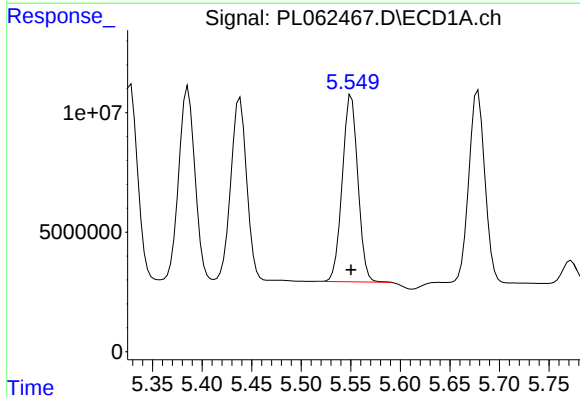


#12 4,4'-DDE

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 85629781
Conc: 51.76 ng/ml

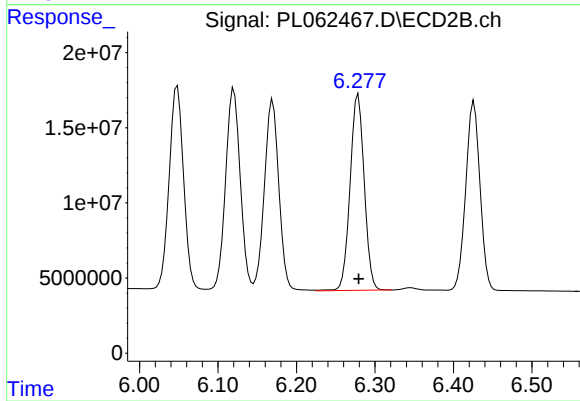

#12 4,4'-DDE


R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 163322291
Conc: 50.69 ng/ml

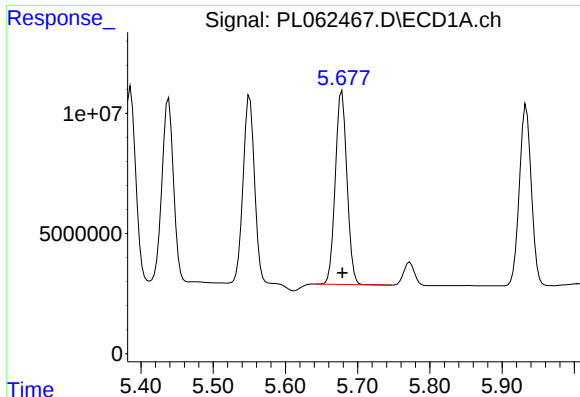

#13 Dieldrin


R.T.: 5.678 min
Delta R.T.: 0.000 min
Response: 90500850
Conc: 51.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

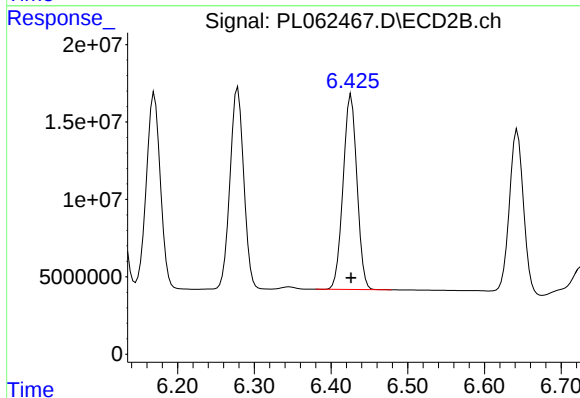


#13 Dieldrin

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 158618675
Conc: 49.56 ng/ml

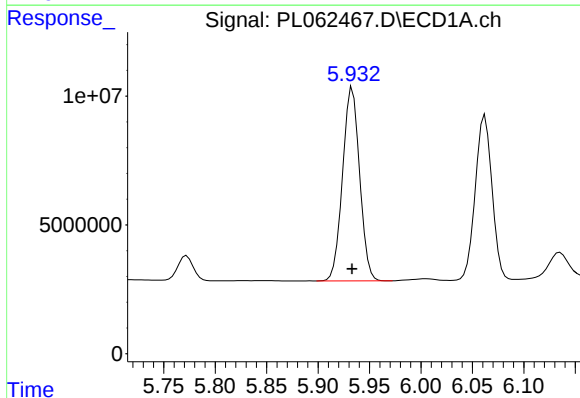


#14 Endrin

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 86647364
Conc: 52.08 ng/ml

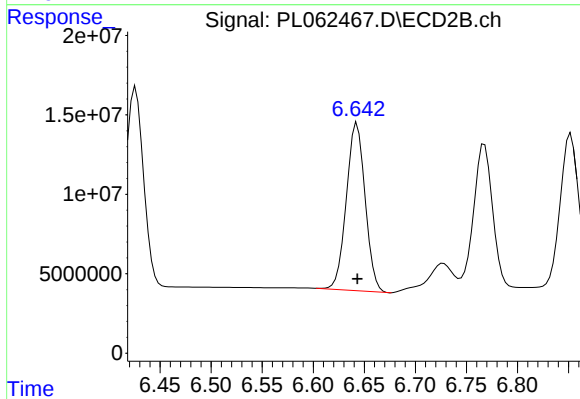

#14 Endrin


R.T.: 6.643 min
Delta R.T.: 0.000 min
Response: 135242716
Conc: 48.45 ng/ml

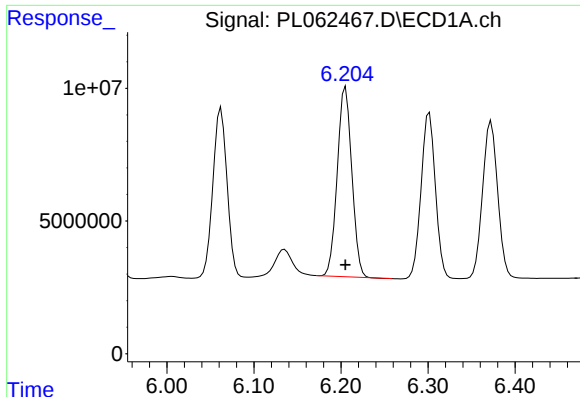

#15 Endosulfan II


R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 82964453
Conc: 50.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

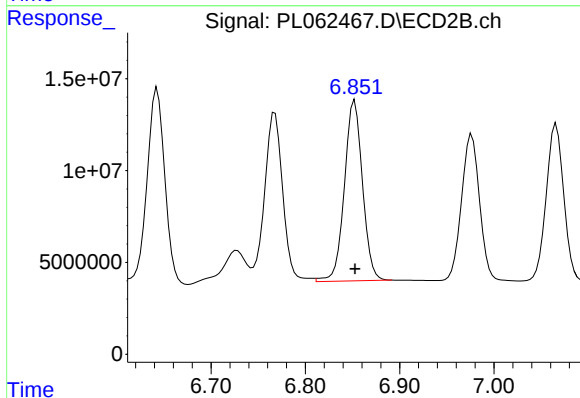


#15 Endosulfan II

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 131244300
Conc: 45.91 ng/ml

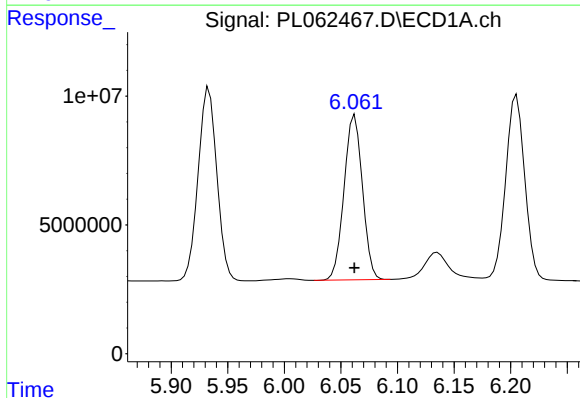


#16 4,4'-DDD

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 72348816
Conc: 51.15 ng/ml

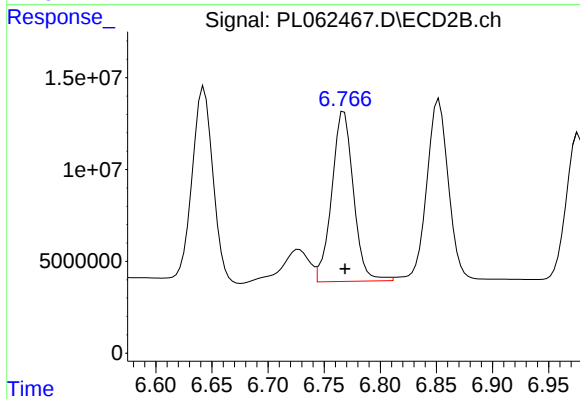

#16 4,4'-DDD


R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 124818985
Conc: 48.76 ng/ml

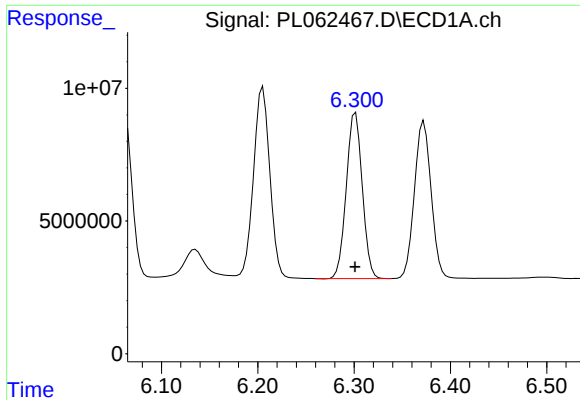

#17 4,4'-DDT


R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 71747860
Conc: 53.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

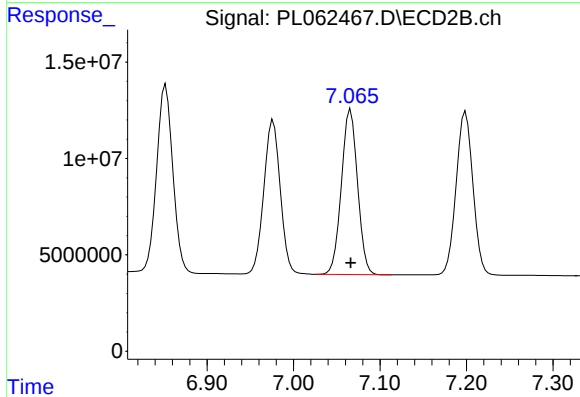


#17 4,4'-DDT

R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 110566876
Conc: 49.24 ng/ml

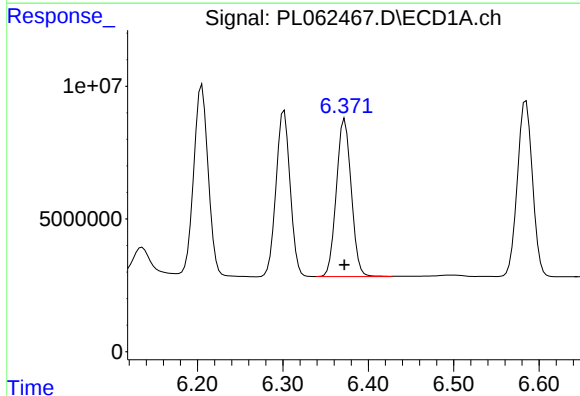


#18 Endrin aldehyde

R.T.: 6.372 min
Delta R.T.: 0.000 min
Response: 72036739
Conc: 49.61 ng/ml

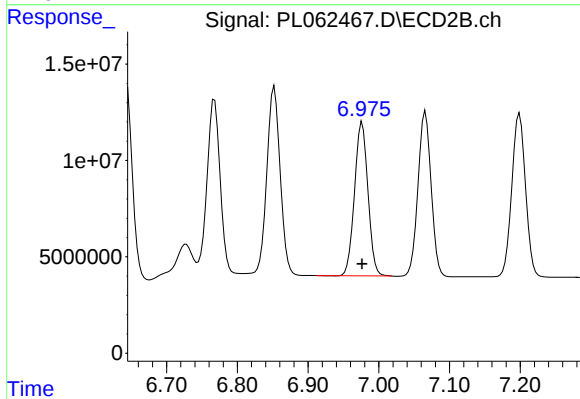

#18 Endrin aldehyde


R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 105179427
Conc: 46.12 ng/ml

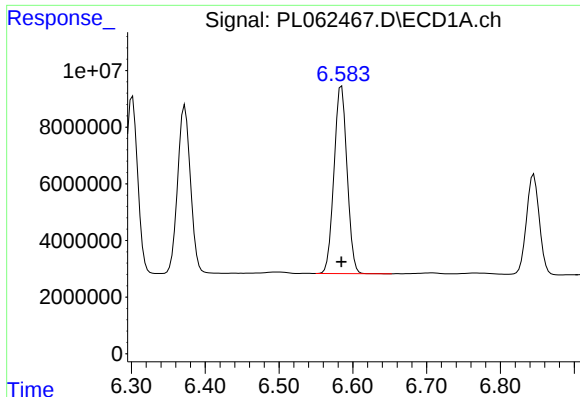

#19 Endosulfan Sulfate


R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 81381809
Conc: 49.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

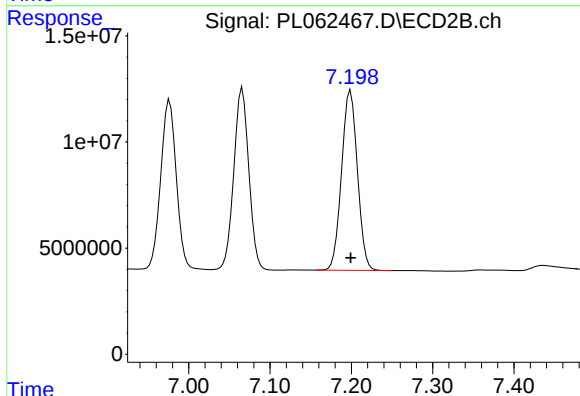


#19 Endosulfan Sulfate

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 114479675
Conc: 47.72 ng/ml

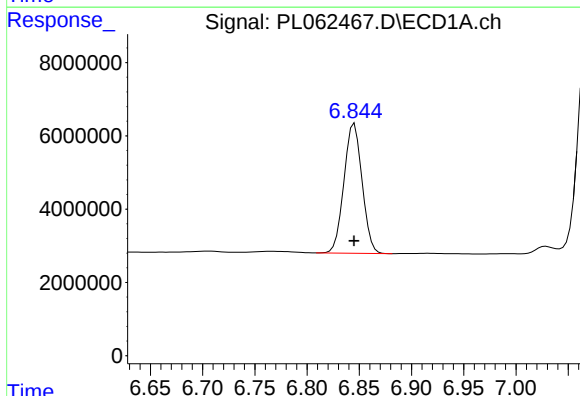


#20 Methoxychlor

R.T.: 6.845 min
Delta R.T.: 0.000 min
Response: 42740154
Conc: 49.62 ng/ml

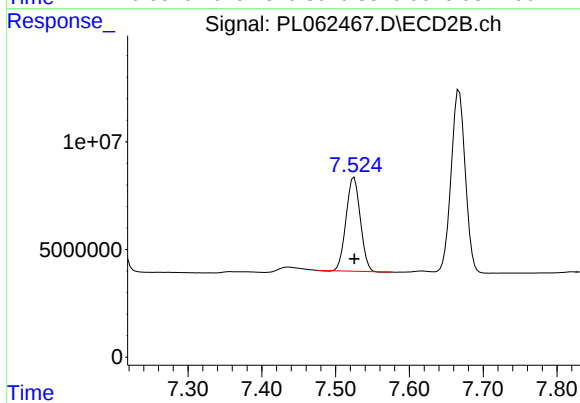

#20 Methoxychlor


R.T.: 7.525 min
Delta R.T.: 0.000 min
Response: 58523909
Conc: 47.37 ng/ml

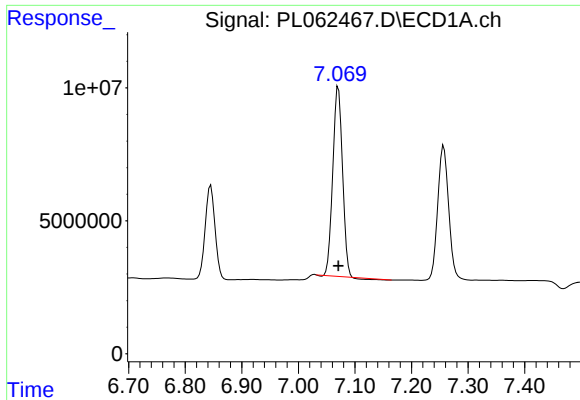

#21 Endrin ketone


R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 84609956
Conc: 46.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

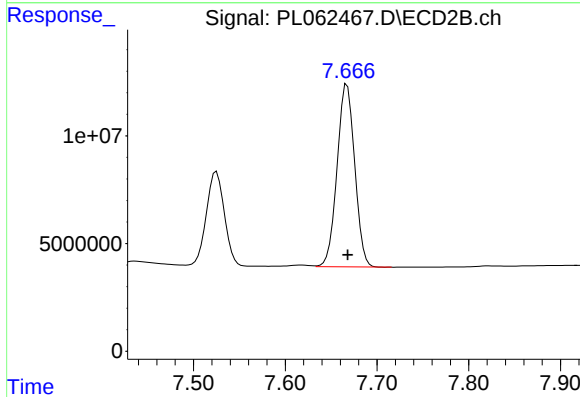


#21 Endrin ketone

R.T.: 7.667 min
Delta R.T.: 0.000 min
Response: 113295031
Conc: 47.81 ng/ml

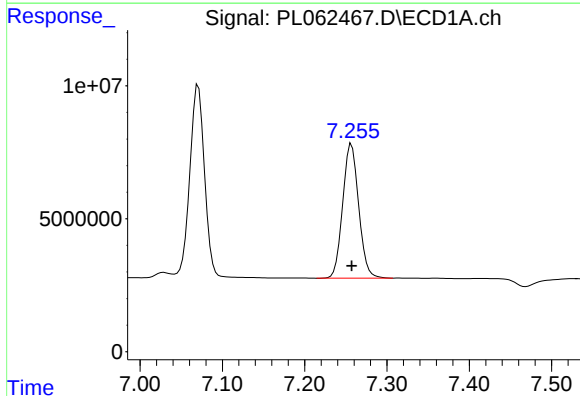


#22 Mirex

R.T.: 7.257 min
Delta R.T.: 0.000 min
Response: 68305320
Conc: 48.18 ng/ml

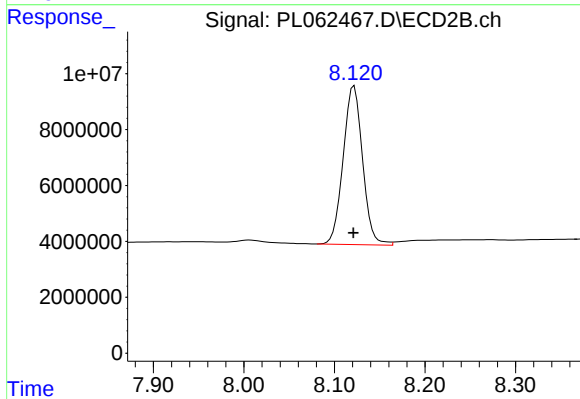

#22 Mirex


R.T.: 8.122 min
Delta R.T.: 0.000 min
Response: 84630212
Conc: 49.66 ng/ml

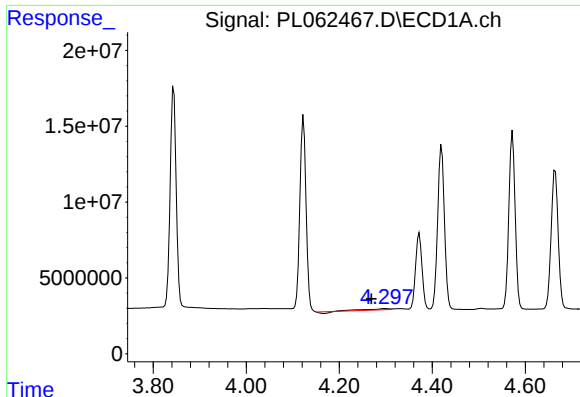

#23 Chlordane-1


R.T.: 4.298 min
Delta R.T.: 0.029 min
Response: 2233590
Conc: 43.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

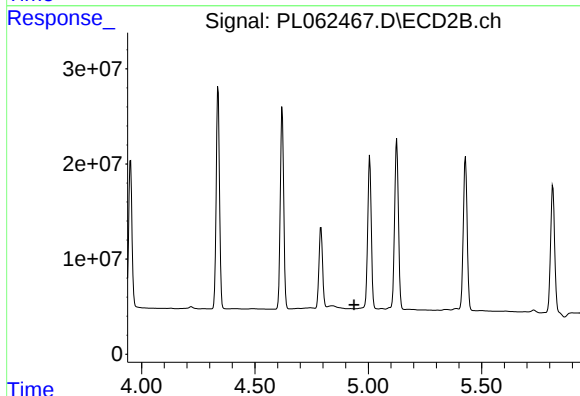


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

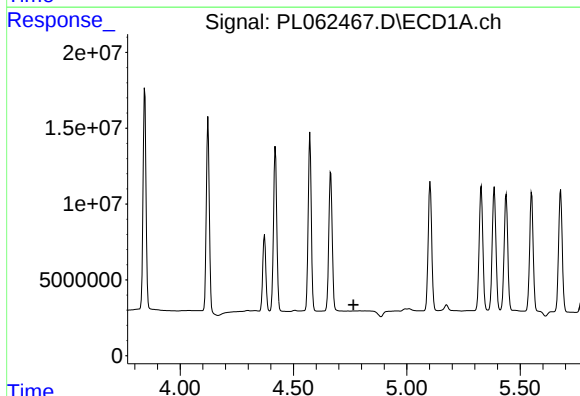


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

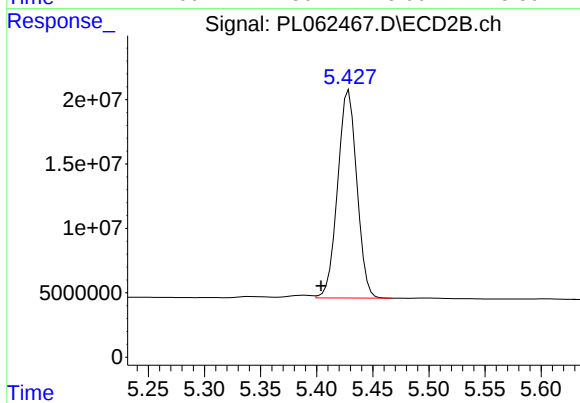

#24 Chlordane-2


R.T.: 5.429 min
Delta R.T.: 0.025 min
Response: 192410662
Conc: 1764.65 ng/ml

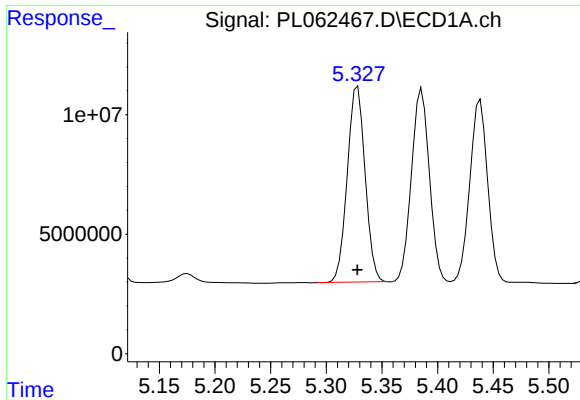

#25 Chlordane-3


R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 91194343
Conc: 595.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

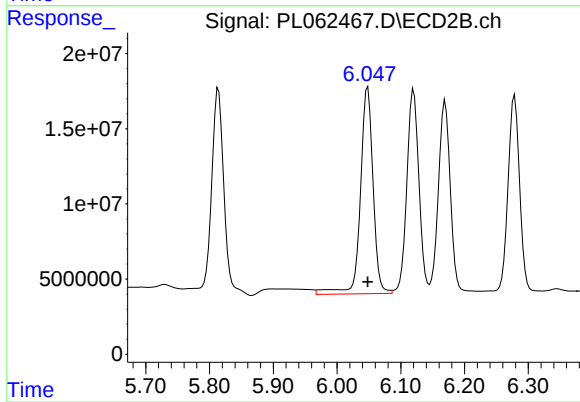


#25 Chlordane-3

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 190594385
Conc: 471.84 ng/ml

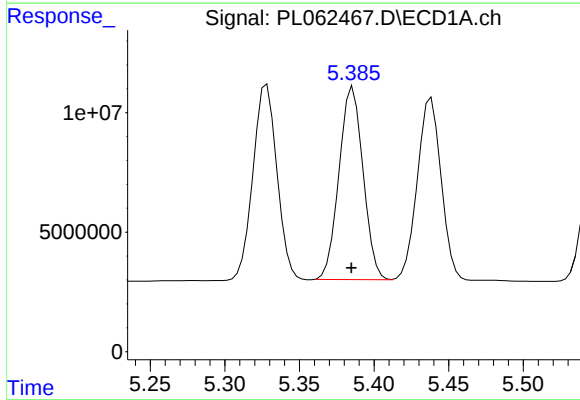


#26 Chlordane-4

R.T.: 5.386 min
Delta R.T.: 0.001 min
Response: 90541850
Conc: 695.08 ng/ml

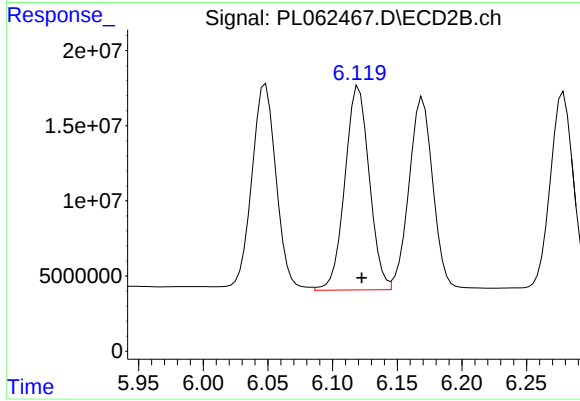

#26 Chlordane-4


R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 177705226
Conc: 366.94 ng/ml

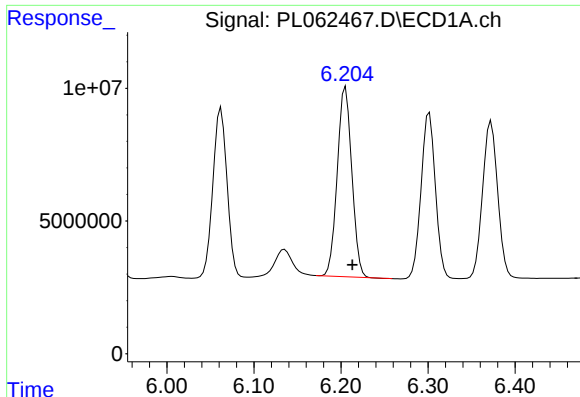

#27 Chlordane-5


R.T.: 6.205 min
Delta R.T.: -0.008 min
Response: 82964453
Conc: 1719.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

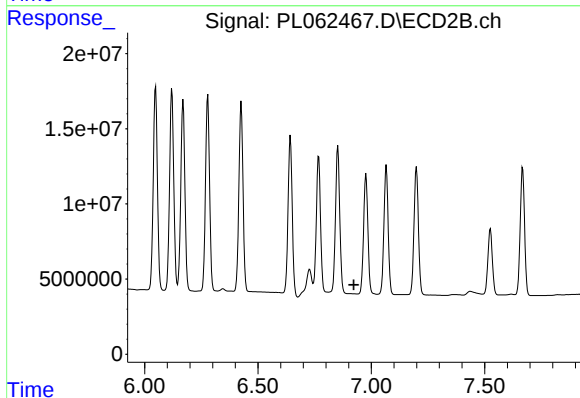


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.923 min
Response: 0
Conc: N.D.

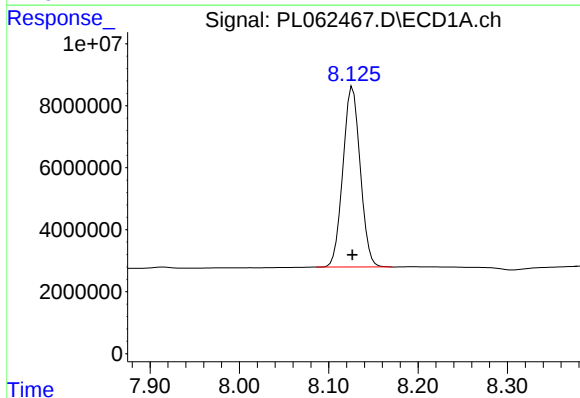

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 78302454
Conc: 48.81 ng/ml

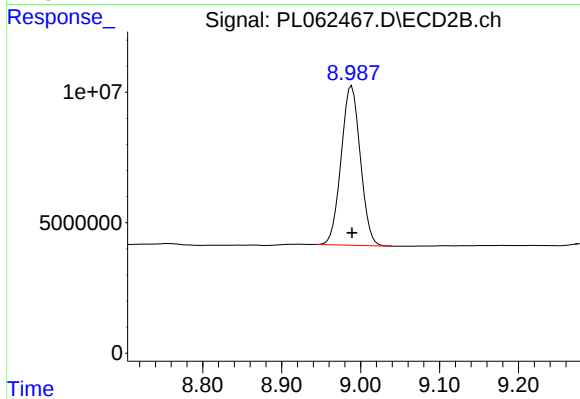

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 103052195
Conc: 49.24 ng/ml