

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 15:10
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 04:22:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:22:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	94337748	142.0E6	50.000	50.000
28)	SA Decachlor...	8.126	8.988	76116194	100.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.269	4.938	25774952	50188317	500.000	500.000
24)	Chlordane-2	4.765	5.404	28819876	54517973	500.000	500.000
25)	Chlordane-3	5.328	6.048	76564468	202.0E6	500.000	500.000
26)	Chlordane-4	5.385	6.123	65130364	242.1E6	500.000	500.000
27)	Chlordane-5	6.213	6.923	24122825	37297400	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 15:10
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 04:22:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:22:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

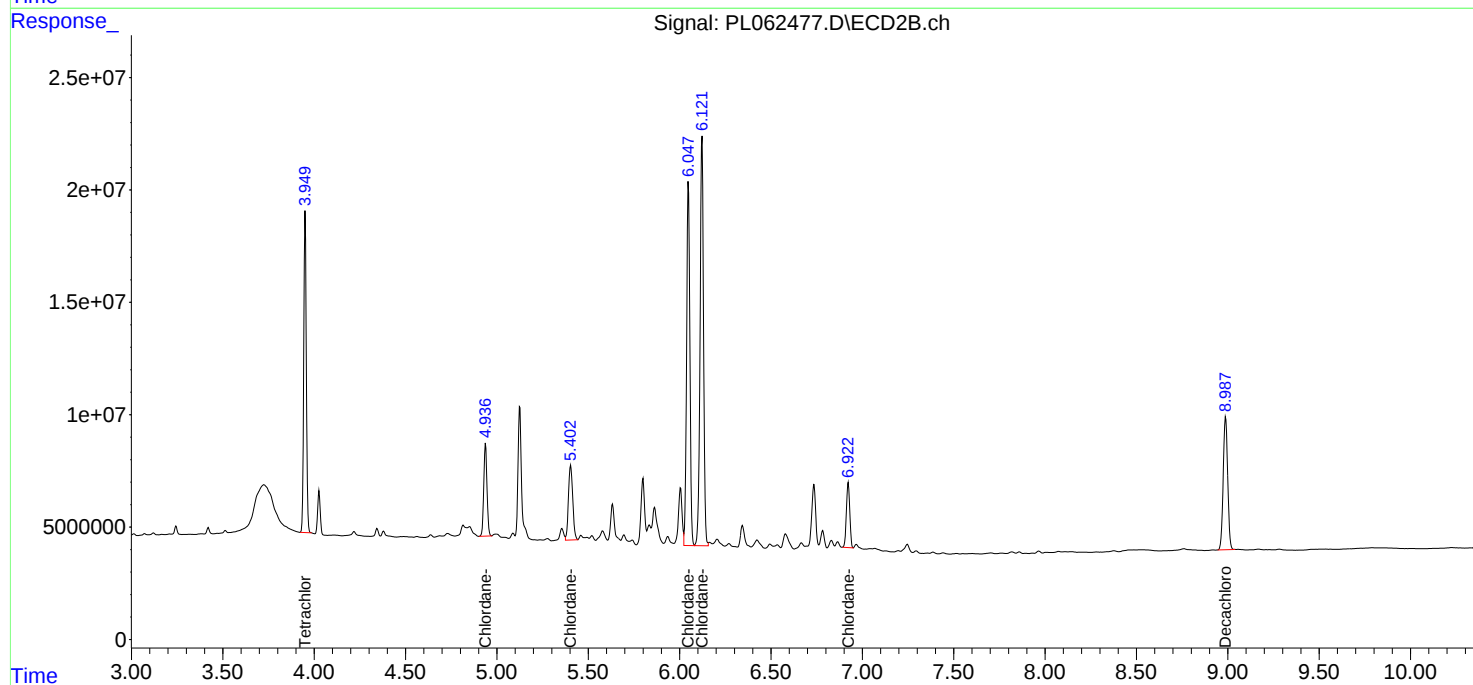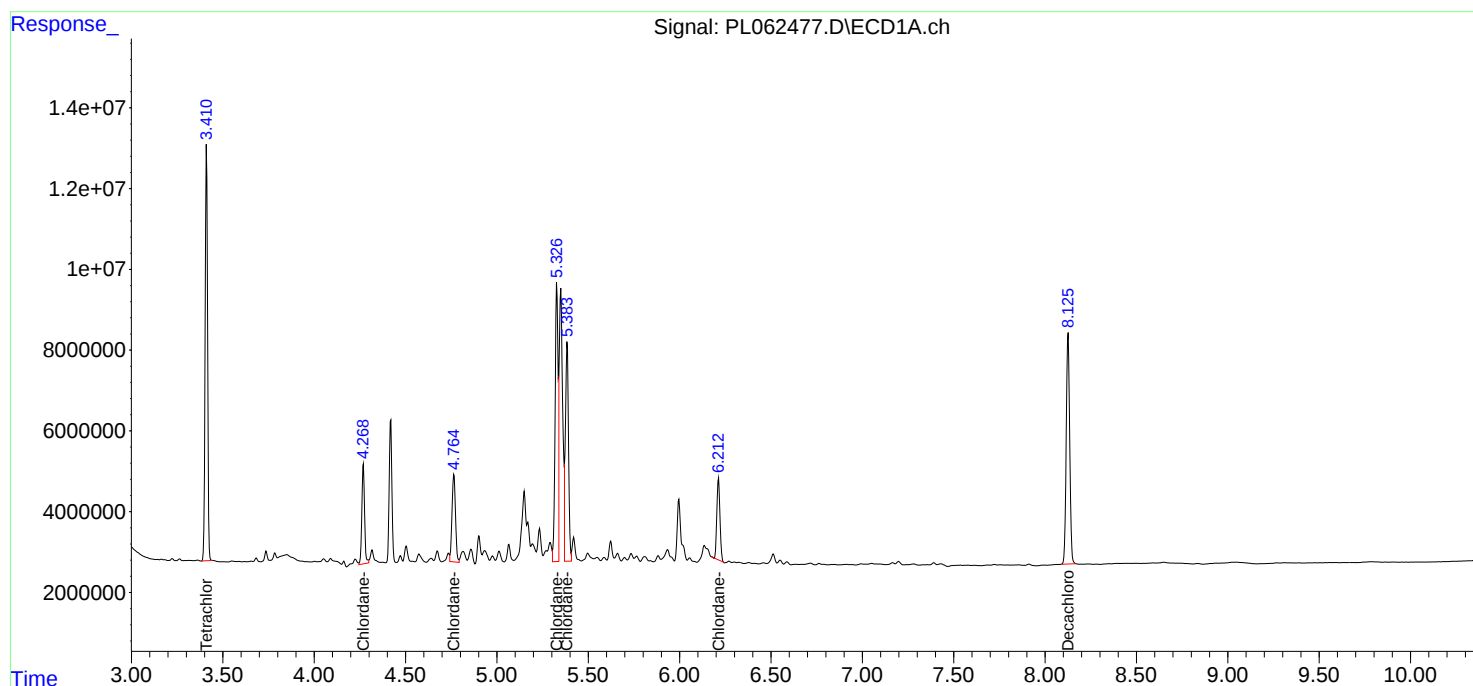


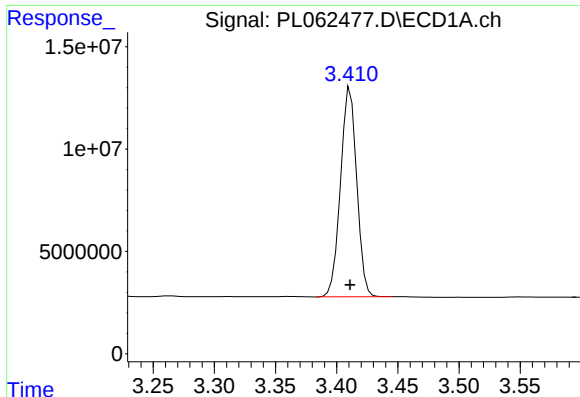

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 94337748
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

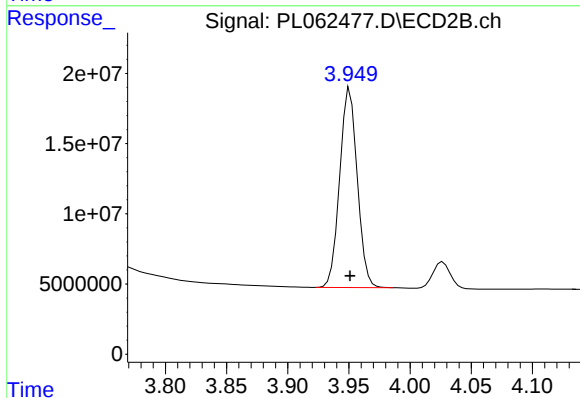


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 142016146
Conc: 50.00 ng/ml

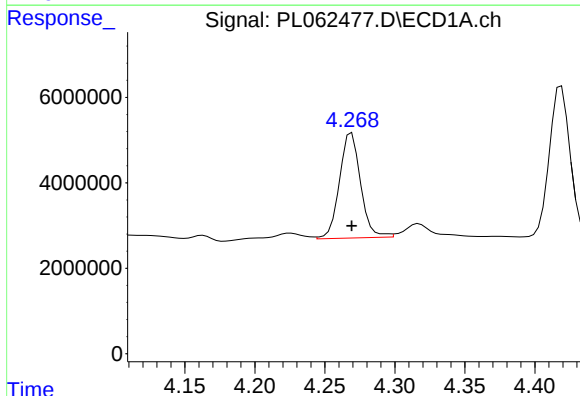


#23 Chlordane-1

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 25774952
Conc: 500.00 ng/ml

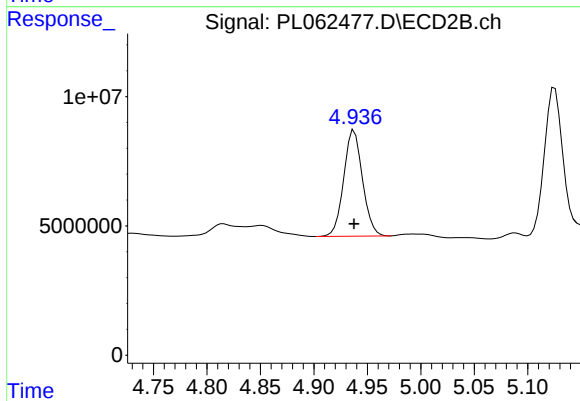

#23 Chlordane-1


R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 50188317
Conc: 500.00 ng/ml

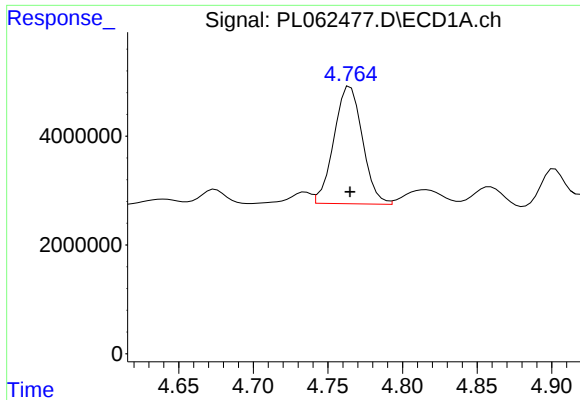

#24 Chlordane-2


R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 28819876
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

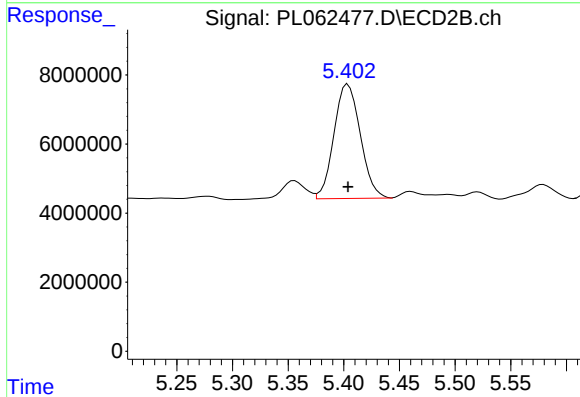


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 54517973
Conc: 500.00 ng/ml

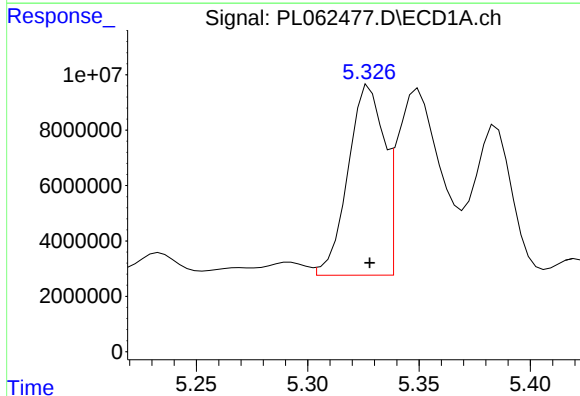


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 76564468
Conc: 500.00 ng/ml

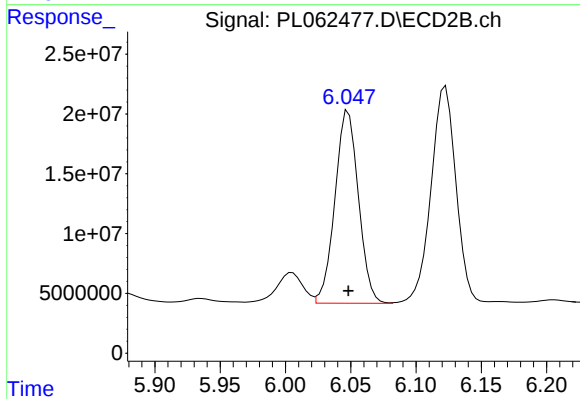

#25 Chlordane-3


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 201970446
Conc: 500.00 ng/ml

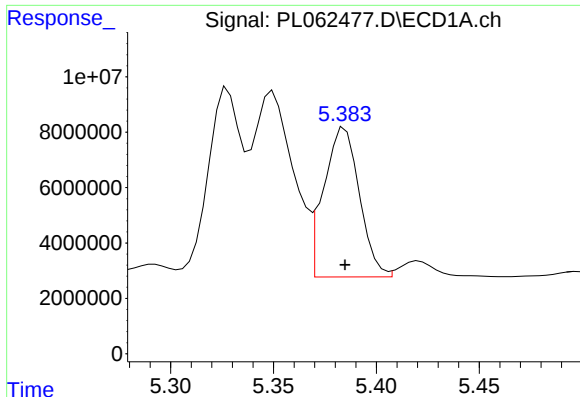

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 65130364
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

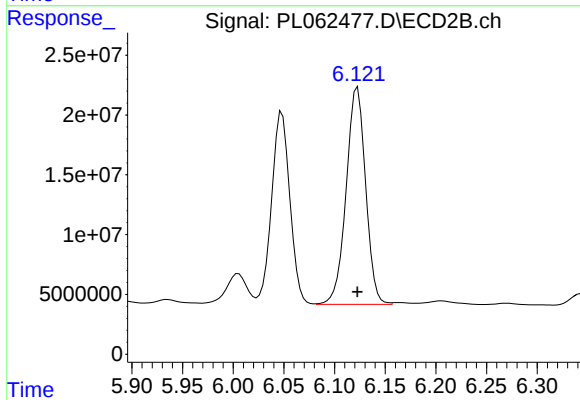


#26 Chlordane-4

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 242143371
Conc: 500.00 ng/ml

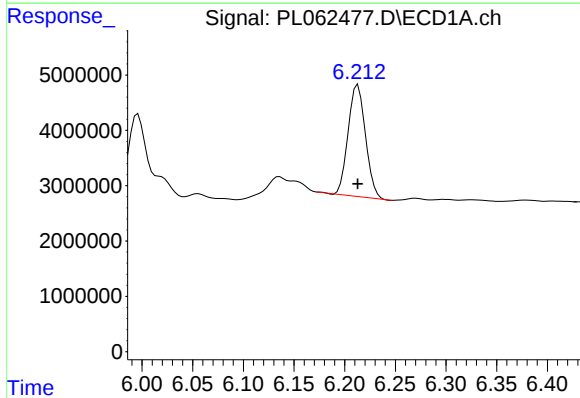


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 24122825
Conc: 500.00 ng/ml

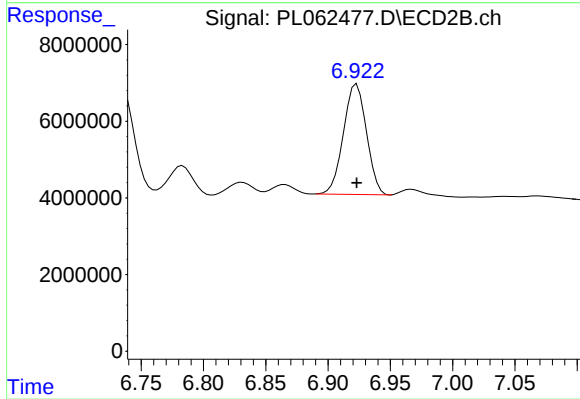

#27 Chlordane-5


R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 37297400
Conc: 500.00 ng/ml

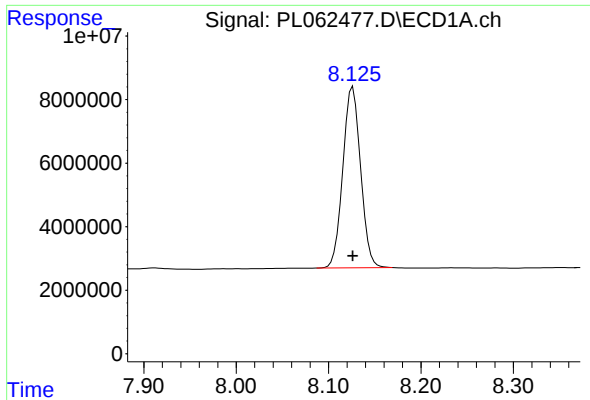

#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 76116194
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

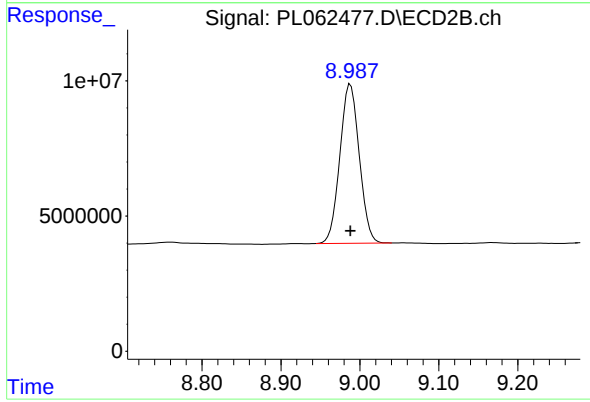

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 100636318
Conc: 50.00 ng/ml