

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 18:01
 Operator : DD\AJ
 Sample : L4467-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 09:14:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	37126702	63335749	21.584	21.552
28)	SA Decachlor...	8.128	8.991	33996082	45432978	21.191	21.708
Target Compounds							
8)	B Heptachlo...	5.115	0.000	1959977	0	1.074	N.D. #
9)	A Endosulfan I	5.460f	0.000	5590388	0	3.344	N.D. #
12)	B 4,4'-DDE	5.553	6.282	3626470	13382422	2.192	4.153 #
14)	MA Endrin	5.936	0.000	2832573	0	1.702	N.D. #
15)	B Endosulfa...	6.222f	6.871f	821217	8703277	0.498	3.045 #
17)	MA 4,4'-DDT	6.301	7.066	3647320	5760309	2.733	2.566
19)	B Endosulfa...	6.605f	0.000	9157279	0	5.549	N.D. #
20)	A Methoxychlor	6.830f	0.000	1000331	0	1.161	N.D. #
23)	Chlordane-1	4.277	0.000	1807396	0	35.061	N.D. #
27)	Chlordane-5	6.222	0.000	821217	0	17.022	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 18:01
Operator : DD\AJ
Sample : L4467-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 09:14:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

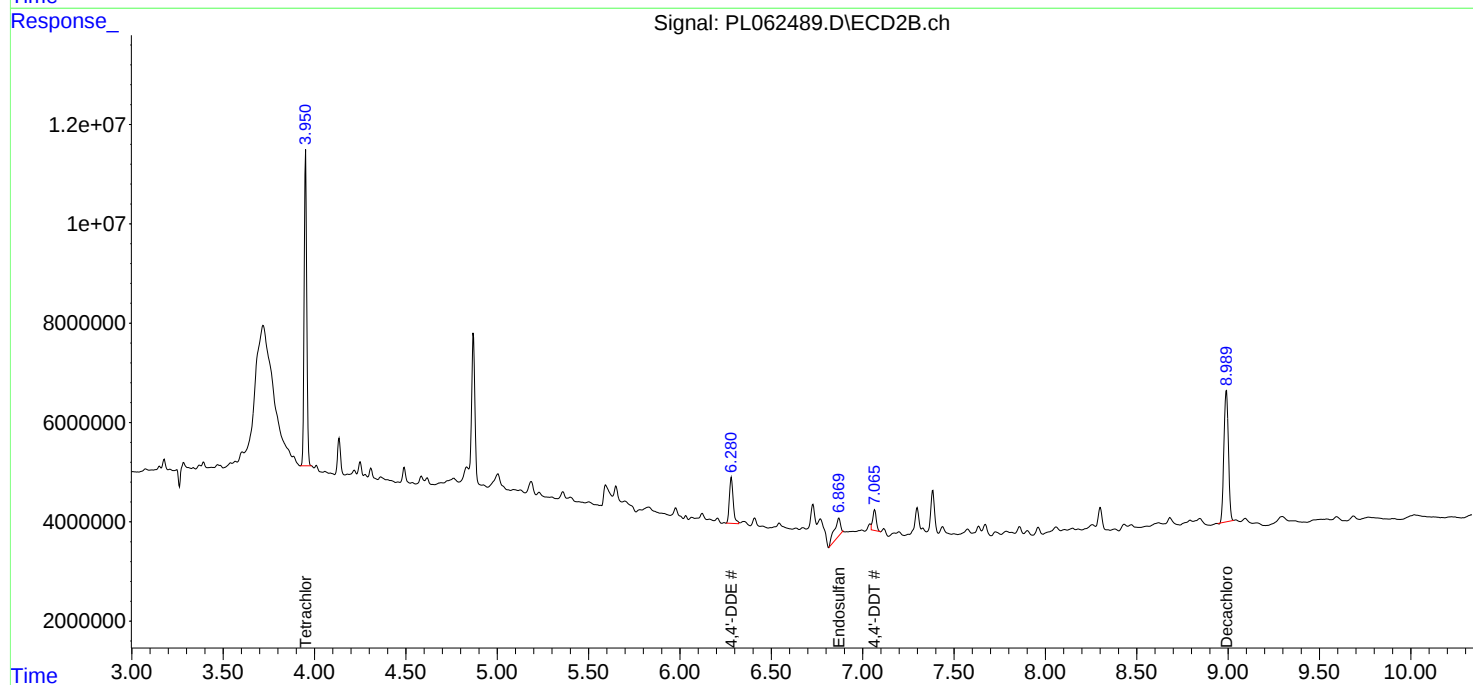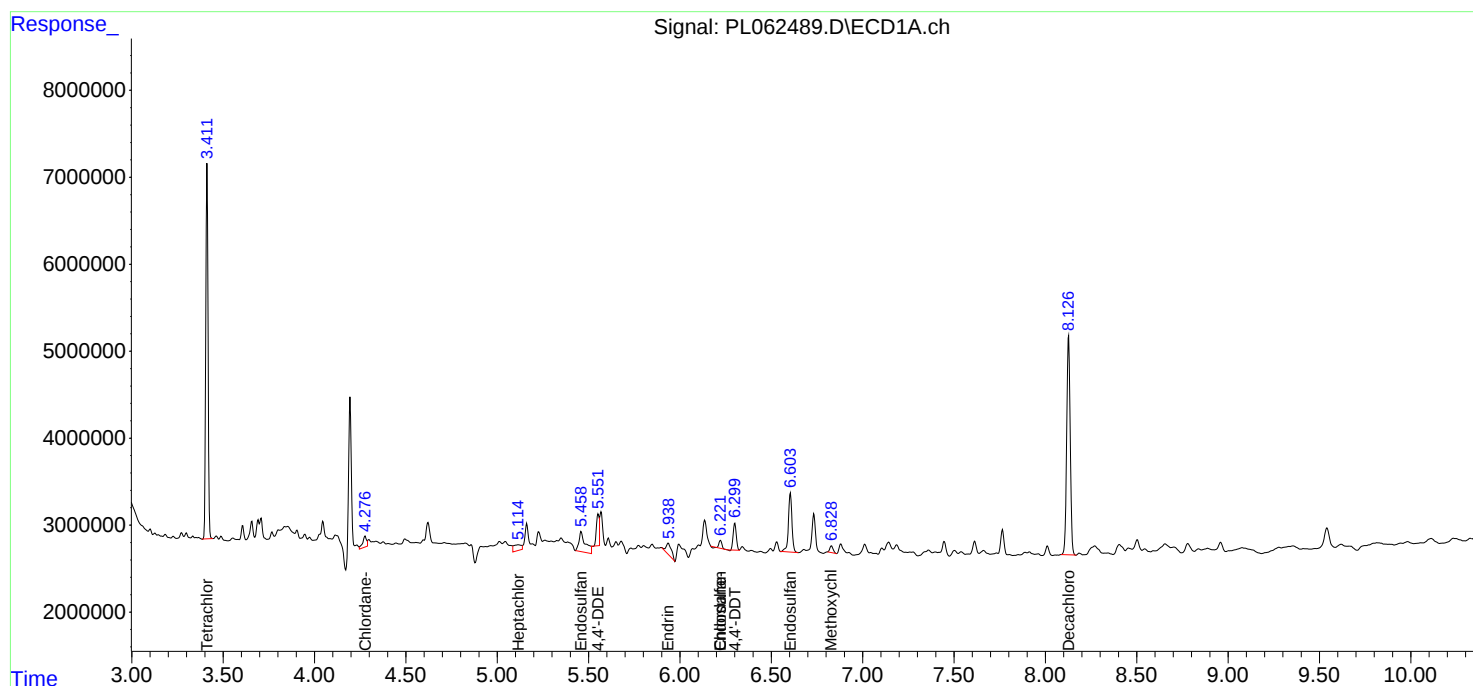


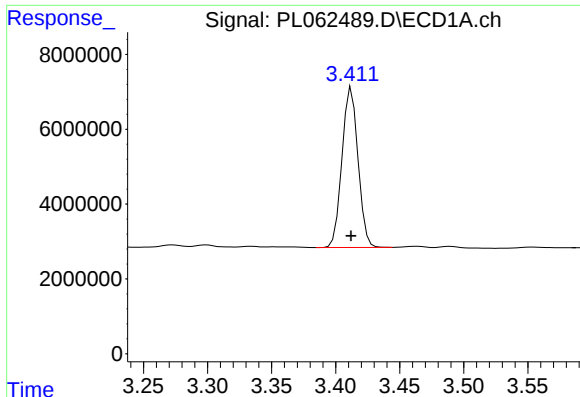

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 37126702
Conc: 21.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

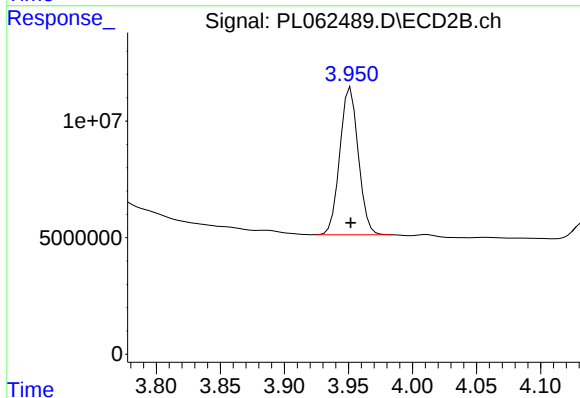


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 63335749
Conc: 21.55 ng/ml

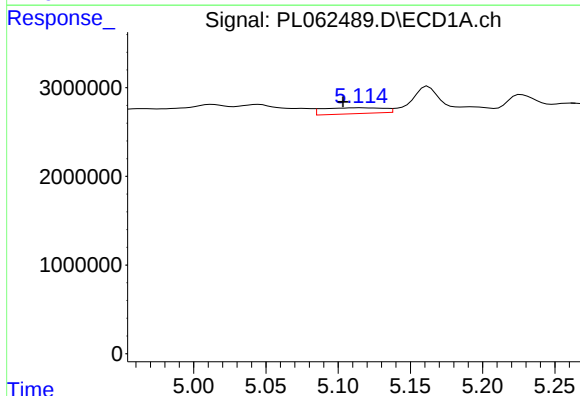


#8 Heptachlor epoxide

R.T.: 5.115 min
Delta R.T.: 0.012 min
Response: 1959977
Conc: 1.07 ng/ml

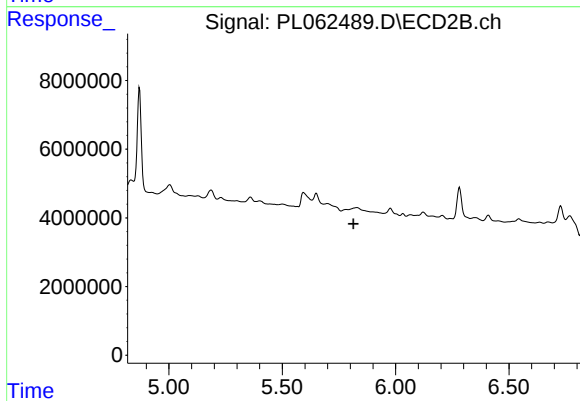

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

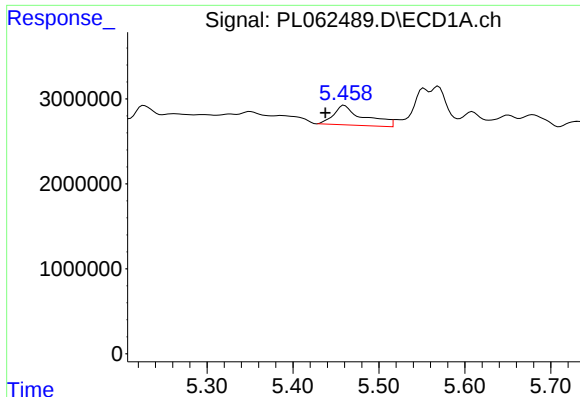

#9 Endosulfan I


R.T.: 5.460 min
Delta R.T.: 0.022 min
Response: 5590388
Conc: 3.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

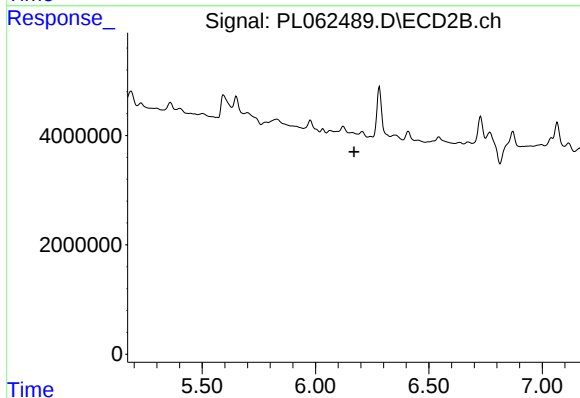


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

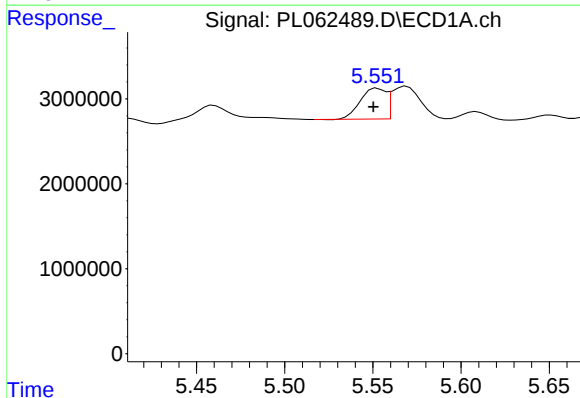


#12 4,4'-DDE

R.T.: 5.553 min
Delta R.T.: 0.002 min
Response: 3626470
Conc: 2.19 ng/ml

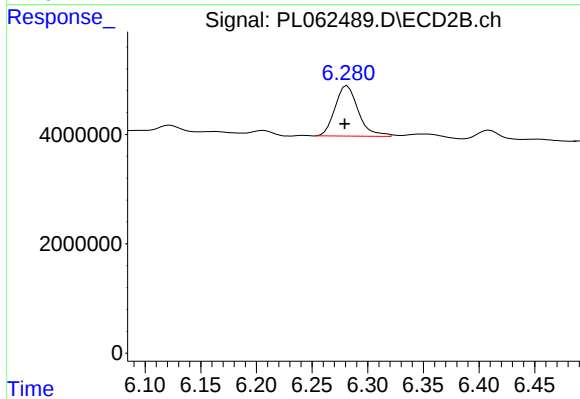

#12 4,4'-DDE


R.T.: 6.282 min
Delta R.T.: 0.002 min
Response: 13382422
Conc: 4.15 ng/ml

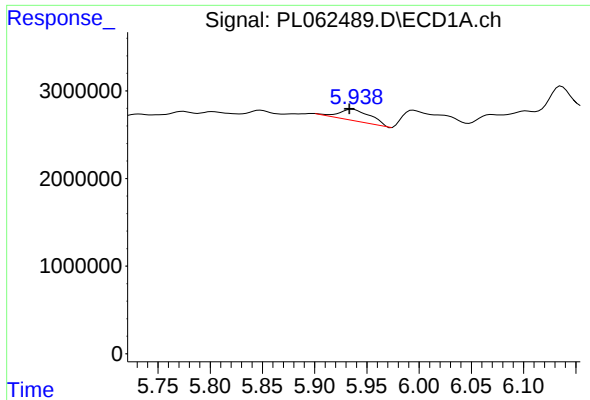

#14 Endrin


R.T.: 5.936 min
Delta R.T.: 0.003 min
Response: 2832573
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

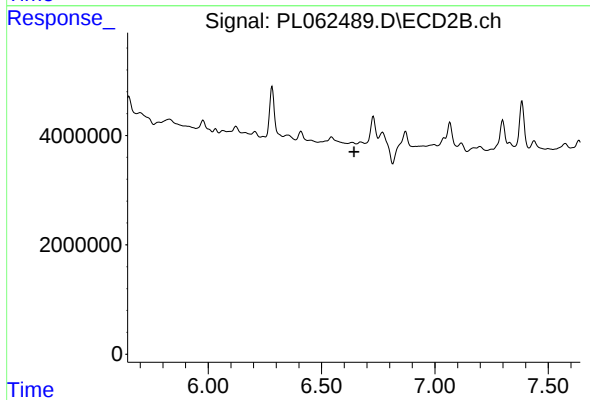


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

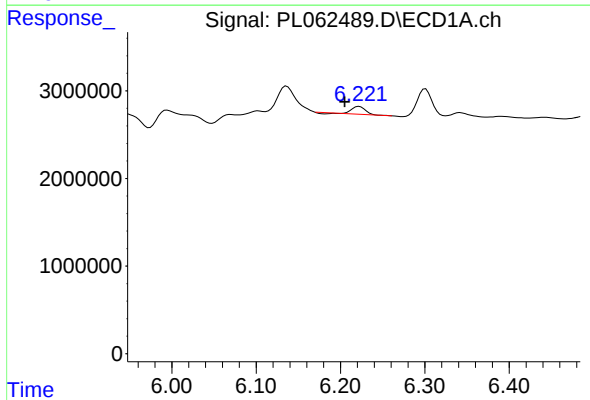


#15 Endosulfan II

R.T.: 6.222 min
Delta R.T.: 0.017 min
Response: 821217
Conc: 0.50 ng/ml

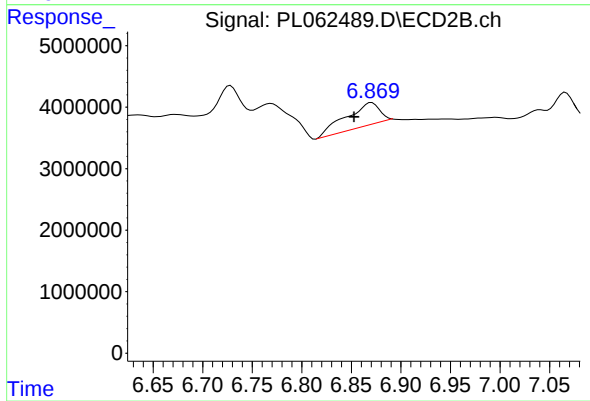

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: 0.018 min
Response: 8703277
Conc: 3.04 ng/ml

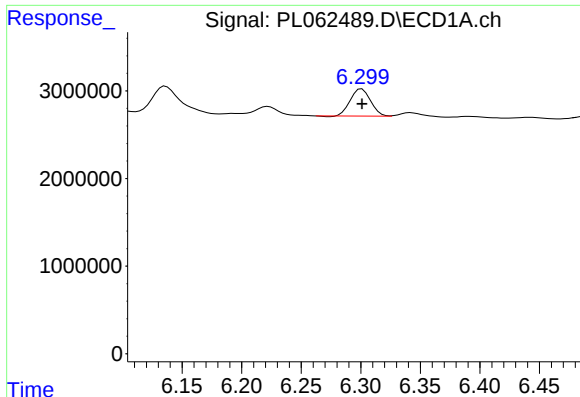

#17 4,4'-DDT


R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 3647320
Conc: 2.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

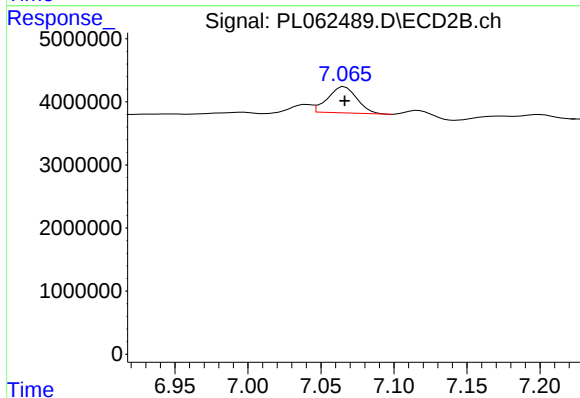


#17 4,4'-DDT

R.T.: 7.066 min
Delta R.T.: 0.000 min
Response: 5760309
Conc: 2.57 ng/ml

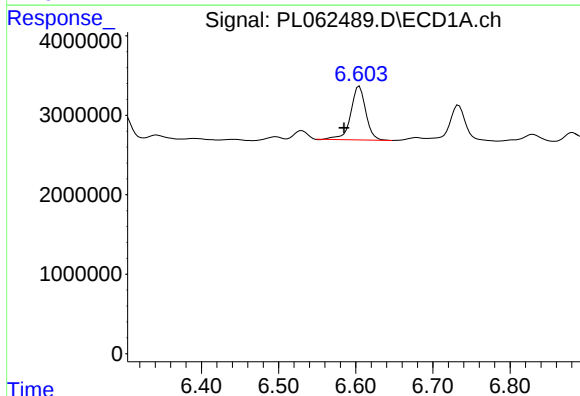


#19 Endosulfan Sulfate

R.T.: 6.605 min
Delta R.T.: 0.020 min
Response: 9157279
Conc: 5.55 ng/ml

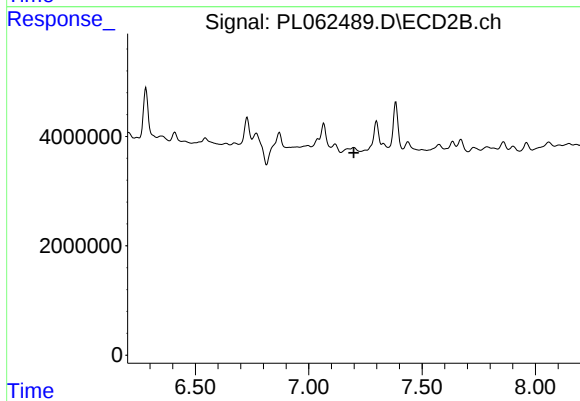

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

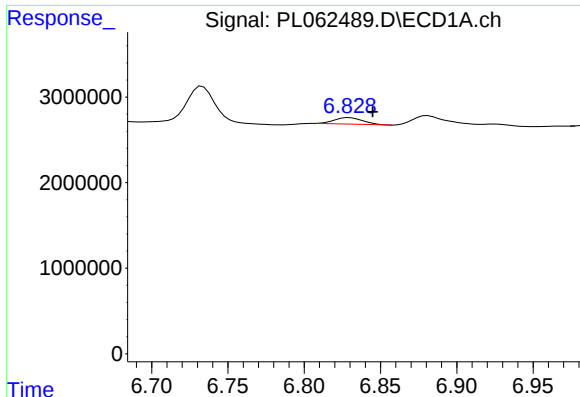

#20 Methoxychlor


R.T.: 6.830 min
Delta R.T.: -0.015 min
Response: 1000331
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

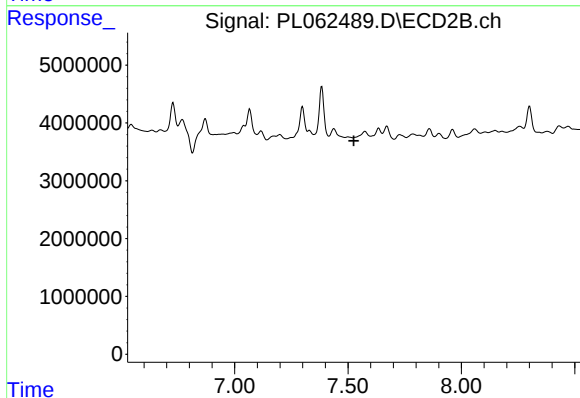


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

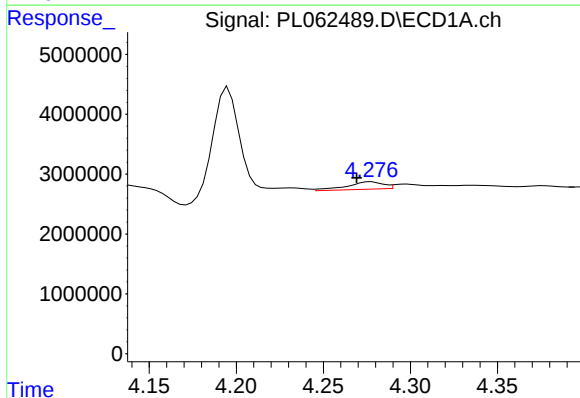


#23 Chlordane-1

R.T.: 4.277 min
Delta R.T.: 0.008 min
Response: 1807396
Conc: 35.06 ng/ml

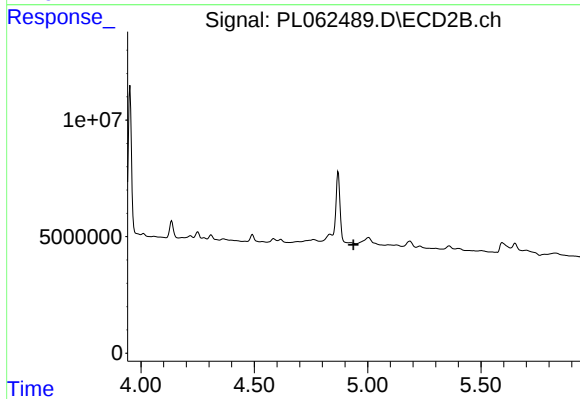

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

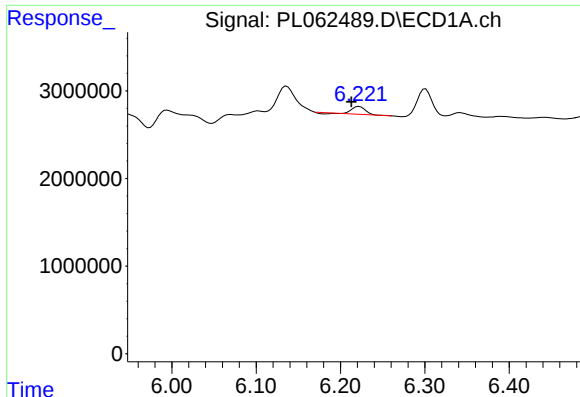

#27 Chlordane-5


R.T.: 6.222 min
Delta R.T.: 0.009 min
Response: 821217
Conc: 17.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

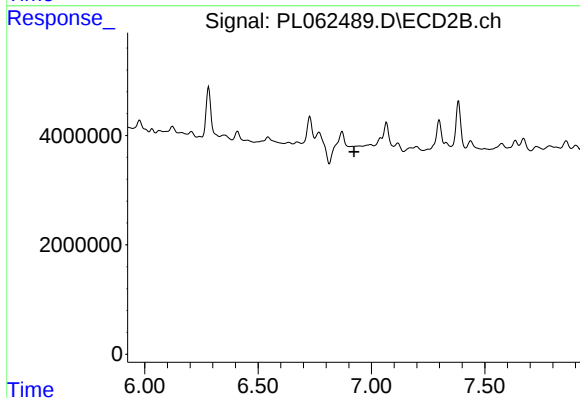


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.923 min
Response: 0
Conc: N.D.

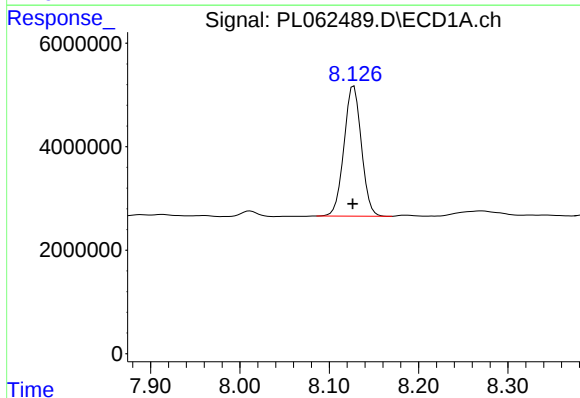

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 33996082
Conc: 21.19 ng/ml

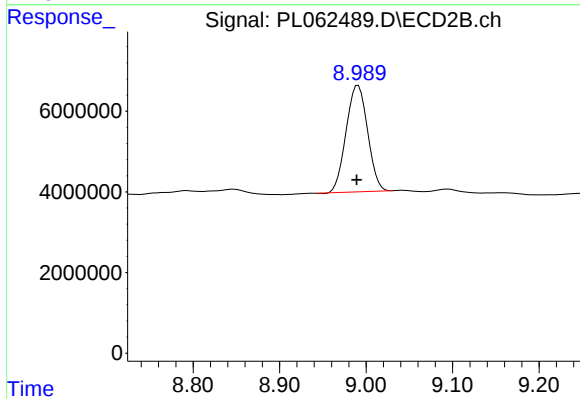

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 45432978
Conc: 21.71 ng/ml