

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
 Data File : PL062503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 21:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 09:17:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.951	35175093	56837233	20.450	19.341
28)	SA Decachlor...	8.127	8.990	28718684	38083397	17.901	18.196
Target Compounds							
8)	B Heptachlo...	0.000	5.811	0	6056242	N.D.	1.870 #
9)	A Endosulfan I	0.000	6.198f	0	2912298	N.D.	0.923 #
11)	B alpha-Chl...	0.000	6.132	0	21150418	N.D.	6.278 #
12)	B 4,4'-DDE	0.000	6.254f	0	1593499	N.D.	0.495 #
15)	B Endosulfa...	0.000	6.871f	0	1754925	N.D.	0.614 #
20)	A Methoxychlor	6.861f	0.000	531932	0	0.618	N.D. #
23)	Chlordane-1	4.299f	0.000	1834175	0	35.581	N.D. #
26)	Chlordane-4	0.000	6.132	0	21150418	N.D.	43.673 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102120\
Data File : PL062503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 21:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 09:17:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

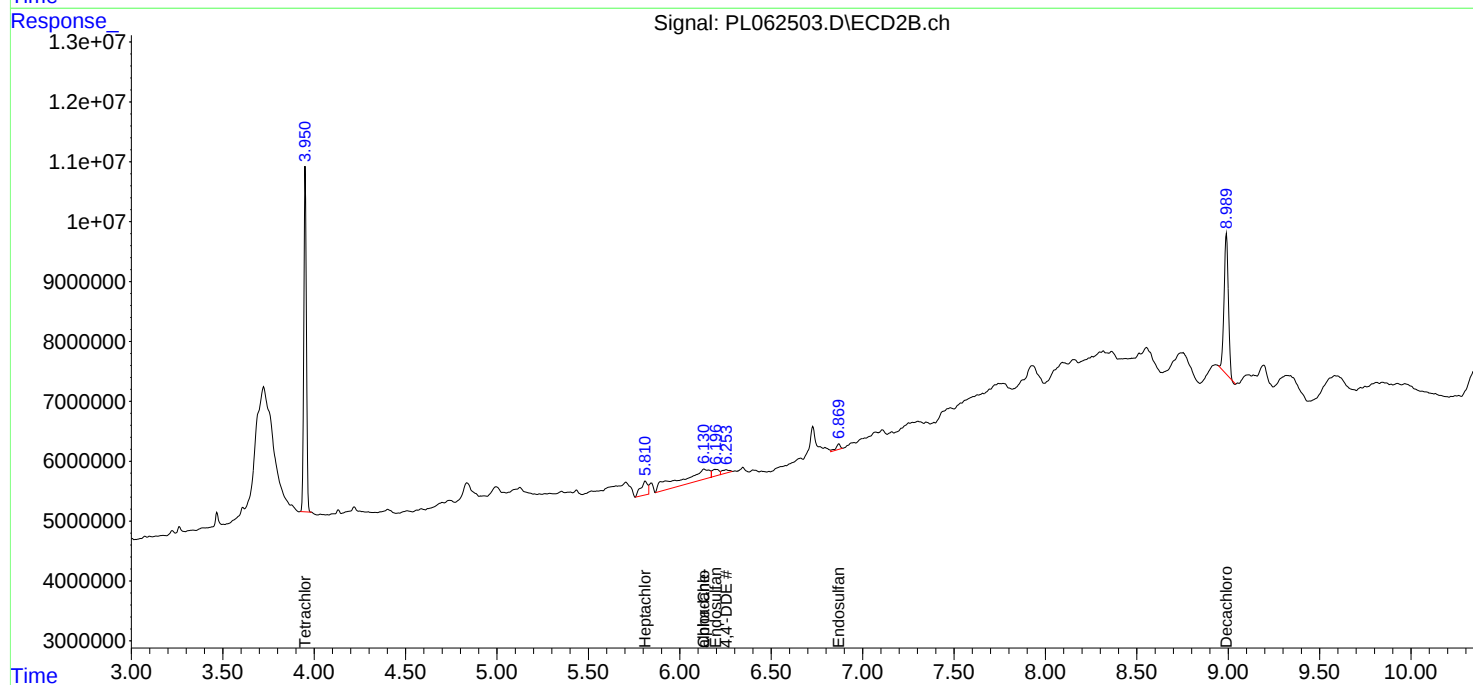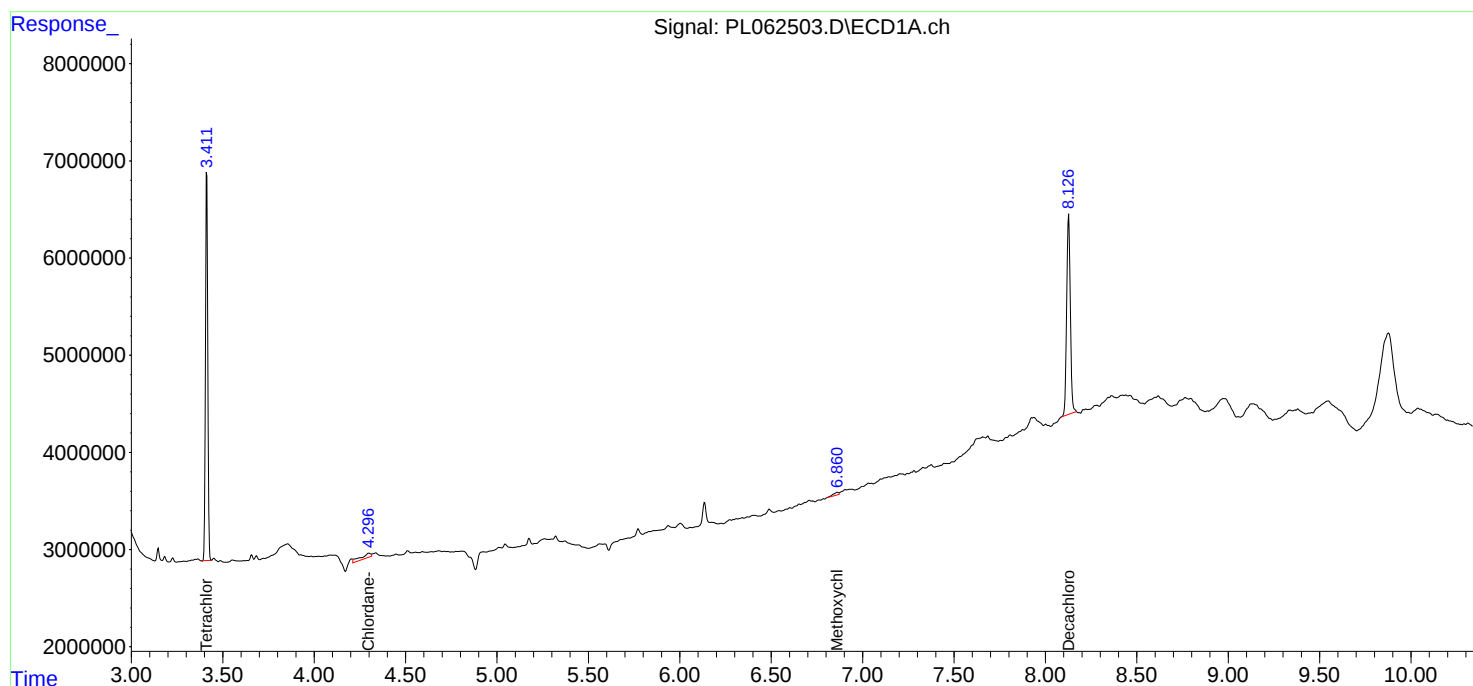


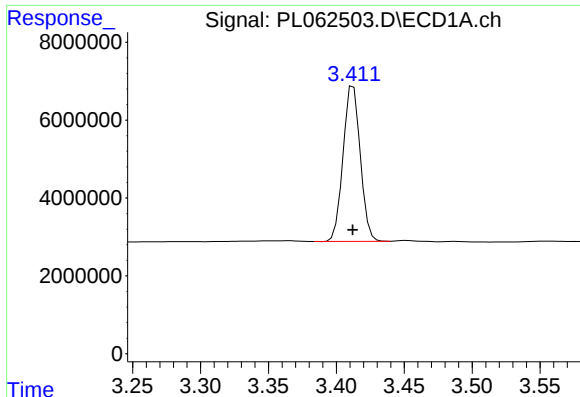

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 35175093
Conc: 20.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

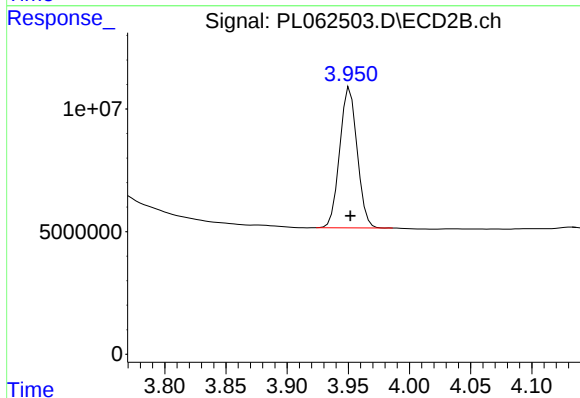


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 56837233
Conc: 19.34 ng/ml

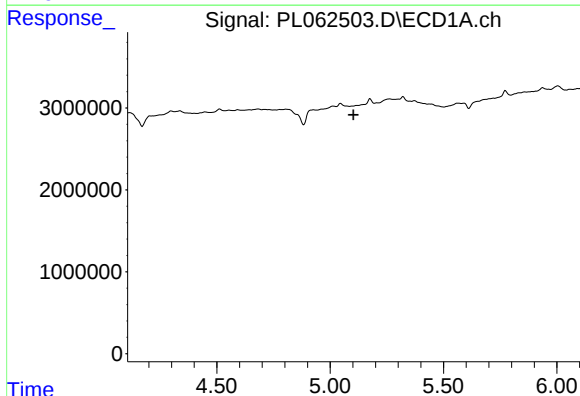


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

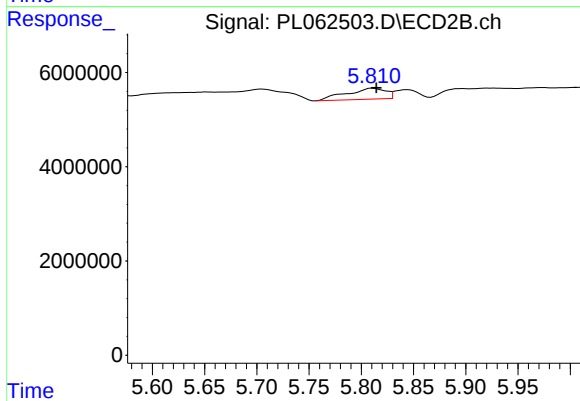

#8 Heptachlor epoxide


R.T.: 5.811 min
Delta R.T.: -0.003 min
Response: 6056242
Conc: 1.87 ng/ml

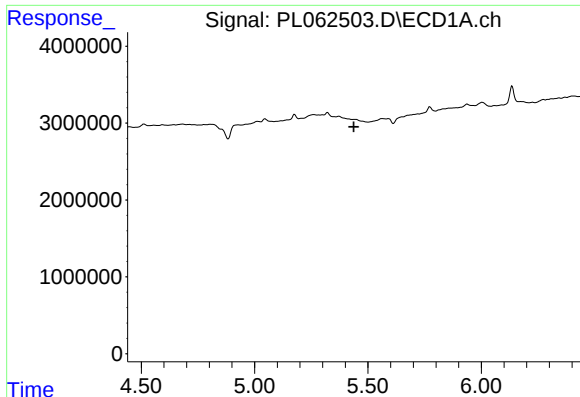

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

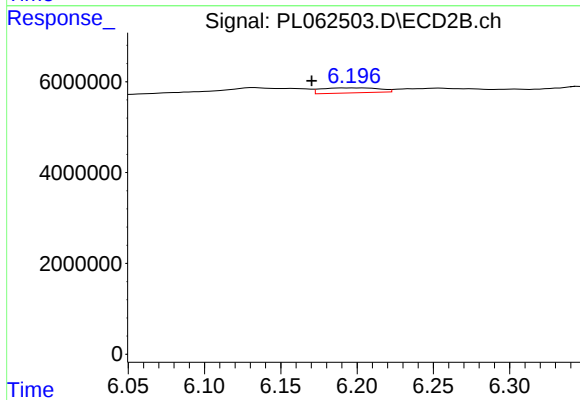


#9 Endosulfan I

R.T.: 6.198 min
Delta R.T.: 0.028 min
Response: 2912298
Conc: 0.92 ng/ml

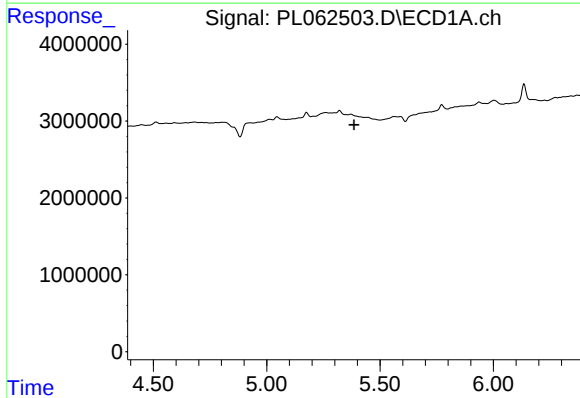


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.386 min
Response: 0
Conc: N.D.

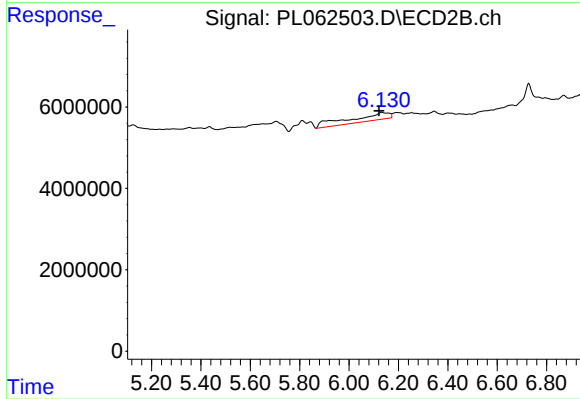

#11 alpha-Chlordane


R.T.: 6.132 min
Delta R.T.: 0.011 min
Response: 21150418
Conc: 6.28 ng/ml

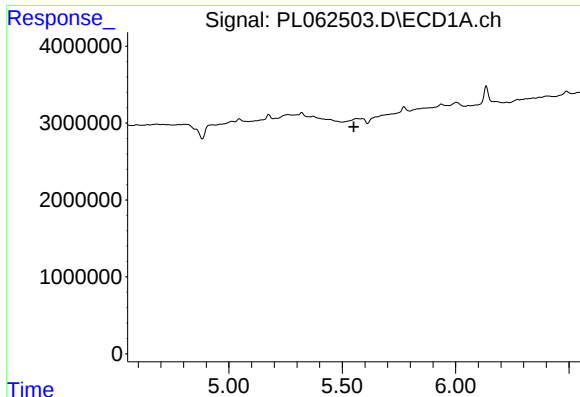

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

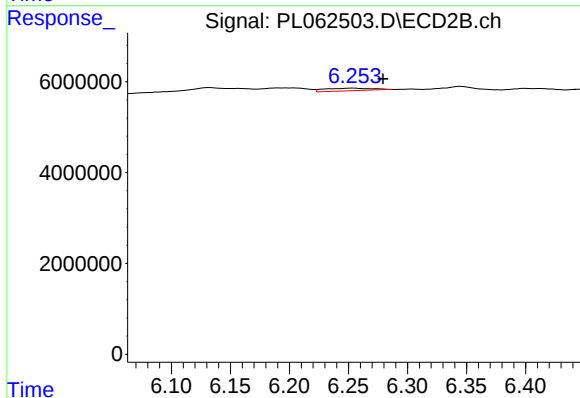


#12 4,4'-DDE

R.T.: 6.254 min
Delta R.T.: -0.025 min
Response: 1593499
Conc: 0.49 ng/ml

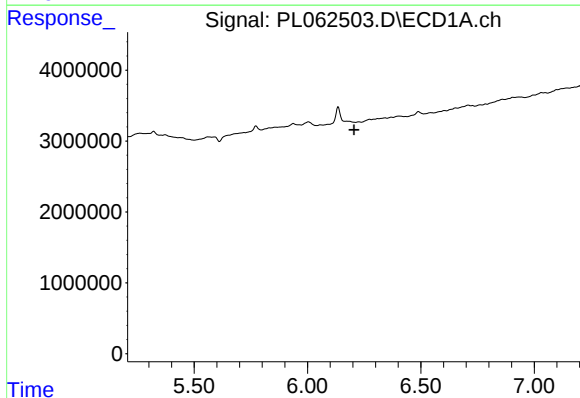


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

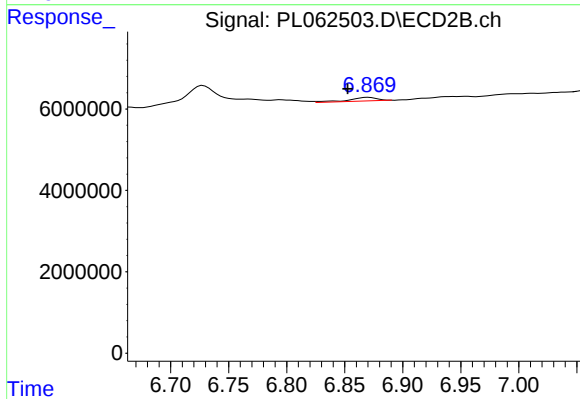

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: 0.018 min
Response: 1754925
Conc: 0.61 ng/ml

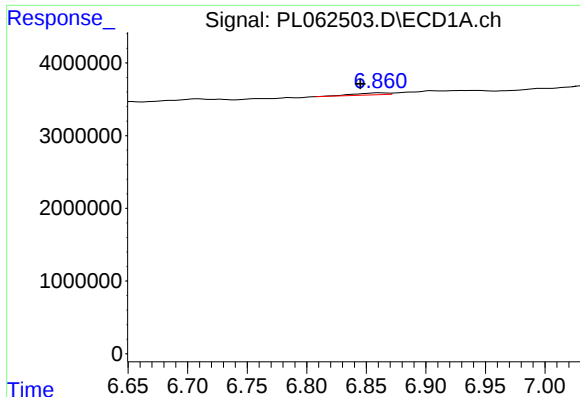

#20 Methoxychlor


R.T.: 6.861 min
Delta R.T.: 0.016 min
Response: 531932
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

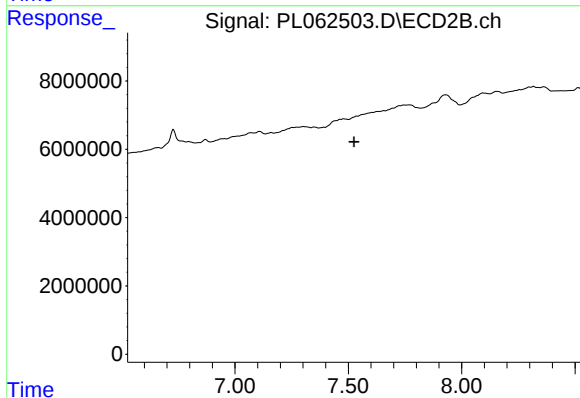


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

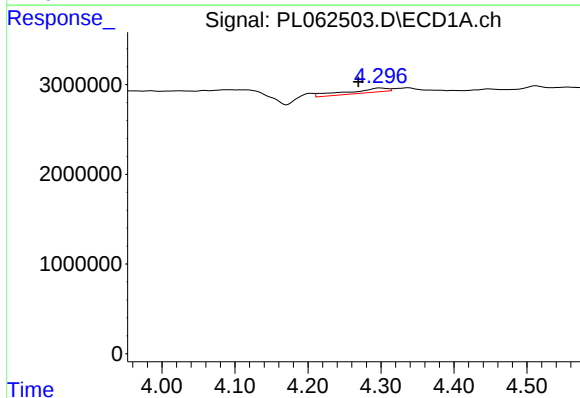


#23 Chlordane-1

R.T.: 4.299 min
Delta R.T.: 0.029 min
Response: 1834175
Conc: 35.58 ng/ml

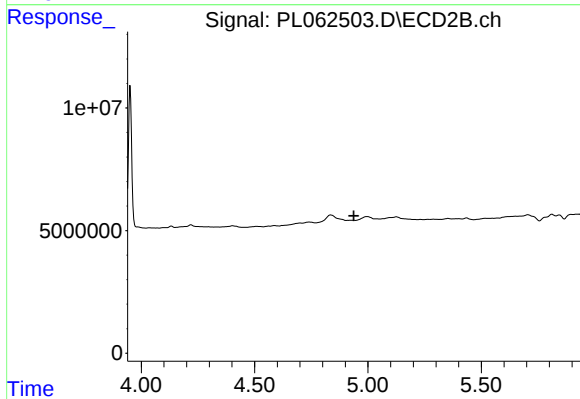

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

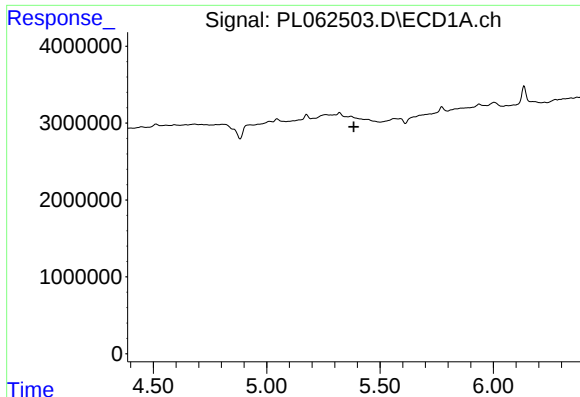

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

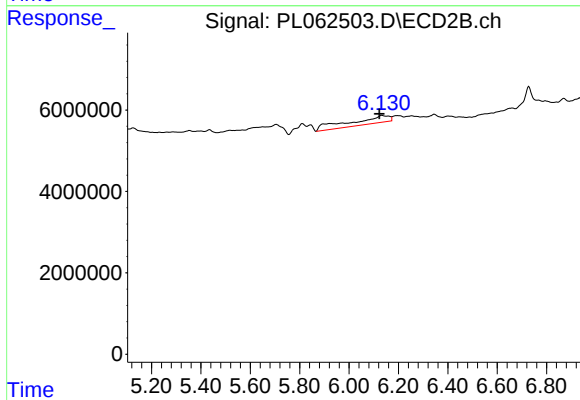


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: 0.010 min
Response: 21150418
Conc: 43.67 ng/ml

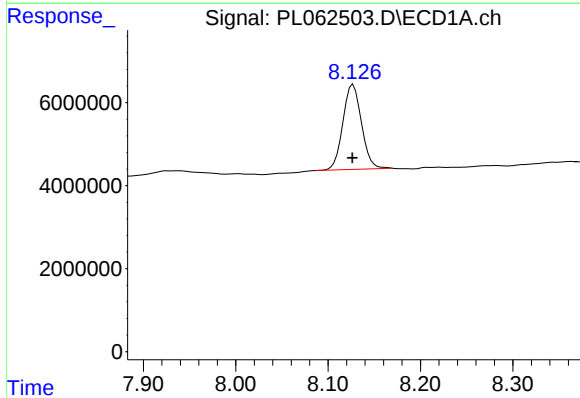

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 28718684
Conc: 17.90 ng/ml

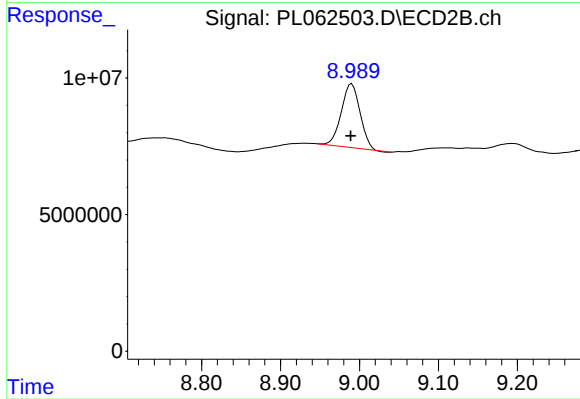

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 38083397
Conc: 18.20 ng/ml